

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060818\
 Data File : BM015571.D
 Acq On : 08 Jun 2018 19:42
 Operator : SJ/JU
 Sample : PB110064BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 08 23:06:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 08 23:05:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.35	152	64352	20.00	ng/ul	0.00
18) Naphthalene-d8	11.17	136	331188	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	209772	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.69	188	557475	20.00	ng/ul	0.00
77) Chrysene-d12	21.79	240	675761	20.00	ng/ul	0.00
85) Perylene-d12	24.20	264	767106	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.55	96	10143	7.66	ng/uL	0.00
5) Phenol-d5	7.49	99	187615	32.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.66	67	132121	37.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.87	132	157862	35.34	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	161401	32.07	ng/ul	0.00
19) Nitrobenzene-d5	9.53	128	81450	36.58	ng/ul	0.00
22) 2-Nitrophenol-d4	10.26	143	86630	36.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.79	165	160116	32.28	ng/ul	0.00
29) 4-Chloroaniline-d4	11.32	131	270225	48.89	ng/ul	0.00
43) Dimethylphthalate-d6	14.36	166	734892	42.32	ng/ul	0.00
46) Acenaphthylene-d8	14.66	160	773571	41.30	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	106980	31.91	ng/ul	0.00
57) Fluorene-d10	15.94	176	574050	39.06	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	86462	25.75	ng/ul	0.00
70) Anthracene-d10	17.78	188	1012226	39.83	ng/ul	0.00
78) Pyrene-d10	20.03	212	1178012	40.53	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.05	264	1529810	39.78	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	9.05	70	4673	1.122	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060818\
Data File : BM015571.D
Acq On : 08 Jun 2018 19:42
Operator : SJ/JU
Sample : PB110064BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 08 23:06:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 08 23:05:23 2018
Response via : Initial Calibration

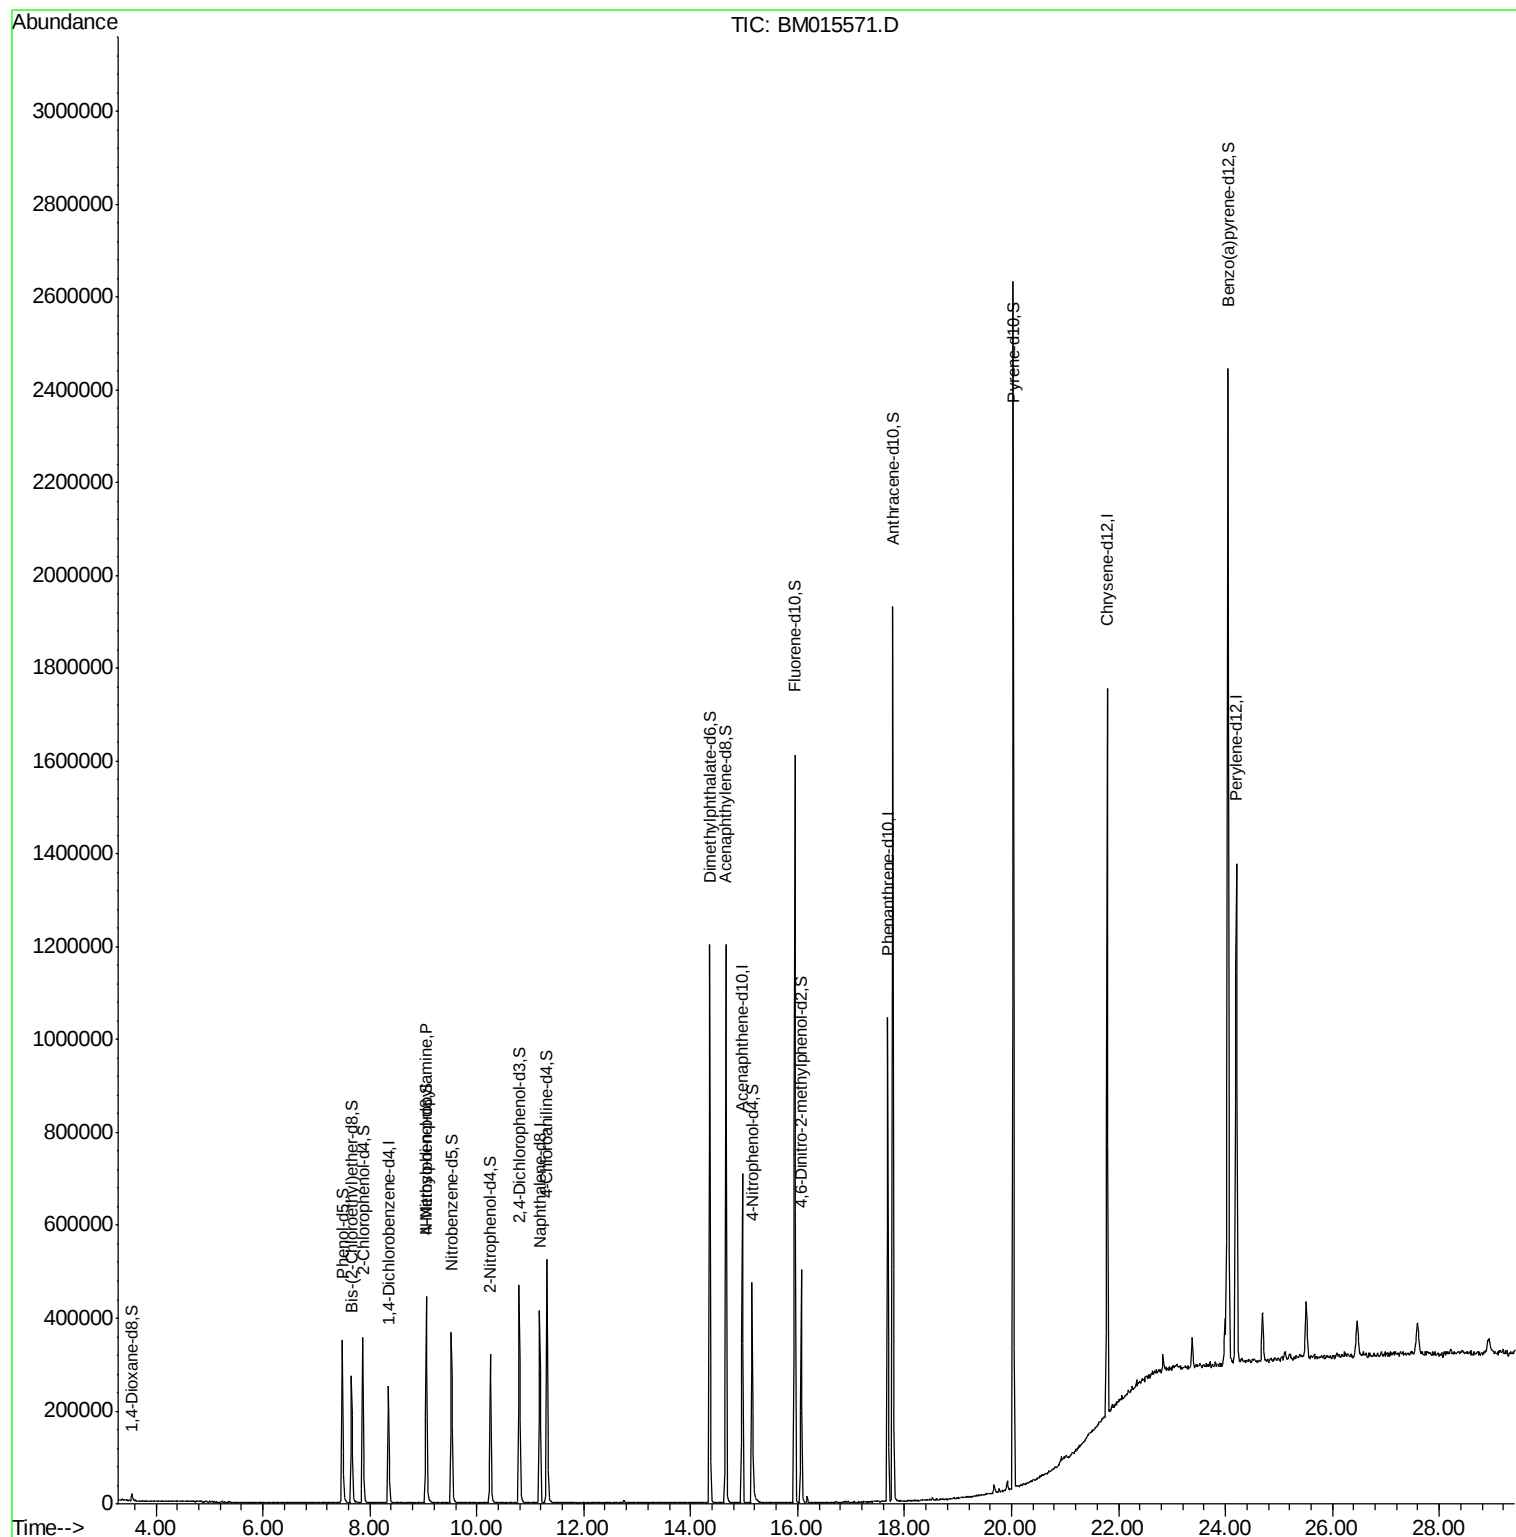

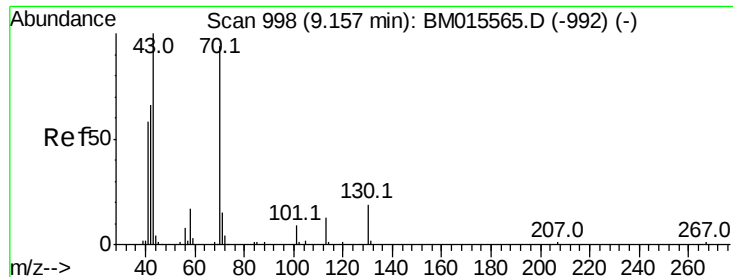

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.122 ng/ul
 RT: 9.05 min Scan# 980
 Delta R.T. -0.11 min
 Lab File: BM015571.D
 Acq: 08 Jun 2018 19:42

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 70 Resp: 4673
 Ion Ratio Lower Upper
 70 100
 42 500.5 35.4 53.0#
 101 0.0 8.4 12.6#
 130 0.0 18.2 27.4#

