

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060818\
 Data File : BM015590.D
 Acq On : 09 Jun 2018 07:29
 Operator : SJ/JU
 Sample : J3346-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 11 00:46:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 09 02:29:49 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.35	152	89238	20.00	ng/ul	0.00
18) Naphthalene-d8	11.17	136	452715	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	294307	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.68	188	733175	20.00	ng/ul	0.00
77) Chrysene-d12	21.79	240	916700	20.00	ng/ul	0.00
85) Perylene-d12	24.20	264	1029902	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.55	96	5723	3.12	ng/uL	0.00
5) Phenol-d5	7.49	99	171015	21.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.66	67	116000	23.70	ng/ul	0.00
9) 2-Chlorophenol-d4	7.87	132	143371	23.15	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	154709	22.17	ng/ul	0.00
19) Nitrobenzene-d5	9.53	128	71204	23.39	ng/ul	0.00
22) 2-Nitrophenol-d4	10.26	143	72508	22.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.79	165	154183	22.74	ng/ul	0.00
29) 4-Chloroaniline-d4	11.32	131	62993	8.34	ng/ul	0.00
43) Dimethylphthalate-d6	14.36	166	554402	22.75	ng/ul	0.00
46) Acenaphthylene-d8	14.66	160	660456	25.13	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	84543	17.97	ng/ul	0.00
57) Fluorene-d10	15.94	176	546357	26.50	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	64639	14.64	ng/ul	0.00
70) Anthracene-d10	17.78	188	900380	26.94	ng/ul	0.00
78) Pyrene-d10	20.03	212	1088044	27.59	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.04	264	1364578	26.43	ng/ul	0.00
Target Compounds						
6) Phenol	7.52	94	19056	2.264	ng/ul#	81
44) Dimethylphthalate	14.40	163	226041	9.085	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060818\
Data File : BM015590.D
Acq On : 09 Jun 2018 07:29
Operator : SJ/JU
Sample : J3346-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 11 00:46:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 09 02:29:49 2018
Response via : Initial Calibration

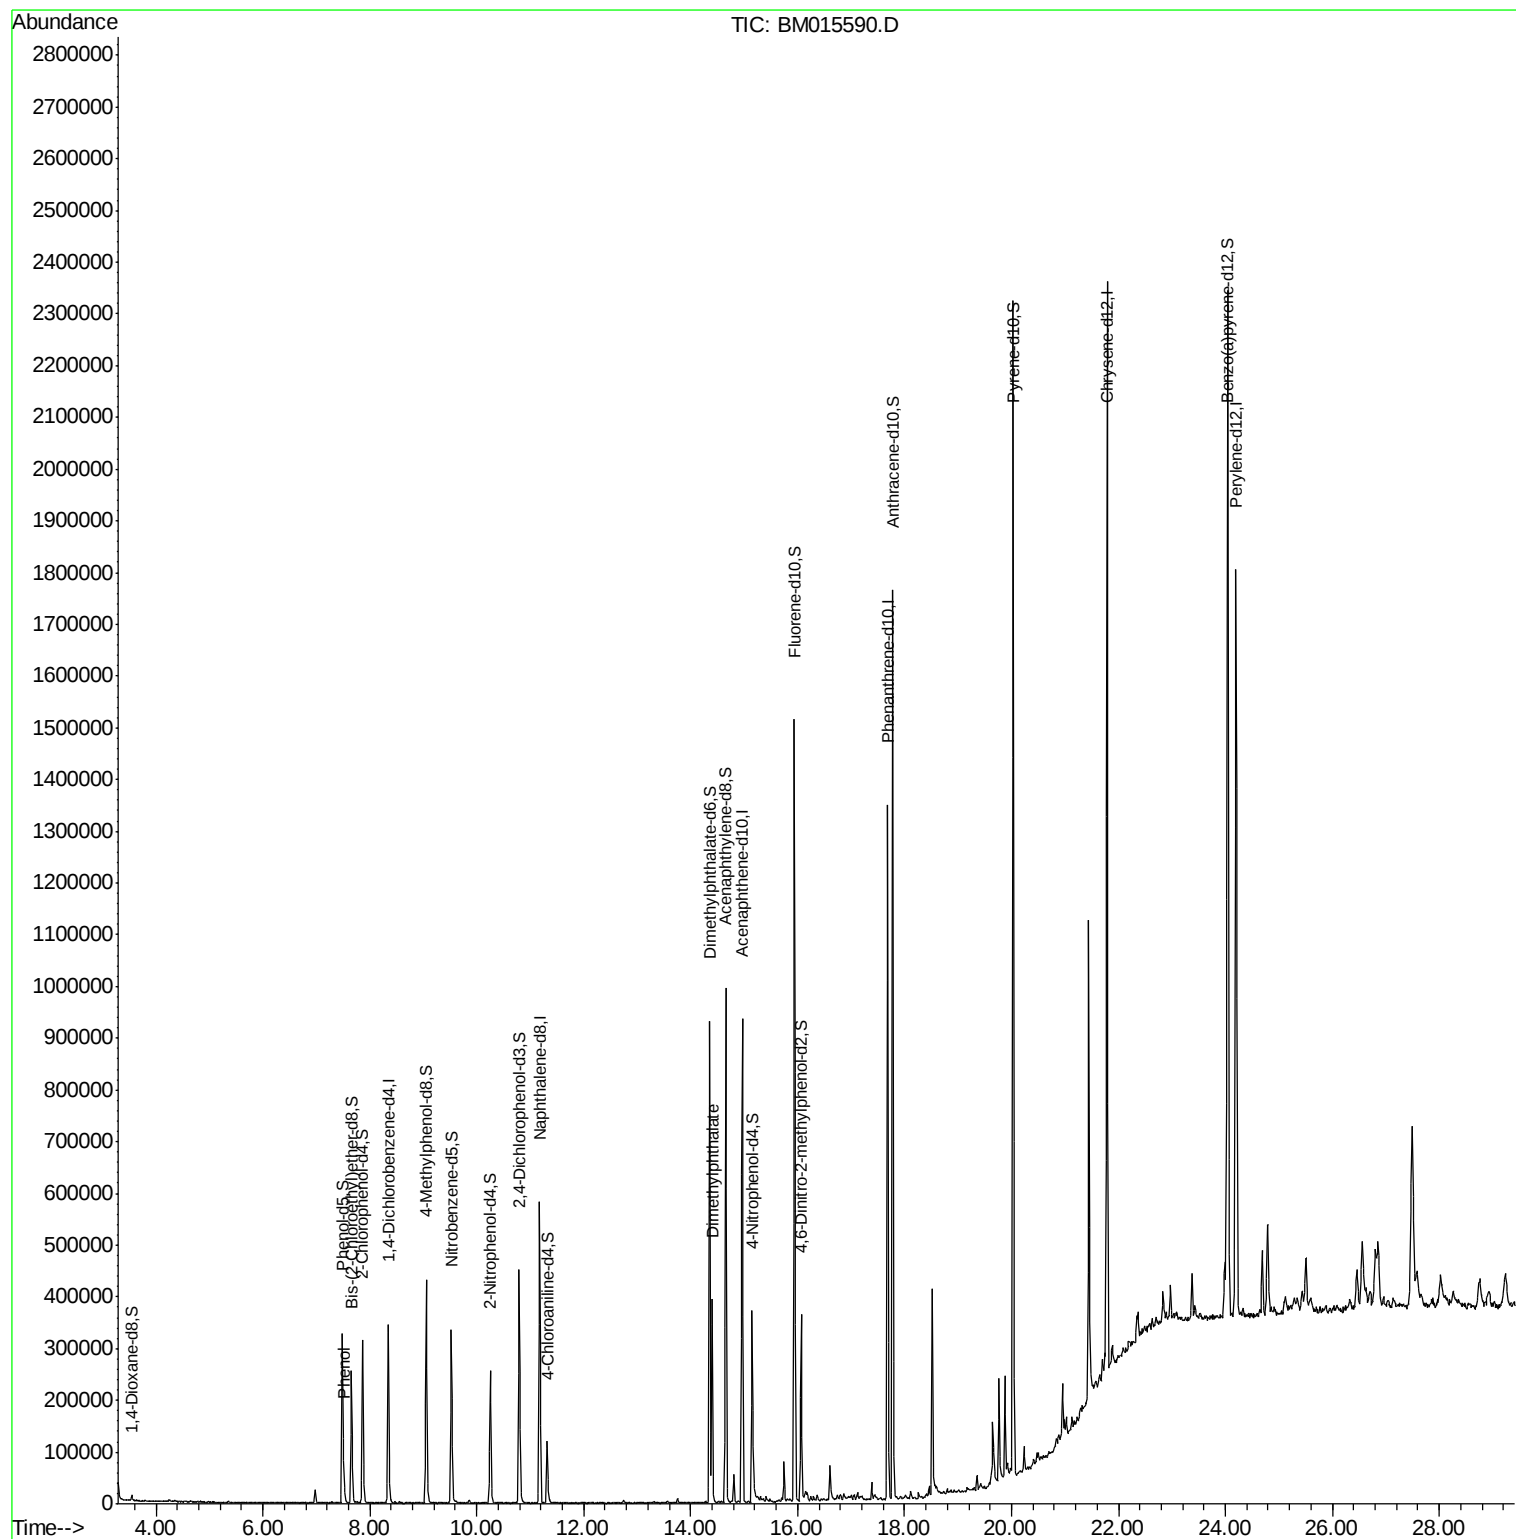

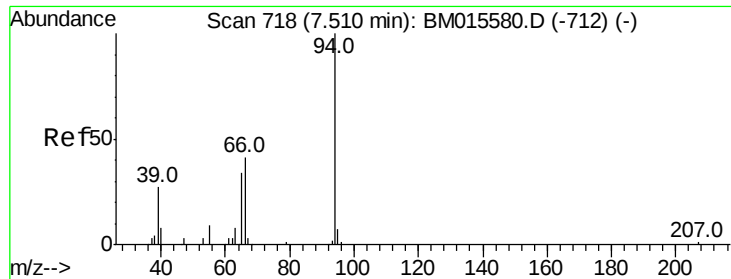

#6

Phenol

Concen: 2.264 ng/ul

RT: 7.52 min Scan# 719

Delta R.T. 0.01 min

Lab File: BM015590.D

Acq: 09 Jun 2018 07:29

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 94 Resp: 19056

Ion Ratio Lower Upper

94 100

65 36.9 21.0 31.6#


66 47.3 29.3 43.9#

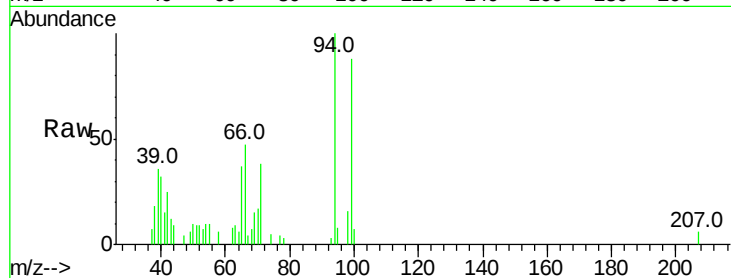



Abundance Ion 94.00 (93.70 to 94.70): BM015580.D (-712) (-)

Ion 65.00 (64.70 to 65.70): BM015580.D (-712) (-)

Ion 66.00 (65.70 to 66.70): BM015580.D (-712) (-)

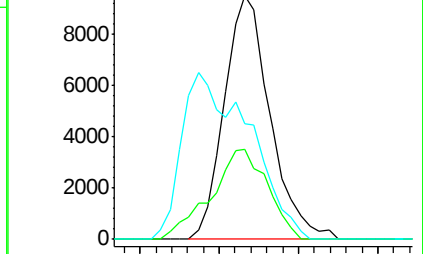

Time-->

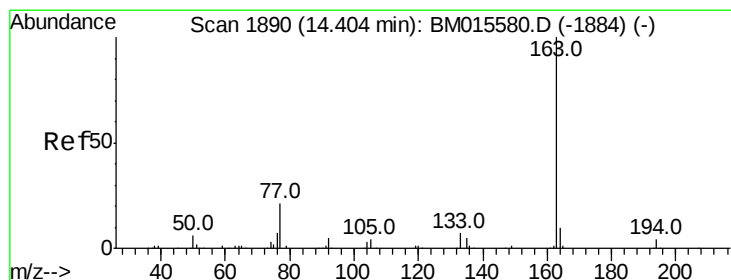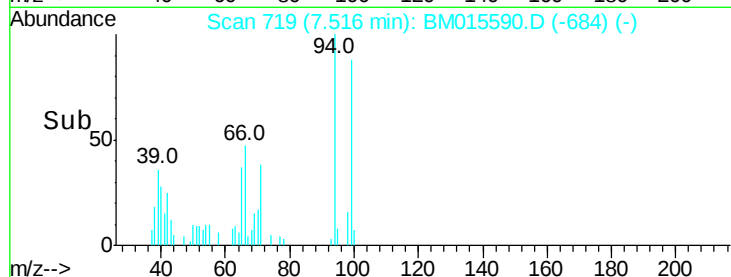

#44

Dimethylphthalate

Concen: 9.085 ng/ul

RT: 14.40 min Scan# 1890

Delta R.T. -0.00 min

Lab File: BM015590.D

Acq: 09 Jun 2018 07:29


Tgt Ion:163 Resp: 226041

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8


164 10.7 7.8 11.8

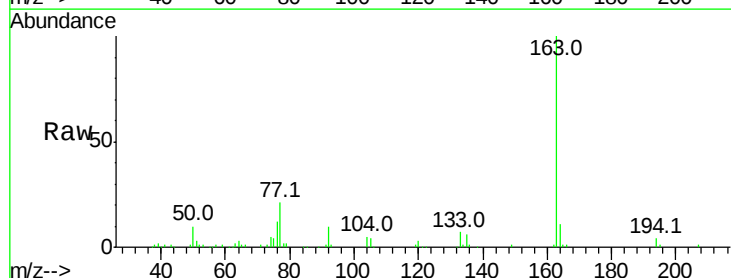

Abundance Ion 163.00 (162.70 to 163.70): BM015580.D (-1884) (-)

Ion 194.00 (193.70 to 194.70): BM015580.D (-1884) (-)

Ion 164.00 (163.70 to 164.70): BM015580.D (-1884) (-)

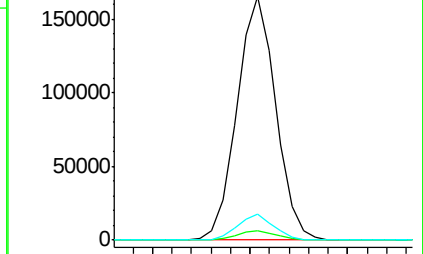

Time-->

