

Quantitation Report (QT Reviewed)


Instrument :
BNA_M
ClientSampled :
DAXH3

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060818\
Data File : BM015594.D
Acq On : 09 Jun 2018 09:57
Operator : SJ/JU
Sample : J3346-11
Misc :
ALS Vial : 37 Sample Multiplier: 1

Manual Integrations
APPROVED

Sohil
6/11/2018 3:59:28 PM

Quant Time: Jun 11 01:58:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 09 02:29:49 2018
Response via : Initial Calibration

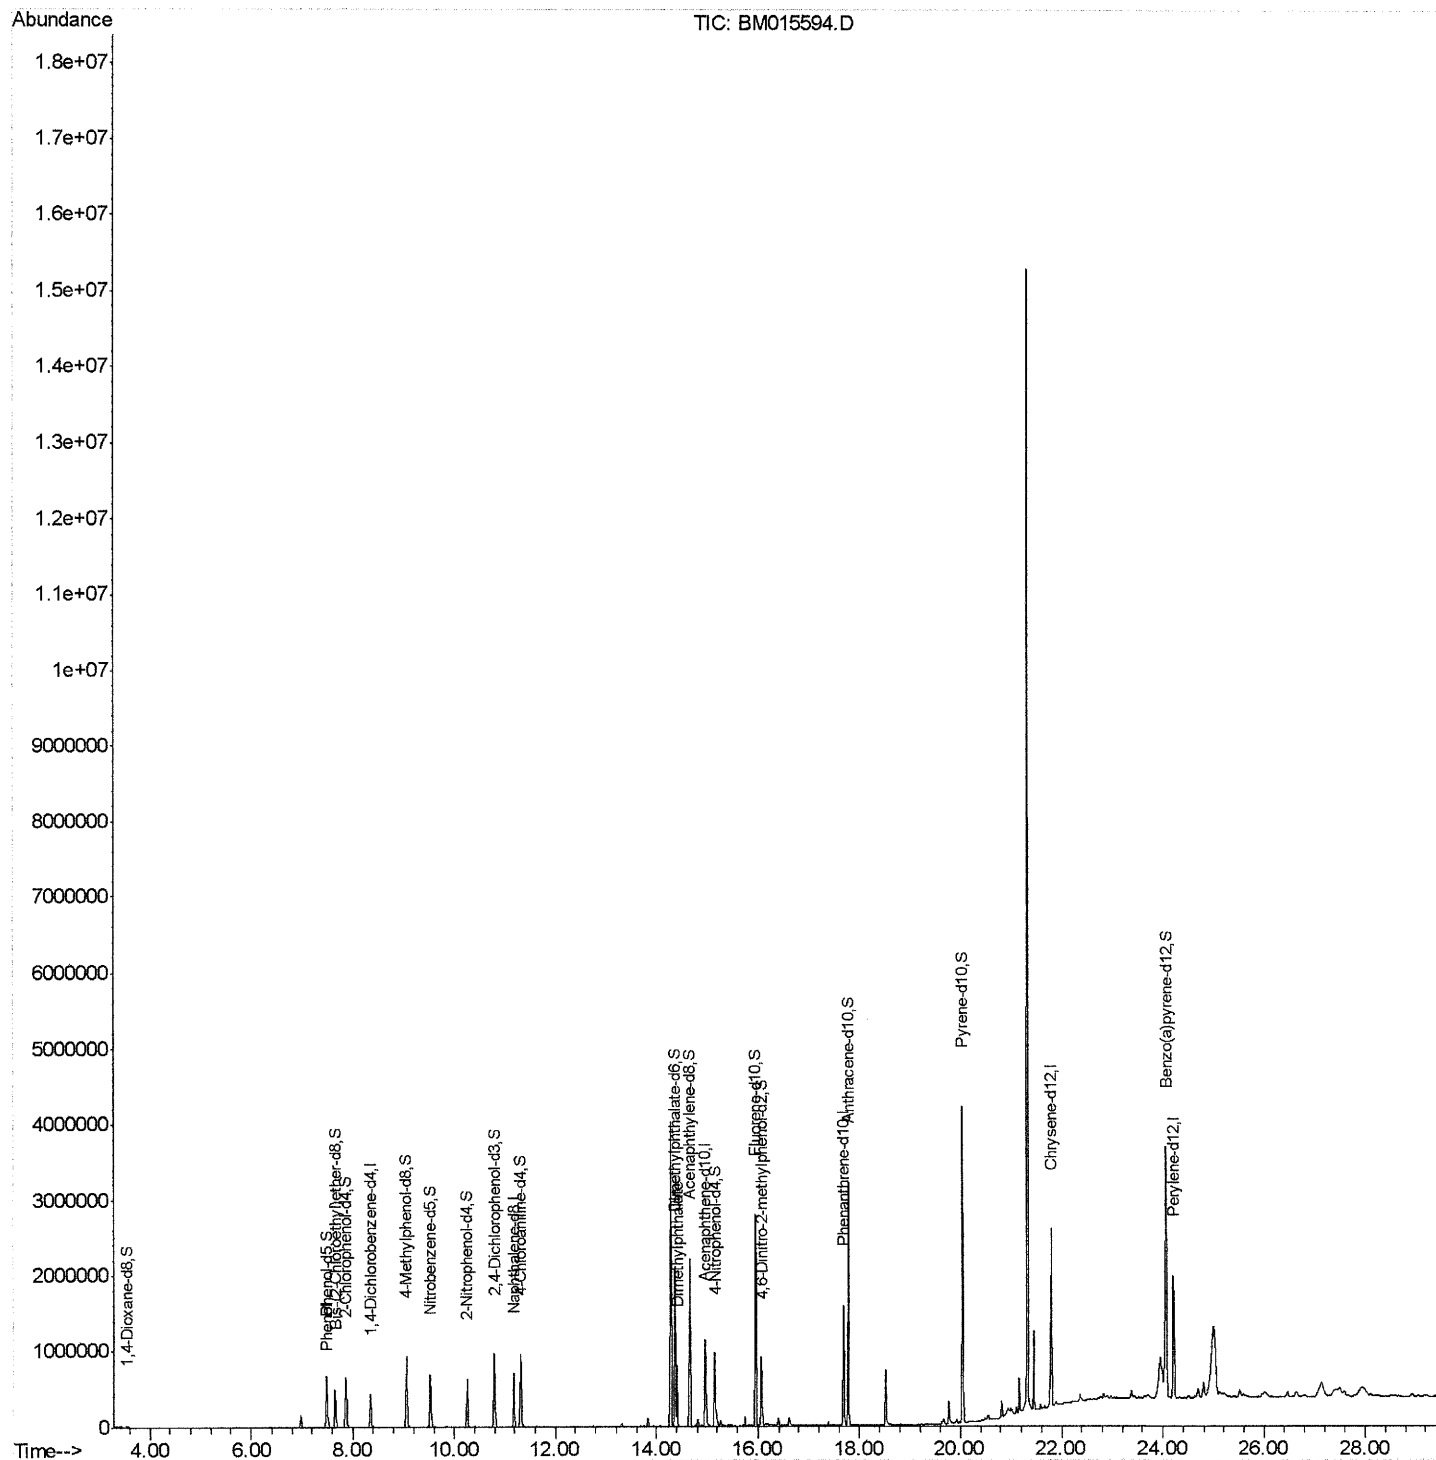

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060818\
 Data File : BM015594.D
 Acq On : 09 Jun 2018 09:57
 Operator : SJ/JU
 Sample : J3346-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DAXH3

Manual Integrations
 APPROVED

Sohil
 6/11/2018 3:59:28 PM

Quant Time: Jun 11 00:47:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 09 02:29:49 2018
 Response via : Initial Calibration

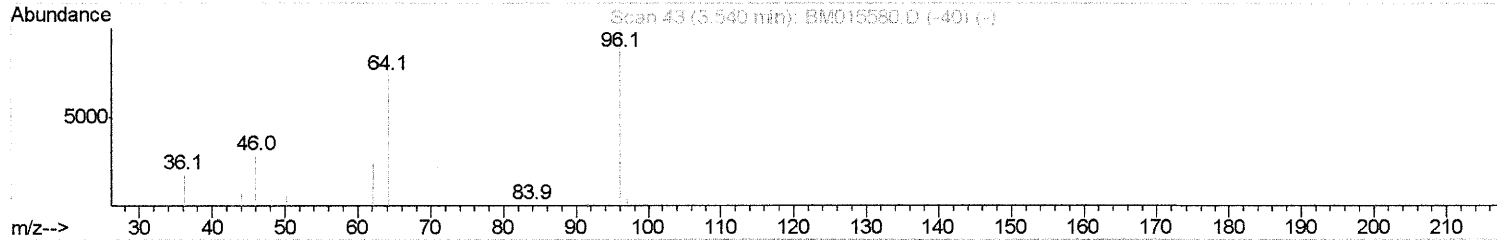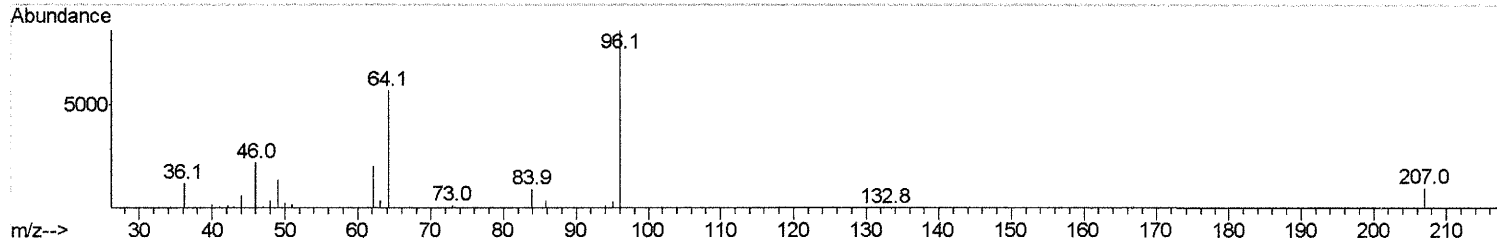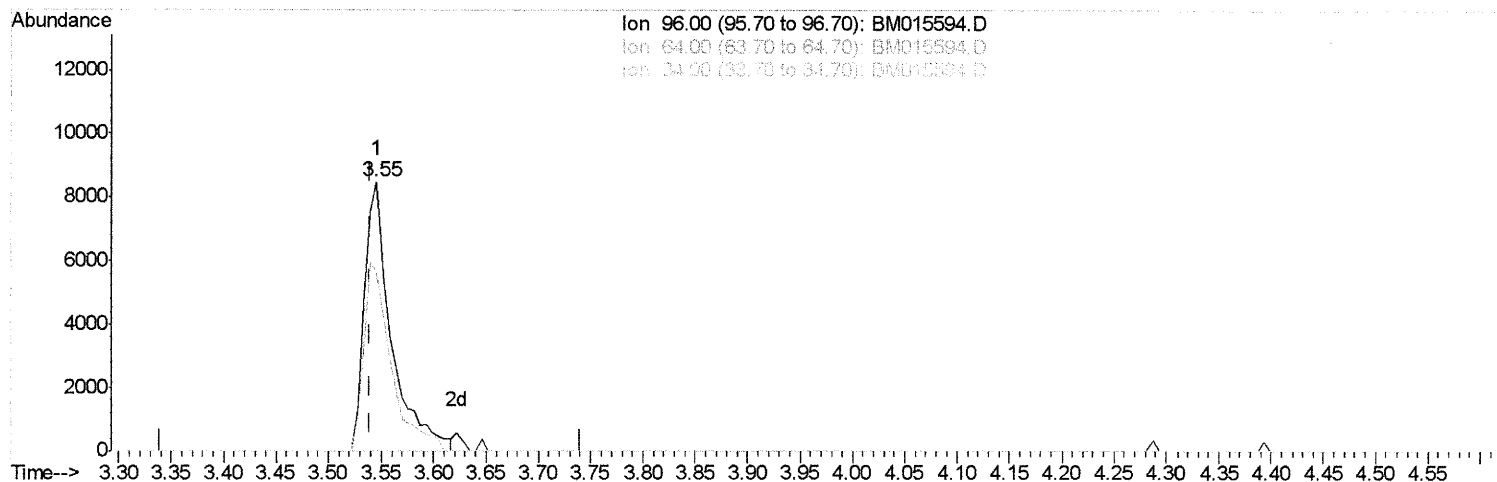

TIC: BM015594.D

(3) 1,4-Dioxane-d8 (S)

3.546min (+0.006) 6.32ng/uL

response 14737

Ion	Exp%	Act%
96.00	100	100
64.00	67.80	71.89
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060818\
 Data File : BM015594.D
 Acq On : 09 Jun 2018 09:57
 Operator : SJ/JU
 Sample : J3346-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DAXH3

Manual Integrations
 APPROVED

Sohil
 6/11/2018 3:59:28 PM

Quant Time: Jun 11 00:47:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 09 02:29:49 2018
 Response via : Initial Calibration

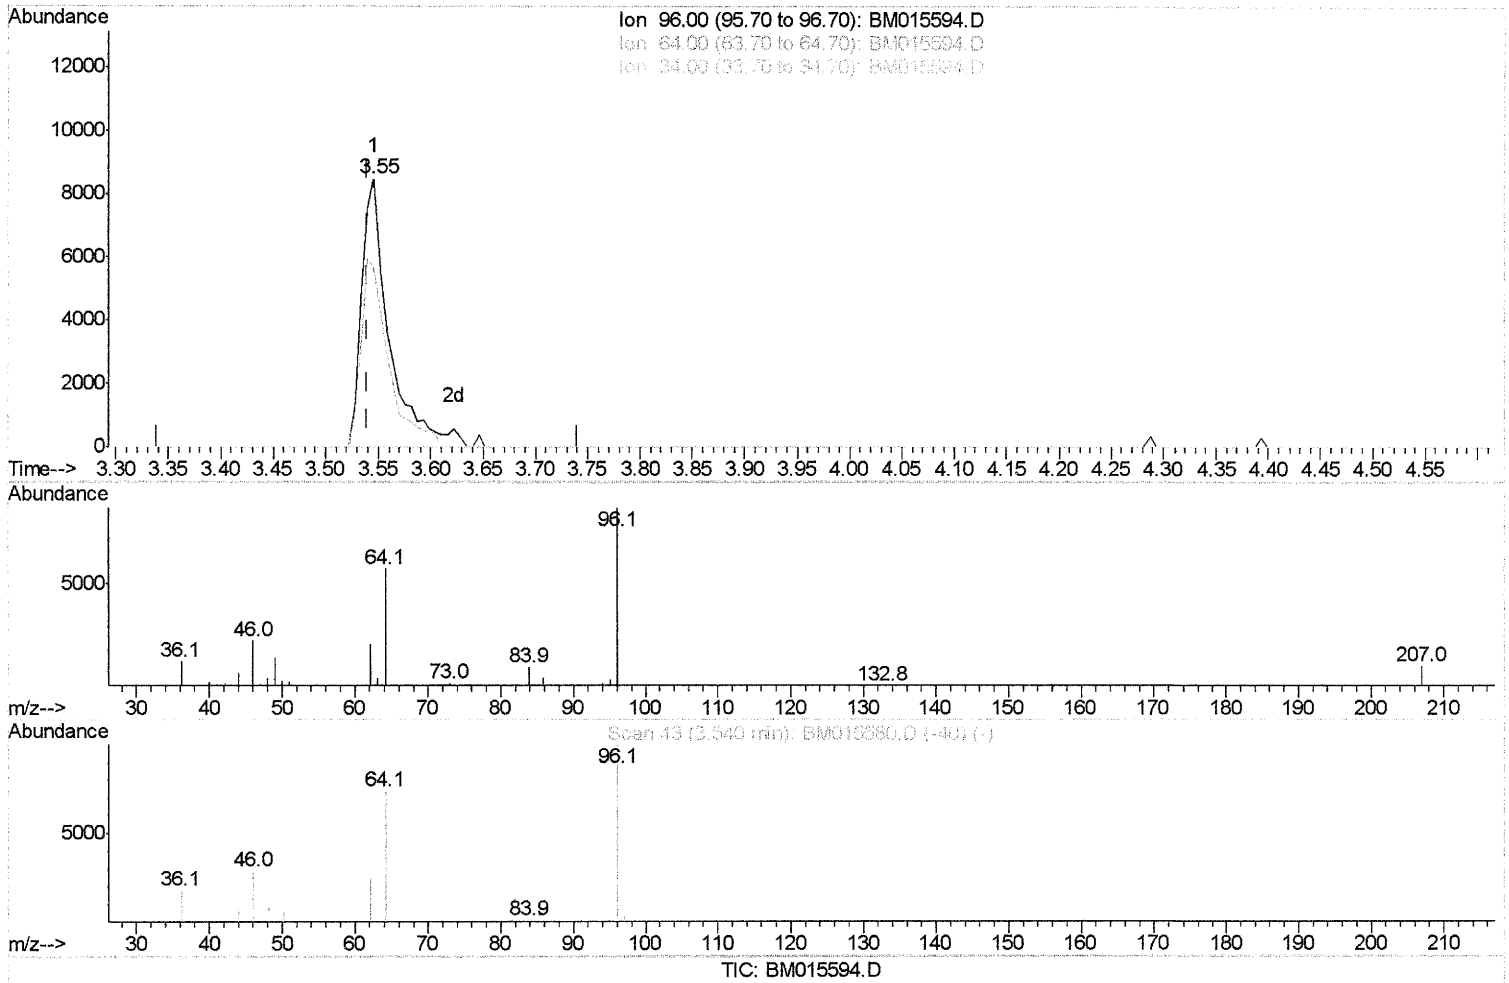

(3) 1,4-Dioxane-d8 (S)

3.546min (+0.006) 6.45ng/uL m

SJ 6/11/18

response 15050

Ion	Exp%	Act%
96.00	100	100
64.00	67.80	70.40
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060818\
 Data File : BM015594.D
 Acq On : 09 Jun 2018 09:57
 Operator : SJ/JU
 Sample : J3346-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 DAXH3

Manual Integrations
 APPROVED

Sohil
 6/11/2018 3:59:28 PM

Quant Time: Jun 11 01:58:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 09 02:29:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.35	152	113301	20.00	ng/ul	0.00
18) Naphthalene-d8	11.17	136	565487	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	357179	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.68	188	864493	20.00	ng/ul	0.00
77) Chrysene-d12	21.79	240	1020766	20.00	ng/ul	0.00
85) Perylene-d12	24.20	264	1140670	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.55	96	15050m	6.45	ng/uL	0.00
5) Phenol-d5	7.49	99	351478	34.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.66	67	226940	36.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.86	132	289072	36.76	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	318280	35.92	ng/ul	0.00
19) Nitrobenzene-d5	9.53	128	150308	39.53	ng/ul	0.00
22) 2-Nitrophenol-d4	10.25	143	171651	41.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.79	165	322218	38.05	ng/ul	0.00
29) 4-Chloroaniline-d4	11.31	131	466691	49.46	ng/ul	0.00
43) Dimethylphthalate-d6	14.36	166	1201825	40.64	ng/ul	0.00
46) Acenaphthylene-d8	14.66	160	1421329	44.56	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	210960	36.96	ng/ul	0.00
57) Fluorene-d10	15.94	176	1028148	41.09	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	160383	30.80	ng/ul	0.00
70) Anthracene-d10	17.78	188	1652092	41.92	ng/ul	0.00
78) Pyrene-d10	20.03	212	1903116	43.34	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.05	264	2390434	41.81	ng/ul	0.00

5/6/11/18

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
6) Phenol	7.51	94	38136	3.569	ng/ul#	82
44) Dimethylphthalate	14.40	163	440687	14.594	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed