

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060818\
 Data File : BM015595.D
 Acq On : 09 Jun 2018 10:34
 Operator : SJ/JU
 Sample : J3261-01DL 5X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C07Q3DL

Manual Integrations
 APPROVED

Sohil
 6/11/2018 3:59:29 PM

Quant Time: Jun 11 12:38:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 09 02:29:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.35	152	100862	20.00	ng/ul	0.00
18) Naphthalene-d8	11.17	136	504303	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	336998	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.68	188	861012	20.00	ng/ul	0.00
77) Chrysene-d12	21.79	240	1039685	20.00	ng/ul	0.00
85) Perylene-d12	24.20	264	1178436	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.54	96	119	0.06	ng/uL	0.00
5) Phenol-d5	7.50	99	11343	1.24	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.66	67	39184	7.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.87	132	38410	5.49	ng/ul	0.00
13) 4-Methylphenol-d8	9.06	113	24535	3.11	ng/ul	0.00
19) Nitrobenzene-d5	9.53	128	24418	7.20	ng/ul	0.00
22) 2-Nitrophenol-d4	10.26	143	25895	7.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.80	165	48460	6.42	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
43) Dimethylphthalate-d6	14.36	166	230179	8.25	ng/ul	0.00
46) Acenaphthylene-d8	14.66	160	235771	7.84	ng/ul	0.00
51) 4-Nitrophenol-d4	15.17	143	4708	0.87	ng/ul	0.02
57) Fluorene-d10	15.94	176	194998	8.26	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	22134	4.27	ng/ul	0.00
70) Anthracene-d10	17.78	188	322497	8.22	ng/ul	0.00
78) Pyrene-d10	20.03	212	390225	8.73	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.04	264	490546	8.30	ng/ul	0.00
Target Compounds						
10) 2-Chlorophenol	7.90	128	9740	1.350	ng/ul#	88
20) Nitrobenzene	9.57	77	226168m	24.693	ng/ul	
72) 1,2,3,4-Tetrachlorobenzene	13.77	216	27778	2.675	ng/uL	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060818\
Data File : BM015595.D
Acq On : 09 Jun 2018 10:34
Operator : SJ/JU
Sample : J3261-01DL 5X
Misc :
ALS Vial : 38 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C07Q3DL

Manual Integrations
APPROVED

Sohil
6/11/2018 3:59:29 PM

Quant Time: Jun 11 12:38:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 09 02:29:49 2018
Response via : Initial Calibration

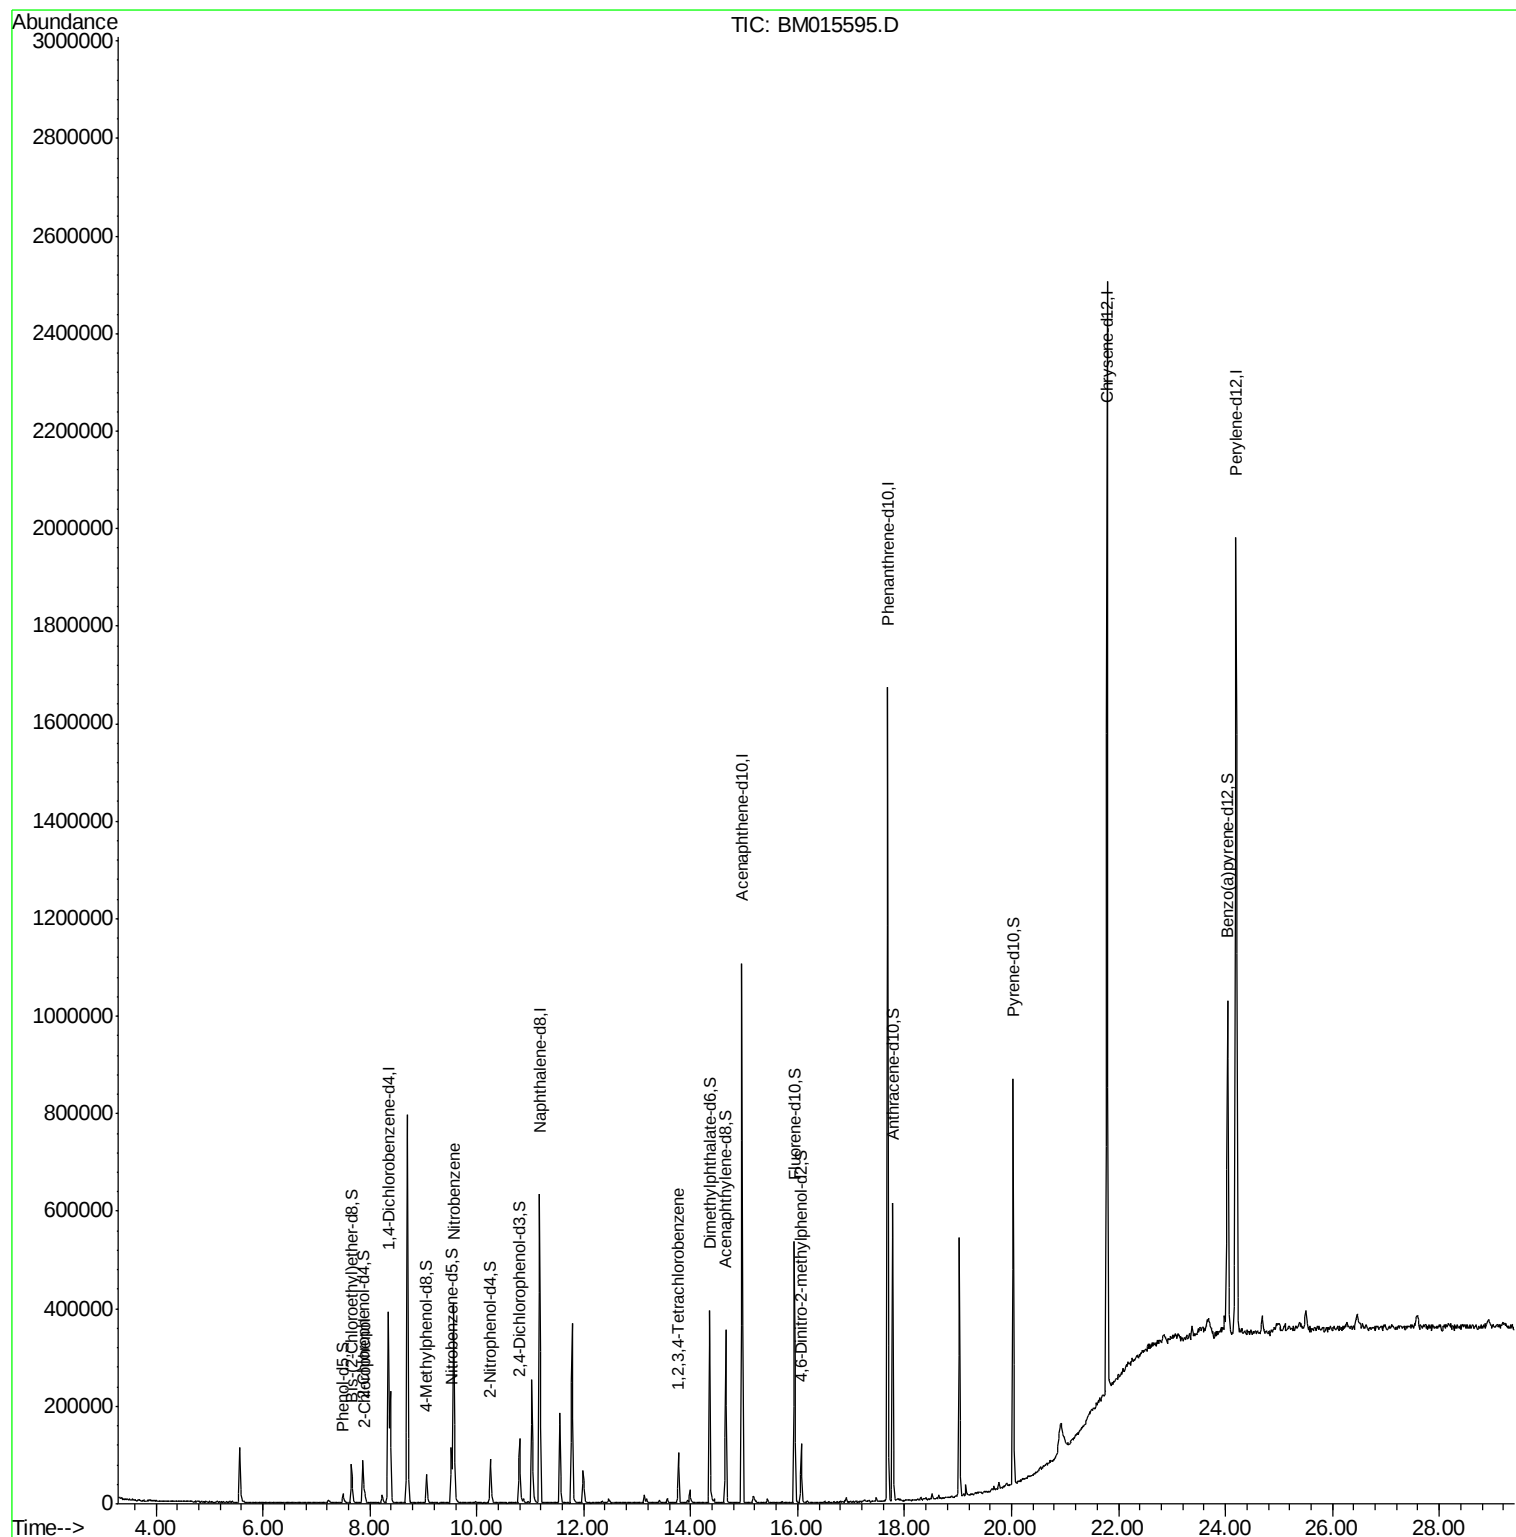

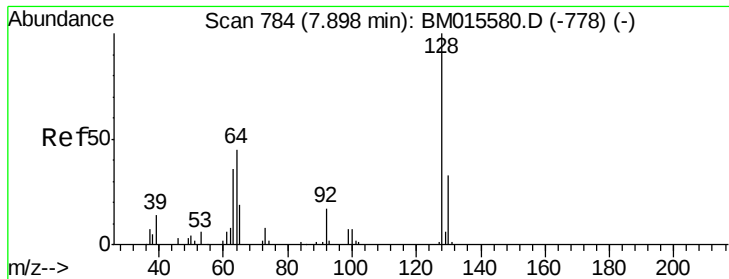





#10
2-Chlorophenol
Concen: 1.350 ng/ul
RT: 7.90 min Scan# 785
Delta R.T. 0.01 min
Lab File: BM015595.D
Acq: 09 Jun 2018 10:34

Instrument :
BNA_M
ClientSampleId :
C07Q3DL

Tot Ion	Ratio	Lower	Upper
128	100		
64	52.7	31.9	47.9#
130	32.4	25.6	38.4




Manual Integrations
APPROVED


Sohil
6/11/2018 3:59:29 PM

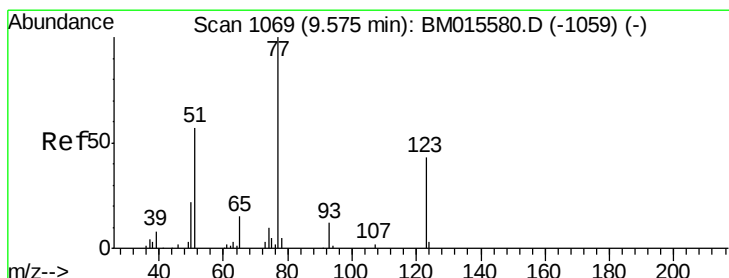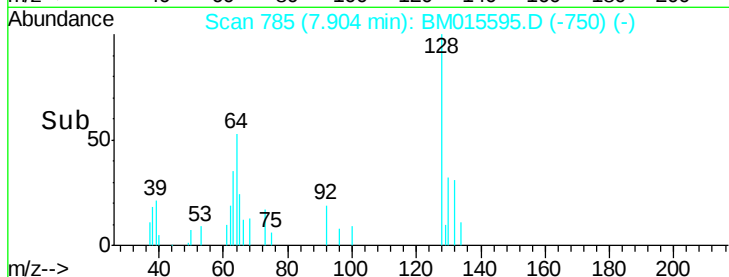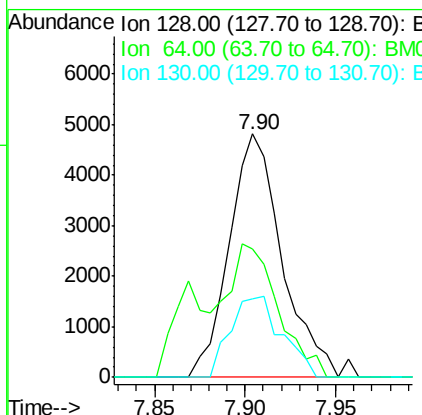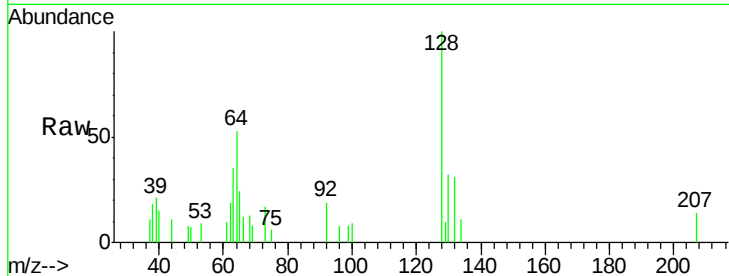

#20
Nitrobenzene
Concen: 24.693 ng/ul m
RT: 9.57 min Scan# 1068
Delta R.T. -0.01 min
Lab File: BM015595.D
Acq: 09 Jun 2018 10:34

Tgt Ion	Ratio	Lower	Upper
77	100		
123	40.2	39.0	58.4
65	13.7	10.4	15.6

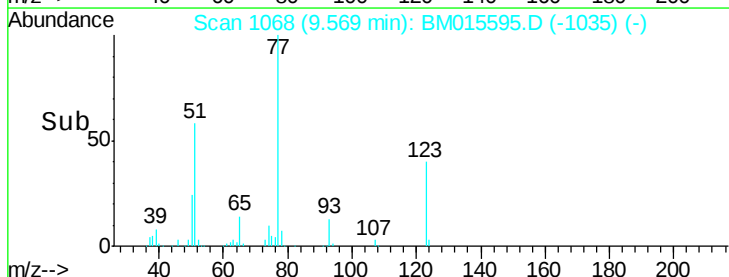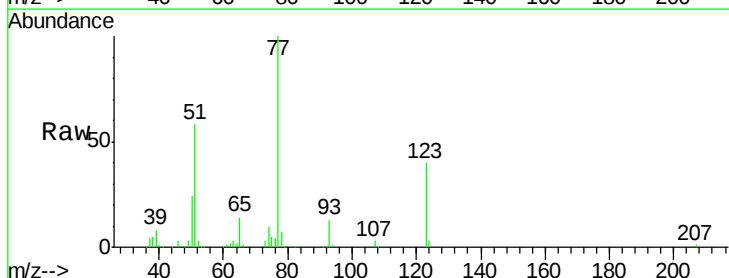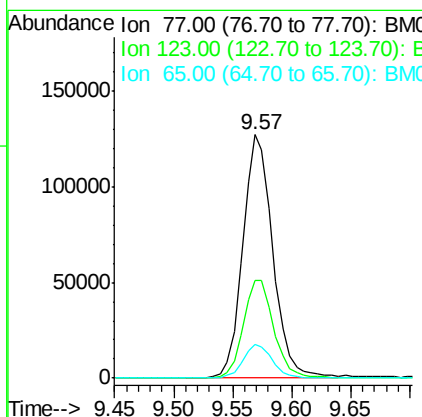

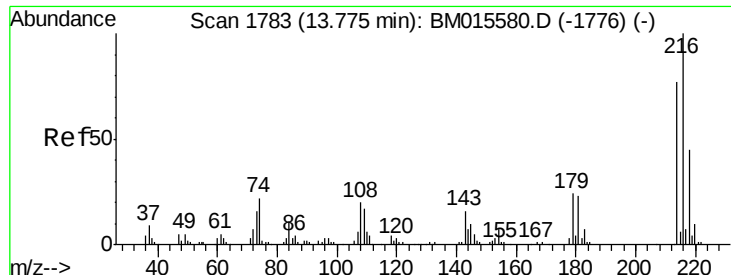

#72

1,2,3,4-Tetrachlorobenzene

Concen: 2.675 ng/uL

RT: 13.77 min Scan# 1782

Delta R.T. -0.01 min

Lab File: BM015595.D

Acq: 09 Jun 2018 10:34

Instrument :

BNA_M

ClientSampleId :

C07Q3DL

Tot Ion:216 Resp: 27778

Ion Ratio Lower Upper

216 100

214 74.7 62.5 93.7


218 48.7 38.4 57.6

Manual Integrations

APPROVED

Sohil

6/11/2018 3:59:29 PM

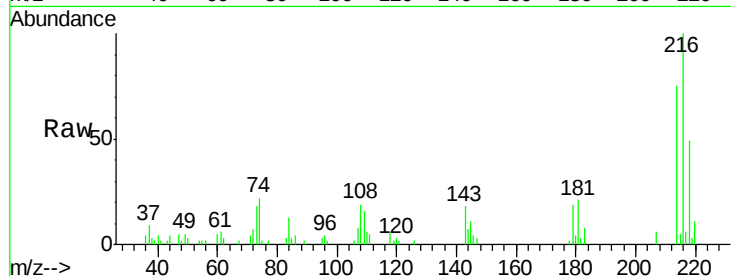

Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

