

Data File : BM020817.D
Acq On : 08 Jun 2019 14:24
Operator : HP/JU
Sample : K3006-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFHD0

Quant Time: Jun 09 01:06:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jun 09 01:02:58 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	279492	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	1178990	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	692081	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	1595802	20.00	ng/ul	0.00
77) Chrysene-d12	21.37	240	1546883	20.00	ng/ul	0.00
85) Perylene-d12	23.66	264	1788857	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.31	96	44373	7.57	ng/uL	0.00
5) Phenol-d5	6.97	99	839475	39.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	506543	39.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	720440	42.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	708623	41.19	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	343919	42.74	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	356671	43.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	734719	42.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	972279	46.73	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	2190925	42.80	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	2822239	43.48	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	257030	29.26	ng/ul	0.00
57) Fluorene-d10	15.44	176	1919913	44.13	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	134403	16.47	ng/ul	0.00
70) Anthracene-d10	17.29	188	3046492	43.71	ng/ul	0.00
78) Pyrene-d10	19.59	212	3285944	43.95	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.52	264	3651496	44.91	ng/ul	0.00


Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	8.51	70	17529	1.252	ng/ul#	1
44) Dimethylphthalate	13.90	163	992086	19.354	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM020817.D
Acq On : 08 Jun 2019 14:24
Operator : HP/JU
Sample : K3006-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFHD0

Quant Time: Jun 09 01:06:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jun 09 01:02:58 2019
Response via : Initial Calibration

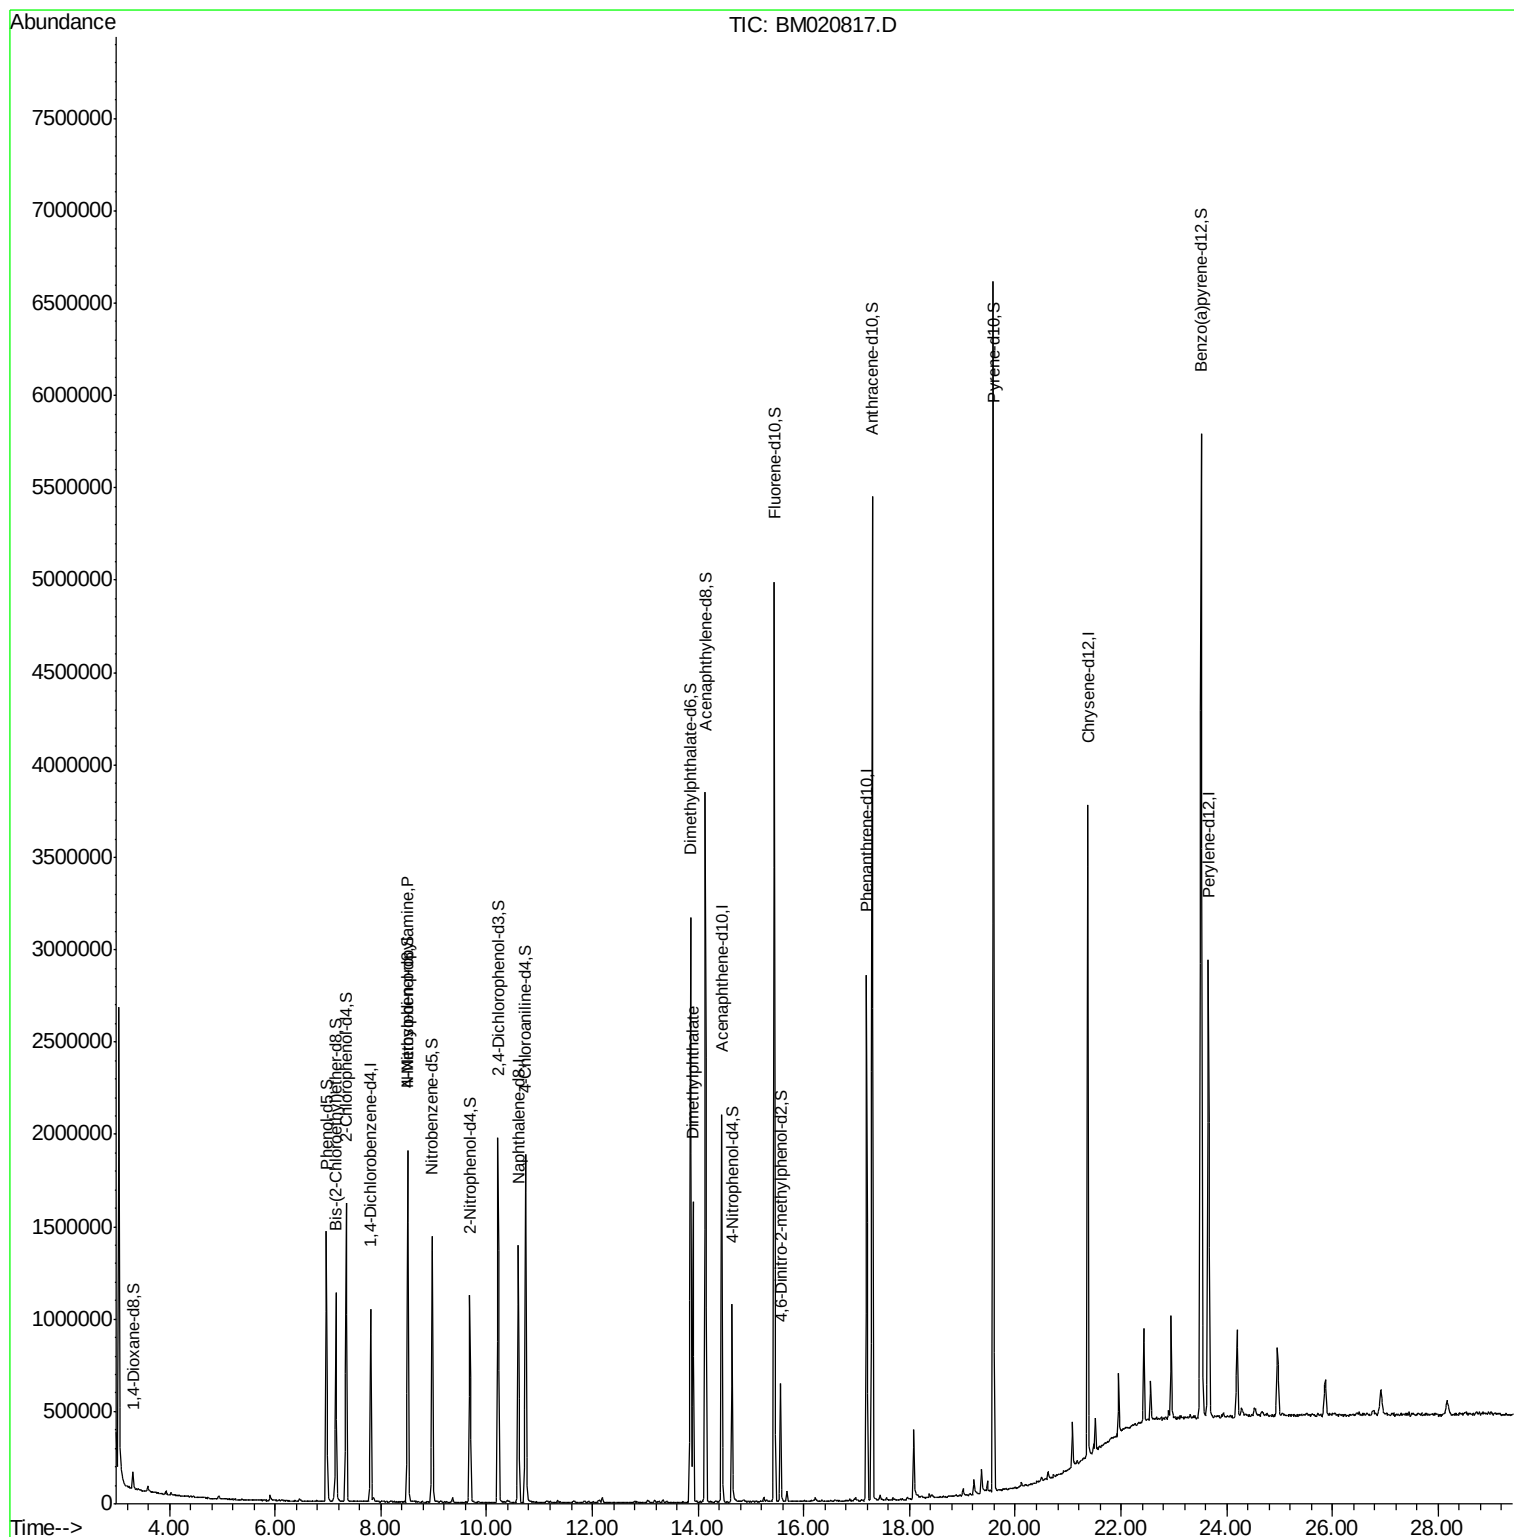

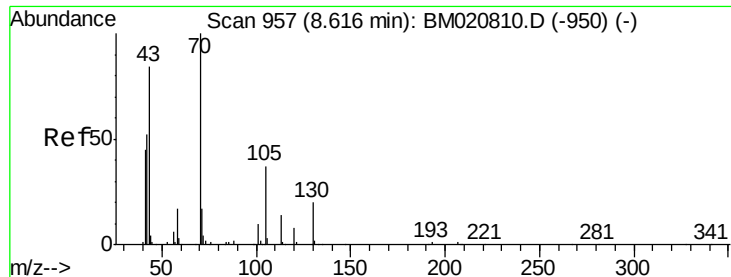

#15

N-Nitroso-di-n-propylamine

Concen: 1.252 ng/ul

RT: 8.51 min Scan# 939

Delta R.T. -0.11 min

Lab File: BM020817.D

Acq: 08 Jun 2019 14:24

Instrument :

BNA_M

ClientSampleId :

BFHD0

Tgt Ion: 70 Resp: 17529





Ion Ratio Lower Upper

70 100

42 384.4 43.6 65.4#

101 0.0 8.2 12.2#

130 0.0 15.8 23.8#

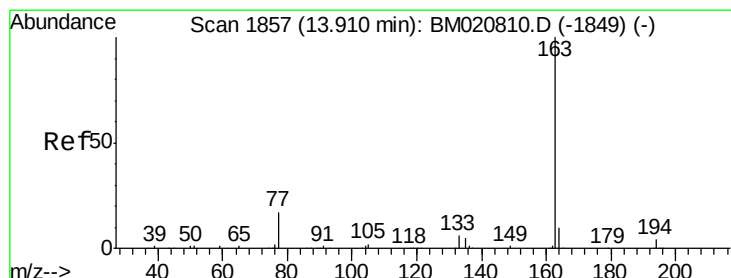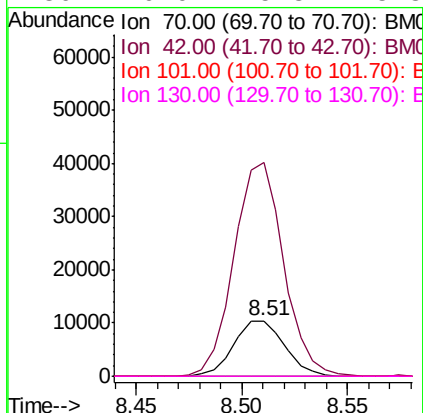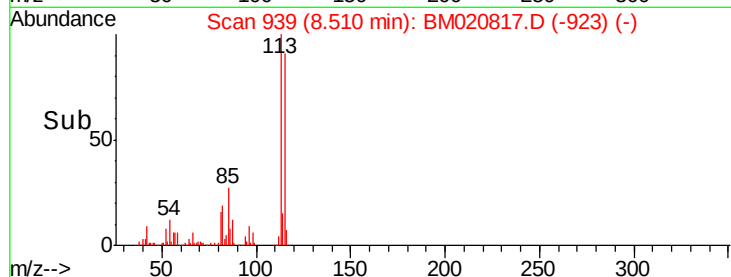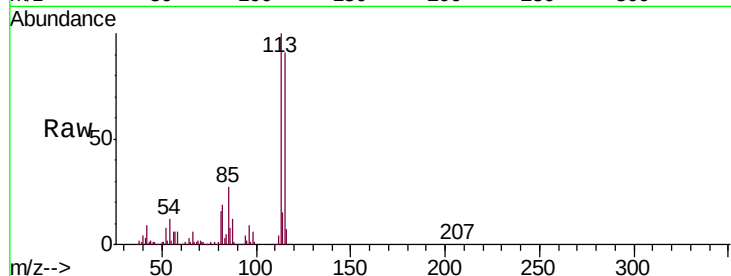

#44

Dimethylphthalate

Concen: 19.354 ng/ul

RT: 13.90 min Scan# 1856

Delta R.T. -0.01 min

Lab File: BM020817.D

Acq: 08 Jun 2019 14:24

Tgt Ion: 163 Resp: 992086

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 10.3 8.0 12.0

