

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060819\
 Data File : BM020813.D
 Acq On : 08 Jun 2019 12:00
 Operator : HP/JU
 Sample : K3006-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFH88

Quant Time: Jun 09 01:05:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jun 09 01:02:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	296646	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	1277681	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	764205	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	1672004	20.00	ng/ul	0.00
77) Chrysene-d12	21.37	240	1178421	20.00	ng/ul	0.00
85) Perylene-d12	23.66	264	1307568	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	26755	4.30	ng/uL	0.00
5) Phenol-d5	6.97	99	440634	19.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	324398	23.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	385472	21.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	348479	19.08	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	211193	24.22	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	225257	25.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	391336	20.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	486304	21.57	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	1515260	26.81	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	1528968	21.33	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	116112	11.97	ng/ul	0.00
57) Fluorene-d10	15.44	176	1154383	24.03	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	69435	8.12	ng/ul	0.00
70) Anthracene-d10	17.29	188	1499774	20.54	ng/ul	0.00
78) Pyrene-d10	19.59	212	1348036	23.67	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.51	264	1097284	18.46	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.90	163	699246	12.354	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060819\
Data File : BM020813.D
Acq On : 08 Jun 2019 12:00
Operator : HP/JU
Sample : K3006-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFH88

Quant Time: Jun 09 01:05:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jun 09 01:02:58 2019
Response via : Initial Calibration

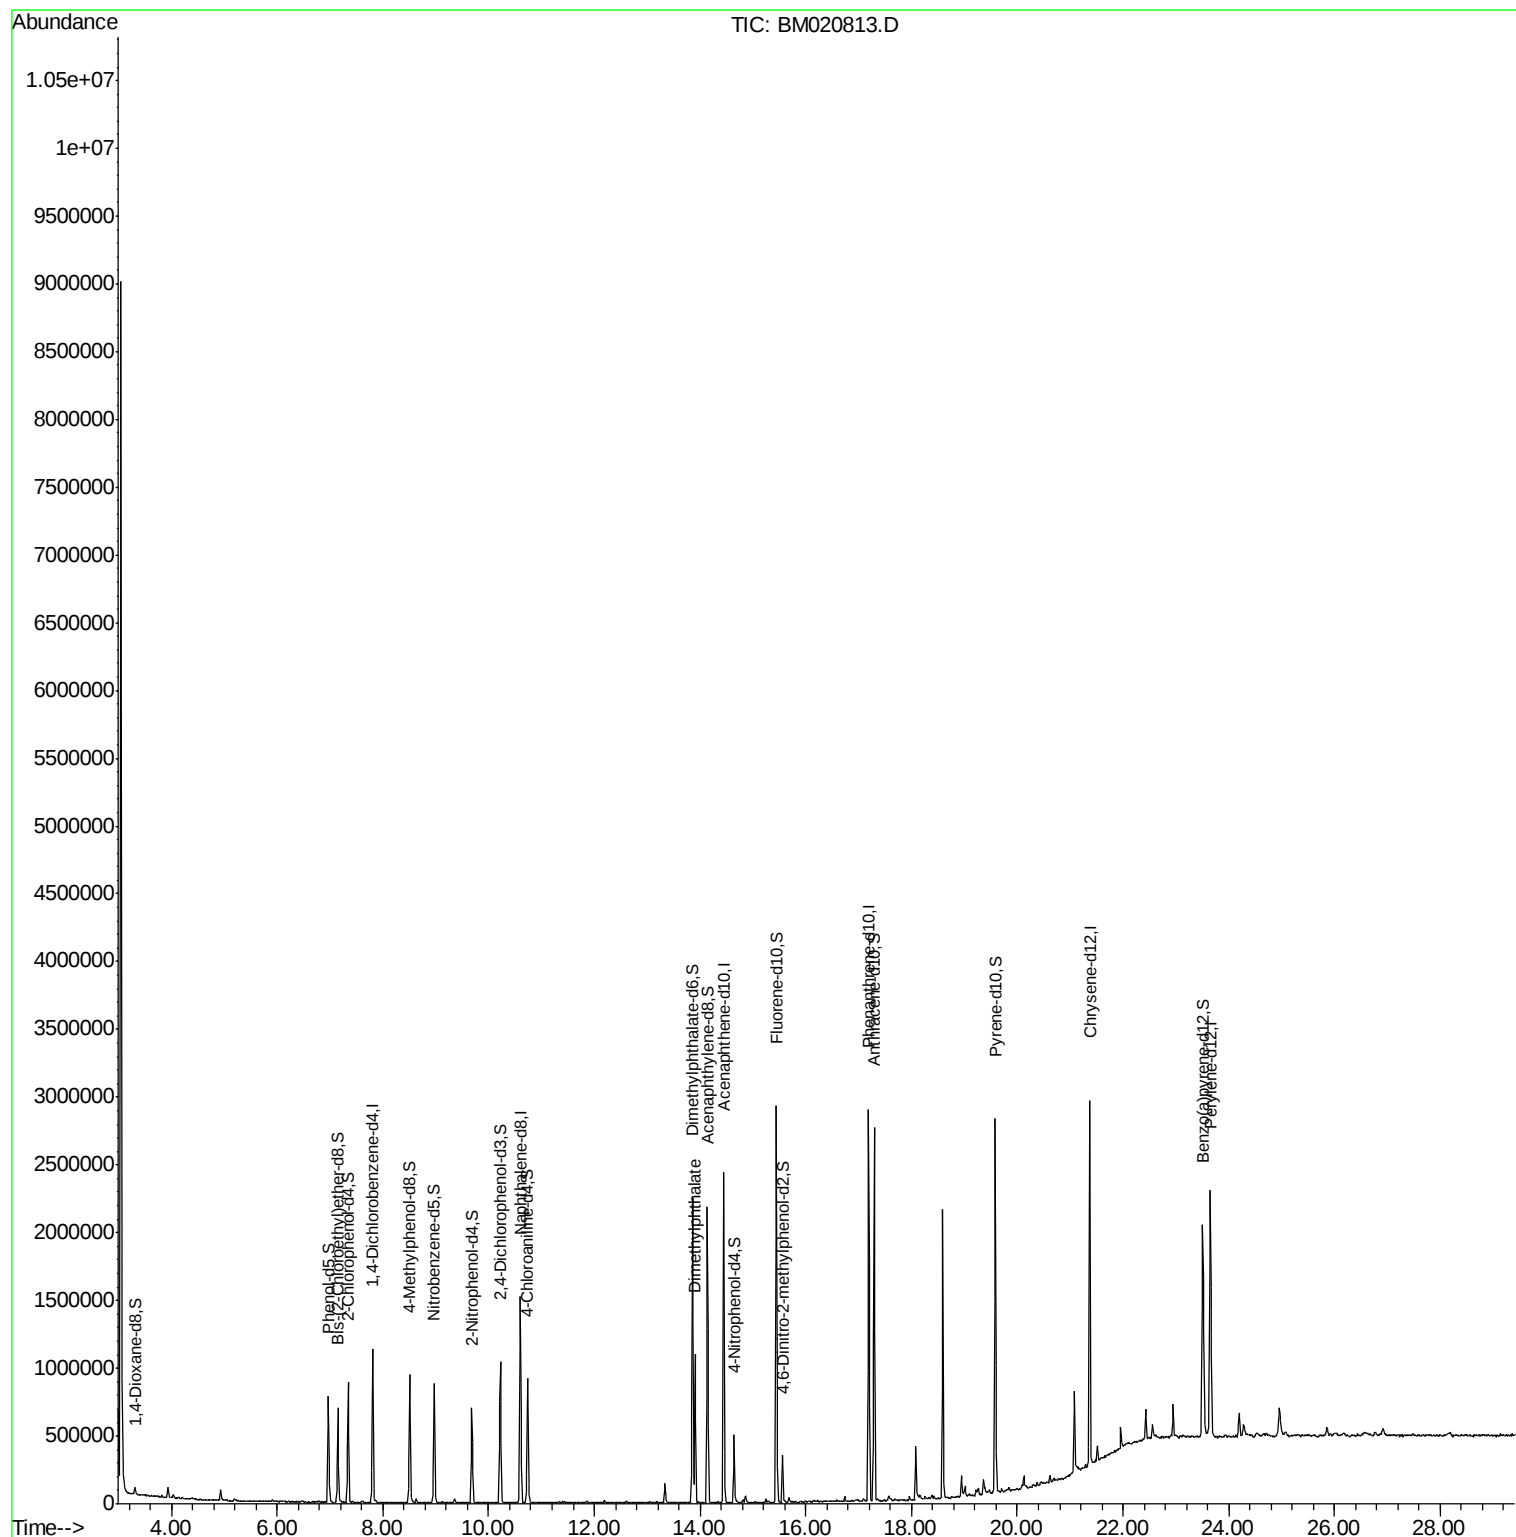

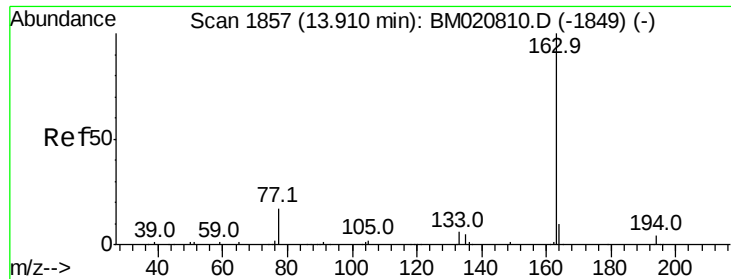

#44

Dimethylphthalate

Concen: 12.354 ng/ul

RT: 13.90 min Scan# 1856

Delta R.T. -0.01 min

Lab File: BM020813.D

Acq: 08 Jun 2019 12:00

Instrument :

BNA_M

ClientSampleId :

BFH88


Tot Ion:163 Resp: 699246

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 9.9 8.0 12.0

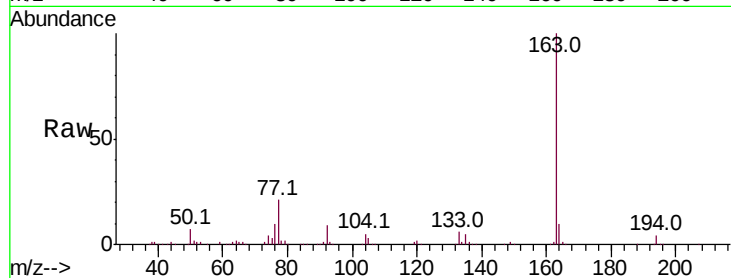

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

