

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060819\
 Data File : BM020811.D
 Acq On : 08 Jun 2019 10:48
 Operator : HP/JU
 Sample : PB120160BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	7	10	17	rVB	197036	236050	3.21%	0.305%
2	3.304	51	54	62	rVB	92250	127969	1.74%	0.165%
3	4.034	173	178	188	rVB	520597	709085	9.63%	0.915%
4	4.445	246	248	255	rVB5	6932	11112	0.15%	0.014%
5	6.922	665	669	671	rBV4	5884	7756	0.11%	0.010%
6	6.975	671	678	691	rVB	1400881	2245392	30.51%	2.898%
7	7.151	700	708	721	rBV	1085126	1749309	23.77%	2.258%
8	7.339	733	740	751	rBV	1529940	2394201	32.53%	3.090%
9	7.810	813	820	831	rVB	1037502	1617971	21.98%	2.089%
10	8.510	930	939	949	rBV	1799657	2822211	38.35%	3.643%
11	8.969	1010	1017	1027	rBV	1341358	2232483	30.33%	2.882%
12	9.686	1132	1139	1148	rBV	1117079	1827511	24.83%	2.359%
13	10.222	1222	1230	1244	rBV	1770590	2997949	40.73%	3.870%
14	10.604	1286	1295	1302	rBV	1338765	2276646	30.93%	2.939%
15	10.739	1310	1318	1333	rBV	1715644	2921424	39.69%	3.771%
16	12.192	1559	1565	1573	rBV2	27350	44615	0.61%	0.058%
17	13.863	1842	1849	1857	rVB	2899140	4054272	55.09%	5.233%
18	14.145	1889	1897	1906	rBV	3468752	5187657	70.49%	6.696%
19	14.451	1942	1949	1957	rBV2	1993524	2984113	40.55%	3.852%
20	14.645	1975	1982	1995	rBV	1235381	1811075	24.61%	2.338%
21	15.445	2111	2118	2128	rVB	4177665	6109645	83.01%	7.886%
22	15.562	2132	2138	2147	rBV	822502	1130603	15.36%	1.459%
23	15.680	2153	2158	2164	rVB2	46704	68737	0.93%	0.089%
24	16.227	2247	2251	2254	rBV3	13965	18687	0.25%	0.024%
25	16.398	2273	2280	2284	rBV5	4518	7426	0.10%	0.010%
26	16.980	2372	2379	2384	rBV3	8856	15245	0.21%	0.020%
27	17.192	2409	2415	2425	rBV2	2285786	3417570	46.44%	4.411%
28	17.292	2425	2432	2443	rBV	4520453	6361760	86.44%	8.212%
29	17.445	2454	2458	2467	rVB5	16211	24318	0.33%	0.031%
30	18.080	2562	2566	2574	rBV7	13791	24546	0.33%	0.032%
31	18.162	2574	2580	2582	rBV5	4732	9129	0.12%	0.012%
32	19.215	2755	2759	2768	rVB	45731	62909	0.85%	0.081%
33	19.362	2781	2784	2787	rBV5	10560	15765	0.21%	0.020%
34	19.474	2799	2803	2808	rBV	40619	53131	0.72%	0.069%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060819\
Data File : BM020811.D
Acq On : 08 Jun 2019 10:48
Operator : HP/JU
Sample : PB120160BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK60

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Title : SVOA CALIBRATION

35	19.586	2816	2822	2829	rBV	5476082	7027536	95.49%	9.071%
36	21.368	3120	3125	3131	rBV	2856236	3665299	49.80%	4.731%
37	23.509	3482	3489	3499	rVB2	3865622	7359774	100.00%	9.500%
38	23.656	3507	3514	3523	rVB	2008667	3838913	52.16%	4.955%


Sum of corrected areas: 77469794

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060819\
Data File : BM020811.D
Acq On : 08 Jun 2019 10:48
Operator : HP/JU
Sample : PB120160BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK60

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

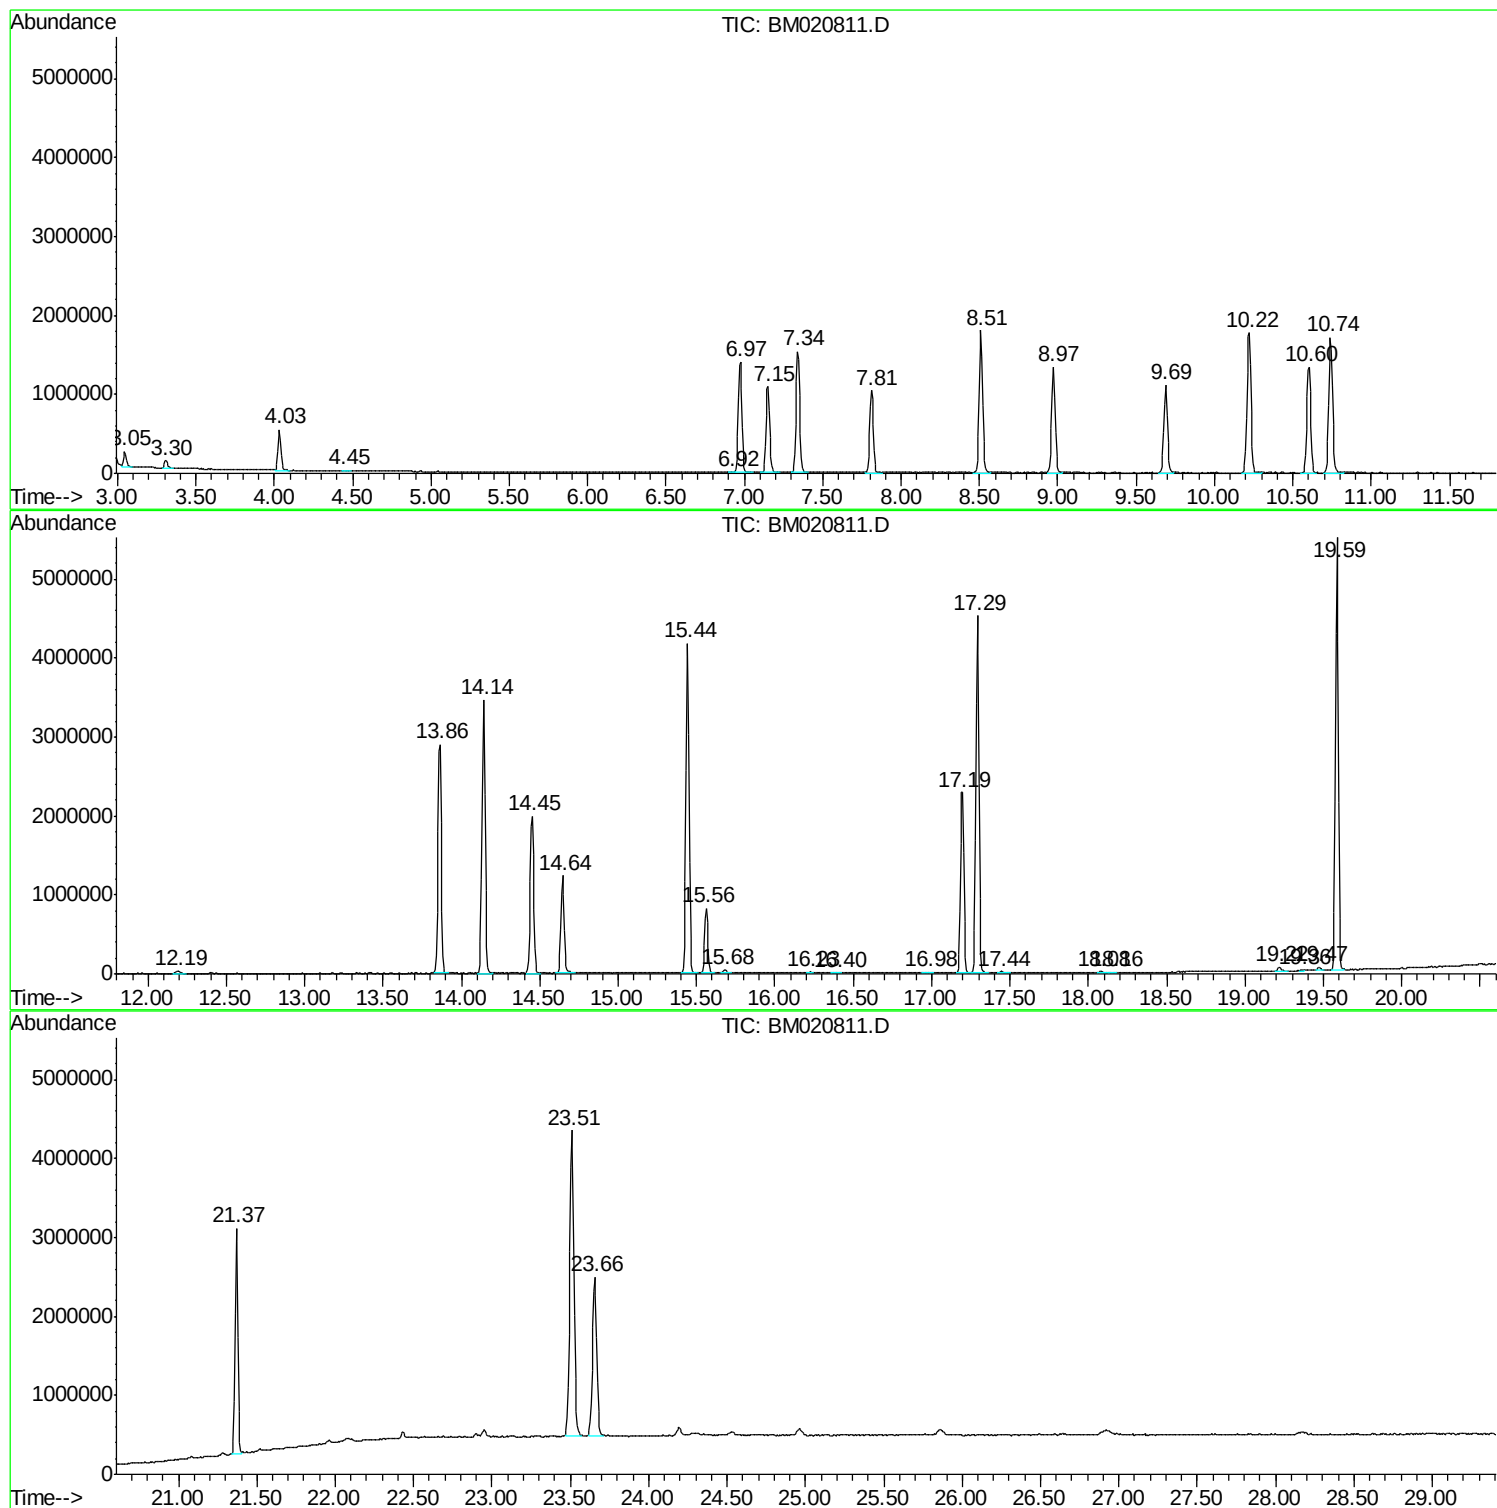

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060819\
Data File : BM020811.D
Acq On : 08 Jun 2019 10:48
Operator : HP/JU
Sample : PB120160BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK60










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.05	2.92 ng/ul	236050	1,4-Dichlorobenzene-d4	7.81

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2		Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	50
3		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
4		N-Ethylformamide	73	C3H7NO	000627-45-2	9
5		Myo-Inositol, 2-C-methyl-	194	C7H14O6	000472-96-8	9

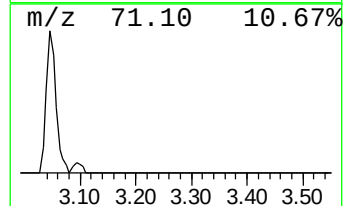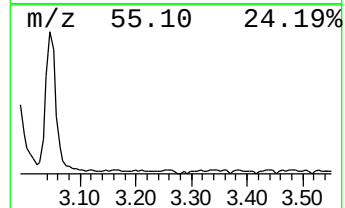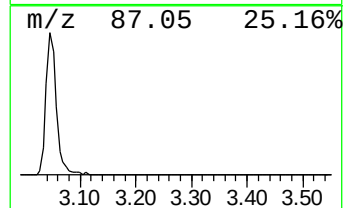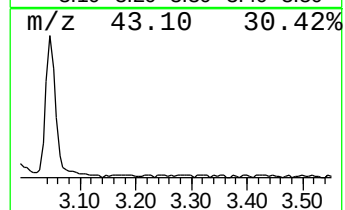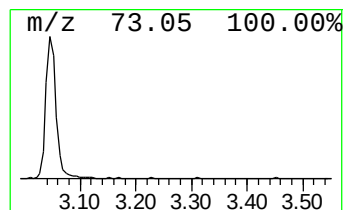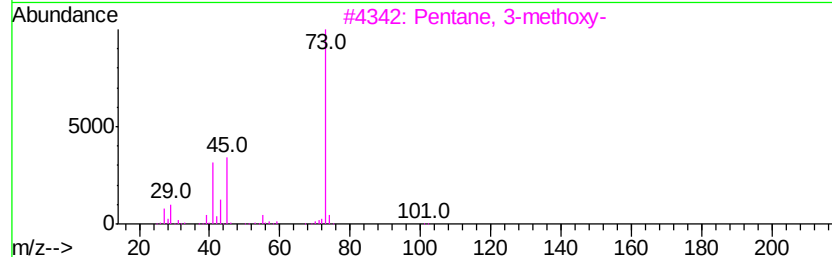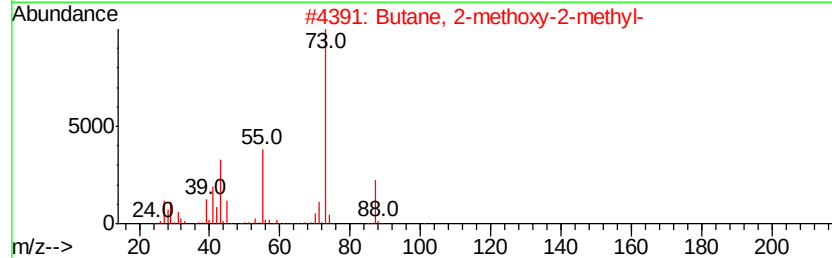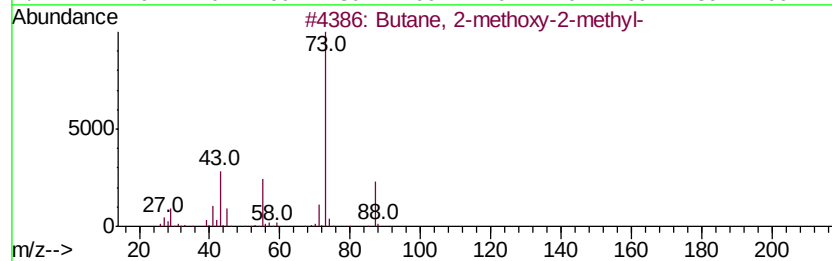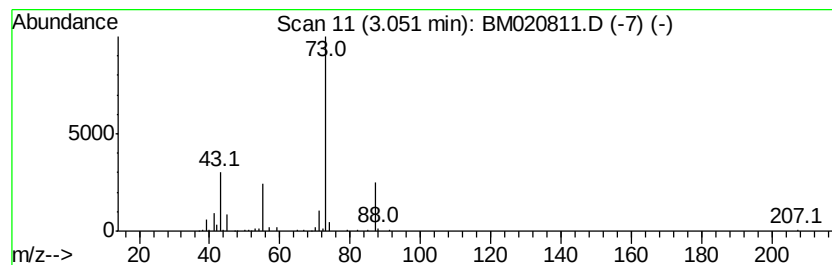

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060819\
Data File : BM020811.D
Acq On : 08 Jun 2019 10:48
Operator : HP/JU
Sample : PB120160BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK60

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	3.05	2.9	ng/ul	236050	1	7.81	1617970	20.0