

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060821\
 Data File : BM030316.D
 Acq On : 08 Jun 2021 09:35
 Operator : CG/JU
 Sample : M2250-02
 Misc : SFAM-MDL-W-02
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT3-2021-06

Quant Time: Jun 08 10:12:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 08 09:51:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	177051	20.000	ng/u1	0.00
20) Naphthalene-d8	10.639	136	764605	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.474	164	503222	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.209	188	1042951	20.000	ng/u1	0.00
79) Chrysene-d12	21.368	240	1006033	20.000	ng/u1	0.00
88) Perylene-d12	23.650	264	922714	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.316	96	22206	4.789	ng/uL	0.00
4) Pyridine-d5	3.734	84	173785	14.264	ng/u1	0.00
7) Phenol-d5	7.004	99	313931	20.401	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	222628	22.416	ng/u1	0.00
11) 2-Chlorophenol-d4	7.381	132	256143	23.017	ng/u1	0.00
15) 4-Methylphenol-d8	8.545	113	248411	20.213	ng/u1	0.00
21) Nitrobenzene-d5	9.004	128	116422	22.244	ng/u1	0.00
24) 2-Nitrophenol-d4	9.722	143	115574	22.234	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.257	165	244575	21.600	ng/u1	0.00
31) 4-Chloroaniline-d4	10.769	131	346894	20.041	ng/u1	0.00
46) Dimethylphthalate-d6	13.880	166	788661	22.837	ng/u1	0.00
49) Acenaphthylene-d8	14.169	160	990434	22.957	ng/u1	0.00
54) 4-Nitrophenol-d4	14.651	143	124370	19.240	ng/u1	0.00
60) Fluorene-d10	15.463	176	715209	23.133	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.574	200	101049	16.785	ng/u1	0.00
73) Anthracene-d10	17.304	188	1074723	22.656	ng/u1	0.00
81) Pyrene-d10	19.586	212	1175998	22.333	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.503	264	1125154	24.454	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.352	88	6570	1.398	ng/uL	97
5) Pyridine	3.757	79	51357	3.993	ng/u1#	78
6) Benzaldehyde	6.992	77	43947	6.094	ng/u1	97
8) Phenol	7.034	94	68785	4.413	ng/u1	97
10) Bis(2-Chloroethyl)ether	7.275	93	58990	4.688	ng/u1	97
12) 2-Chlorophenol	7.416	128	54562	4.753	ng/u1	99
13) 2-Methylphenol	8.287	108	46370	4.001	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.375	45	92873	4.582	ng/u1	98
16) Acetophenone	8.669	105	87622	4.509	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.651	70	42386	4.488	ng/u1	94
18) 4-Methylphenol	8.604	108	54831	4.291	ng/u1	96
19) Hexachloroethane	8.928	117	21964	4.522	ng/u1	95
22) Nitrobenzene	9.045	77	66009	4.913	ng/u1	97
23) Isophorone	9.569	82	105730	4.304	ng/u1	99
25) 2-Nitrophenol	9.757	139	27486	4.773	ng/u1	97
26) 2,4-Dimethylphenol	9.810	107	59754	4.584	ng/u1	96
27) Bis(2-Chloroethoxy)met...	10.051	93	75242	4.600	ng/u1	99
29) 2,4-Dichlorophenol	10.281	162	52986	4.805	ng/u1	92
30) Naphthalene	10.686	128	188235	4.857	ng/u1	99
32) 4-Chloroaniline	10.798	127	77441	4.470	ng/u1	98
33) Hexachlorobutadiene	10.980	225	35623	5.077	ng/u1	94
34) Caprolactam	11.586	113	13307	3.769	ng/u1	91
35) 4-Chloro-3-methylphenol	11.910	107	47289	4.214	ng/u1	98
36) 2-Methylnaphthalene	12.298	142	132264	4.797	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060821\
 Data File : BM030316.D
 Acq On : 08 Jun 2021 09:35
 Operator : CG/JU
 Sample : M2250-02
 Misc : SFAM-MDL-W-02
 ALS Vial : 4 Sample Multiplier: 1


Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT3-2021-06

Quant Time: Jun 08 10:12:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 08 09:51:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.522	142	131752	4.708	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.669	216	70466	4.817	ng/ul	98
40) Hexachlorocyclopentadiene	12.651	237	37119	4.015	ng/ul	99
41) 2,4,6-Trichlorophenol	12.904	196	34779	3.957	ng/ul	96
42) 2,4,5-Trichlorophenol	12.969	196	40350	4.214	ng/ul	96
43) 1,1'-Biphenyl	13.310	154	174711	4.765	ng/ul	99
44) 2-Chloronaphthalene	13.351	162	135684	4.795	ng/ul	99
45) 2-Nitroaniline	13.551	65	26610	3.762	ng/ul	96
47) Dimethylphthalate	13.927	163	165831	4.916	ng/ul	100
48) 2,6-Dinitrotoluene	14.045	165	23988	3.968	ng/ul	95
50) Acenaphthylene	14.192	152	202340	4.910	ng/ul	99
51) 3-Nitroaniline	14.374	138	25549	3.707	ng/ul	98
52) Acenaphthene	14.539	153	146079	4.772	ng/ul	99
53) 2,4-Dinitrophenol	14.574	184	19944	4.944	ng/ul	97
55) 4-Nitrophenol	14.663	109	22087	4.361	ng/ul	93
56) Dibenzofuran	14.868	168	206704	4.853	ng/ul	100
57) 2,4-Dinitrotoluene	14.827	165	35323	4.131	ng/ul	95
58) 2,3,4,6-Tetrachlorophenol	15.092	232	33337	4.350	ng/ul	95
59) Diethylphthalate	15.286	149	154467	4.640	ng/ul	99
61) Fluorene	15.515	166	170231	4.760	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.510	204	85479	4.963	ng/ul	98
63) 4-Nitroaniline	15.533	138	24633	3.817	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.586	198	23811	3.989	ng/ul#	84
67) N-Nitrosodiphenylamine	15.721	169	139451	4.539	ng/ul	97
68) 4-Bromophenyl-phenylether	16.404	248	46927	4.626	ng/ul	97
69) Hexachlorobenzene	16.515	284	54520	4.728	ng/ul	98
70) Atrazine	16.668	200	42198	3.827	ng/ul	100
71) Pentachlorophenol	16.857	266	29257	4.141	ng/ul	95
72) Phenanthrene	17.251	178	263535	4.673	ng/ul	99
74) Anthracene	17.339	178	267915	4.707	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.274	216	69441	4.627	ng/ul	97
76) Pentachlorobenzene	14.792	250	67435	4.666	ng/ul	99
77) Carbazole	17.604	167	216028	4.274	ng/ul	98
78) Di-n-butylphthalate	18.168	149	216046	4.081	ng/ul	99
80) Fluoranthene	19.256	202	290318	4.487	ng/ul	99
82) Pyrene	19.615	202	320438	4.683	ng/ul	99
83) Butylbenzylphthalate	20.509	149	78188	3.641	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.286	252	66248	3.641	ng/ul	99
85) Benzo(a)anthracene	21.350	228	286832	4.719	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.280	149	111813	3.432	ng/ul	99
87) Chrysene	21.403	228	288107	4.807	ng/ul	99
89) Di-n-octyl phthalate	22.168	149	179559	3.021	ng/ul	100
90) Benzo(b)fluoranthene	22.962	252	271613	4.579	ng/ul	97
91) Benzo(k)fluoranthene	23.003	252	262679	4.637	ng/ul	99
93) Benzo(a)pyrene	23.550	252	247218	4.769	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	25.968	276	272107	4.265	ng/ul	99
95) Dibenzo(a,h)anthracene	25.974	278	225725	4.202	ng/ul	99
96) Benzo(g,h,i)perylene	26.674	276	225505	4.301	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Abundance Scan 45 (3.351 min): BM030314.D\data.ms (-40)


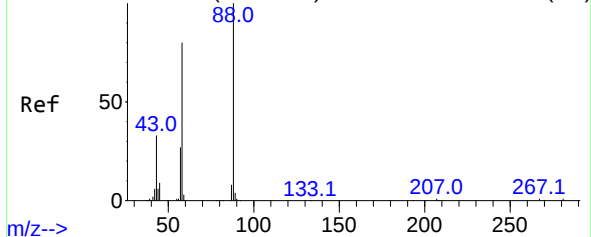


#2
1,4-Dioxane
Concen: 1.398 ng/uL
RT: 3.352 min Scan# 45
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35


Tgt Ion:	88	Resp:	6570
Ion	Ratio	Lower	Upper
88	100		
43	37.3	27.3	40.9
58	78.9	64.2	96.2

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Abundance Scan 45 (3.352 min): BM030316.D\data.ms

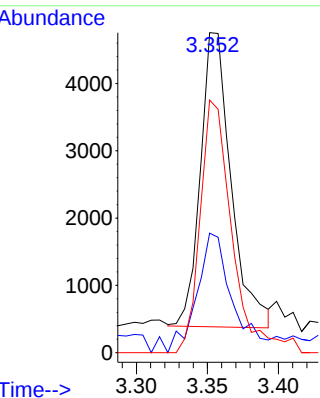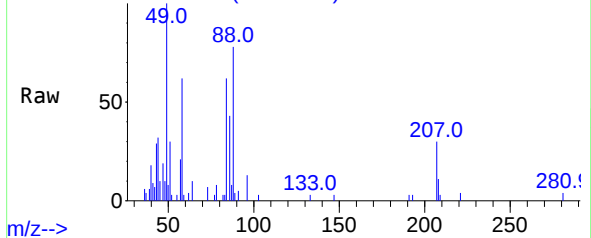

Abundance Scan 45 (3.352 min): BM030316.D\data.ms (-11)

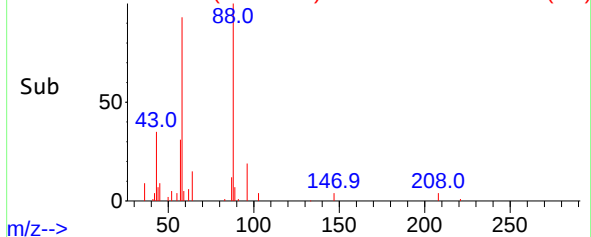



Abundance Scan 112 (3.746 min): BM030314.D\data.ms (-10)

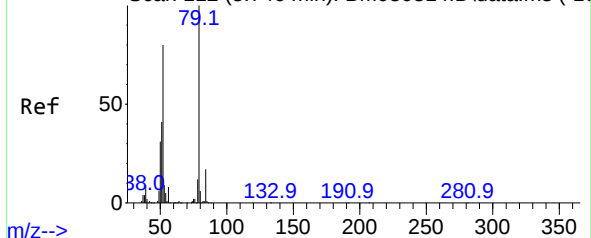


#5
Pyridine
Concen: 3.993 ng/uL
RT: 3.757 min Scan# 114
Delta R.T. 0.012 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35


Tgt Ion:	79	Resp:	51357
Ion	Ratio	Lower	Upper
79	100		
52	108.4	66.1	99.1#
51	43.9	31.0	46.4

Abundance Scan 114 (3.757 min): BM030316.D\data.ms

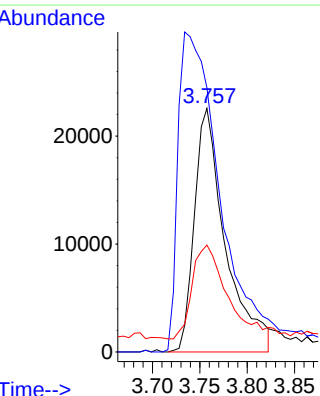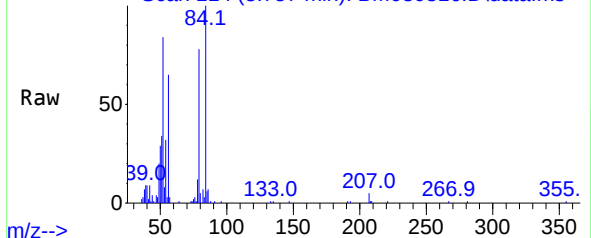

Abundance Scan 114 (3.757 min): BM030316.D\data.ms (-95)




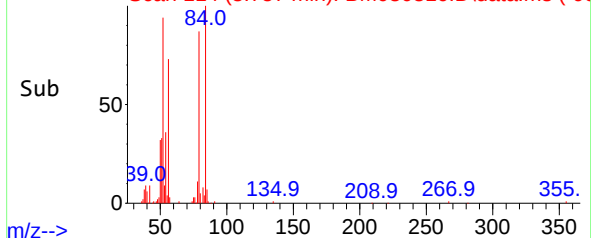




#6
Benzaldehyde
Concen: 6.094 ng/ul
RT: 6.992 min Scan# 664
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion: 77 Resp: 43947
Ion Ratio Lower Upper
77 100
105 97.9 74.5 111.7
106 88.7 70.2 105.2



#8
Phenol
Concen: 4.413 ng/ul
RT: 7.034 min Scan# 671
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion: 94 Resp: 68785
Ion Ratio Lower Upper
94 100
65 27.9 24.2 36.4
66 38.4 29.5 44.3









#10

Bis(2-Chloroethyl)ether
Concen: 4.688 ng/ul
RT: 7.275 min Scan# 712
Delta R.T. 0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06




Tgt Ion: 93	Resp: 58990
Ion Ratio	Lower Upper
93 100	
63 85.1	66.6 99.8
95 35.6	25.8 38.6

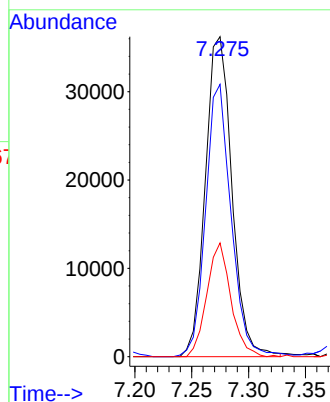


#12

2-Chlorophenol
Concen: 4.753 ng/ul
RT: 7.416 min Scan# 736
Delta R.T. 0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion: 128	Resp: 54562
Ion Ratio	Lower Upper
128 100	
64 46.6	37.7 56.5
130 31.8	25.6 38.4


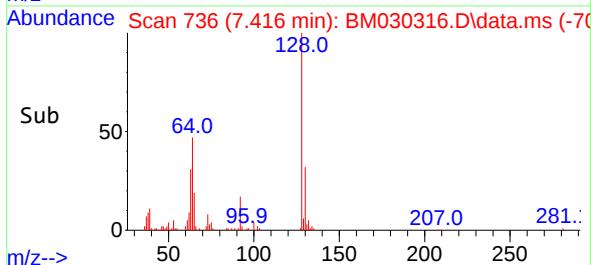






#13
2-Methylphenol
Concen: 4.001 ng/ul
RT: 8.287 min Scan# 884
Delta R.T. 0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:108 Resp: 46370
Ion Ratio Lower Upper
108 100
107 86.8 70.8 106.2

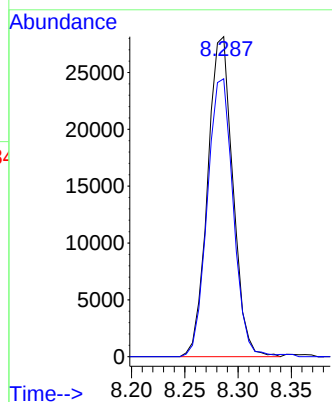

#14
2,2'-oxybis(1-Chloropropane)
Concen: 4.582 ng/ul
RT: 8.375 min Scan# 899
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion: 45 Resp: 92873
Ion Ratio Lower Upper
45 100
77 14.1 9.9 14.9
79 9.5 7.7 11.5



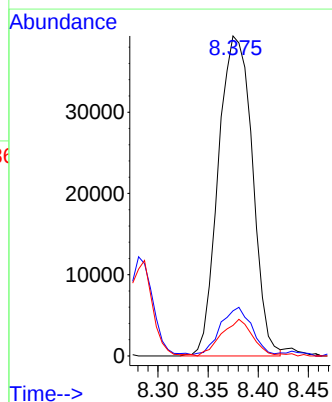





#16
Acetophenone
Concen: 4.509 ng/ul
RT: 8.669 min Scan# 949
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:	105	Resp:	87622
Ion	Ratio	Lower	Upper
105	100		
77	77.2	62.6	93.8
51	29.3	24.3	36.5



#17
N-Nitroso-di-n-propylamine
Concen: 4.488 ng/ul
RT: 8.651 min Scan# 946
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:	70	Resp:	42386
Ion	Ratio	Lower	Upper
70	100		
42	69.0	51.0	76.6
101	9.0	7.4	11.2
130	22.2	15.8	23.6



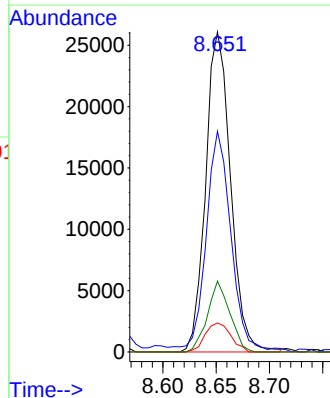





#18
4-Methylphenol
Concen: 4.291 ng/ul
RT: 8.604 min Scan# 938
Delta R.T. -0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:108 Resp: 54831
Ion Ratio Lower Upper
108 100
107 105.3 87.9 131.9

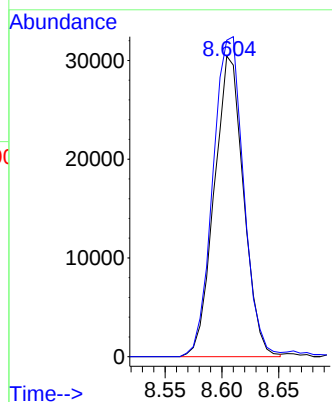

#19
Hexachloroethane
Concen: 4.522 ng/ul
RT: 8.928 min Scan# 993
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:117 Resp: 21964
Ion Ratio Lower Upper
117 100
201 98.8 81.0 121.6
199 68.4 49.1 73.7









#22
Nitrobenzene
Concen: 4.913 ng/ul
RT: 9.045 min Scan# 1013
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion: 77 Resp: 66009
Ion Ratio Lower Upper
77 100
123 41.1 34.6 51.8
65 11.9 10.2 15.2



#23
Isophorone
Concen: 4.304 ng/ul
RT: 9.569 min Scan# 1102
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion: 82 Resp: 105730
Ion Ratio Lower Upper
82 100
95 7.5 5.7 8.5
138 18.1 14.0 21.0









#25
2-Nitrophenol
Concen: 4.773 ng/ul
RT: 9.757 min Scan# 1134
Delta R.T. 0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:139 Resp: 27486
Ion Ratio Lower Upper
139 100
65 52.5 43.0 64.4
109 32.0 23.8 35.6



#26
2,4-Dimethylphenol
Concen: 4.584 ng/ul
RT: 9.810 min Scan# 1143
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:107 Resp: 59754
Ion Ratio Lower Upper
107 100
121 55.2 40.2 60.4
122 88.9 69.2 103.8









#27
Bis(2-Chloroethoxy)methane
Concen: 4.600 ng/ul
RT: 10.051 min Scan# 1184
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06

Tgt Ion: 93 Resp: 75242




Ion	Ratio	Lower	Upper
93	100		
95	33.3	26.2	39.2
123	11.0	9.0	13.6

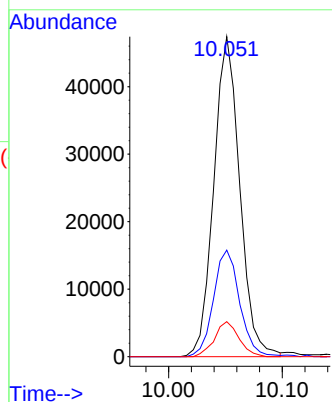


#29
2,4-Dichlorophenol
Concen: 4.805 ng/ul
RT: 10.281 min Scan# 1223
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion: 162 Resp: 52986

Ion	Ratio	Lower	Upper
162	100		
164	73.7	51.5	77.3
98	35.7	27.8	41.8









#30
Naphthalene
Concen: 4.857 ng/ul
RT: 10.686 min Scan# 1292
Delta R.T. -0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:128 Resp: 188235
Ion Ratio Lower Upper
128 100
129 10.7 8.6 13.0
127 12.0 10.2 15.2



#32
4-Chloroaniline
Concen: 4.470 ng/ul
RT: 10.798 min Scan# 1311
Delta R.T. 0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:127 Resp: 77441
Ion Ratio Lower Upper
127 100
129 34.5 26.6 39.8


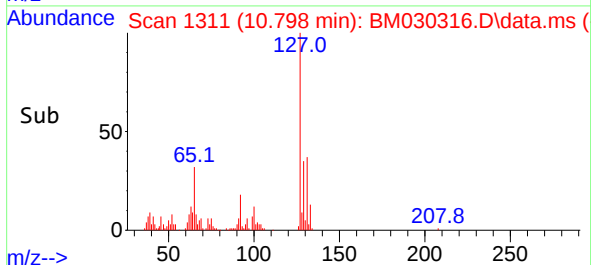

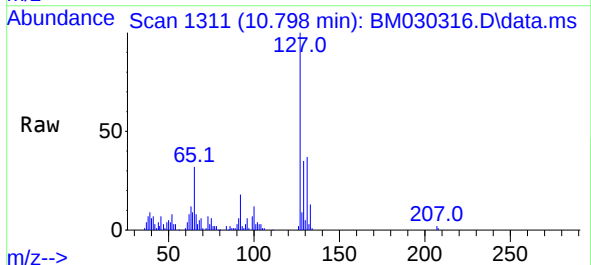




#33
Hexachlorobutadiene
Concen: 5.077 ng/ul
RT: 10.980 min Scan# 1342
Delta R.T. 0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:	225	Resp:	35623
Ion	Ratio	Lower	Upper
225	100		
223	61.0	52.2	78.2
227	62.1	54.2	81.4

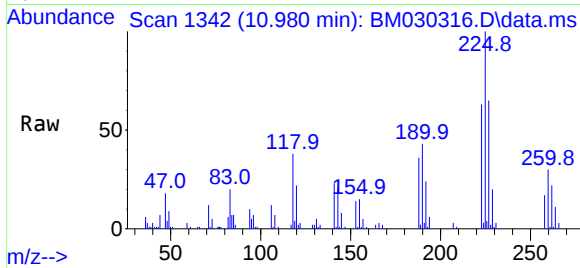

#34
Caprolactam
Concen: 3.769 ng/ul
RT: 11.586 min Scan# 1445
Delta R.T. 0.024 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:	113	Resp:	13307
Ion	Ratio	Lower	Upper
113	100		
55	175.6	150.3	225.5
56	126.3	110.9	166.3


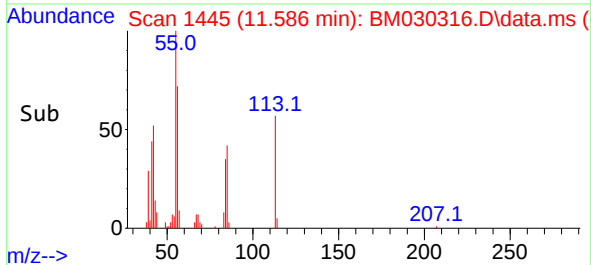

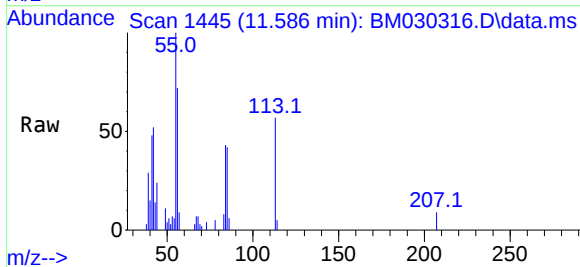




#35
4-Chloro-3-methylphenol
Concen: 4.214 ng/ul
RT: 11.910 min Scan# 1500
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:	107	Resp:	47289
Ion	Ratio	Lower	Upper
107	100		
144	29.6	22.3	33.5
142	85.8	67.8	101.6

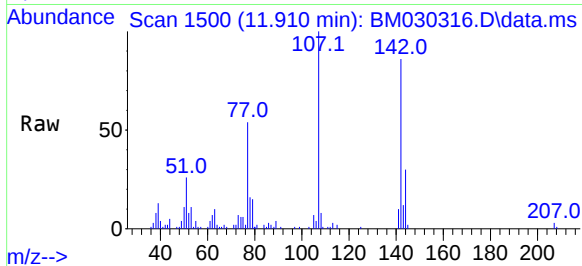

#36
2-Methylnaphthalene
Concen: 4.797 ng/ul
RT: 12.298 min Scan# 1566
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:	142	Resp:	132264
Ion	Ratio	Lower	Upper
142	100		
141	89.5	70.8	106.2



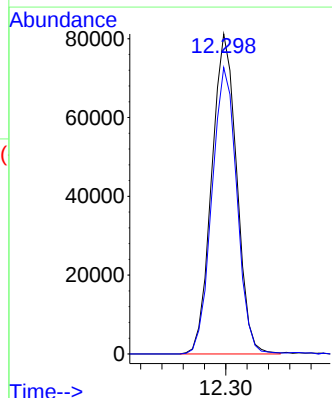
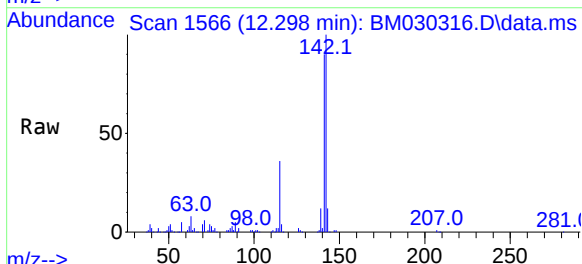




#37
1-Methylnaphthalene
Concen: 4.708 ng/ul
RT: 12.522 min Scan# 1604
Delta R.T. 0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:142 Resp: 131752
Ion Ratio Lower Upper
142 100
141 91.5 74.2 111.2
116 3.8 3.3 4.9

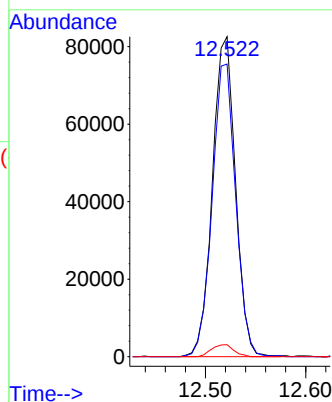

#39
1,2,4,5-Tetrachlorobenzene
Concen: 4.817 ng/ul
RT: 12.669 min Scan# 1629
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:216 Resp: 70466
Ion Ratio Lower Upper
216 100
214 77.1 63.0 94.6
179 20.7 16.8 25.2
108 18.3 14.2 21.2









#40
Hexachlorocyclopentadiene
Concen: 4.015 ng/ul
RT: 12.651 min Scan# 1626
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:	237	Resp:	37119
Ion	Ratio	Lower	Upper
237	100		
235	66.0	51.9	77.9
272	13.0	9.8	14.8

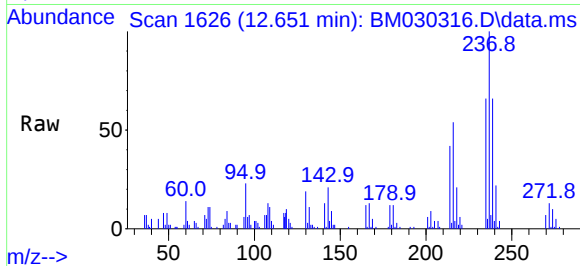

#41
2,4,6-Trichlorophenol
Concen: 3.957 ng/ul
RT: 12.904 min Scan# 1669
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:	196	Resp:	34779
Ion	Ratio	Lower	Upper
196	100		
198	99.3	75.8	113.6
200	32.0	24.4	36.6




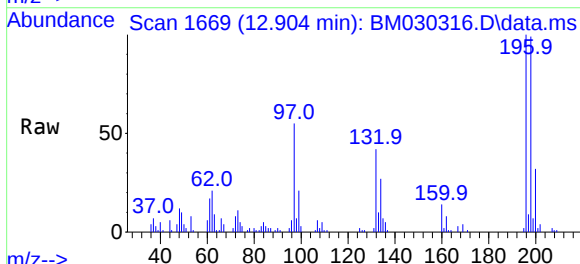




#42
2,4,5-Trichlorophenol
Concen: 4.214 ng/ul
RT: 12.969 min Scan# 1680
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:	196	Resp:	40350
Ion	Ratio	Lower	Upper
196	100		
198	92.7	77.5	116.3
200	33.0	25.1	37.7



#43
1,1'-Biphenyl
Concen: 4.765 ng/ul
RT: 13.310 min Scan# 1738
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:	154	Resp:	174711
Ion	Ratio	Lower	Upper
154	100		
153	38.9	31.5	47.3
76	12.7	10.8	16.2




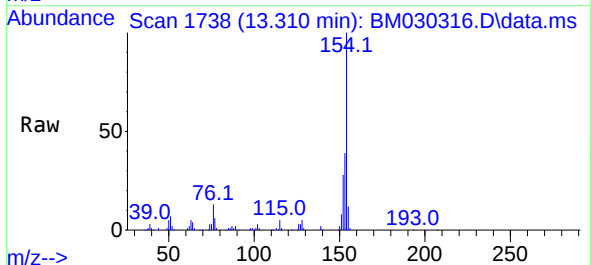




#44
2-Chloronaphthalene
Concen: 4.795 ng/ul
RT: 13.351 min Scan# 1745
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:162 Resp: 135684
Ion Ratio Lower Upper
162 100
164 32.9 26.0 39.0
127 37.0 28.6 42.8



#45
2-Nitroaniline
Concen: 3.762 ng/ul
RT: 13.551 min Scan# 1779
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion: 65 Resp: 26610
Ion Ratio Lower Upper
65 100
92 72.8 54.4 81.6
138 107.9 84.1 126.1









#47
Dimethylphthalate
Concen: 4.916 ng/ul
RT: 13.927 min Scan# 1843
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06

Tgt Ion:163 Resp: 165831




Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.2	4.8
164	10.0	8.0	12.0




#48
2,6-Dinitrotoluene
Concen: 3.968 ng/ul
RT: 14.045 min Scan# 1863
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:165 Resp: 23988

Ion	Ratio	Lower	Upper
165	100		
89	58.2	49.8	74.6
121	25.1	18.6	27.8









#50
Acenaphthylene
Concen: 4.910 ng/ul
RT: 14.192 min Scan# 1888
Delta R.T. -0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:152 Resp: 202340
Ion Ratio Lower Upper
152 100
151 20.4 15.9 23.9
153 13.3 10.5 15.7



#51
3-Nitroaniline
Concen: 3.707 ng/ul
RT: 14.374 min Scan# 1919
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:138 Resp: 25549
Ion Ratio Lower Upper
138 100
108 11.9 8.7 13.1
92 115.3 94.1 141.1









#52
Acenaphthene
Concen: 4.772 ng/ul
RT: 14.539 min Scan# 1947
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:153 Resp: 146079
Ion Ratio Lower Upper
153 100
152 47.9 39.0 58.4
154 88.0 71.7 107.5

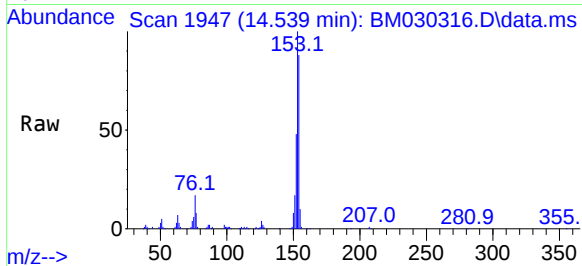

#53
2,4-Dinitrophenol
Concen: 4.944 ng/ul
RT: 14.574 min Scan# 1953
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:184 Resp: 19944
Ion Ratio Lower Upper
184 100
63 67.9 53.9 80.9
154 55.3 47.4 71.0




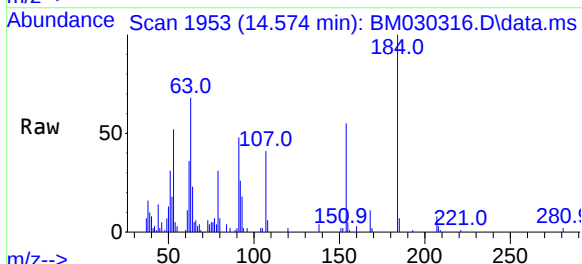




#55
4-Nitrophenol
Concen: 4.361 ng/ul
RT: 14.663 min Scan# 1968
Delta R.T. -0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:109 Resp: 22087
Ion Ratio Lower Upper
109 100
139 137.1 110.1 165.1
65 157.4 112.4 168.6

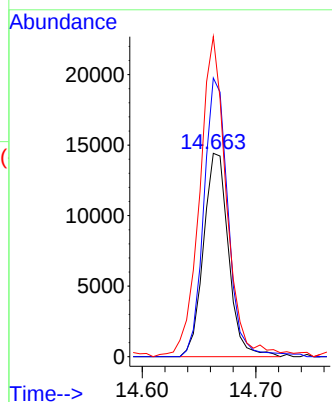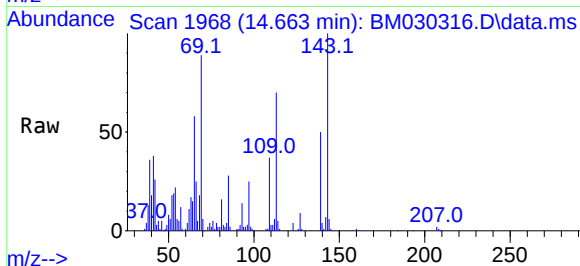

#56
Dibenzofuran
Concen: 4.853 ng/ul
RT: 14.868 min Scan# 2003
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:168 Resp: 206704
Ion Ratio Lower Upper
168 100
139 36.5 29.4 44.0



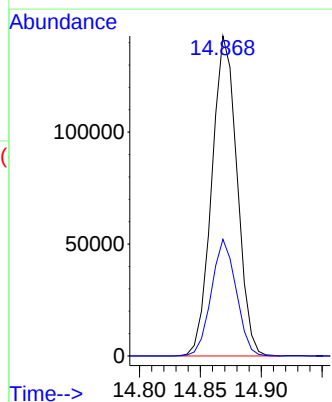
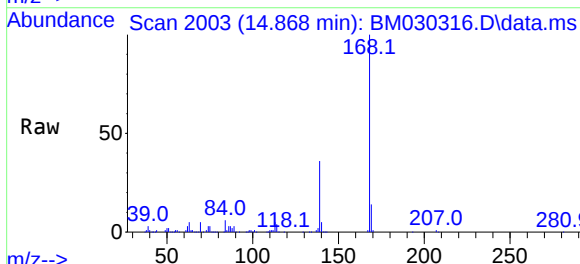




#57
2,4-Dinitrotoluene
Concen: 4.131 ng/ul
RT: 14.827 min Scan# 1996
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:165 Resp: 35323
Ion Ratio Lower Upper
165 100
63 46.4 34.2 51.4
182 2.5 2.1 3.1

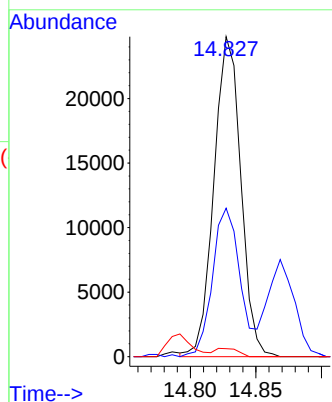

#58
2,3,4,6-Tetrachlorophenol
Concen: 4.350 ng/ul
RT: 15.092 min Scan# 2041
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:232 Resp: 33337
Ion Ratio Lower Upper
232 100
131 49.5 35.7 53.5
130 2.2 1.8 2.6
166 32.2 25.4 38.2


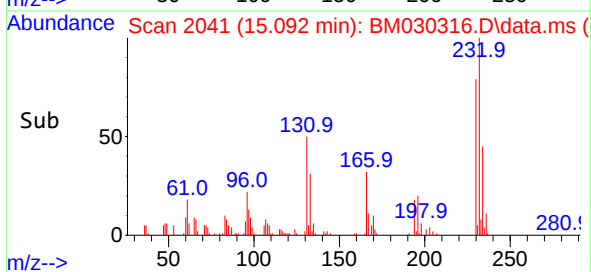






#59
Diethylphthalate
Concen: 4.640 ng/ul
RT: 15.286 min Scan# 2074
Delta R.T. -0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:149 Resp: 154467
Ion Ratio Lower Upper
149 100
177 22.0 17.4 26.0
150 12.8 10.0 15.0



#61
Fluorene
Concen: 4.760 ng/ul
RT: 15.515 min Scan# 2113
Delta R.T. -0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:166 Resp: 170231
Ion Ratio Lower Upper
166 100
165 96.7 77.0 115.6
167 13.3 10.5 15.7









#62
4-Chlorophenyl-phenylether
Concen: 4.963 ng/ul
RT: 15.510 min Scan# 2112
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:204 Resp: 85479
Ion Ratio Lower Upper
204 100
206 31.7 26.1 39.1
141 56.6 44.0 66.0



#63
4-Nitroaniline
Concen: 3.817 ng/ul
RT: 15.533 min Scan# 2116
Delta R.T. 0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:138 Resp: 24633
Ion Ratio Lower Upper
138 100
92 50.9 41.2 61.8
108 74.7 61.3 91.9









#66
4,6-Dinitro-2-methylphenol
Concen: 3.989 ng/ul
RT: 15.586 min Scan# 2125
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:198 Resp: 23811
Ion Ratio Lower Upper
198 100
182 6.5 3.7 5.5#
77 33.2 19.5 29.3#



#67
N-Nitrosodiphenylamine
Concen: 4.539 ng/ul
RT: 15.721 min Scan# 2148
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:169 Resp: 139451
Ion Ratio Lower Upper
169 100
168 69.9 53.8 80.8
167 38.0 29.0 43.6




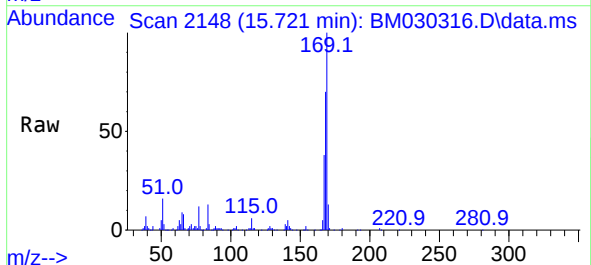




#68
4-Bromophenyl-phenylether
Concen: 4.626 ng/ul
RT: 16.404 min Scan# 2264
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:248	Resp:	46927
Ion Ratio	Lower	Upper
248	100	
250	100.3	78.6 117.8
141	68.1	57.8 86.6

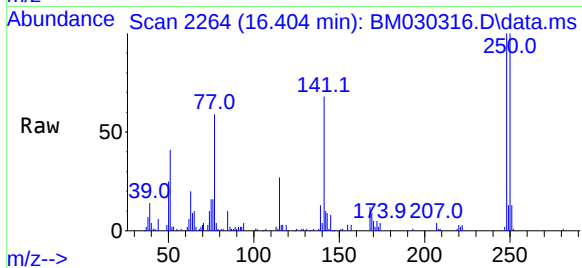

#69
Hexachlorobenzene
Concen: 4.728 ng/ul
RT: 16.515 min Scan# 2283
Delta R.T. -0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:284	Resp:	54520
Ion Ratio	Lower	Upper
284	100	
142	38.7	29.6 44.4
249	30.7	24.0 36.0




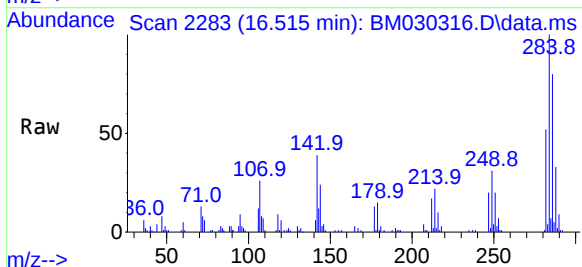




#70
Atrazine
Concen: 3.827 ng/ul
RT: 16.668 min Scan# 2309
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:	200	Resp:	42198
Ion Ratio	Lower	Upper	
200	100		
173	25.0	20.1	30.1
215	48.2	38.3	57.5



#71
Pentachlorophenol
Concen: 4.141 ng/ul
RT: 16.857 min Scan# 2341
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:	266	Resp:	29257
Ion Ratio	Lower	Upper	
266	100		
264	63.1	51.5	77.3
268	72.3	52.3	78.5









#72
Phenanthrene
Concen: 4.673 ng/u1
RT: 17.251 min Scan# 2408
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:178 Resp: 263535
Ion Ratio Lower Upper
178 100
179 15.6 12.2 18.2
176 19.5 15.0 22.6

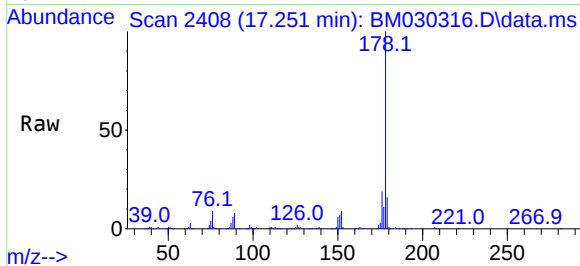

#74
Anthracene
Concen: 4.707 ng/u1
RT: 17.339 min Scan# 2423
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:178 Resp: 267915
Ion Ratio Lower Upper
178 100
179 16.1 12.5 18.7
176 18.2 15.0 22.4




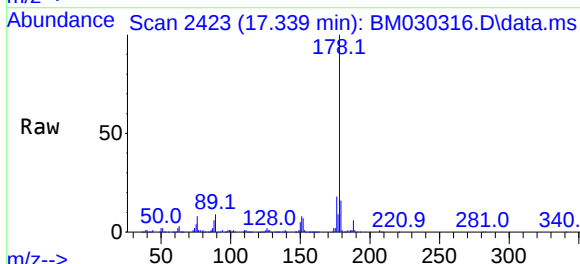




#75
1,2,3,4-Tetrachlorobenzene
Concen: 4.627 ng/uL
RT: 13.274 min Scan# 1732
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:	216	Resp:	69441
Ion Ratio	Lower	Upper	
216	100		
214	77.3	63.9	95.9
218	49.3	38.1	57.1



#76
Pentachlorobenzene
Concen: 4.666 ng/uL
RT: 14.792 min Scan# 1990
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:	250	Resp:	67435
Ion Ratio	Lower	Upper	
250	100		
248	61.9	50.3	75.5
252	64.5	50.6	75.8

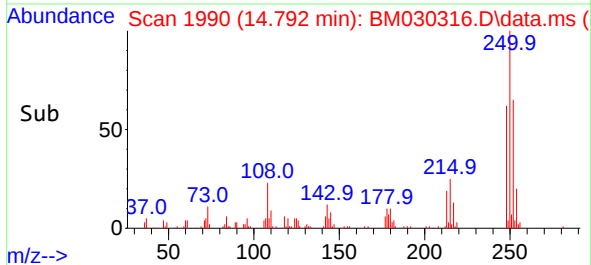







#77
 Carbazole
 Concen: 4.274 ng/ul
 RT: 17.604 min Scan# 2468
 Delta R.T. -0.006 min
 Lab File: BM030316.D
 Acq: 08 Jun 2021 09:35

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT3-2021-06

Tgt Ion:167 Resp: 216028




Ion	Ratio	Lower	Upper
167	100		
166	22.2	16.7	25.1
139	12.9	9.8	14.8

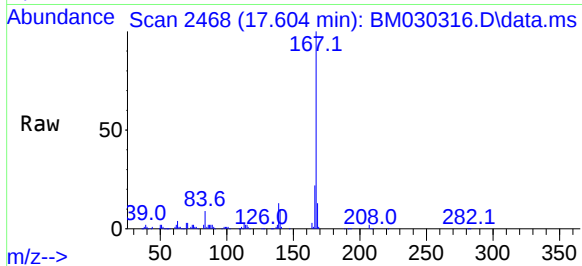


#78
 Di-n-butylphthalate
 Concen: 4.081 ng/ul
 RT: 18.168 min Scan# 2564
 Delta R.T. 0.000 min
 Lab File: BM030316.D
 Acq: 08 Jun 2021 09:35

Tgt Ion:149 Resp: 216046

Ion	Ratio	Lower	Upper
149	100		
150	9.0	7.4	11.2
104	5.5	4.1	6.1




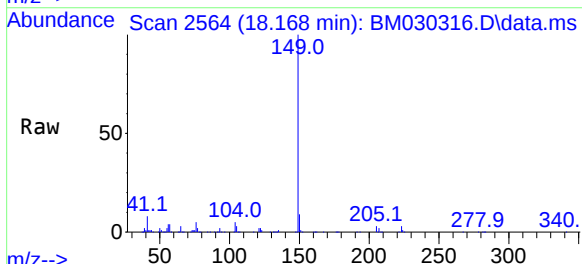




#80
Fluoranthene
Concen: 4.487 ng/ul
RT: 19.256 min Scan# 2749
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:202 Resp: 290318
Ion Ratio Lower Upper
202 100
101 10.4 8.7 13.1
100 8.4 6.6 10.0



#82
Pyrene
Concen: 4.683 ng/ul
RT: 19.615 min Scan# 2810
Delta R.T. -0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:202 Resp: 320438
Ion Ratio Lower Upper
202 100
101 13.8 10.8 16.2
100 11.2 9.1 13.7



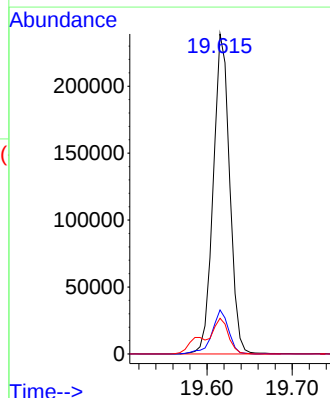





#83
Butylbenzylphthalate
Concen: 3.641 ng/ul
RT: 20.509 min Scan# 2962
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:	149	Resp:	78188
Ion	Ratio	Lower	Upper
149	100		
91	71.5	57.4	86.2
206	20.4	17.3	25.9

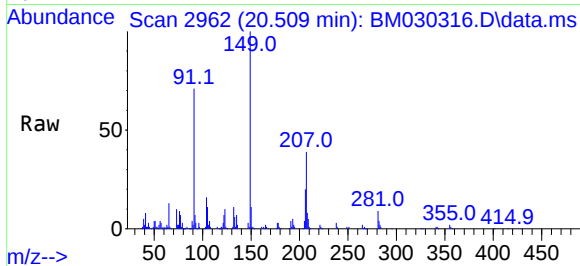

#84
3,3'-Dichlorobenzidine
Concen: 3.641 ng/ul
RT: 21.286 min Scan# 3094
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:	252	Resp:	66248
Ion	Ratio	Lower	Upper
252	100		
254	63.8	51.3	76.9
126	11.4	10.0	15.0



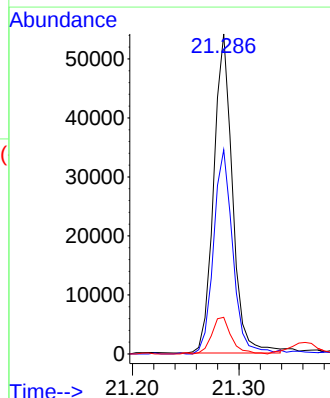
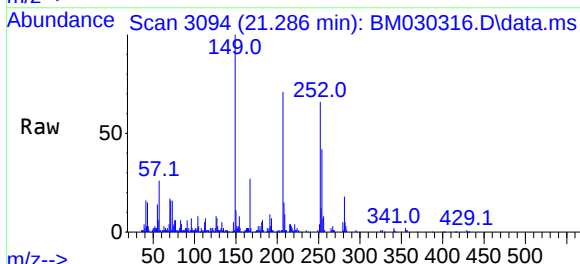




#85
Benzo(a)anthracene
Concen: 4.719 ng/ul
RT: 21.350 min Scan# 3105
Delta R.T. -0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:228 Resp: 286832
Ion Ratio Lower Upper
228 100
229 19.0 15.6 23.4
226 26.9 22.2 33.2

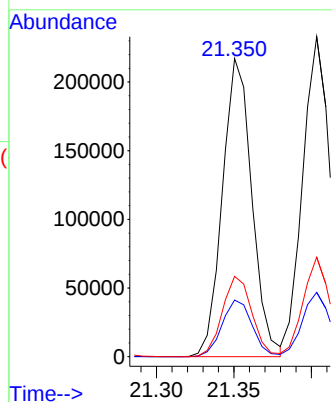

#86
Bis(2-ethylhexyl)phthalate
Concen: 3.432 ng/ul
RT: 21.280 min Scan# 3093
Delta R.T. -0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:149 Resp: 111813
Ion Ratio Lower Upper
149 100
167 26.3 20.9 31.3
279 4.2 3.0 4.6









#87
Chrysene
Concen: 4.807 ng/ul
RT: 21.403 min Scan# 3114
Delta R.T. -0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:	228	Resp:	288107
Ion	Ratio	Lower	Upper
228	100		
226	31.1	24.2	36.2
229	20.1	15.8	23.6

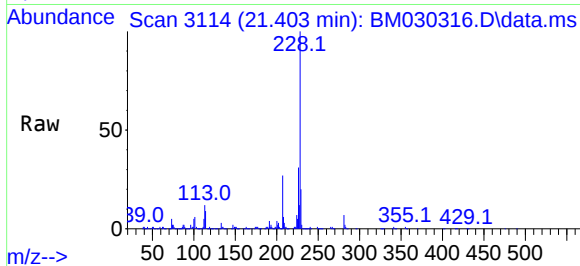

#89
Di-n-octyl phthalate
Concen: 3.021 ng/ul
RT: 22.168 min Scan# 3244
Delta R.T. -0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:149 Resp: 179559




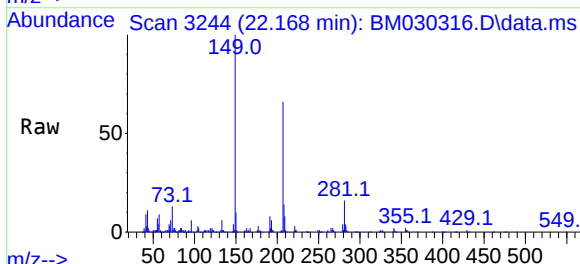




#90
Benzo(b)fluoranthene
Concen: 4.579 ng/ul
RT: 22.962 min Scan# 3379
Delta R.T. 0.000 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt	Ion:252	Resp:	271613
Ion	Ratio	Lower	Upper
252	100		
253	21.3	18.0	27.0
125	9.6	8.6	13.0



#91
Benzo(k)fluoranthene
Concen: 4.637 ng/ul
RT: 23.003 min Scan# 3386
Delta R.T. -0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt	Ion:252	Resp:	262679
Ion	Ratio	Lower	Upper
252	100		
253	22.7	17.9	26.9
125	11.3	8.4	12.6









#93
Benzo(a)pyrene
Concen: 4.769 ng/ul
RT: 23.550 min Scan# 3479
Delta R.T. -0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06


Tgt Ion:	252	Resp:	247218
Ion Ratio	Lower	Upper	
252	100		
253	22.0	17.8	26.8
125	11.6	9.5	14.3

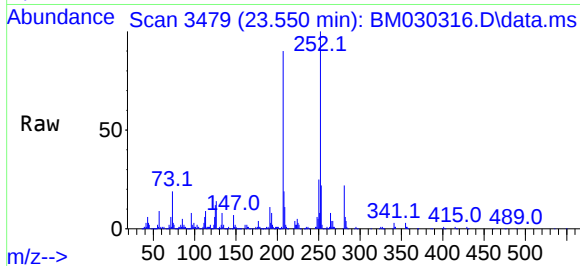

#94
Indeno(1,2,3-cd)pyrene
Concen: 4.265 ng/ul
RT: 25.968 min Scan# 3890
Delta R.T. -0.006 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:	276	Resp:	272107
Ion Ratio	Lower	Upper	
276	100		
138	26.3	21.8	32.6
277	24.8	20.3	30.5



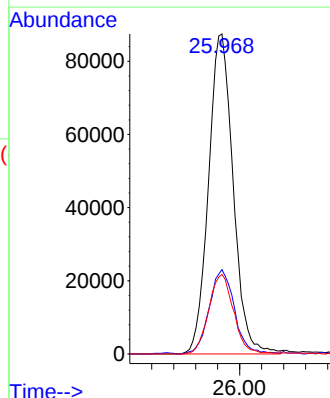
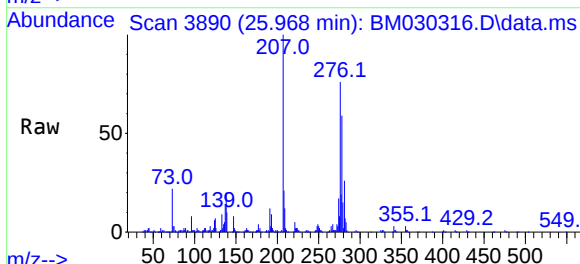




#95
Dibenzo(a,h)anthracene
Concen: 4.202 ng/ul
RT: 25.974 min Scan# 3891
Delta R.T. -0.012 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT3-2021-06

Tgt Ion:	278	Resp:	225725
Ion	Ratio	Lower	Upper
278	100		
139	16.8	13.4	20.2
279	24.2	18.6	28.0

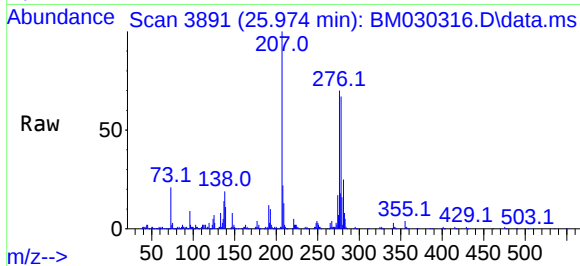

#96
Benzo(g,h,i)perylene
Concen: 4.301 ng/ul
RT: 26.674 min Scan# 4010
Delta R.T. -0.012 min
Lab File: BM030316.D
Acq: 08 Jun 2021 09:35

Tgt Ion:	276	Resp:	225505
Ion	Ratio	Lower	Upper
276	100		
138	22.7	18.7	28.1
277	23.9	18.6	28.0

