
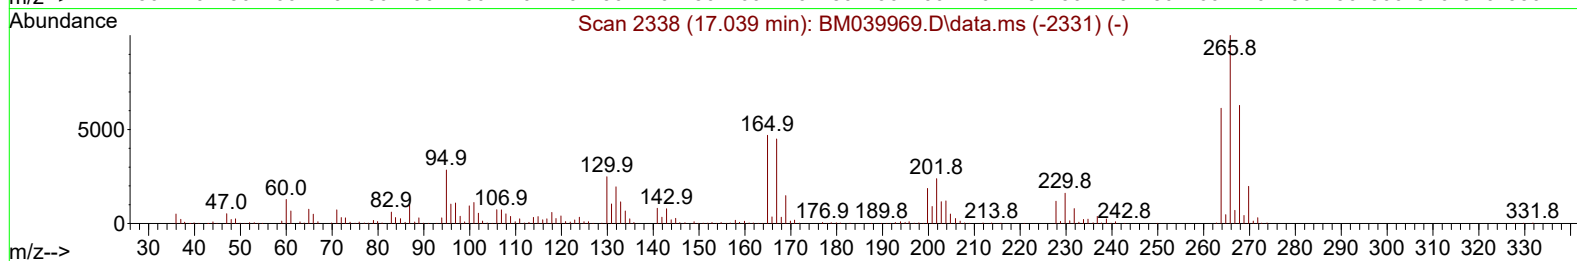
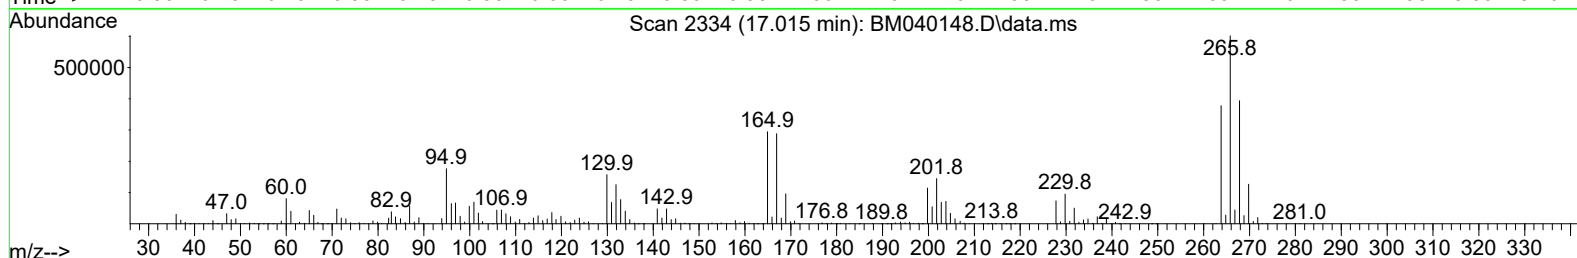


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040148.D
Acq On : 08 Jun 2023 08:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 09:13:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 06 16:45:42 2023
Response via : Initial Calibration

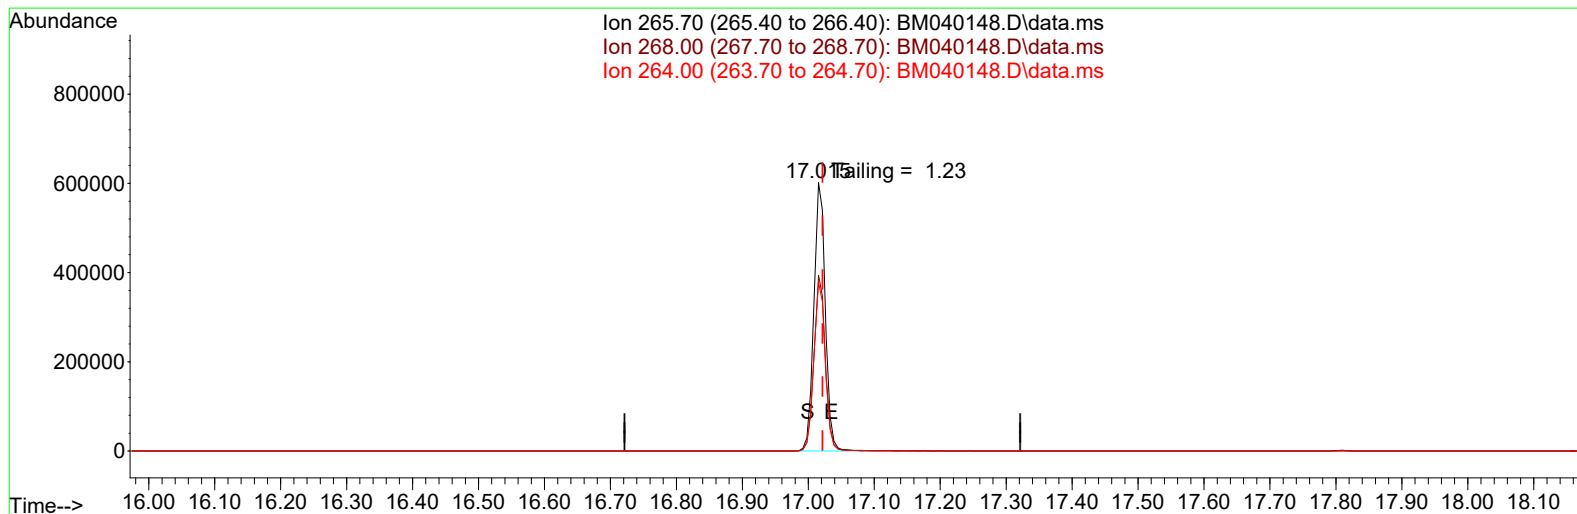

TIC: BM040148.D\data.ms

(70) Pentachlorophenol (C)




17.015min (-0.006) 222839.05 ng

response 731478

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	65.45
264.00	61.30	62.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040148.D
Acq On : 08 Jun 2023 08:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 09:13:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 06 16:45:42 2023
Response via : Initial Calibration

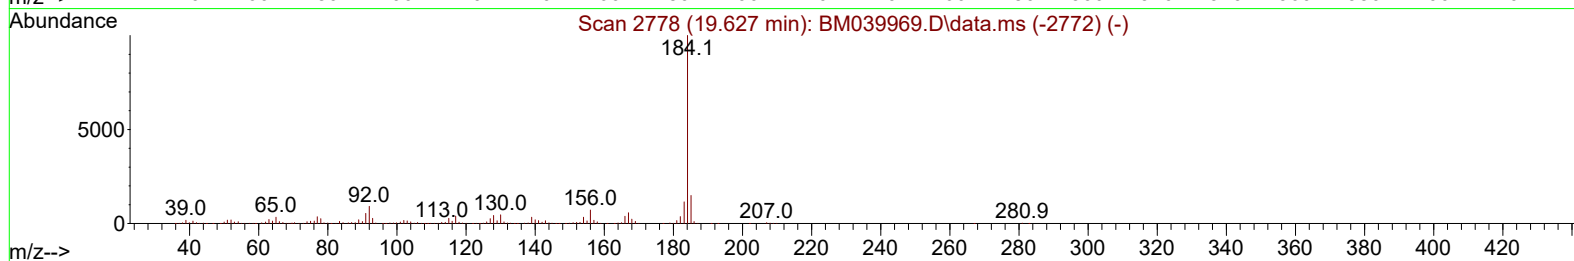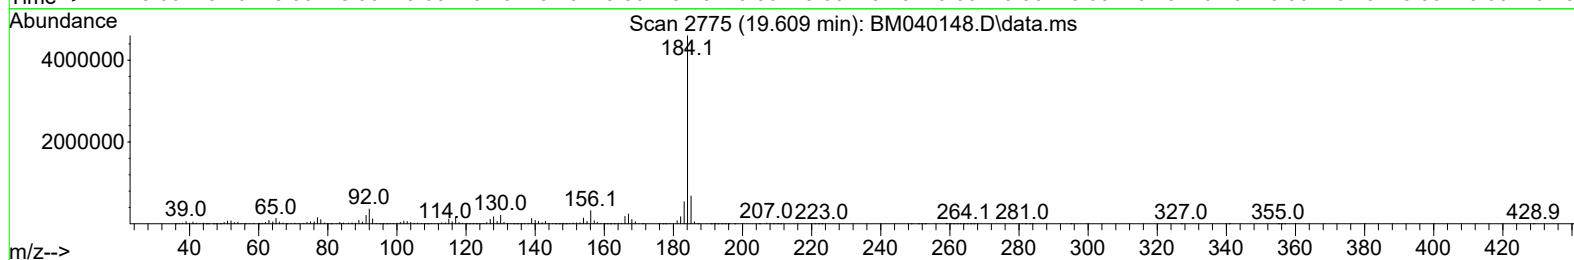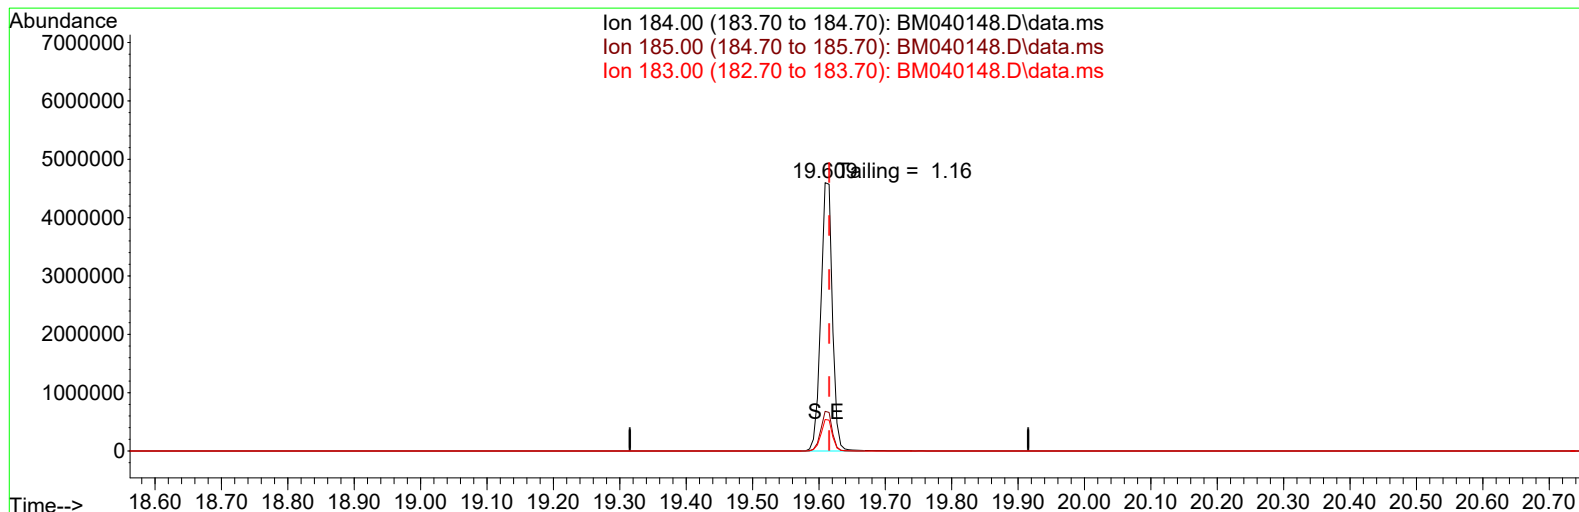

TIC: BM040148.D\data.ms

(77) Benzidine**19.609min (-0.006) 853163.81 ng****response 5564458**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.82
183.00	11.50	11.77
0.00	0.00	0.00