
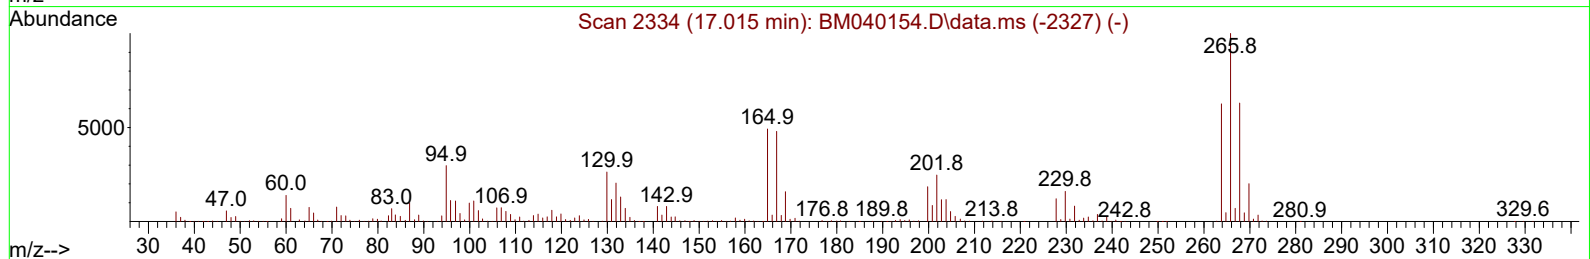
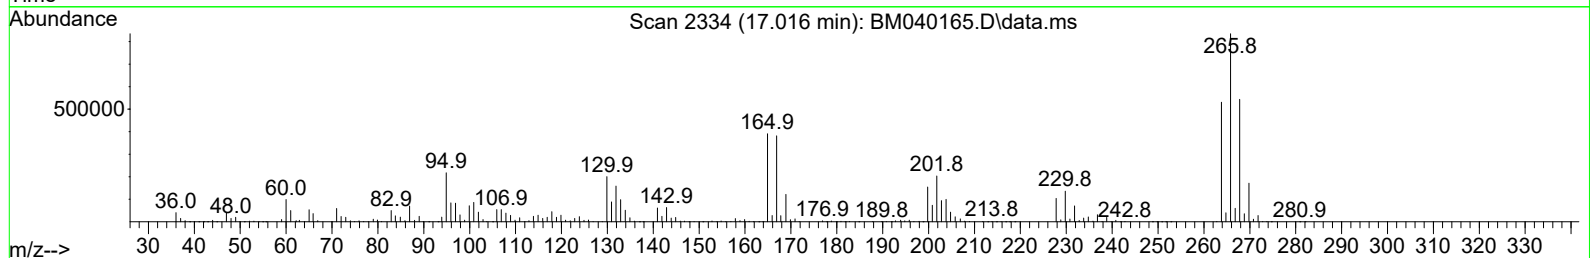


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040165.D
Acq On : 08 Jun 2023 19:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 03:50:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 23:25:50 2023
Response via : Initial Calibration

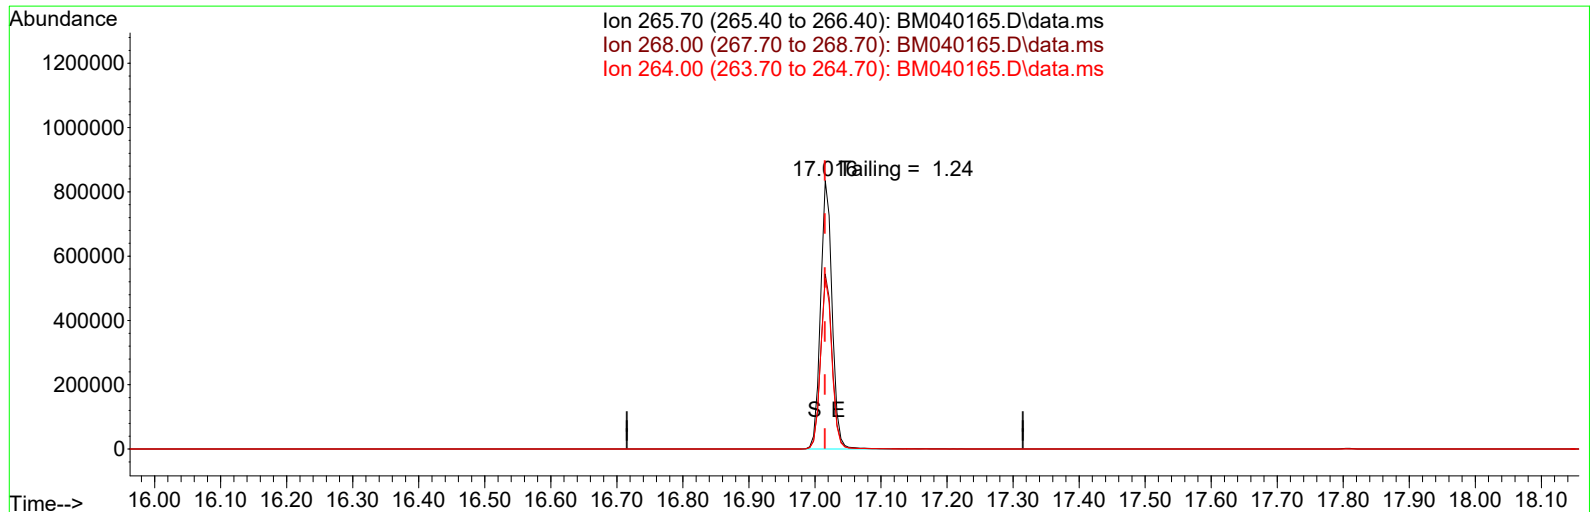

TIC: BM040165.D\data.ms

(70) Pentachlorophenol (C)




17.016min (+ 0.001) 198385.69 ng

response 1018213

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	65.14
264.00	62.60	63.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
 Data File : BM040165.D
 Acq On : 08 Jun 2023 19:43
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 03:50:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 08 23:25:50 2023
 Response via : Initial Calibration

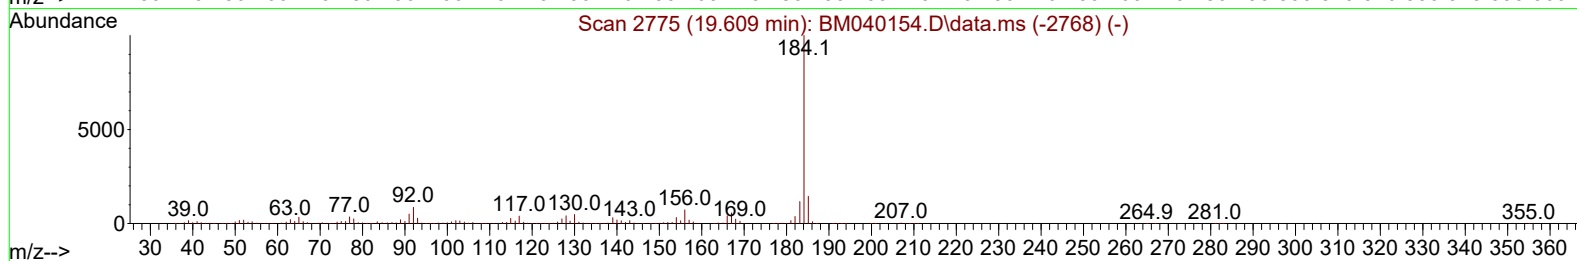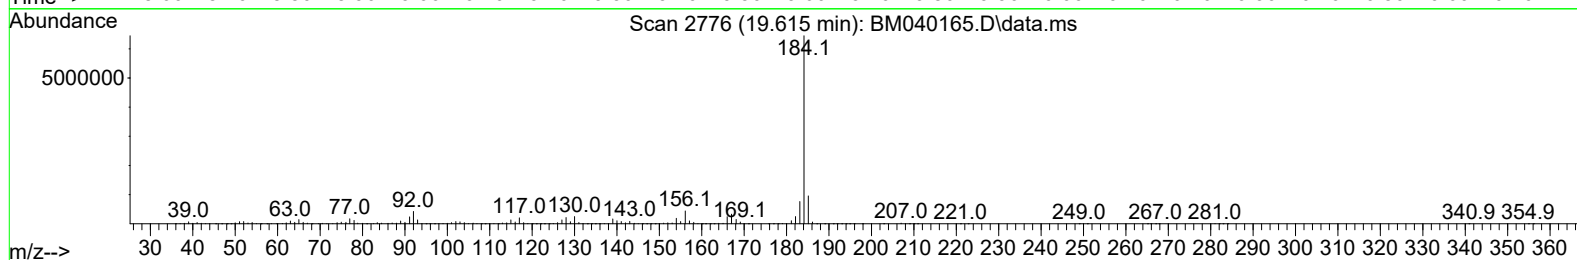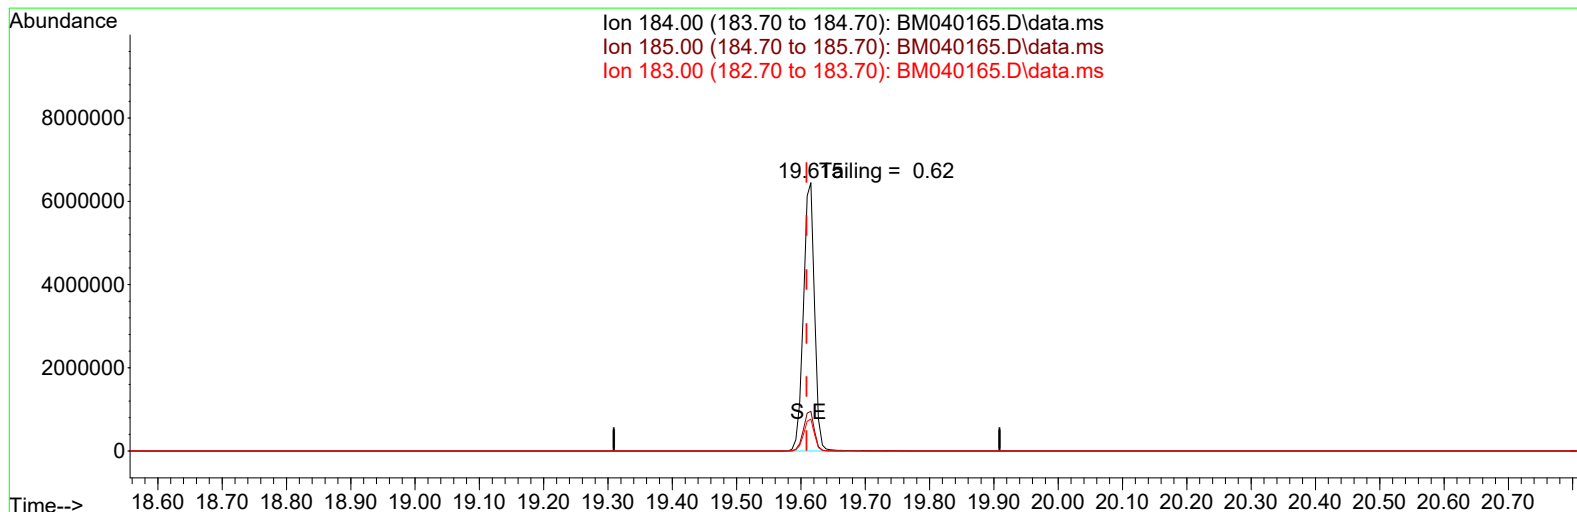

TIC: BM040165.D\data.ms

(77) Benzidine**19.615min (+ 0.006) 622924.65 ng****response 7767976**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.83
183.00	11.70	11.86
0.00	0.00	0.00