

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
 Data File : BM040167.D
 Acq On : 08 Jun 2023 21:32
 Operator : MA/JU
 Sample : PB153236BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB153236BL

Quant Time: Jun 09 02:24:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 08 23:25:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.987	152	309320	20.000	ng	0.00
21) Naphthalene-d8	10.804	136	1258853	20.000	ng	0.00
39) Acenaphthene-d10	14.627	164	682820	20.000	ng	0.00
64) Phenanthrene-d10	17.368	188	1431038	20.000	ng	0.00
76) Chrysene-d12	21.545	240	1179661	20.000	ng	0.00
86) Perylene-d12	23.980	264	1371688	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.540	112	2837328	136.964	ng	0.00
7) Phenol-d6	7.145	99	3474762	122.925	ng	0.00
23) Nitrobenzene-d5	9.157	82	1843649	79.270	ng	0.00
42) 2,4,6-Tribromophenol	16.110	330	1258609	122.511	ng	0.00
45) 2-Fluorobiphenyl	13.257	172	4406459	85.294	ng	0.00
79) Terphenyl-d14	19.986	244	7793005	121.778	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040167.D
Acq On : 08 Jun 2023 21:32
Operator : MA/JU
Sample : PB153236BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153236BL

Quant Time: Jun 09 02:24:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 23:25:50 2023
Response via : Initial Calibration




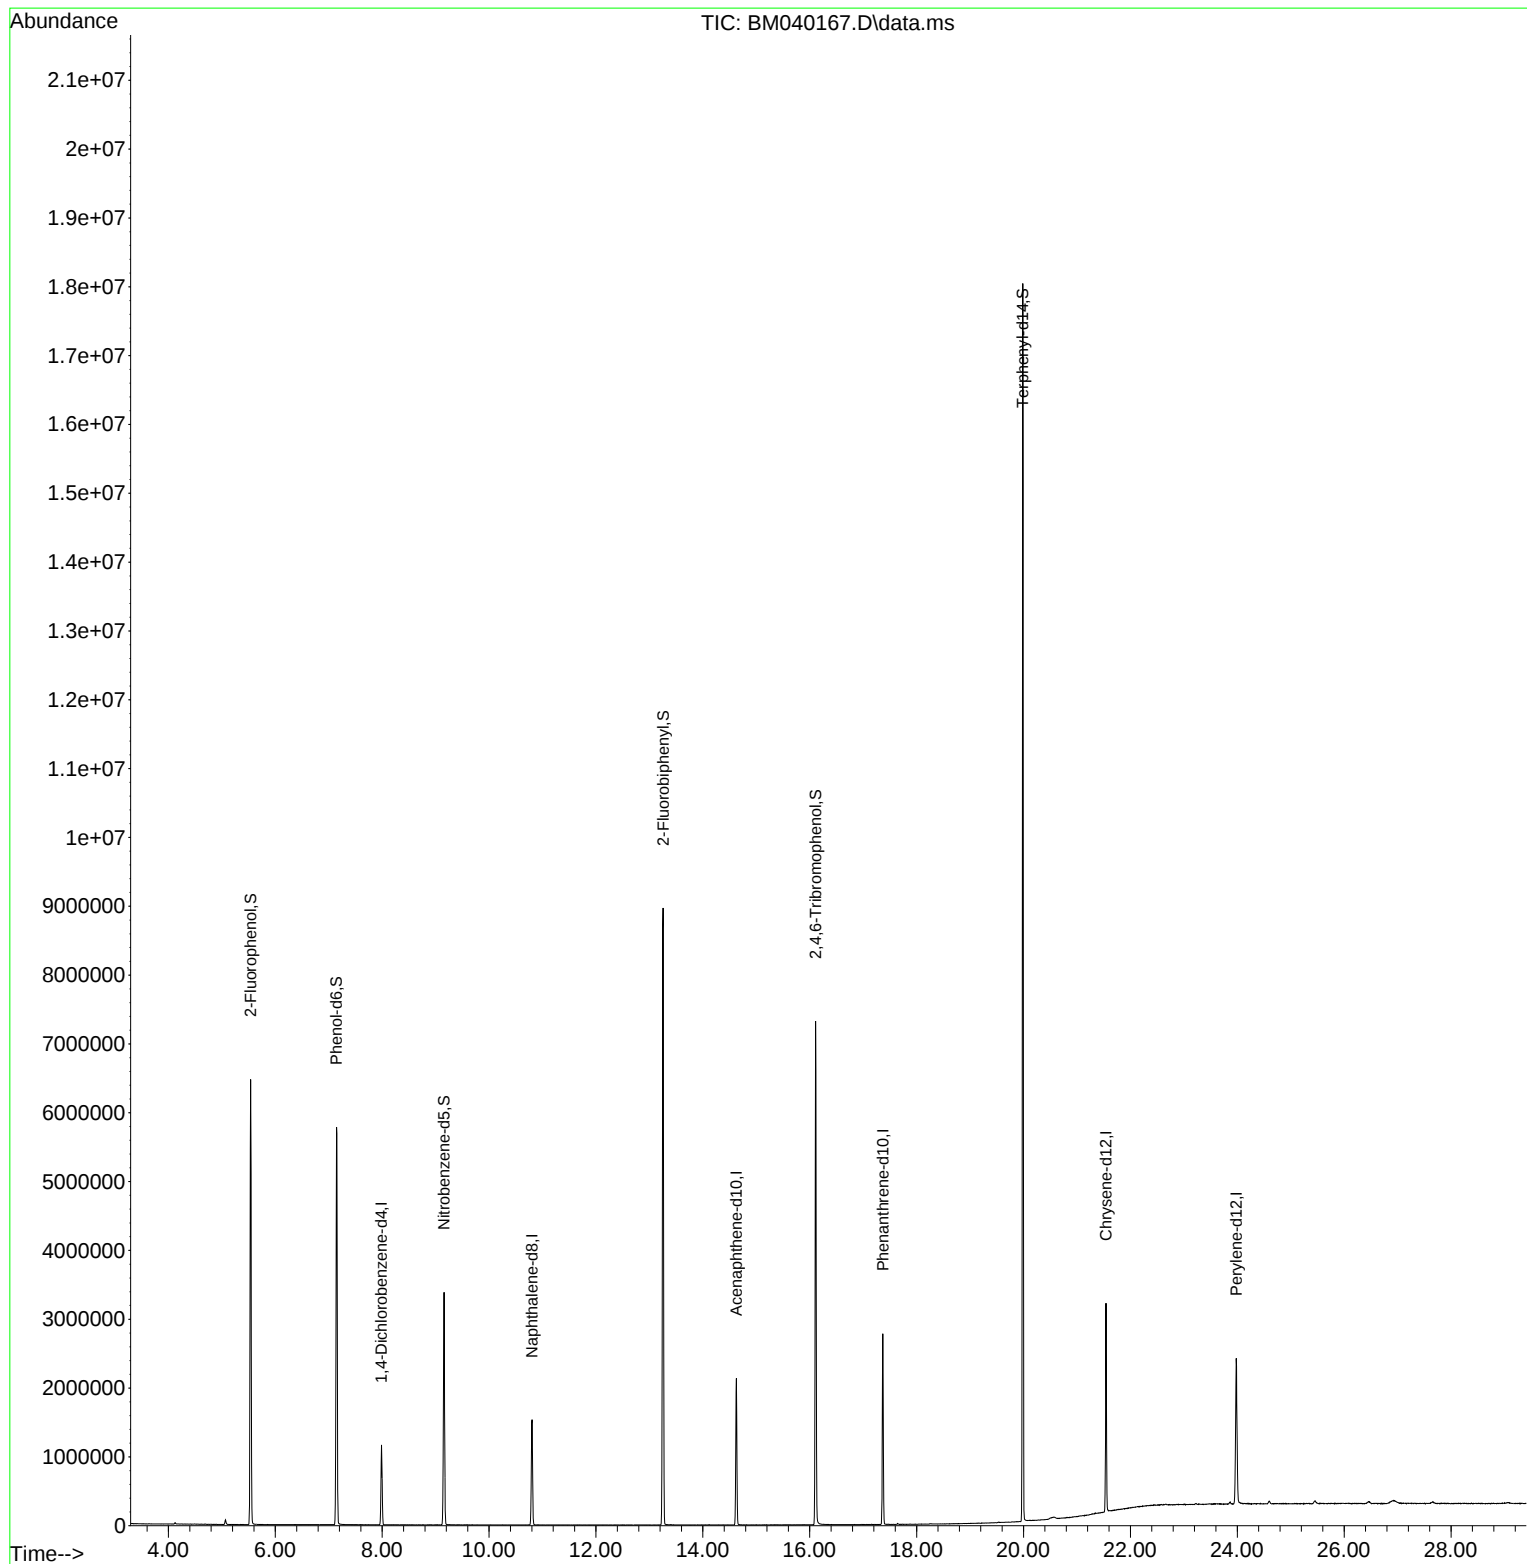


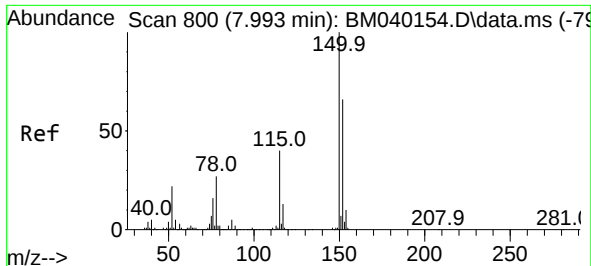

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.987 min Scan# 79
Delta R.T. -0.006 min
Lab File: BM040167.D
Acq: 08 Jun 2023 21:32




Instrument :
BNA_M
ClientSampleId :
PB153236BL


Tgt Ion:152 Resp: 309320
Ion Ratio Lower Upper
152 100
150 153.5 121.4 182.0
115 59.3 48.2 72.4

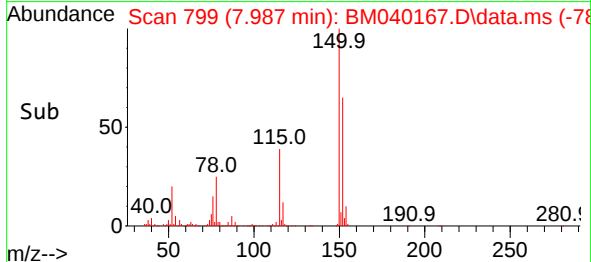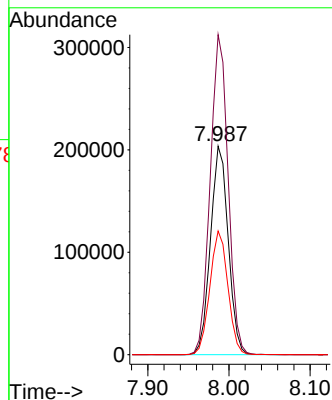

#5
2-Fluorophenol
Concen: 136.964 ng
RT: 5.540 min Scan# 383
Delta R.T. 0.006 min
Lab File: BM040167.D
Acq: 08 Jun 2023 21:32

Tgt Ion:112 Resp: 2837328
Ion Ratio Lower Upper
112 100
64 51.4 43.8 65.6
63 26.4 22.8 34.2

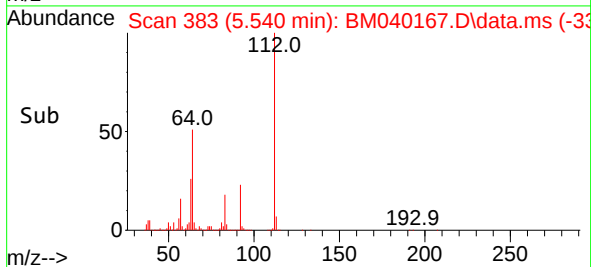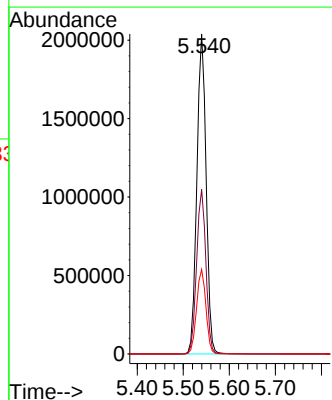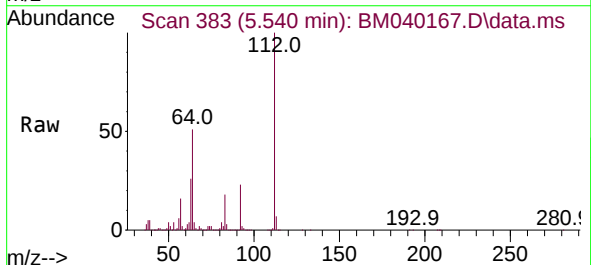




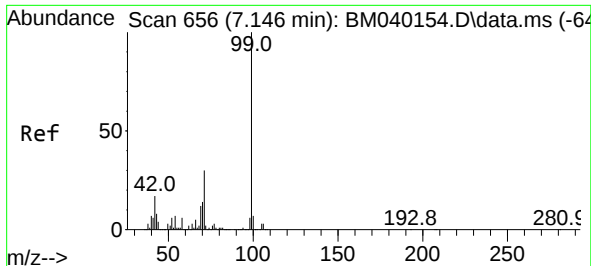


#7
Phenol-d6
Concen: 122.925 ng
RT: 7.145 min Scan# 61
Delta R.T. -0.000 min
Lab File: BM040167.D
Acq: 08 Jun 2023 21:32

Instrument :
BNA_M
ClientSampleId :
PB153236BL

Tgt Ion: 99 Resp: 3474762




Ion	Ratio	Lower	Upper
99	100		
42	16.3	13.4	20.2
71	30.4	24.3	36.5

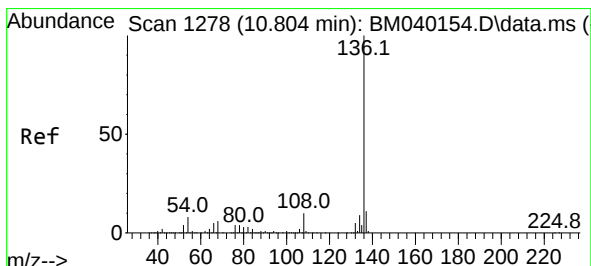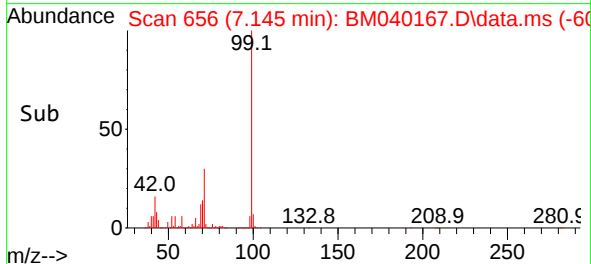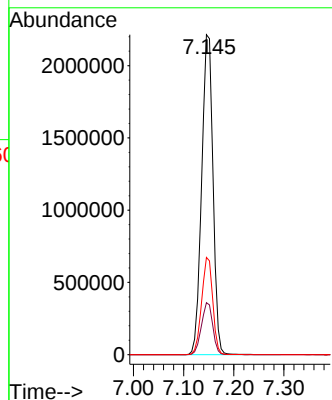


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.804 min Scan# 1278
Delta R.T. 0.000 min
Lab File: BM040167.D
Acq: 08 Jun 2023 21:32

Tgt Ion: 136 Resp: 1258853

Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.8	13.2
54	6.9	6.2	9.4
68	5.8	5.0	7.4


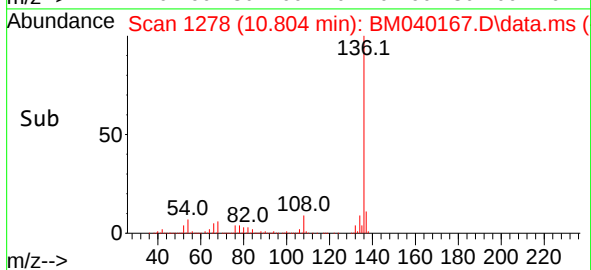
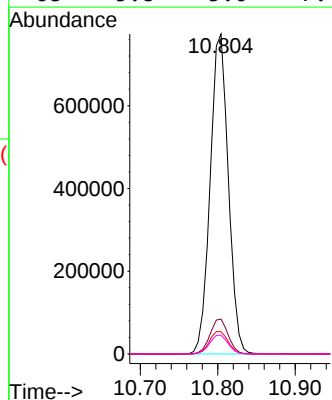
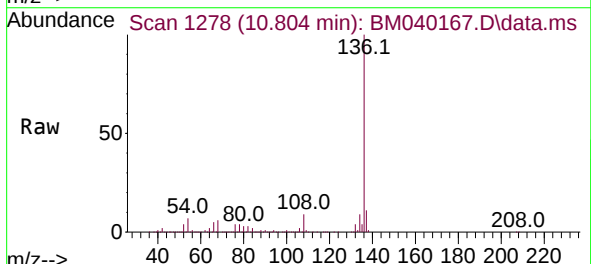


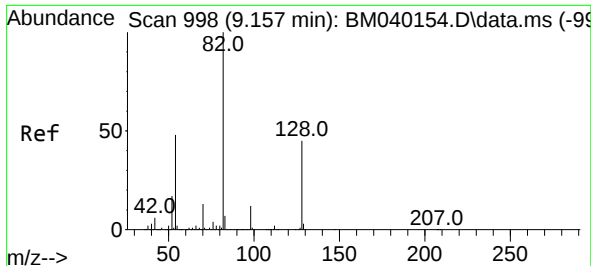

#23
 Nitrobenzene-d5
 Concen: 79.270 ng
 RT: 9.157 min Scan# 998
 Delta R.T. -0.000 min
 Lab File: BM040167.D
 Acq: 08 Jun 2023 21:32




Instrument :
 BNA_M
 ClientSampleId :
 PB153236BL


Tgt Ion: 82 Resp: 1843649
 Ion Ratio Lower Upper
 82 100
 128 46.5 36.0 54.0
 54 46.1 38.5 57.7

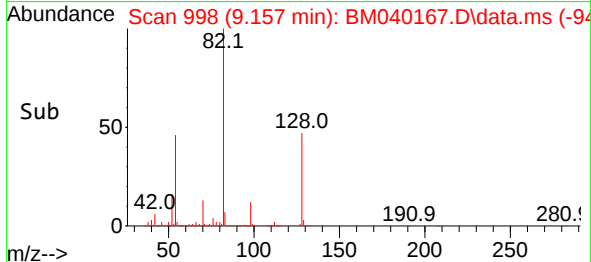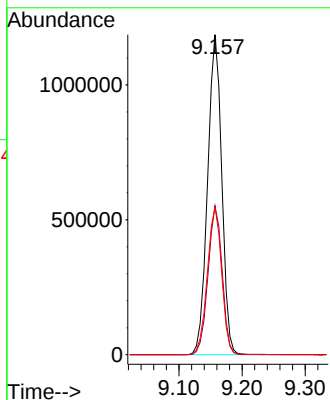

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.627 min Scan# 1928
 Delta R.T. 0.000 min
 Lab File: BM040167.D
 Acq: 08 Jun 2023 21:32

Tgt Ion: 164 Resp: 682820
 Ion Ratio Lower Upper
 164 100
 162 101.9 80.4 120.6
 160 46.2 35.9 53.9


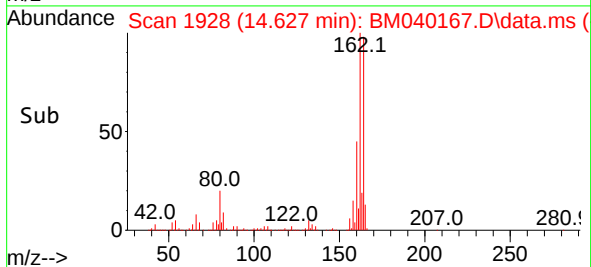
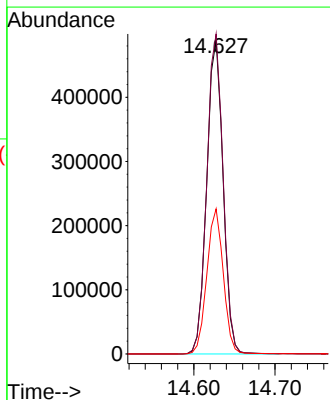
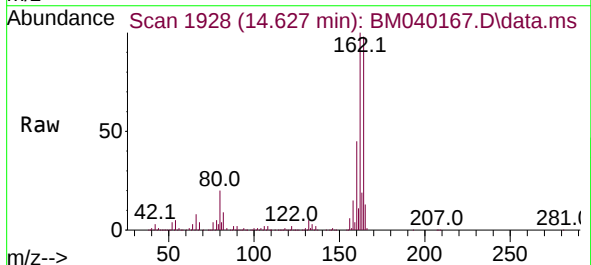


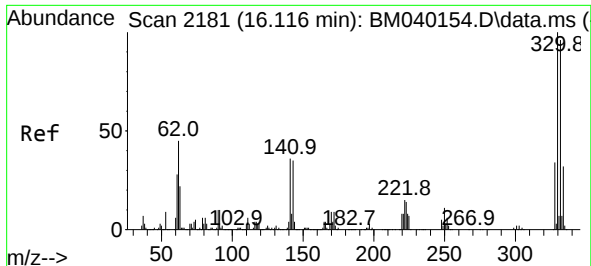

#42
2,4,6-Tribromophenol
Concen: 122.511 ng
RT: 16.110 min Scan# 2181
Delta R.T. -0.006 min
Lab File: BM040167.D
Acq: 08 Jun 2023 21:32




Instrument :
BNA_M
ClientSampleId :
PB153236BL


Tgt Ion:330 Resp: 1258609
Ion Ratio Lower Upper
330 100
332 96.5 77.1 115.7
141 35.8 31.6 47.4

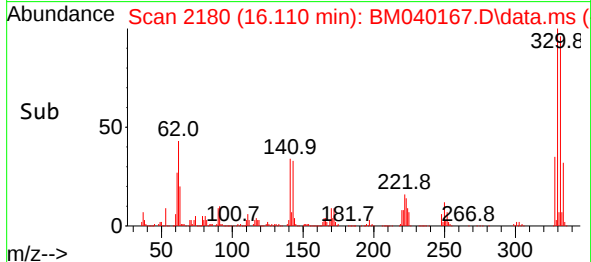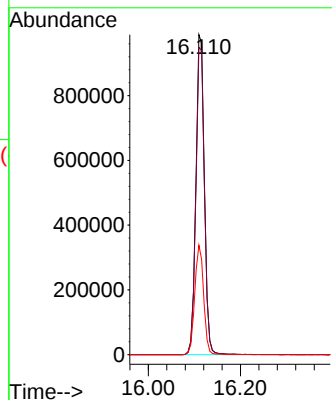

#45
2-Fluorobiphenyl
Concen: 85.294 ng
RT: 13.257 min Scan# 1695
Delta R.T. -0.000 min
Lab File: BM040167.D
Acq: 08 Jun 2023 21:32

Tgt Ion:172 Resp: 4406459
Ion Ratio Lower Upper
172 100
171 35.7 28.8 43.2
170 24.7 19.8 29.6


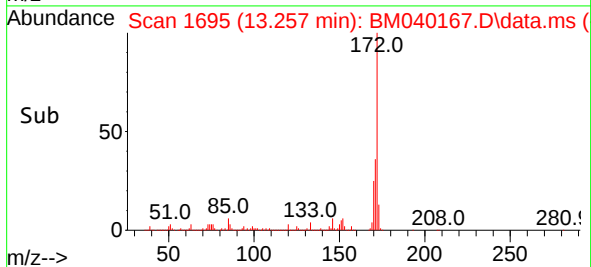
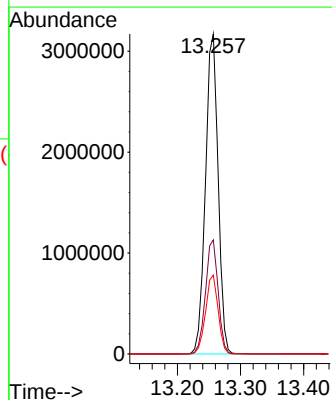
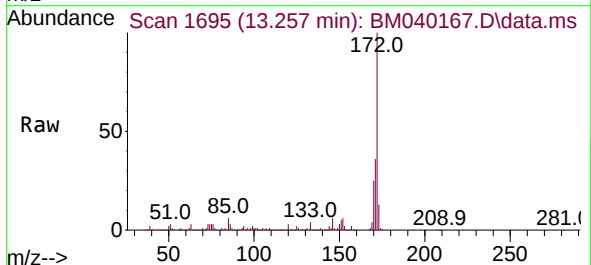


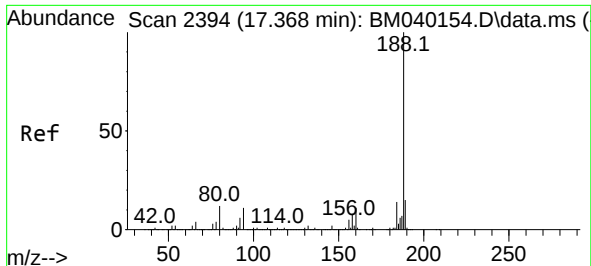

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.368 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM040167.D
Acq: 08 Jun 2023 21:32




Instrument :
BNA_M
ClientSampleId :
PB153236BL


Tgt Ion:188 Resp: 1431038
Ion Ratio Lower Upper
188 100
94 10.3 8.9 13.3
80 11.1 9.6 14.4

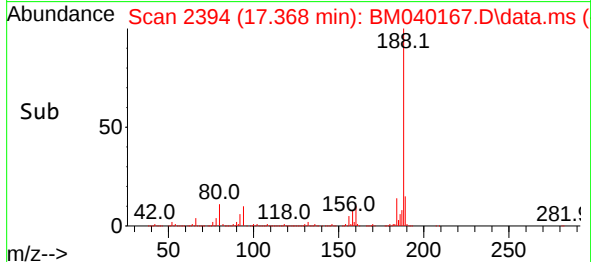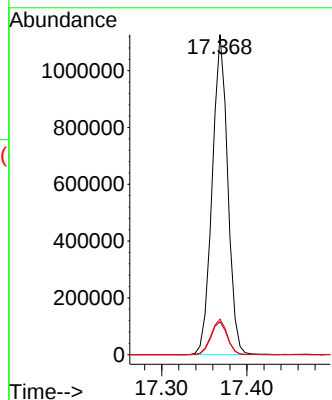

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.545 min Scan# 3104
Delta R.T. -0.006 min
Lab File: BM040167.D
Acq: 08 Jun 2023 21:32

Tgt Ion:240 Resp: 1179661
Ion Ratio Lower Upper
240 100
120 12.9 9.9 14.9
236 26.2 21.1 31.7


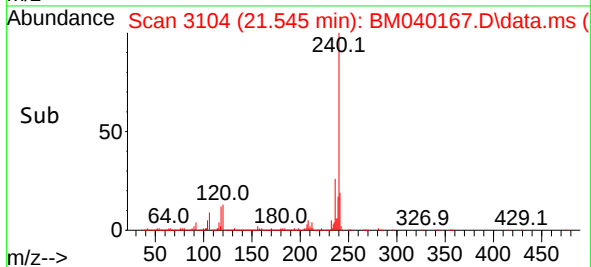
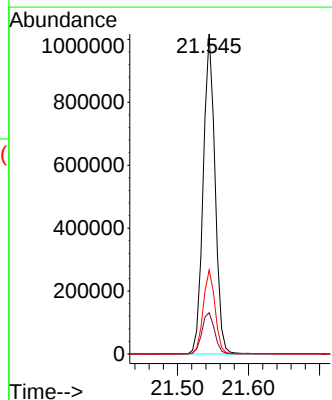
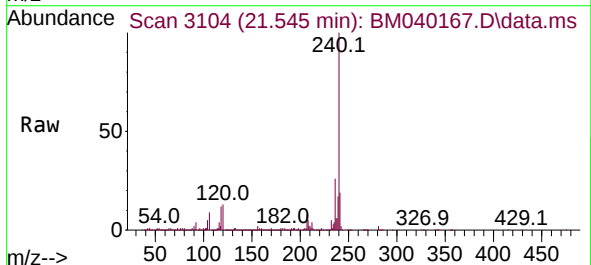


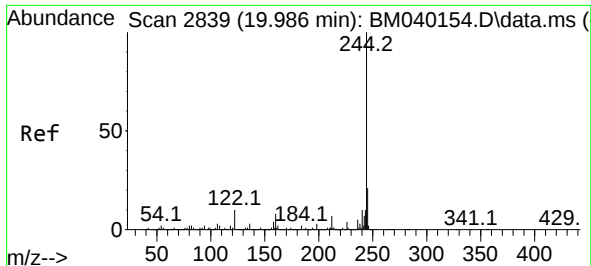

#79
 Terphenyl-d14
 Concen: 121.778 ng
 RT: 19.986 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BM040167.D
 Acq: 08 Jun 2023 21:32

Instrument :
 BNA_M
 ClientSampleId :
 PB153236BL

Tgt Ion:244 Resp: 7793005
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.7 8.5
 122 9.5 7.9 11.9

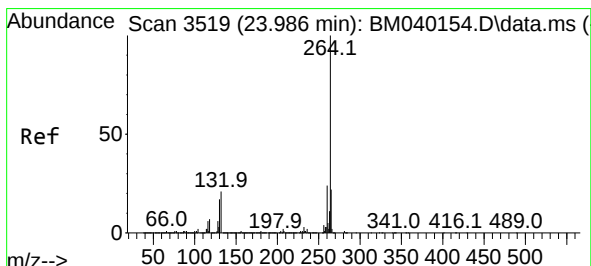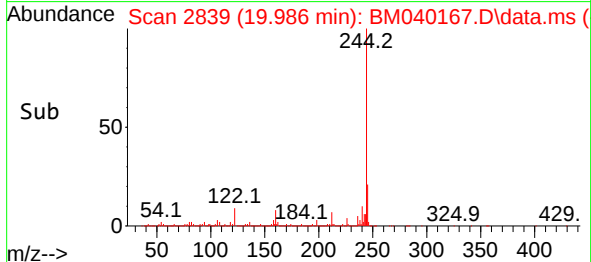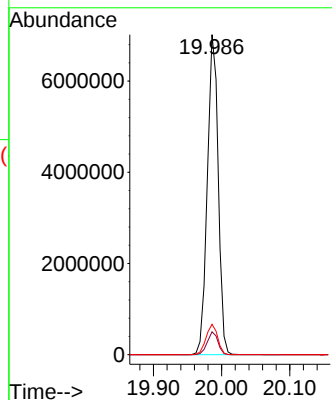

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.980 min Scan# 3518
 Delta R.T. -0.006 min
 Lab File: BM040167.D
 Acq: 08 Jun 2023 21:32

Tgt Ion:264 Resp: 1371688
 Ion Ratio Lower Upper
 264 100
 260 23.9 19.1 28.7
 265 21.6 17.7 26.5

