

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
 Data File : BM040161.D
 Acq On : 08 Jun 2023 16:41
 Operator : MA/JU
 Sample : 03074-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GT-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040161.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.540	376	383	399	rBV	3771047	5445644	41.25%	8.954%
2	7.146	648	656	667	rBV	3735670	5609993	42.49%	9.225%
3	7.987	790	799	806	rBV	1020216	1627279	12.33%	2.676%
4	9.157	989	998	1006	rBV	2034489	3262823	24.71%	5.365%
5	10.804	1268	1278	1287	rBV	1408137	2300942	17.43%	3.783%
6	13.257	1688	1695	1705	rBV	5764721	8083064	61.23%	13.291%
7	14.627	1921	1928	1938	rBV	2018186	2852863	21.61%	4.691%
8	15.980	2152	2158	2165	rBV	479339	617575	4.68%	1.015%
9	16.110	2174	2180	2198	rBV	4483007	5949439	45.06%	9.783%
10	17.368	2387	2394	2403	rBV	2559932	3437024	26.03%	5.652%
11	18.257	2541	2545	2553	rBV2	84328	132861	1.01%	0.218%
12	19.986	2833	2839	2852	rBV	12155523	13202154	100.00%	21.708%
13	21.245	3049	3053	3059	rBV	211782	299001	2.26%	0.492%
14	21.545	3099	3104	3113	rBV	3236015	3789287	28.70%	6.231%
15	23.986	3512	3519	3530	rVB	2148793	4205963	31.86%	6.916%




Sum of corrected areas: 60815912

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040161.D
Acq On : 08 Jun 2023 16:41
Operator : MA/JU
Sample : 03074-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GT-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

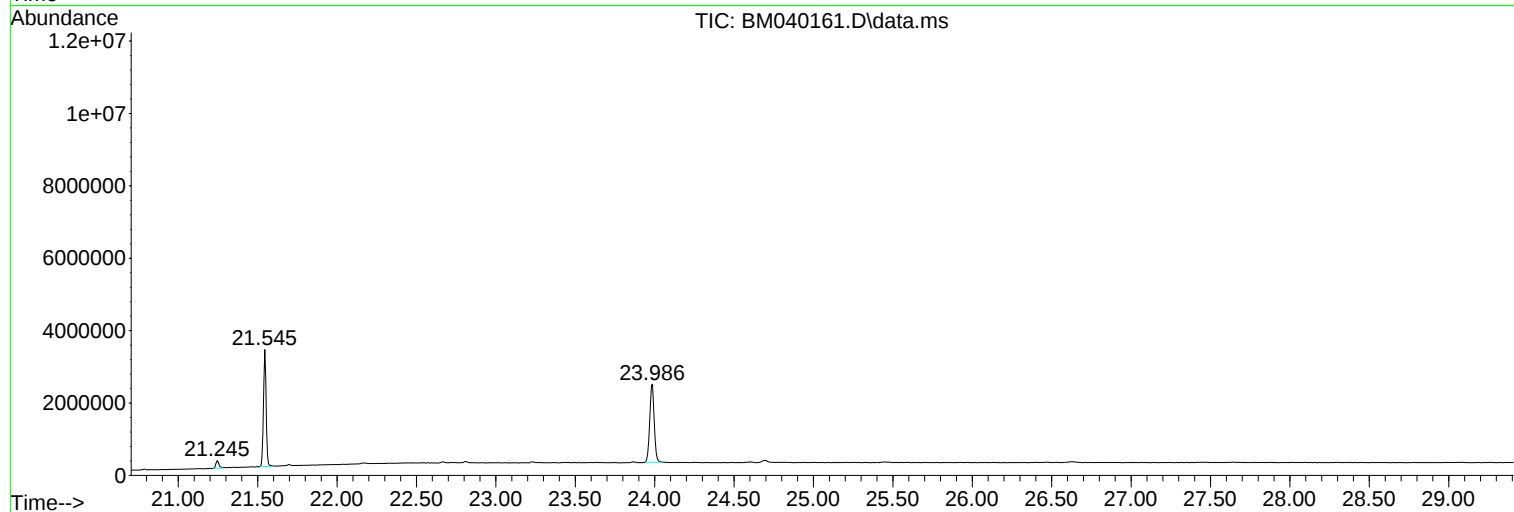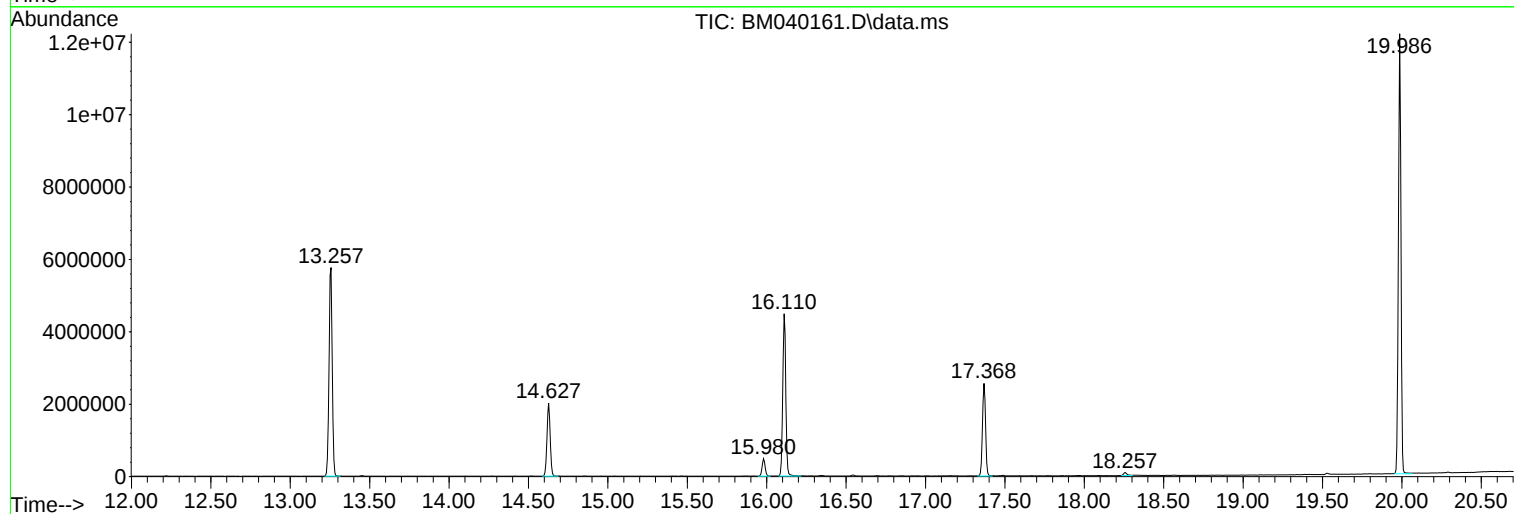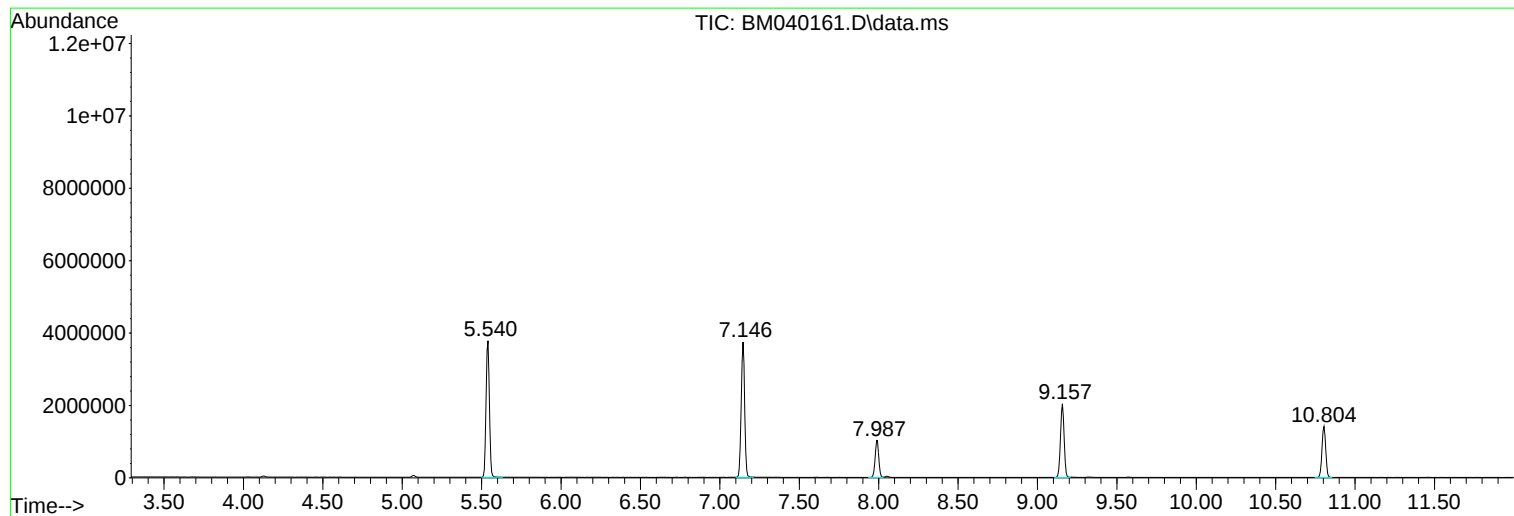

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040161.D
Acq On : 08 Jun 2023 16:41
Operator : MA/JU
Sample : 03074-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GT-01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.980	4.33 ng	617575	Acenaphthene-d10	14.627

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			1,2,4,5-Tetroxane, 3,3,6,6-tetra...	396	C26H20O4	016204-36-7	78
3			Azobenzene	182	C12H10N2	000103-33-3	64
4			Benzeneacetic acid, .alpha.-oxo-...	164	C9H8O3	015206-55-0	53
5			Phenyl 4-pyridyl ketone	183	C12H9NO	014548-46-0	50

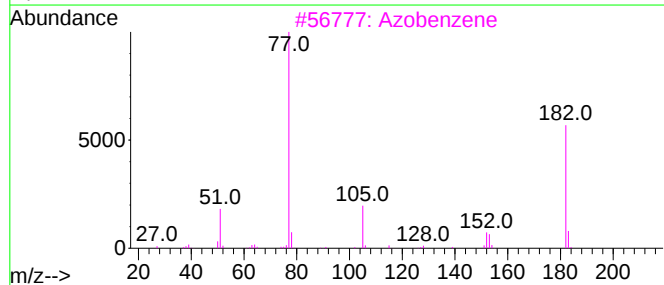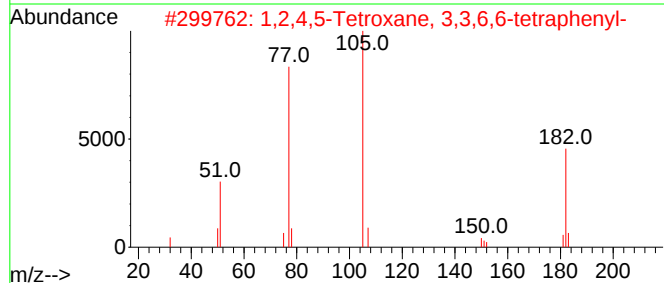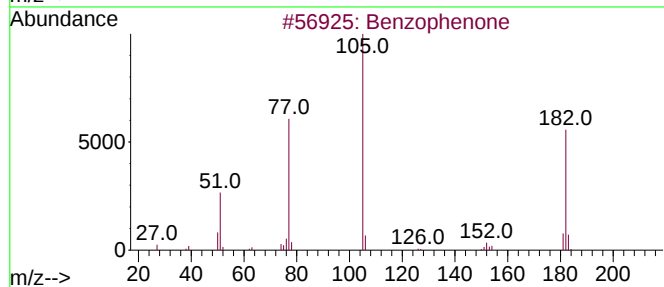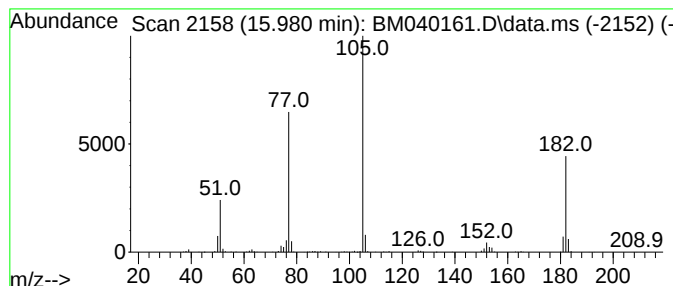

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040161.D
Acq On : 08 Jun 2023 16:41
Operator : MA/JU
Sample : 03074-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GT-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.980	4.3	ng	617575	3	14.627	2852860	20.0