

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
 Data File : BM040162.D
 Acq On : 08 Jun 2023 17:17
 Operator : MA/JU
 Sample : 03074-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GT-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.540	376	383	393	rBV	3462373	4968445	39.82%	8.502%
2	7.145	648	656	666	rBV	3525359	5238193	41.98%	8.964%
3	7.987	791	799	806	rBV	1020831	1612481	12.92%	2.759%
4	9.157	990	998	1006	rBV	1938707	3037550	24.34%	5.198%
5	10.804	1269	1278	1288	rBV	1422123	2321165	18.60%	3.972%
6	13.257	1687	1695	1704	rBV	5301129	7625083	61.11%	13.049%
7	14.627	1921	1928	1940	rVB	2084240	2903436	23.27%	4.969%
8	15.980	2152	2158	2166	rBV	447172	588017	4.71%	1.006%
9	16.110	2174	2180	2199	rBV	4334730	5663552	45.39%	9.692%
10	17.368	2388	2394	2405	rBV	2653692	3511540	28.14%	6.009%
11	18.257	2540	2545	2552	rBV	104297	160911	1.29%	0.275%
12	19.986	2833	2839	2844	rBV	11631529	12477300	100.00%	21.352%
13	21.245	3049	3053	3060	rBV2	213712	309608	2.48%	0.530%
14	21.545	3099	3104	3113	rBV	3181032	3814499	30.57%	6.528%
15	23.986	3511	3519	3531	rVB	2145732	4203608	33.69%	7.194%




Sum of corrected areas: 58435388

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040162.D
Acq On : 08 Jun 2023 17:17
Operator : MA/JU
Sample : 03074-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GT-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

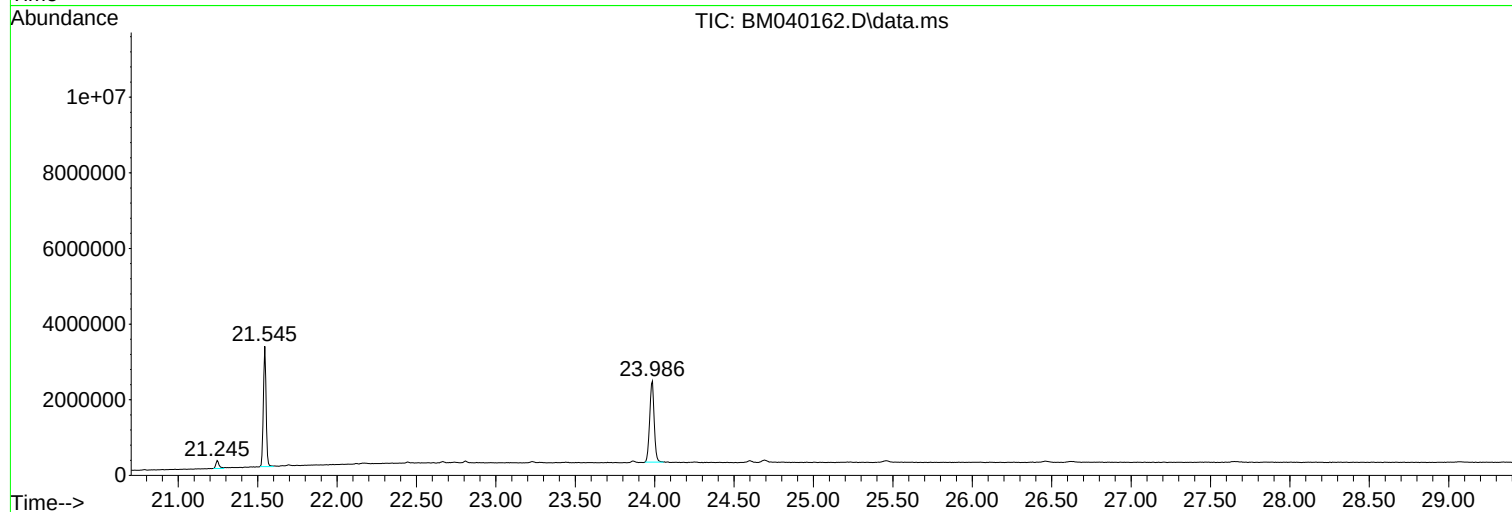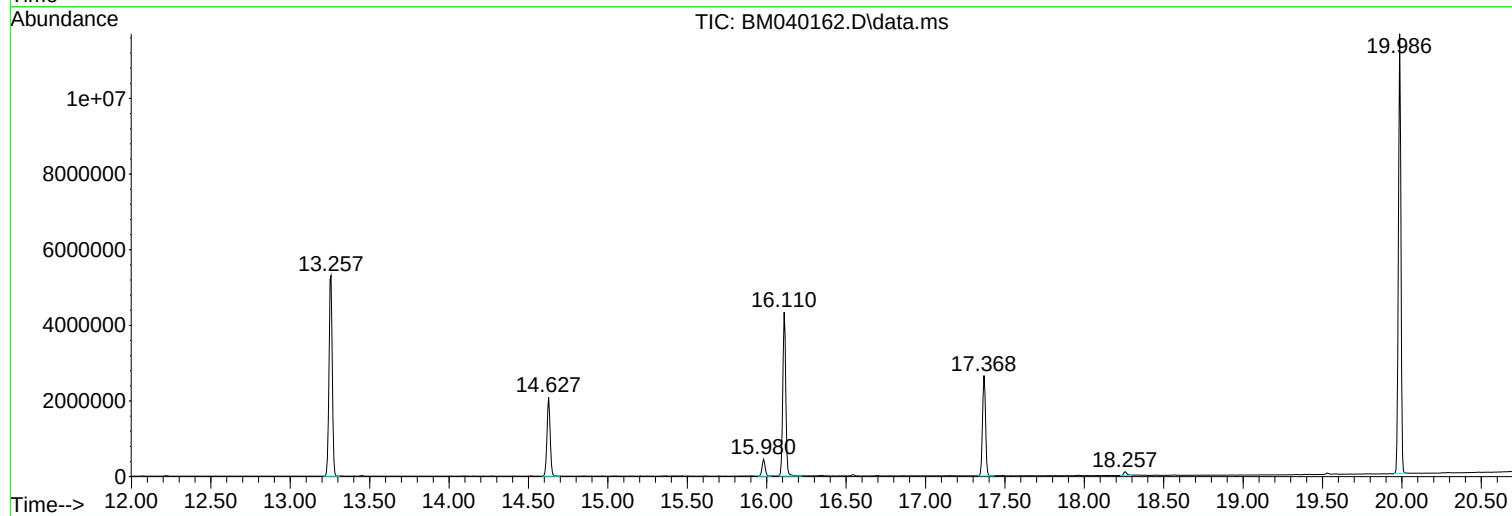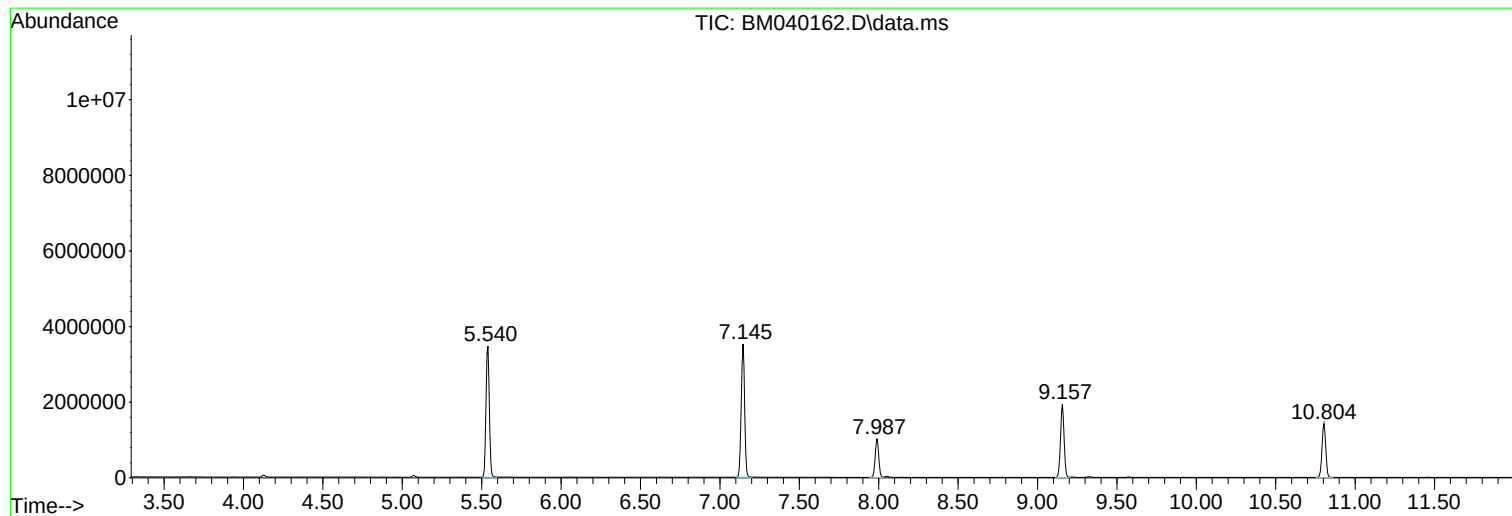

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040162.D
Acq On : 08 Jun 2023 17:17
Operator : MA/JU
Sample : 03074-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GT-02










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.980	4.05 ng	588017	Acenaphthene-d10	14.627

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzenecarbothioic acid, S-methy...	152	C8H8OS	005925-68-8	50
3			Acetophenone, 2-chloro-	154	C8H7ClO	000532-27-4	49
4			Disulfide, dibenzoyl	274	C14H10O2S2	000644-32-6	47
5			1,2-Propanedione, 1-phenyl-	148	C9H8O2	000579-07-7	47

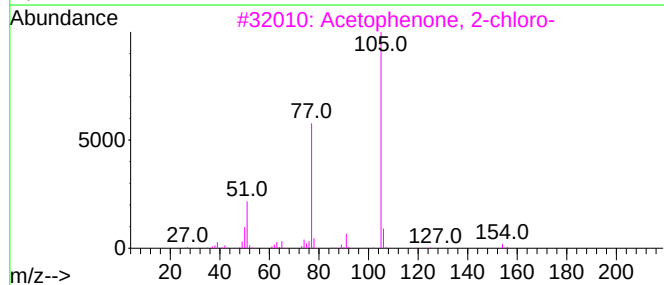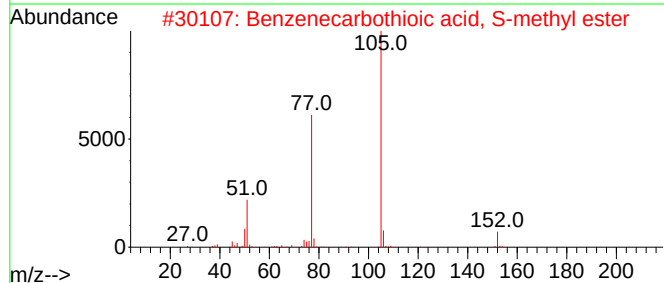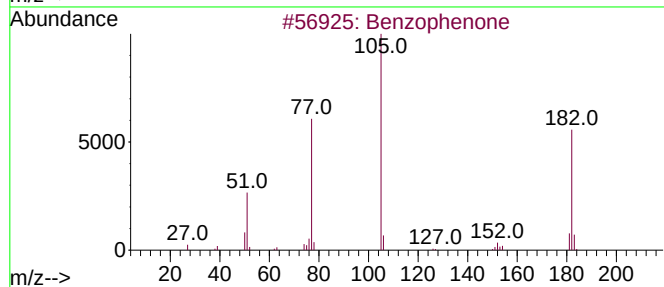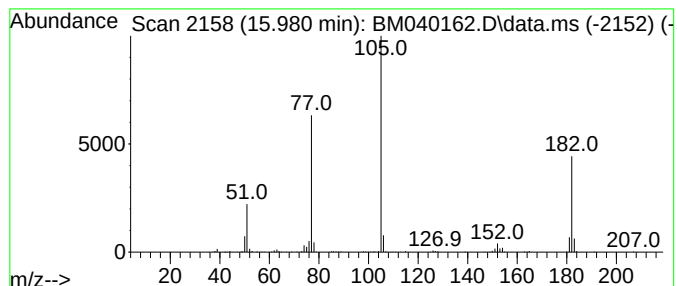

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040162.D
Acq On : 08 Jun 2023 17:17
Operator : MA/JU
Sample : 03074-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GT-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.980	4.0	ng	588017	3	14.627	2903440	20.0