

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
 Data File : BM040167.D
 Acq On : 08 Jun 2023 21:32
 Operator : MA/JU
 Sample : PB153236BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB153236BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040167.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.540	376	383	397	rBV	6464946	9038614	44.44%	10.674%
2	7.145	649	656	674	rBV	5776360	9134482	44.91%	10.788%
3	7.987	792	799	810	rVB	1160596	1790328	8.80%	2.114%
4	9.157	990	998	1010	rBV	3379760	5288501	26.00%	6.246%
5	10.804	1269	1278	1289	rBV	1529037	2511595	12.35%	2.966%
6	13.257	1687	1695	1706	rBV	8963625	12719506	62.54%	15.021%
7	14.627	1921	1928	1940	rBV	2129606	3044211	14.97%	3.595%
8	16.110	2174	2180	2202	rBV	7317432	9632176	47.36%	11.375%
9	17.368	2388	2394	2405	rVB	2770668	3576900	17.59%	4.224%
10	19.986	2833	2839	2845	rBV	17987482	20339496	100.00%	24.020%
11	21.545	3099	3104	3113	rBV	3031771	3636206	17.88%	4.294%
12	23.980	3511	3518	3527	rBV	2107346	3964357	19.49%	4.682%




Sum of corrected areas: 84676372

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040167.D
Acq On : 08 Jun 2023 21:32
Operator : MA/JU
Sample : PB153236BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153236BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

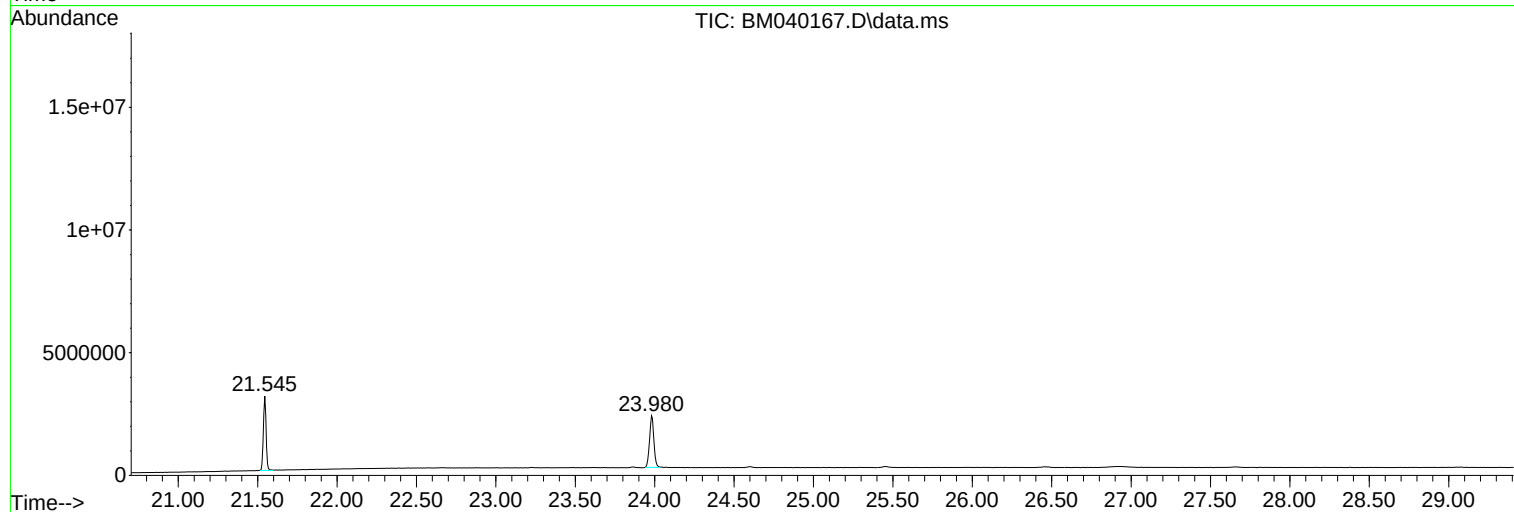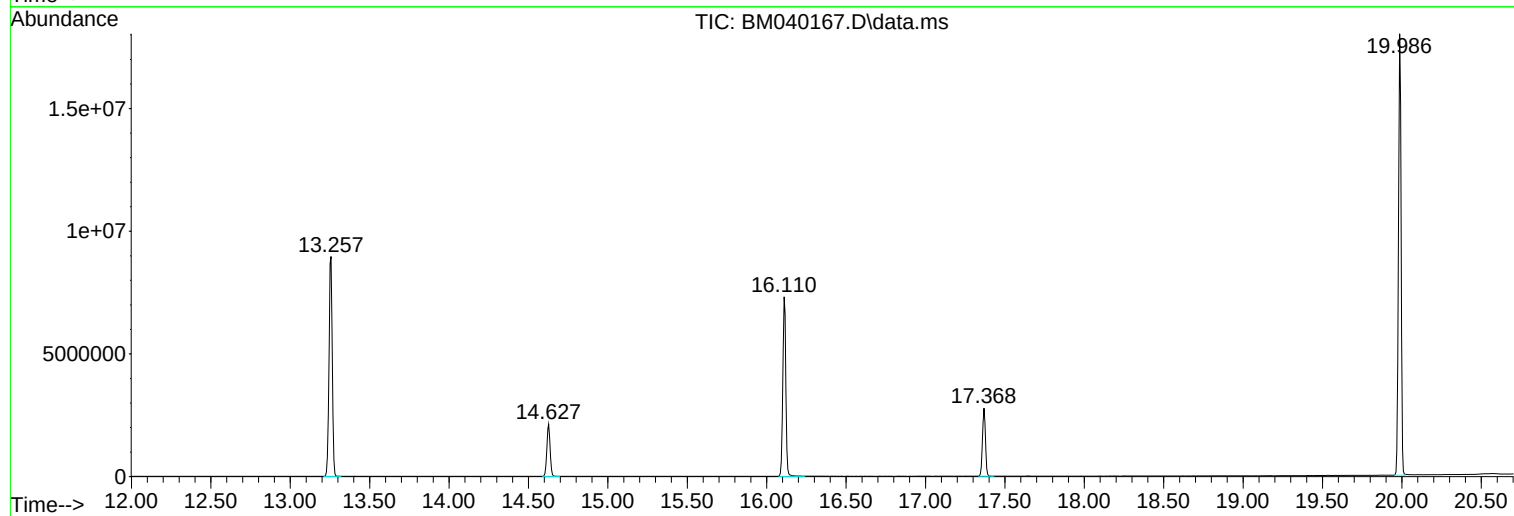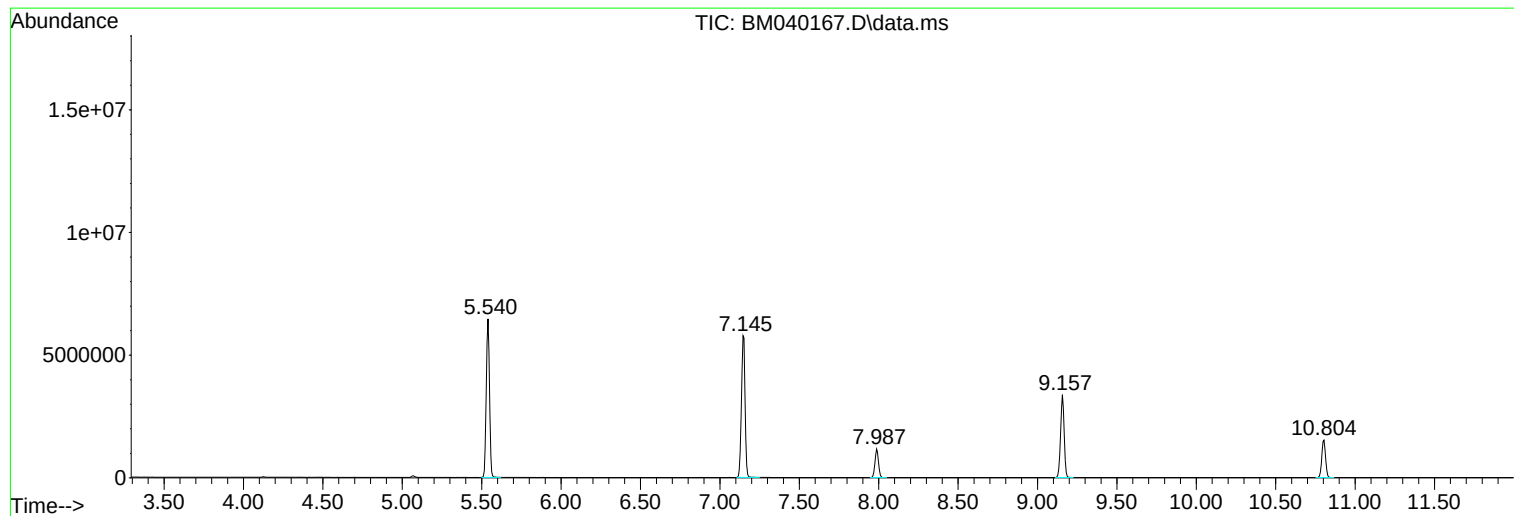

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040167.D
Acq On : 08 Jun 2023 21:32
Operator : MA/JU
Sample : PB153236BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153236BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040167.D
Acq On : 08 Jun 2023 21:32
Operator : MA/JU
Sample : PB153236BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153236BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------