

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
 Data File : BM040171.D
 Acq On : 08 Jun 2023 23:57
 Operator : MA/JU
 Sample : 03074-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GT-06

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040171.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.534	376	382	394	rBV	3229503	4736490	39.55%	9.003%
2	7.145	648	656	670	rBV	3248580	5026906	41.97%	9.555%
3	7.987	792	799	806	rBV	831059	1278850	10.68%	2.431%
4	9.151	989	997	1005	rBV	1789389	2898391	24.20%	5.509%
5	10.798	1268	1277	1285	rBV	1115815	1860780	15.54%	3.537%
6	13.251	1687	1694	1703	rBV	5182656	7132448	59.55%	13.557%
7	14.627	1921	1928	1941	rBV	1555376	2286675	19.09%	4.346%
8	15.980	2151	2158	2163	rBV	272875	356762	2.98%	0.678%
9	16.110	2173	2180	2198	rBV	4082222	5317943	44.40%	10.108%
10	17.368	2387	2394	2407	rBV	2051611	2784058	23.25%	5.292%
11	19.986	2833	2839	2850	rBV	10753492	11976481	100.00%	22.764%
12	21.244	3049	3053	3060	rBV	185437	257500	2.15%	0.489%
13	21.544	3098	3104	3113	rBV	2490411	3147993	26.28%	5.983%
14	23.980	3511	3518	3531	rVB	1824117	3550547	29.65%	6.749%




Sum of corrected areas: 52611824

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040171.D
Acq On : 08 Jun 2023 23:57
Operator : MA/JU
Sample : 03074-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GT-06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

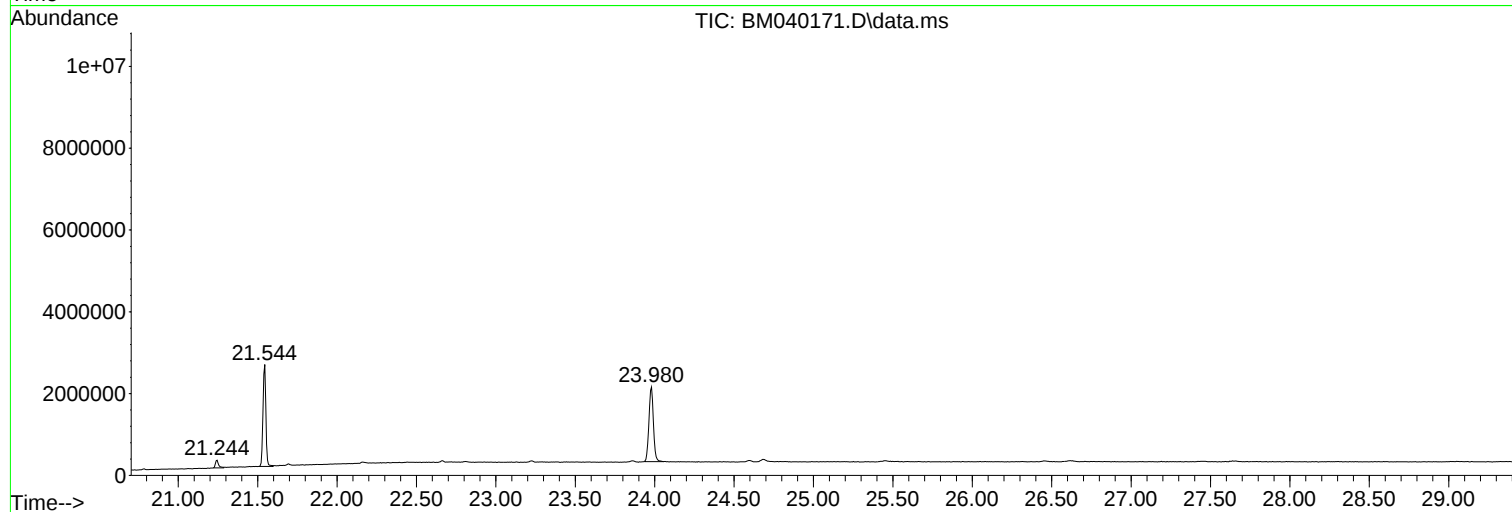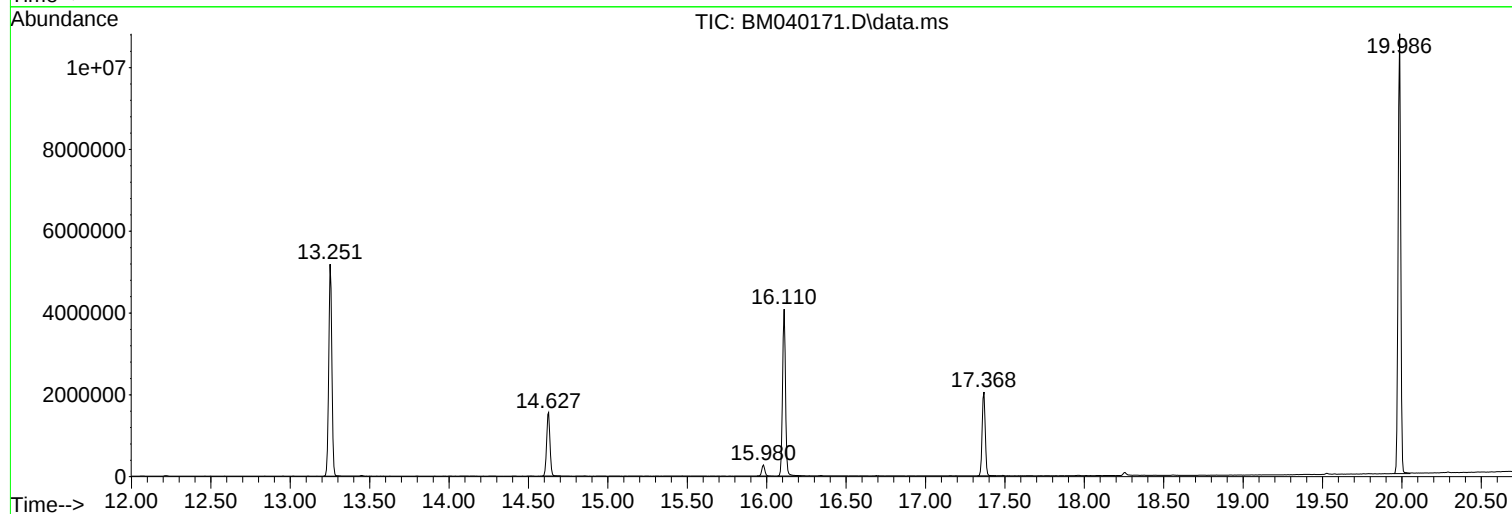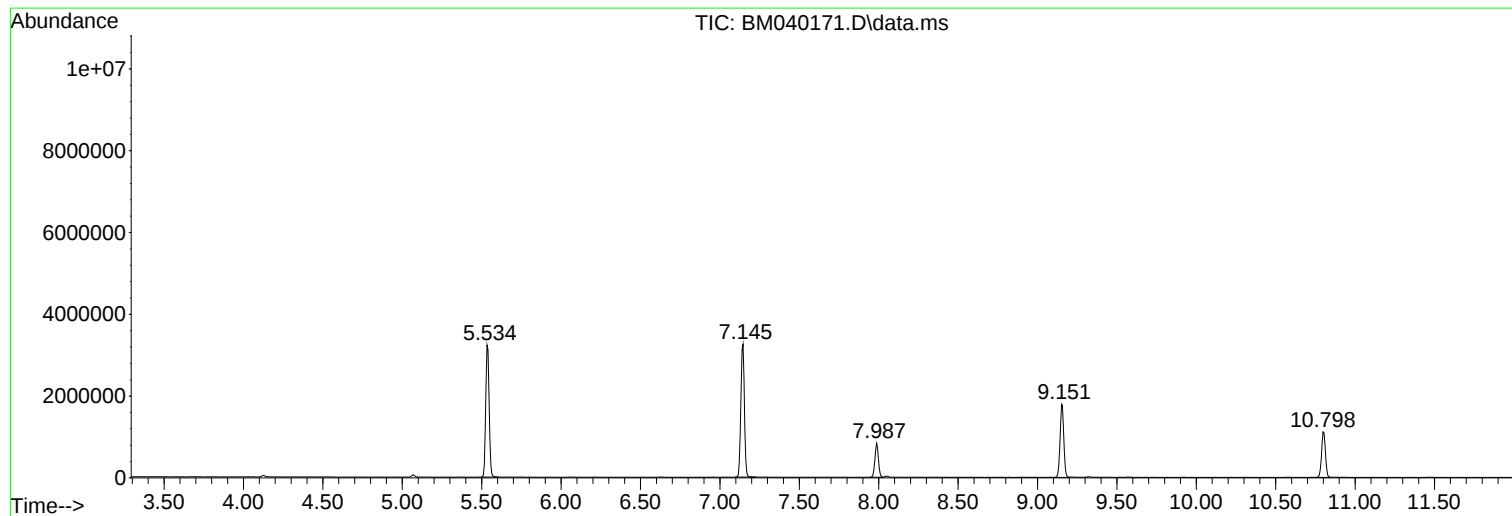

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040171.D
Acq On : 08 Jun 2023 23:57
Operator : MA/JU
Sample : 03074-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GT-06










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.980	3.12 ng	356762	Acenaphthene-d10	14.627

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzenecarbothioic acid, S-methy...	152	C8H8OS	005925-68-8	50
3			Acetophenone, 2-chloro-	154	C8H7ClO	000532-27-4	49
4			Benzenecarboxylic acid, .alpha.-oxo-...	164	C9H8O3	015206-55-0	47
5			Benzoic acid, pentafluorophenyl ...	288	C13H5F5O2	1000360-67-9	47

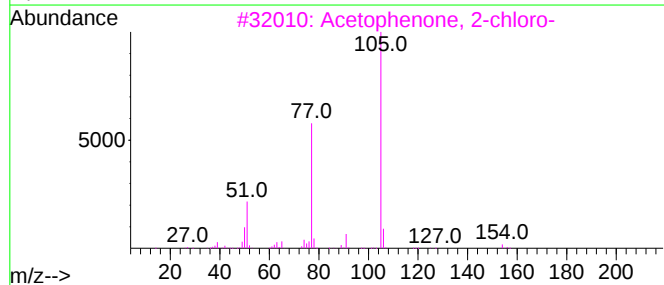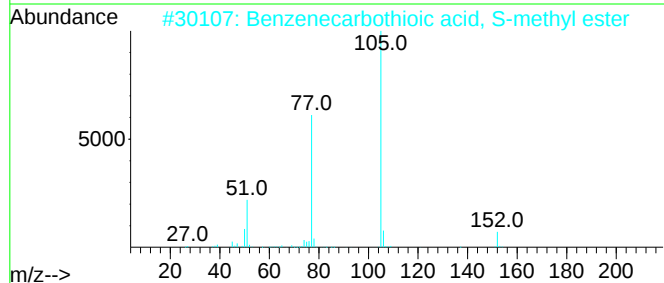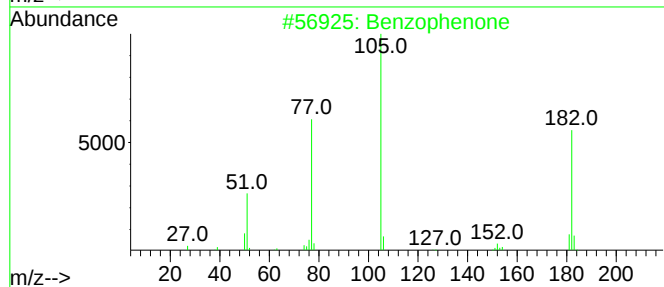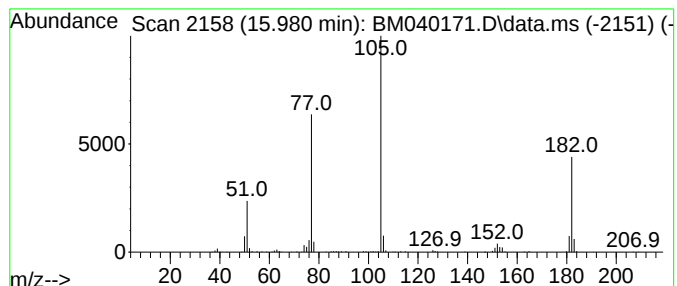

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040171.D
Acq On : 08 Jun 2023 23:57
Operator : MA/JU
Sample : 03074-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GT-06

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.980	3.1	ng	356762	3	14.627	2286680	20.0