


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
 Data File : BM040148.D
 Acq On : 08 Jun 2023 08:35
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 08 23:25:50 2023

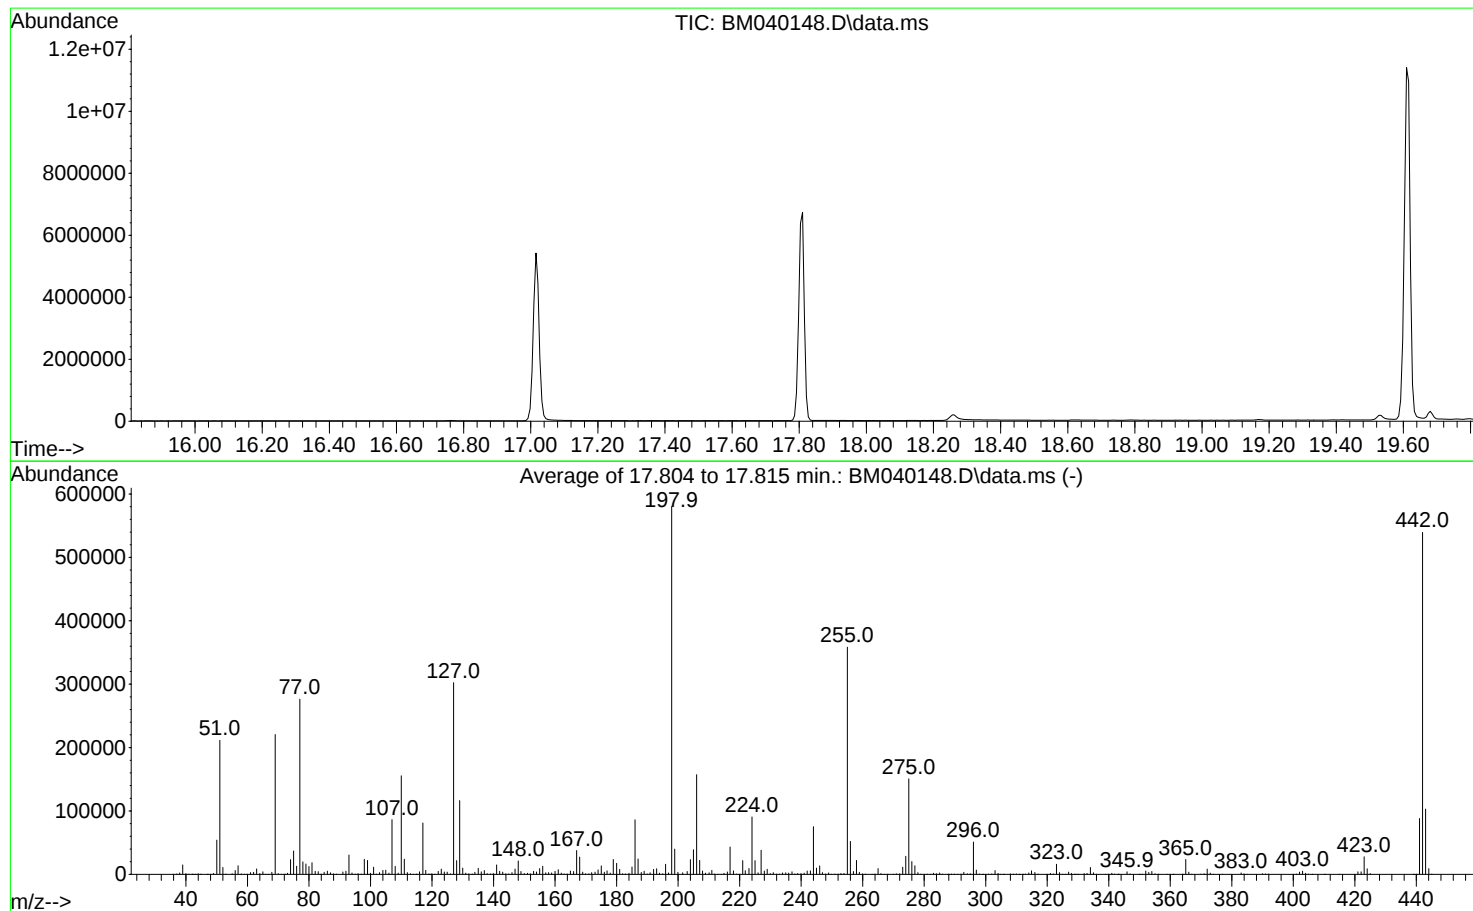

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	211528	PASS
68	69	0.00	2	1.5	3405	PASS
69	198	0.00	100	38.0	220656	PASS
70	69	0.00	2	0.5	1189	PASS
127	198	10	80	52.1	302400	PASS
197	198	0.00	2	0.4	2403	PASS
198	198	100	100	100.0	580288	PASS
199	198	5	9	6.9	39800	PASS
275	198	10	60	26.0	150701	PASS
365	198	1	100	4.1	23593	PASS
441	198	0.01	100	15.2	88029	PASS
442	442	50	100	100.0	539435	PASS
443	442	15	24	19.1	103128	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/8/2023	BNA_M	<u>BM040148.D</u>
Compound Name	Response	Retention Time
DDT	2322041	20.839
DDD	11448	20.456
DDE	365	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11813	2333854	0.51

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
 Data File : BM040148.D
 Acq On : 08 Jun 2023 08:35
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 08 09:13:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 06 16:45:42 2023
 Response via : Initial Calibration

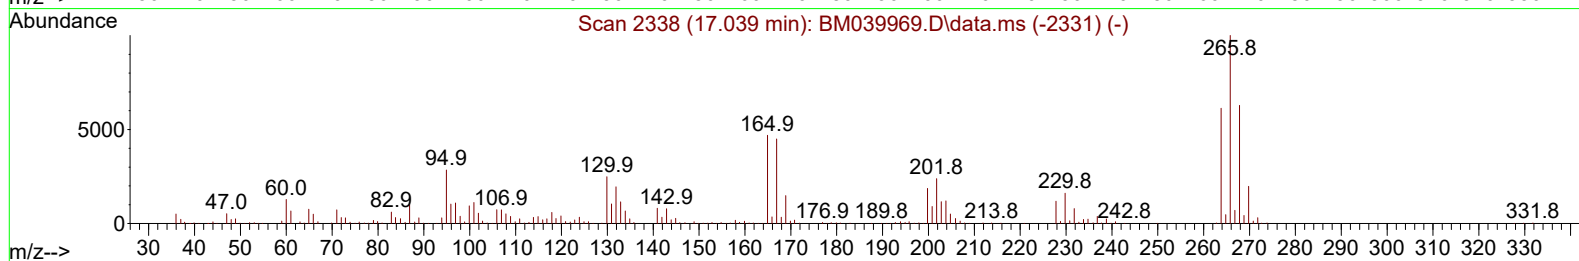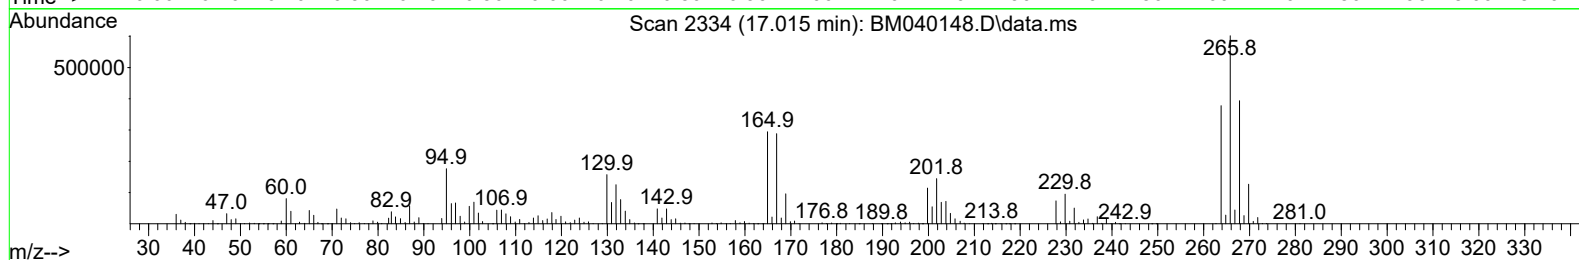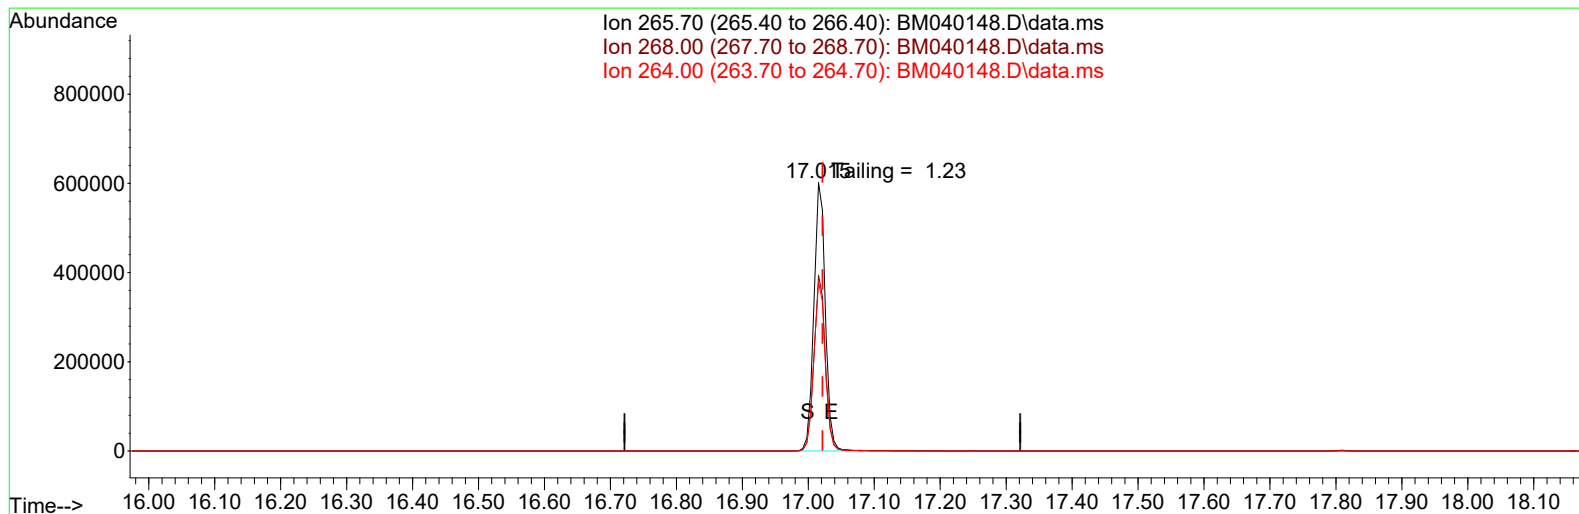

TIC: BM040148.D\data.ms

(70) Pentachlorophenol (C)

17.015min (-0.006) 222839.05 ng




response 731478

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	65.45
264.00	61.30	62.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040148.D
Acq On : 08 Jun 2023 08:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 08 09:13:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 06 16:45:42 2023
Response via : Initial Calibration

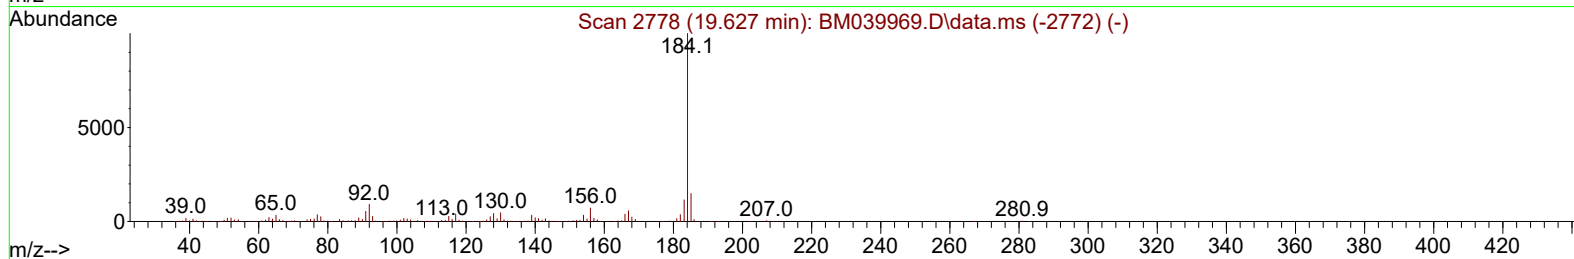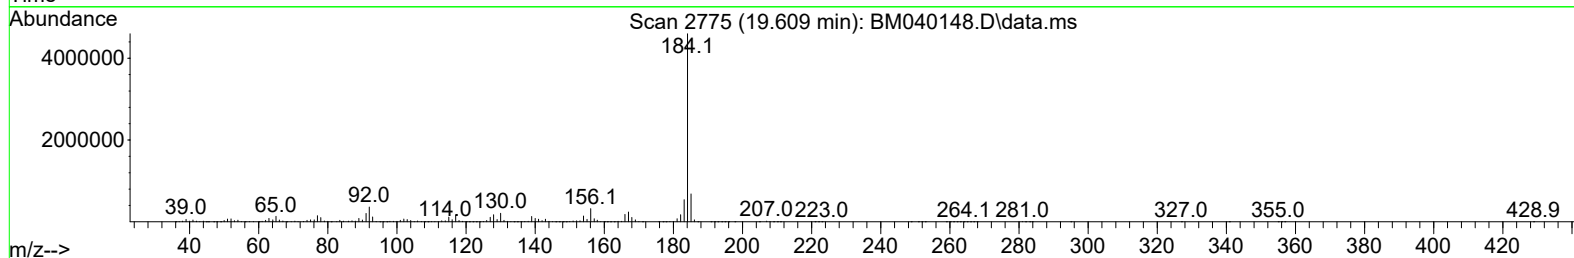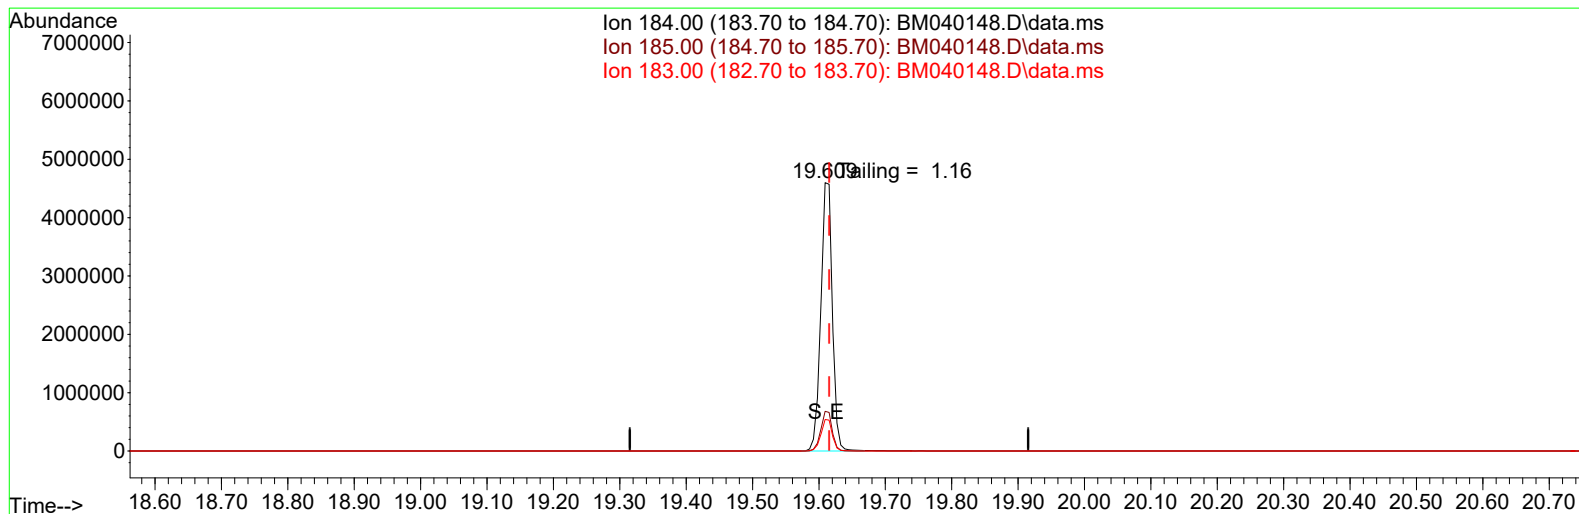

TIC: BM040148.D\data.ms

(77) Benzidine

19.609min (-0.006) 853163.81 ng

response 5564458

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.82
183.00	11.50	11.77
0.00	0.00	0.00