
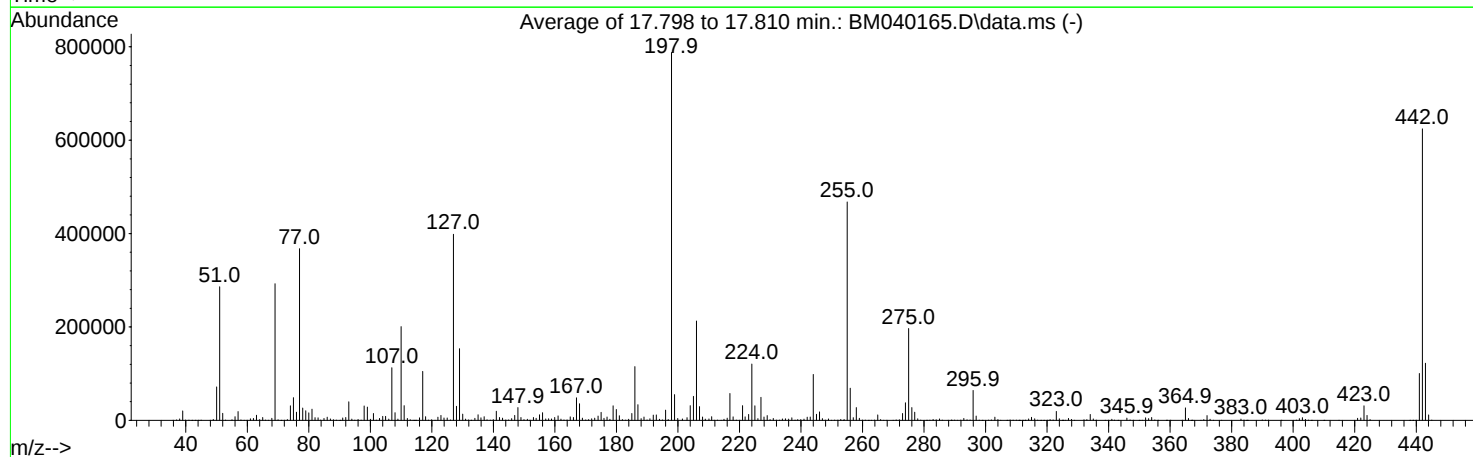


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
Data File : BM040165.D
Acq On : 08 Jun 2023 19:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 08 23:25:50 2023

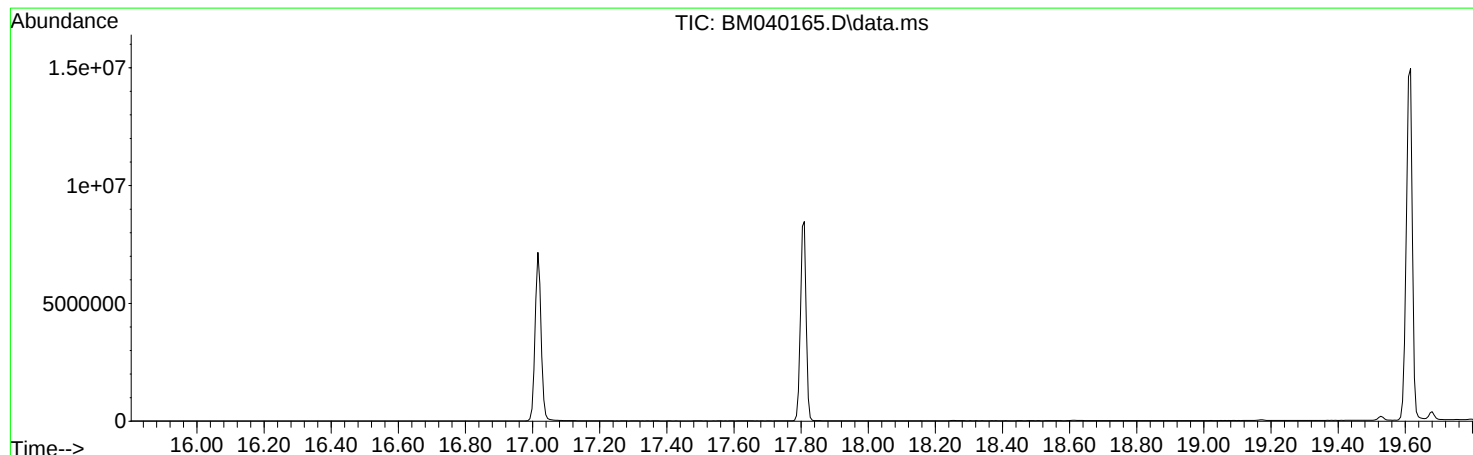

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	285961	PASS
68	69	0.00	2	1.5	4325	PASS
69	198	0.00	100	37.2	292779	PASS
70	69	0.00	2	0.5	1515	PASS
127	198	10	80	50.6	398592	PASS
197	198	0.00	2	0.2	1354	PASS
198	198	100	100	100.0	787712	PASS
199	198	5	9	7.0	55032	PASS
275	198	10	60	25.0	196560	PASS
365	198	1	100	3.4	26592	PASS
441	198	0.01	100	12.8	100525	PASS
442	442	50	100	100.0	624277	PASS
443	442	15	24	19.6	122192	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/8/2023	BNA_M	<u>BM040165.D</u>
Compound Name	Response	Retention Time
DDT	3245433	20.839
DDD	29637	20.398
DDE	825	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30462	3275895	0.93

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
 Data File : BM040165.D
 Acq On : 08 Jun 2023 19:43
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 09 03:50:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 08 23:25:50 2023
 Response via : Initial Calibration

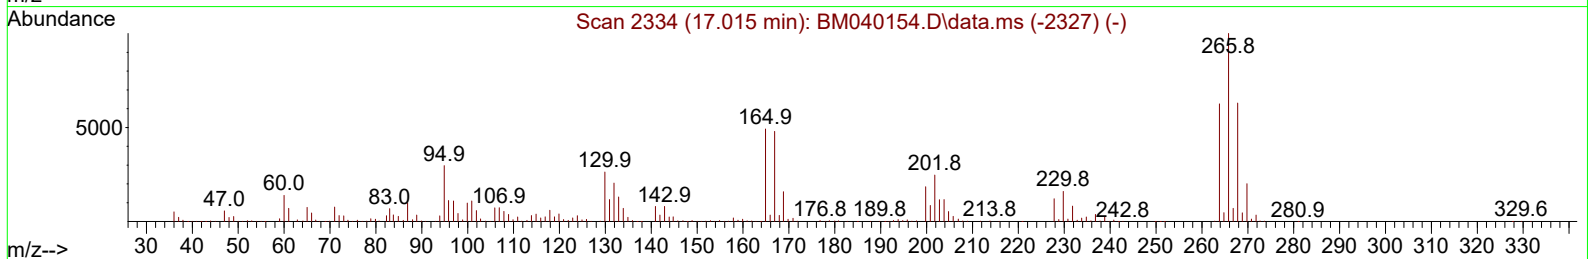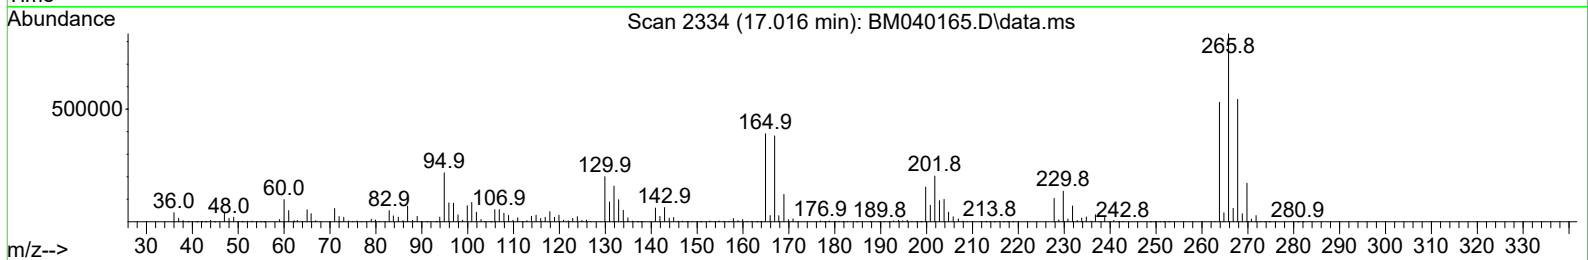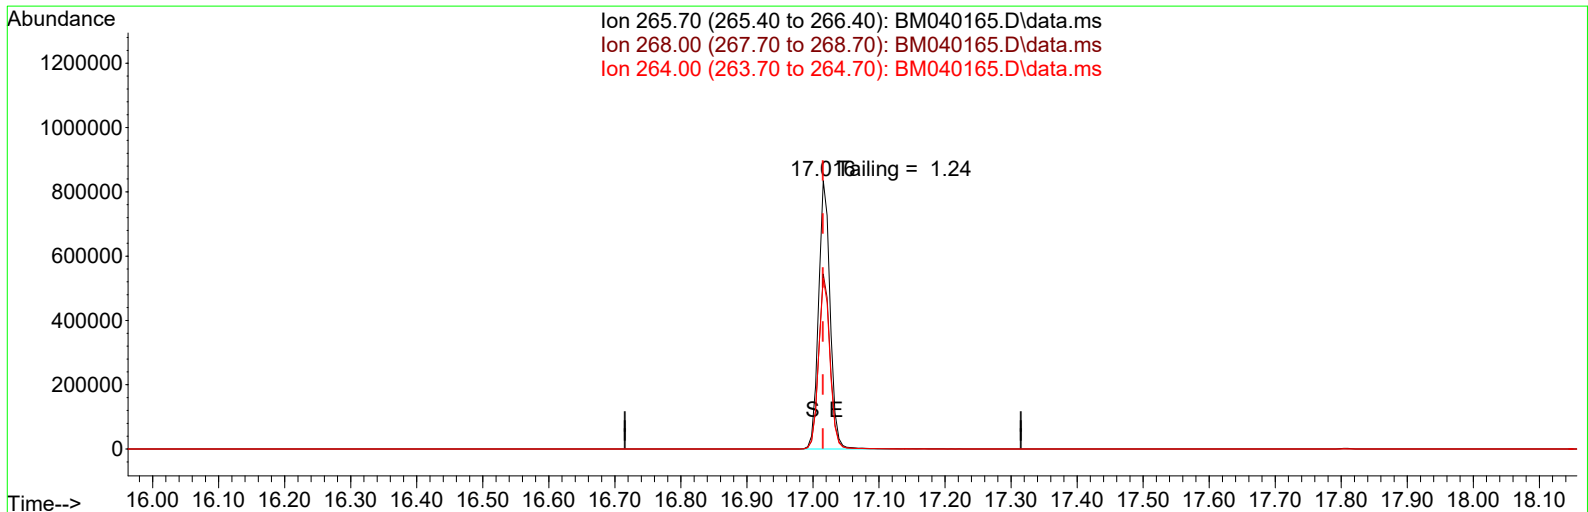

TIC: BM040165.D\data.ms

(70) Pentachlorophenol (C)

17.016min (+ 0.001) 198385.69 ng




response 1018213

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	65.14
264.00	62.60	63.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060823\
 Data File : BM040165.D
 Acq On : 08 Jun 2023 19:43
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 09 03:50:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 08 23:25:50 2023
 Response via : Initial Calibration

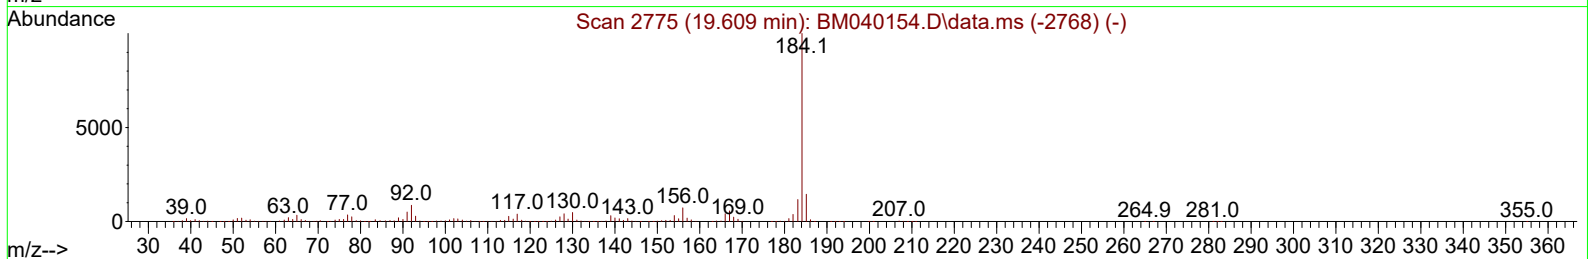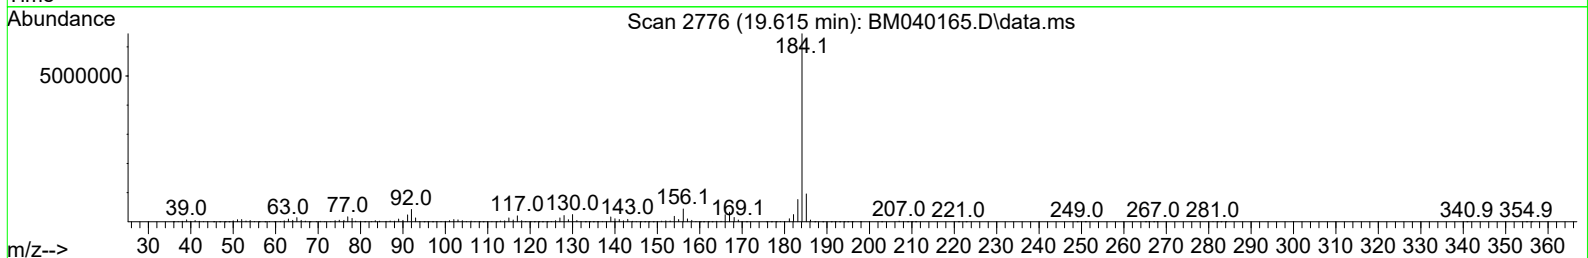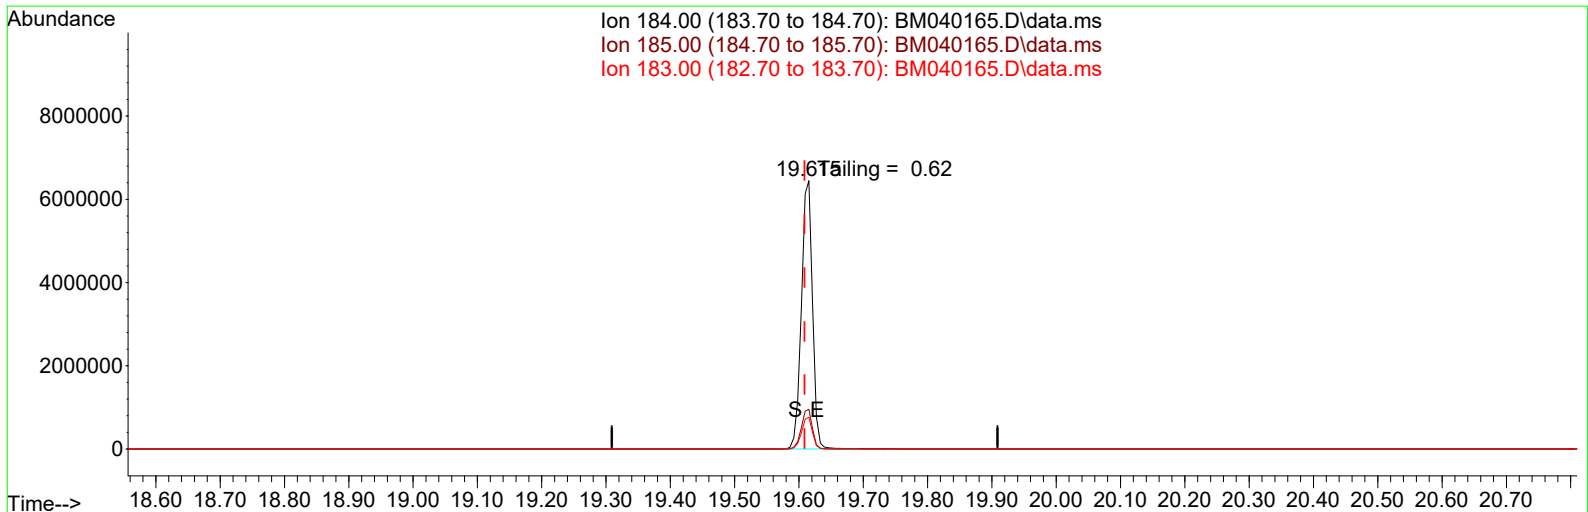

TIC: BM040165.D\data.ms

(77) Benzidine

19.615min (+ 0.006) 622924.65 ng

response 7767976

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.83
183.00	11.70	11.86
0.00	0.00	0.00