

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
 Data File : BM030347.D
 Acq On : 09 Jun 2021 18:03
 Operator : CG/JU
 Sample : PB136946BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB136946BL

Quant Time: Jun 09 18:52:59 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 08 20:51:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	189390	20.000	ng	0.00
21) Naphthalene-d8	10.639	136	745932	20.000	ng	# 0.00
39) Acenaphthene-d10	14.474	164	491351	20.000	ng	0.00
64) Phenanthrene-d10	17.204	188	1120152	20.000	ng	# 0.00
76) Chrysene-d12	21.368	240	1243661	20.000	ng	0.00
86) Perylene-d12	23.650	264	1311474	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.434	112	1781878	152.950	ng	0.00
7) Phenol-d6	7.010	99	2289101	135.731	ng	0.00
23) Nitrobenzene-d5	9.004	82	1350367	88.194	ng	0.00
42) 2,4,6-Tribromophenol	15.957	330	917406	148.504	ng	0.00
45) 2-Fluorobiphenyl	13.098	172	3292239	88.114	ng	0.00
79) Terphenyl-d14	19.821	244	6338194	89.515	ng	0.00
Target Compounds						
						Qvalue
48) 2-Nitroaniline	13.445	65	54	4.026	ng	# 4
80) Butylbenzylphthalate	20.497	149	330	4.313	ng	# 58
84) Bis(2-ethylhexyl)phtha...	21.280	149	894	4.288	ng	# 83
85) Di-n-octyl phthalate	22.162	149	236	4.167	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030347.D
Acq On : 09 Jun 2021 18:03
Operator : CG/JU
Sample : PB136946BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136946BL

Quant Time: Jun 09 18:52:59 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 08 20:51:08 2021
Response via : Initial Calibration




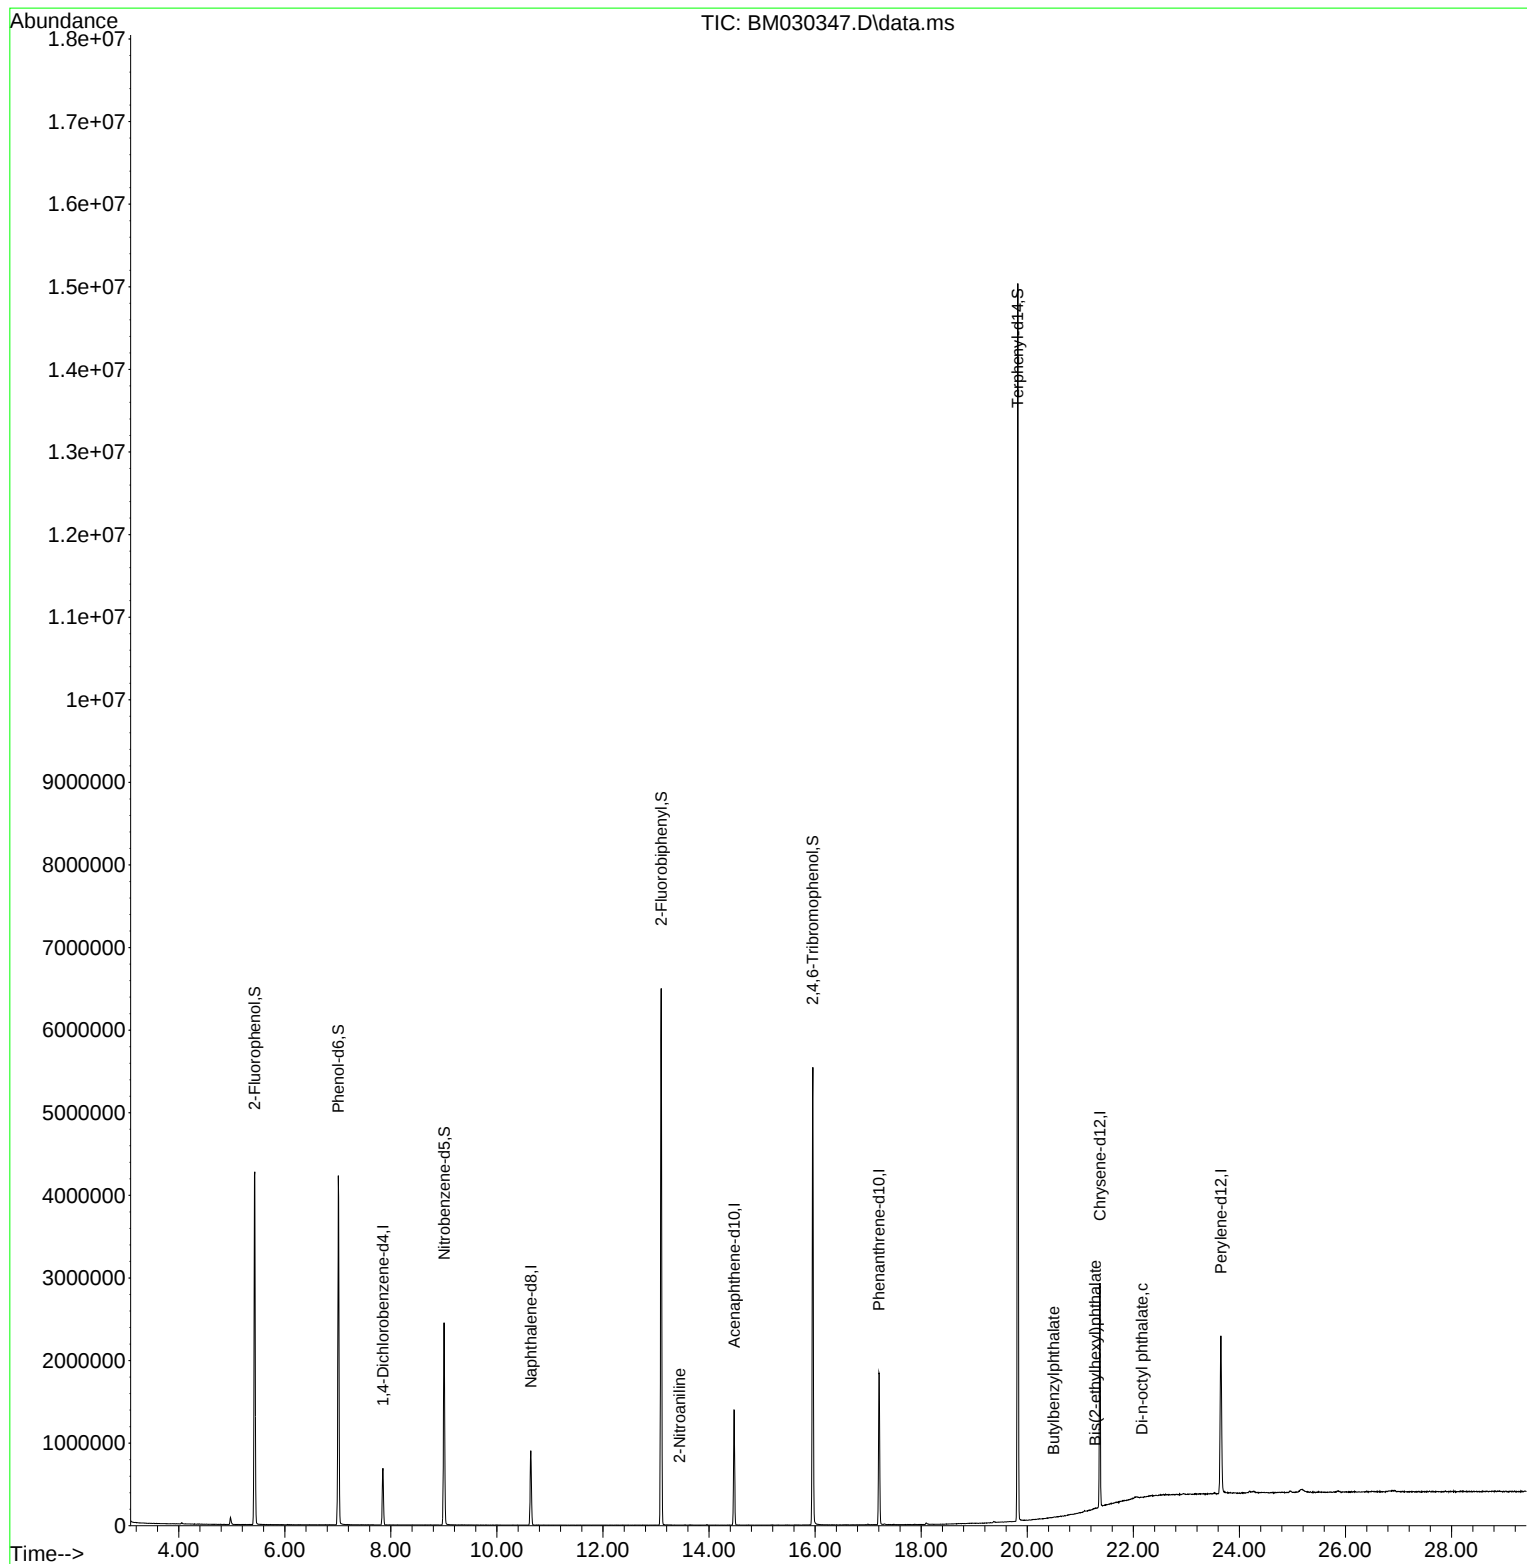


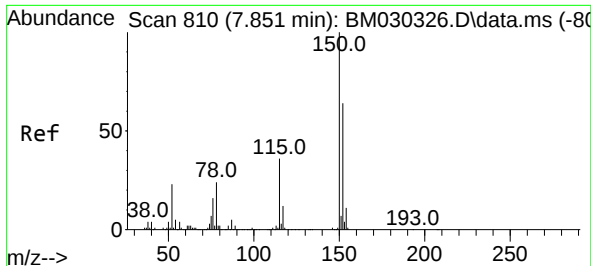

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.851 min Scan# 810
Delta R.T. 0.000 min
Lab File: BM030347.D
Acq: 09 Jun 2021 18:03




Instrument :
BNA_M
ClientSampleId :
PB136946BL


Tgt Ion:152 Resp: 189390
Ion Ratio Lower Upper
152 100
150 154.8 125.9 188.9
115 55.2 44.6 67.0

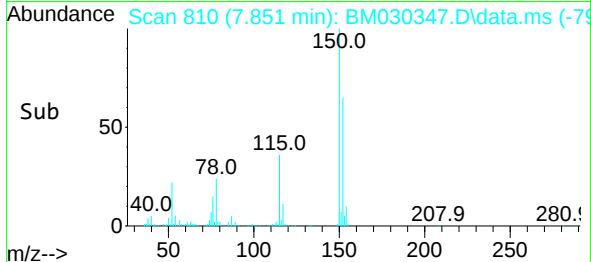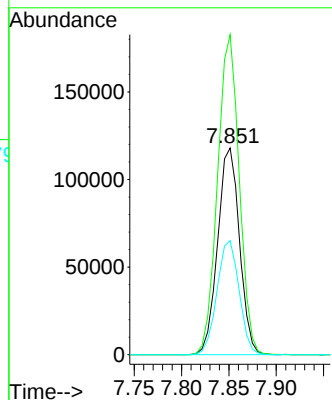

#5
2-Fluorophenol
Concen: 152.950 ng
RT: 5.434 min Scan# 399
Delta R.T. 0.006 min
Lab File: BM030347.D
Acq: 09 Jun 2021 18:03

Tgt Ion:112 Resp: 1781878
Ion Ratio Lower Upper
112 100
64 59.8 47.1 70.7
63 31.3 27.3 40.9

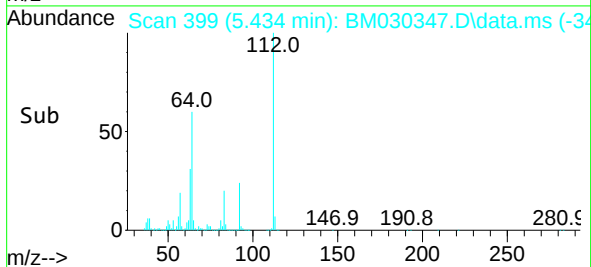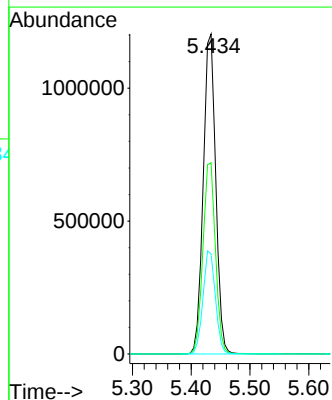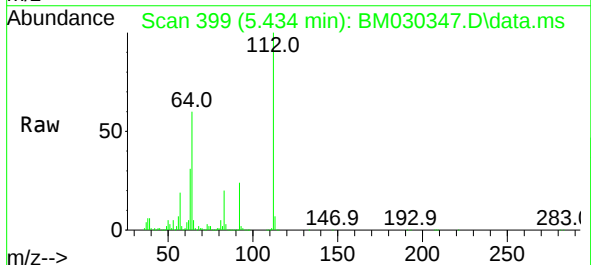




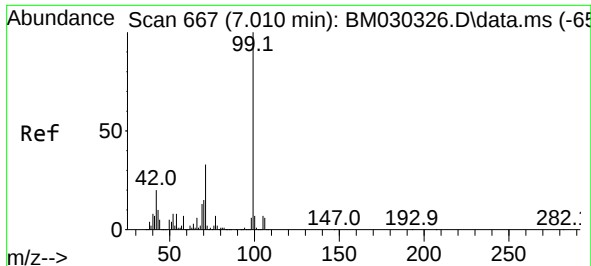


#7
Phenol-d6
Concen: 135.731 ng
RT: 7.010 min Scan# 667
Delta R.T. 0.000 min
Lab File: BM030347.D
Acq: 09 Jun 2021 18:03

Instrument :
BNA_M
ClientSampleId :
PB136946BL

Tgt Ion: 99 Resp: 2289101




Ion	Ratio	Lower	Upper
99	100		
42	20.3	18.0	27.0
71	33.1	30.9	46.3

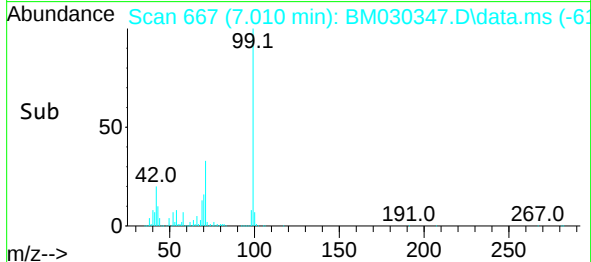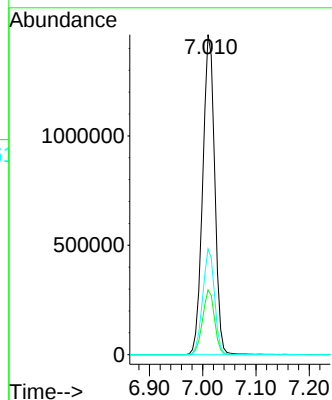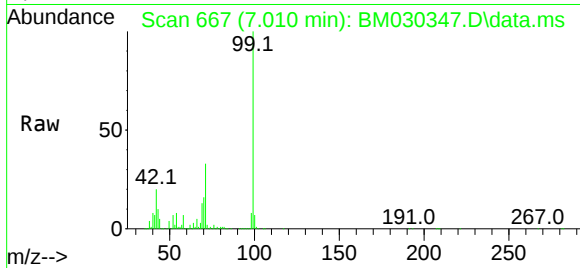


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.639 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BM030347.D
Acq: 09 Jun 2021 18:03

Tgt Ion: 136 Resp: 745932

Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.4	12.6
54	8.8	5.5	8.3#
68	5.9	4.2	6.2


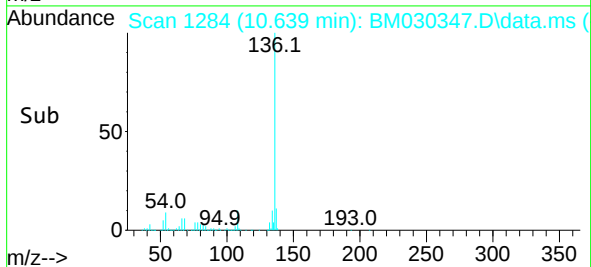
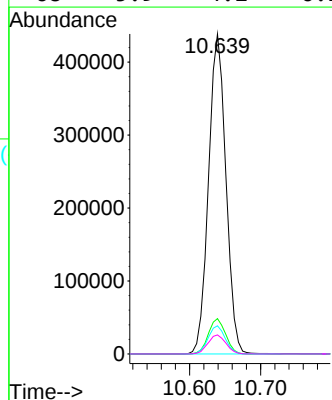
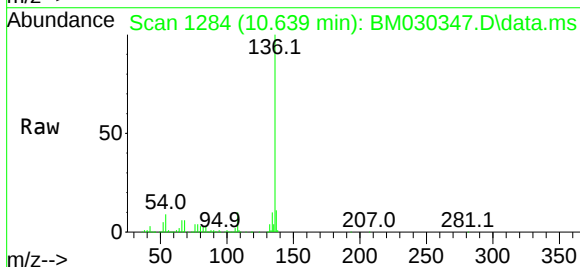


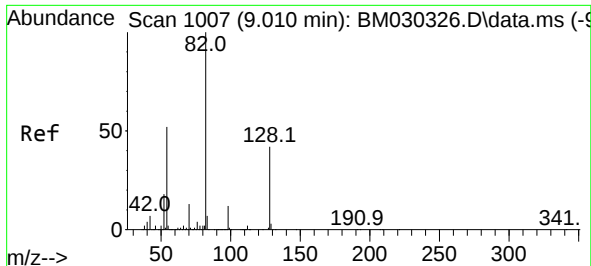

#23
Nitrobenzene-d5
Concen: 88.194 ng
RT: 9.004 min Scan# 1006
Delta R.T. -0.006 min
Lab File: BM030347.D
Acq: 09 Jun 2021 18:03




Instrument :
BNA_M
ClientSampleId :
PB136946BL


Tgt Ion: 82 Resp: 1350367
Ion Ratio Lower Upper
82 100
128 40.6 31.1 46.7
54 52.2 37.3 55.9

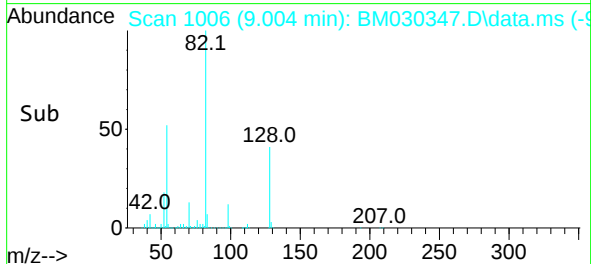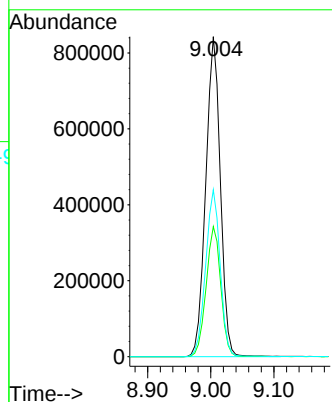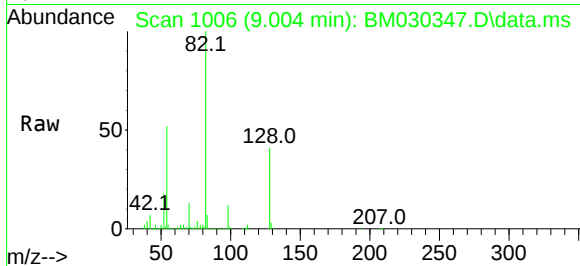

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.474 min Scan# 1936
Delta R.T. 0.000 min
Lab File: BM030347.D
Acq: 09 Jun 2021 18:03

Tgt Ion: 164 Resp: 491351
Ion Ratio Lower Upper
164 100
162 101.6 83.4 125.0
160 44.5 37.2 55.8


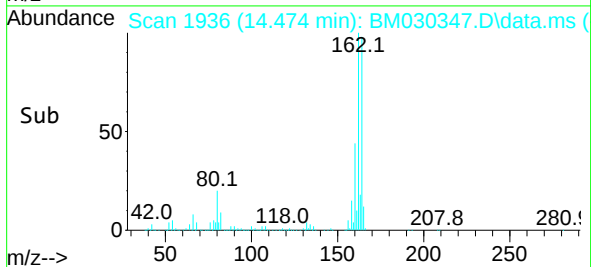
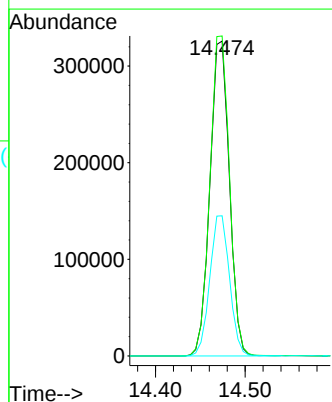
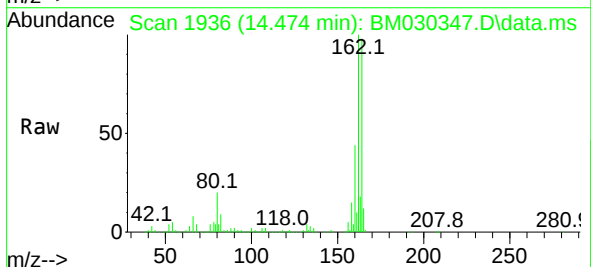


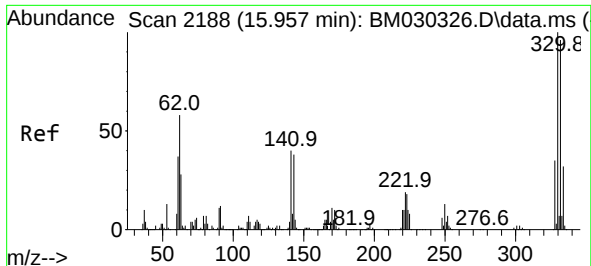

#42
2,4,6-Tribromophenol
Concen: 148.504 ng
RT: 15.957 min Scan# 2188
Delta R.T. 0.000 min
Lab File: BM030347.D
Acq: 09 Jun 2021 18:03




Instrument :
BNA_M
ClientSampleId :
PB136946BL


Tgt Ion:330 Resp: 917406
Ion Ratio Lower Upper
330 100
332 95.9 77.0 115.4
141 37.6 30.2 45.2

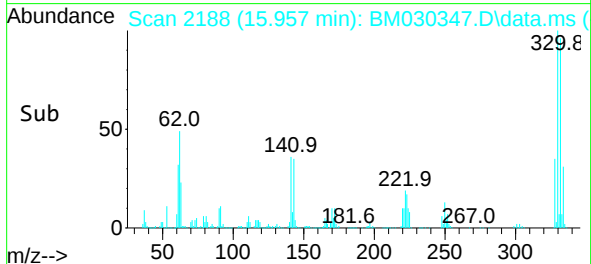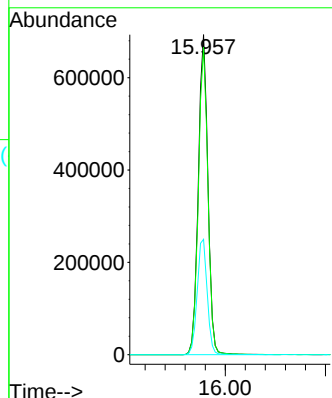

#45
2-Fluorobiphenyl
Concen: 88.114 ng
RT: 13.098 min Scan# 1702
Delta R.T. 0.000 min
Lab File: BM030347.D
Acq: 09 Jun 2021 18:03

Tgt Ion:172 Resp: 3292239
Ion Ratio Lower Upper
172 100
171 35.3 28.6 43.0
170 23.7 18.4 27.6



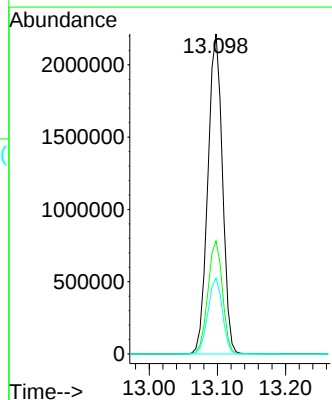
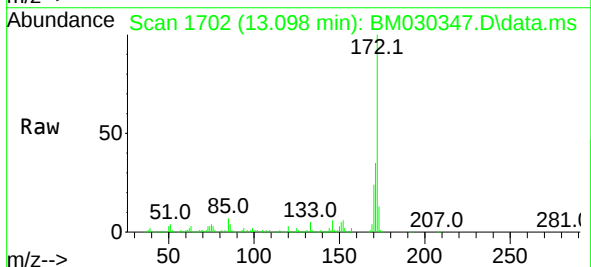




#48
2-Nitroaniline
Concen: 4.026 ng
RT: 13.445 min Scan# 1761
Delta R.T. -0.106 min
Lab File: BM030347.D
Acq: 09 Jun 2021 18:03




Instrument :
BNA_M
ClientSampleId :
PB136946BL


Tgt Ion: 65 Resp: 54
Ion Ratio Lower Upper
65 100
92 0.0 55.5 83.3#
138 0.0 85.7 128.5#

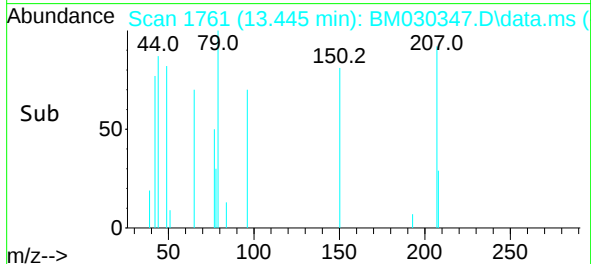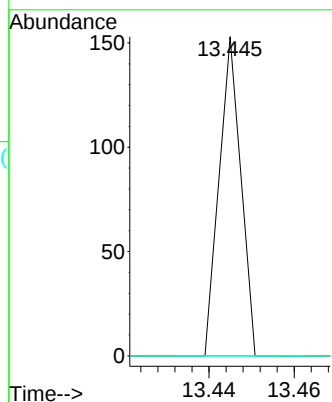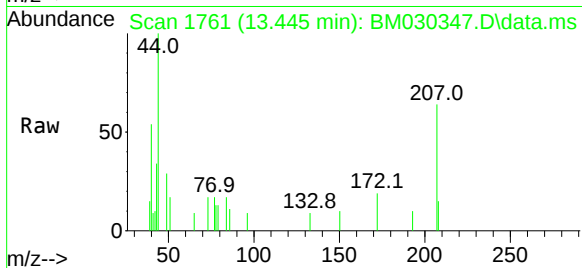

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.204 min Scan# 2400
Delta R.T. -0.005 min
Lab File: BM030347.D
Acq: 09 Jun 2021 18:03

Tgt Ion: 188 Resp: 1120152
Ion Ratio Lower Upper
188 100
94 9.4 6.0 9.0#
80 10.0 6.6 9.8#

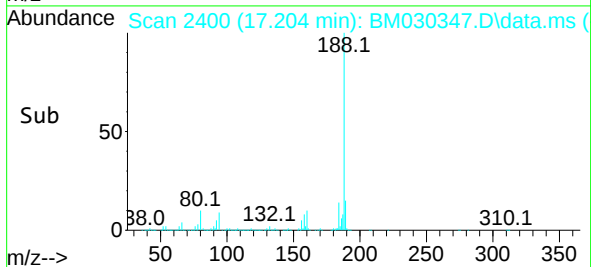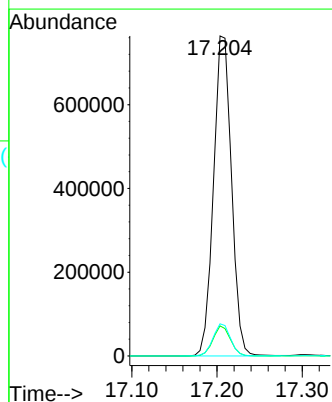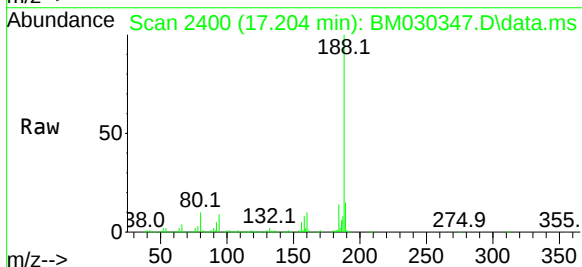



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.368 min Scan# 3108

Delta R.T. -0.000 min

Lab File: BM030347.D

Acq: 09 Jun 2021 18:03





Tgt Ion:240 Resp: 1243661

Ion Ratio Lower Upper

240 100

120 10.4 7.0 10.6

236 25.5 21.0 31.4

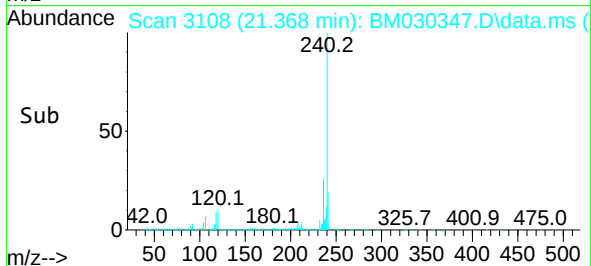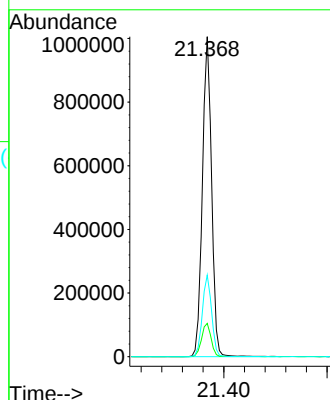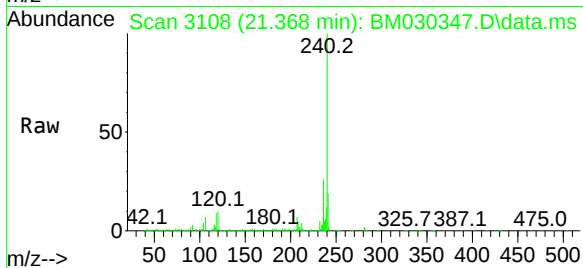

#79

Terphenyl-d14

Concen: 89.515 ng

RT: 19.821 min Scan# 2845

Delta R.T. 0.000 min

Lab File: BM030347.D

Acq: 09 Jun 2021 18:03




Tgt Ion:244 Resp: 6338194


Ion Ratio Lower Upper

244 100

212 8.0 6.3 9.5

122 11.2 6.9 10.3#


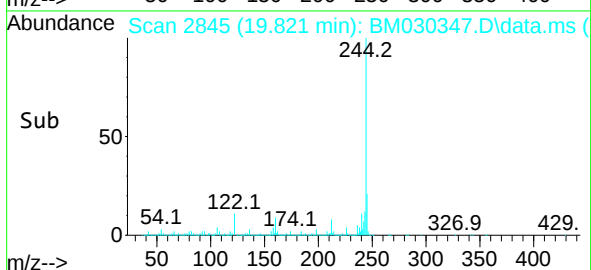
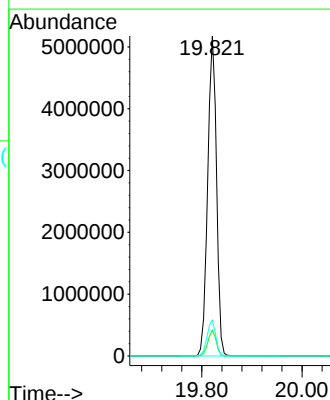
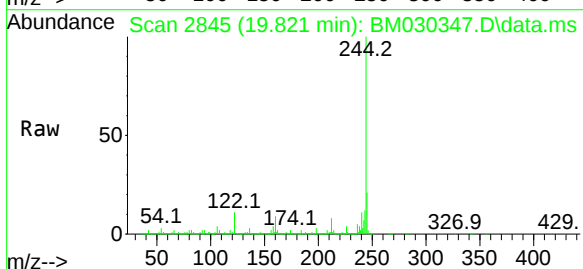


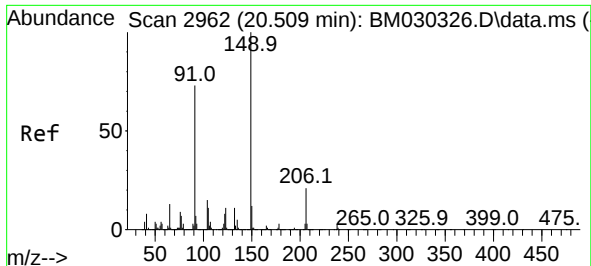

#80
Butylbenzylphthalate
Concen: 4.313 ng
RT: 20.497 min Scan# 2960
Delta R.T. -0.012 min
Lab File: BM030347.D
Acq: 09 Jun 2021 18:03




Instrument :
BNA_M
ClientSampleId :
PB136946BL


Tgt Ion:149 Resp: 330
Ion Ratio Lower Upper
149 100
91 31.7 57.4 86.0#
206 29.8 16.6 25.0#

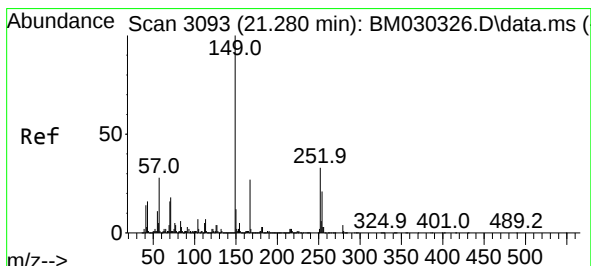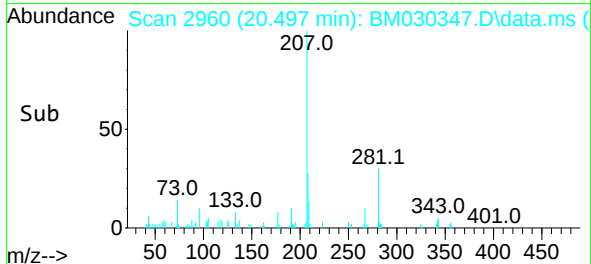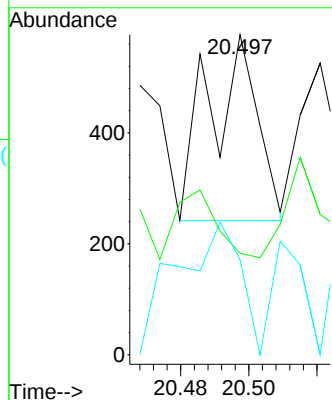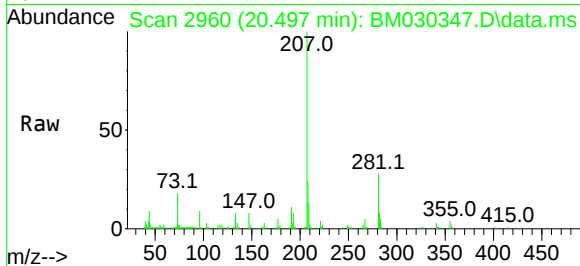

#84
Bis(2-ethylhexyl)phthalate
Concen: 4.288 ng
RT: 21.280 min Scan# 3093
Delta R.T. -0.000 min
Lab File: BM030347.D
Acq: 09 Jun 2021 18:03

Tgt Ion:149 Resp: 894
Ion Ratio Lower Upper
149 100
167 19.7 22.6 33.8#
279 13.3 3.8 5.8#


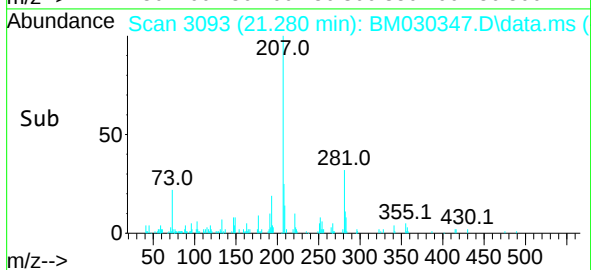
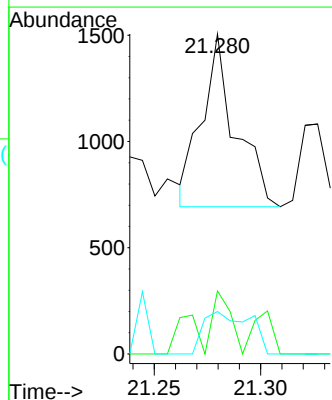
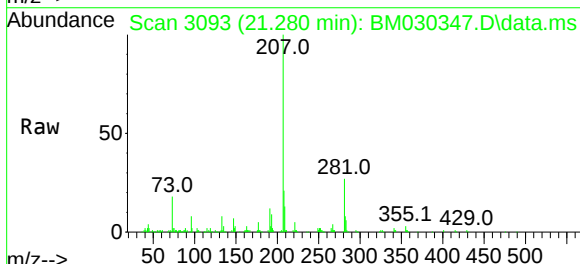


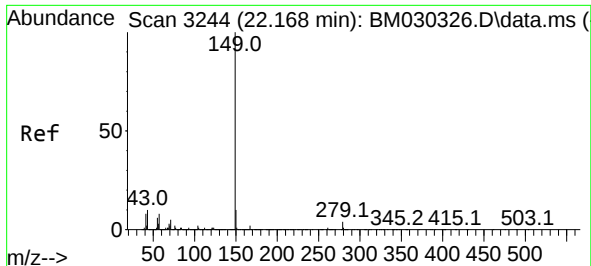

#85
Di-n-octyl phthalate
Concen: 4.167 ng
RT: 22.162 min Scan# 3243
Delta R.T. -0.006 min
Lab File: BM030347.D
Acq: 09 Jun 2021 18:03

Instrument :
BNA_M
ClientSampleId :
PB136946BL

Tgt Ion:149 Resp: 236
Ion Ratio Lower Upper
149 100
167 0.0 1.3 1.9#
43 119.9 7.4 11.0#

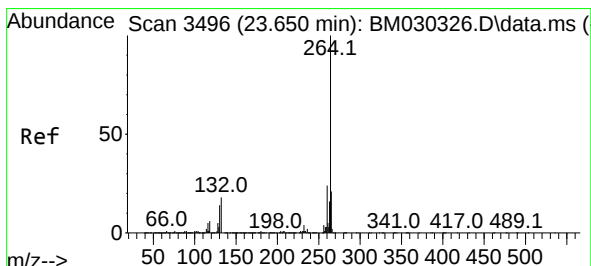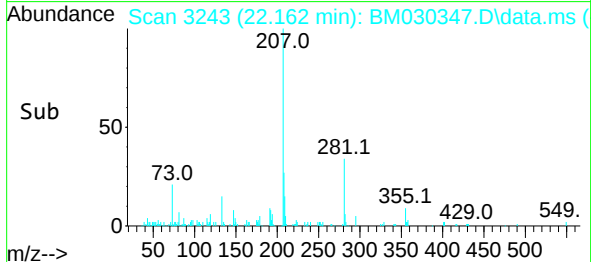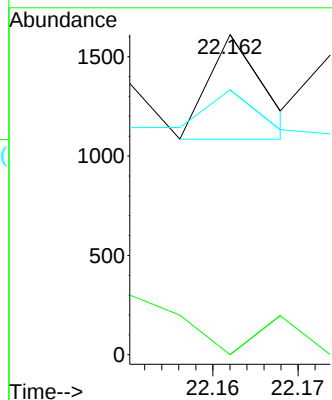

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.650 min Scan# 3496
Delta R.T. 0.000 min
Lab File: BM030347.D
Acq: 09 Jun 2021 18:03

Tgt Ion:264 Resp: 1311474
Ion Ratio Lower Upper
264 100
260 24.0 19.8 29.8
265 22.2 17.7 26.5

