
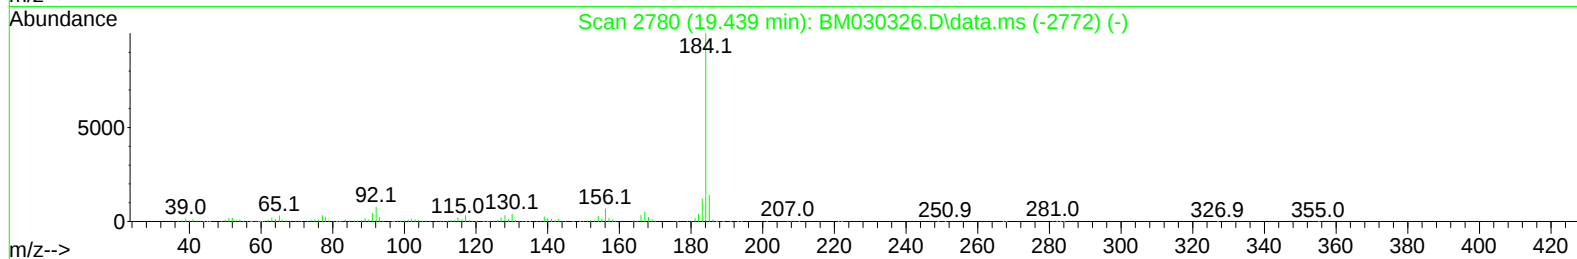
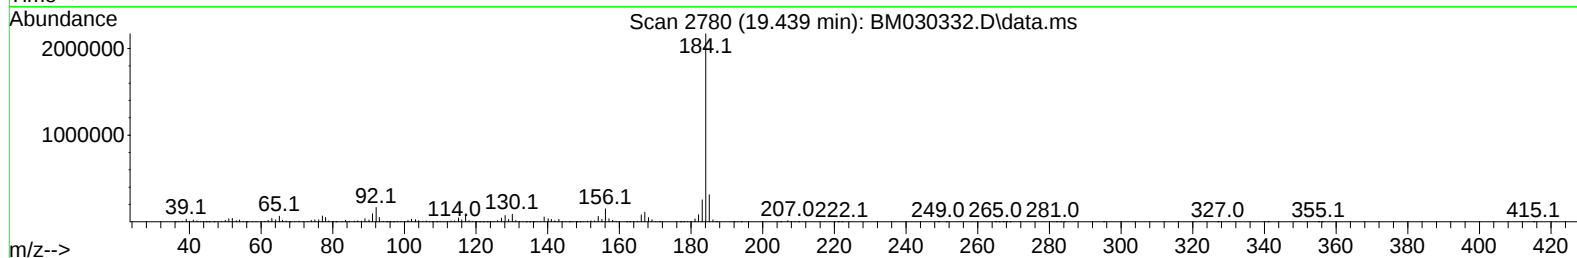


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030332.D
Acq On : 09 Jun 2021 08:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 14:11:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 08 20:51:08 2021
Response via : Initial Calibration

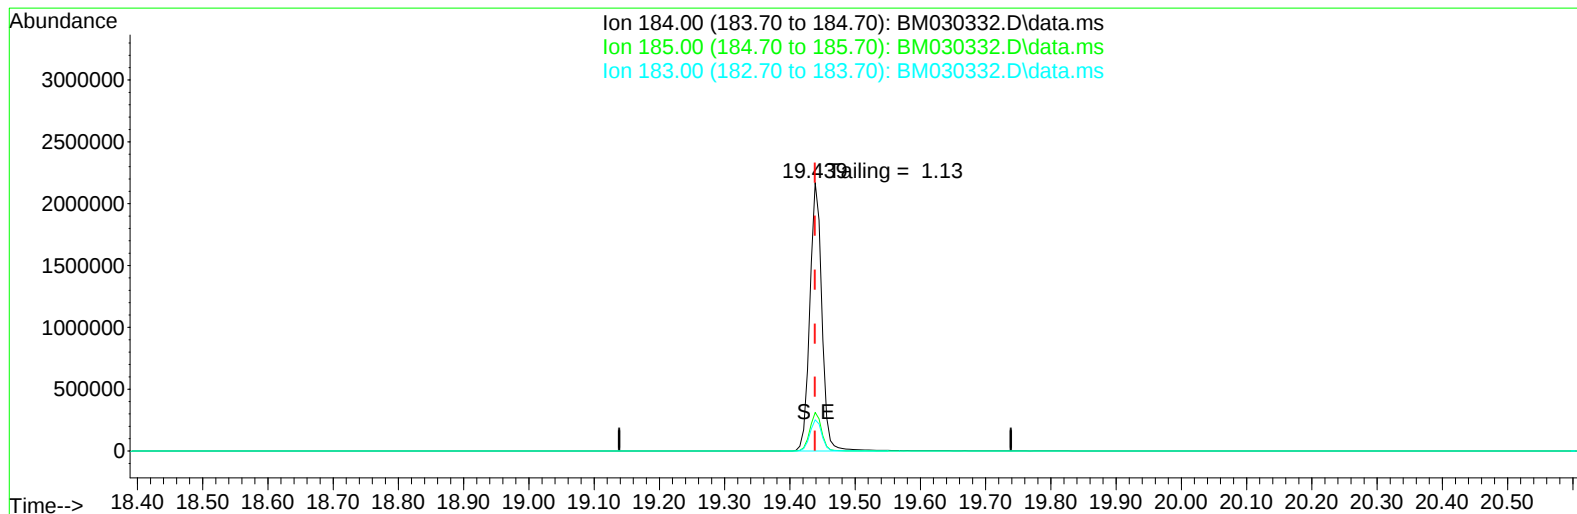




TIC: BM030332.D\data.ms

(77) Benzidine**19.439min (+ 0.000) 11454.42 ng****response 2798455**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.40
183.00	12.30	11.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030332.D
Acq On : 09 Jun 2021 08:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 14:11:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 08 20:51:08 2021
Response via : Initial Calibration

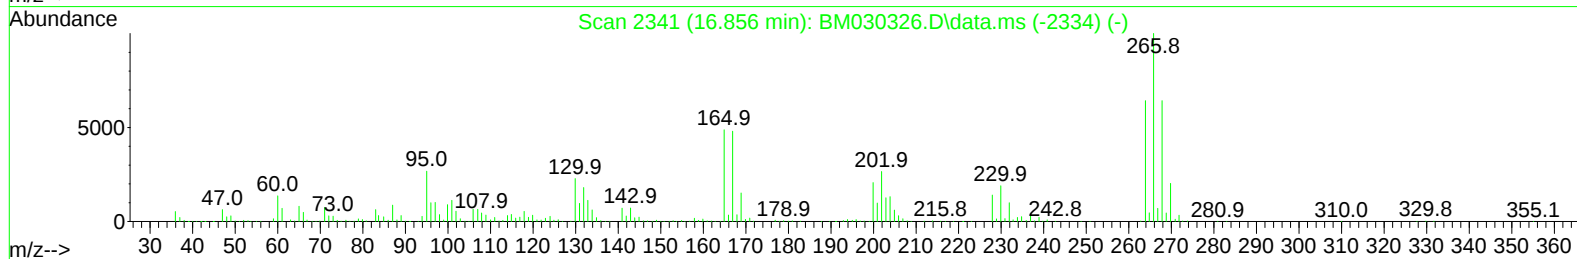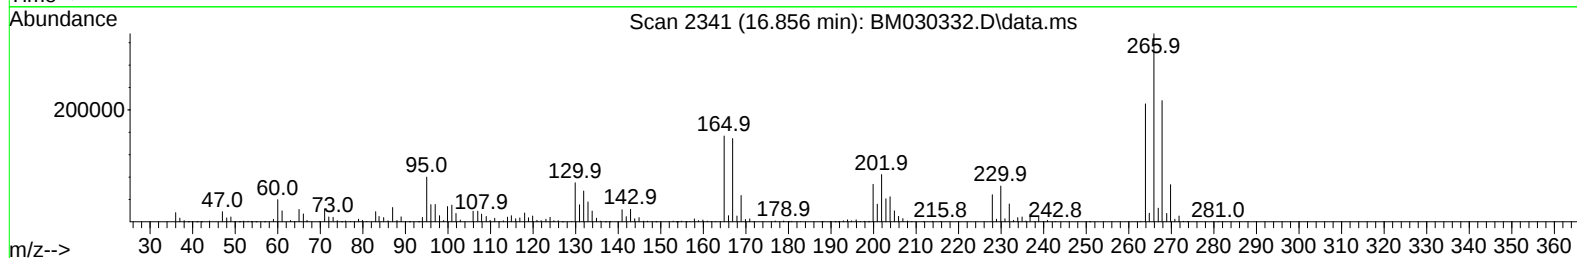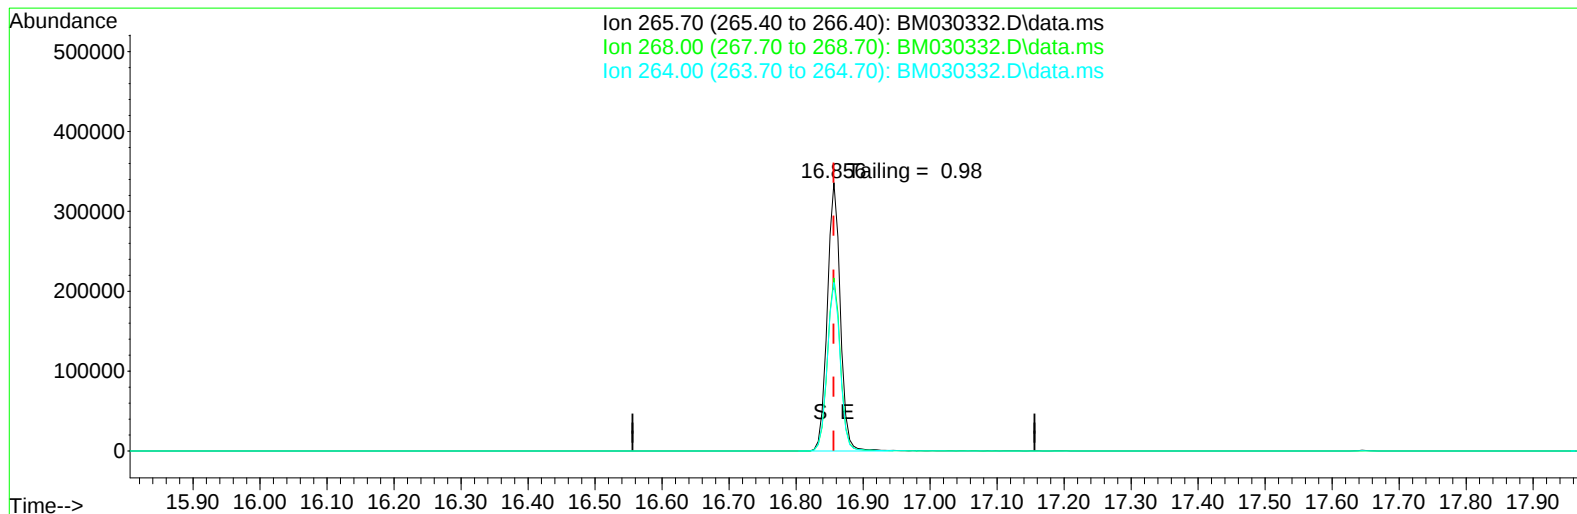

TIC: BM030332.D\data.ms

(70) Pentachlorophenol (C)

16.856min (+ 0.000) 95335.07 ng

response 454185

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	64.48
264.00	64.90	62.76
0.00	0.00	0.00