

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
 Data File : BM030338.D
 Acq On : 09 Jun 2021 12:24
 Operator : CG/JU
 Sample : M2598-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 13

Quant Time: Jun 09 14:56:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 08 20:51:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	166731	20.000	ng	0.00
21) Naphthalene-d8	10.639	136	726864	20.000	ng	# 0.00
39) Acenaphthene-d10	14.474	164	505802	20.000	ng	0.00
64) Phenanthrene-d10	17.203	188	1192459	20.000	ng	# 0.00
76) Chrysene-d12	21.368	240	1315131	20.000	ng	0.00
86) Perylene-d12	23.650	264	1058777	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.428	112	1047365	102.120	ng	0.00
7) Phenol-d6	7.010	99	1415315	95.325	ng	0.00
23) Nitrobenzene-d5	9.004	82	875904	58.707	ng	0.00
42) 2,4,6-Tribromophenol	15.956	330	626324	98.489	ng	0.00
45) 2-Fluorobiphenyl	13.098	172	2302639	59.867	ng	0.00
79) Terphenyl-d14	19.821	244	4453014	59.473	ng	0.00
Target Compounds						
84) Bis(2-ethylhexyl)phtha...	21.280	149	15899	4.508	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030338.D
Acq On : 09 Jun 2021 12:24
Operator : CG/JU
Sample : M2598-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
13

Quant Time: Jun 09 14:56:55 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 08 20:51:08 2021
Response via : Initial Calibration




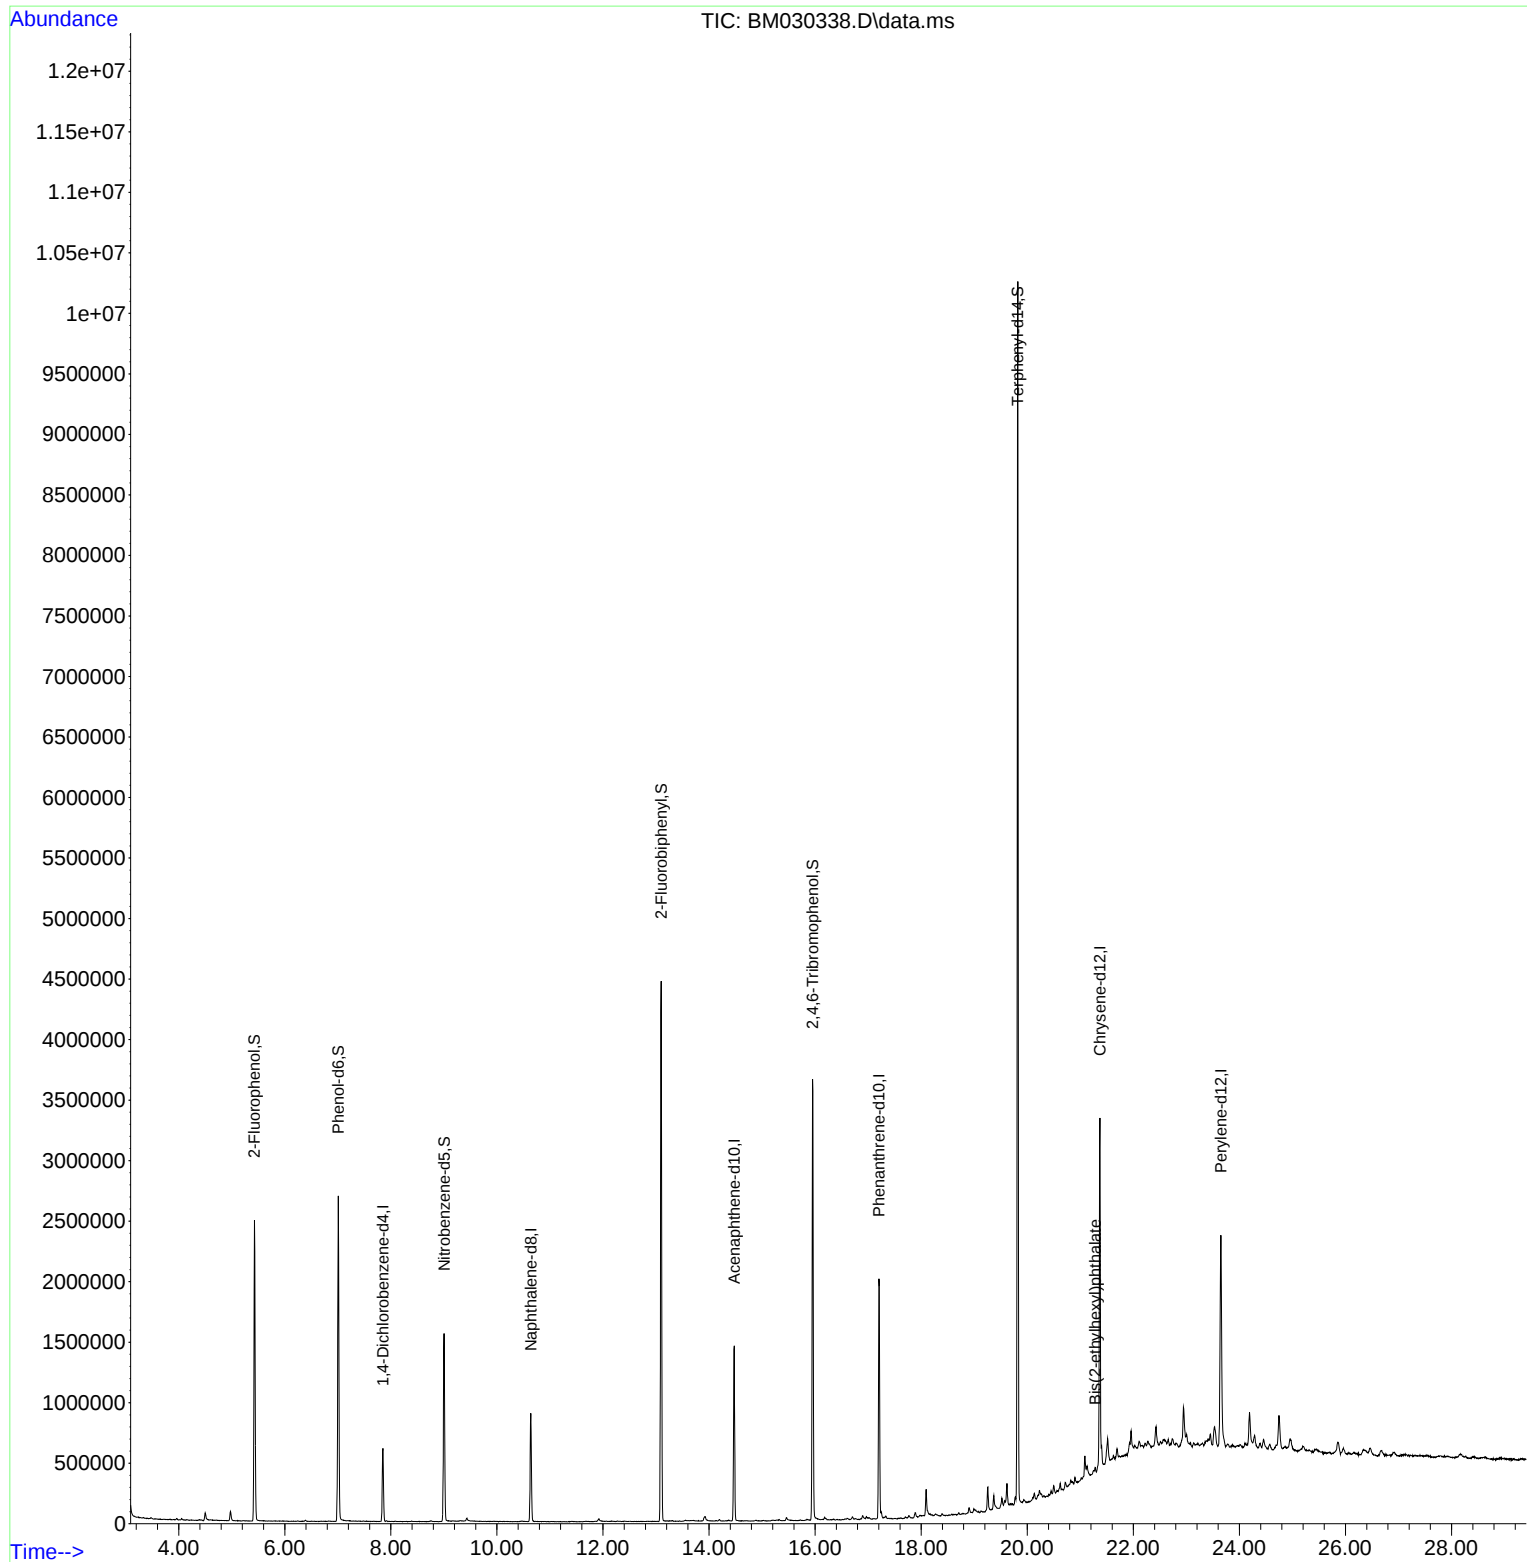




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.851 min Scan# 810
Delta R.T. 0.000 min
Lab File: BM030338.D
Acq: 09 Jun 2021 12:24




Instrument :
BNA_M
ClientSampleId :
13


Tgt Ion:152 Resp: 166731
Ion Ratio Lower Upper
152 100
150 157.4 125.9 188.9
115 57.7 44.6 67.0

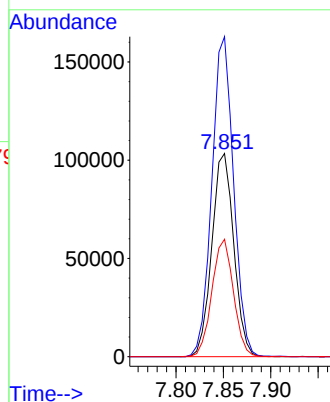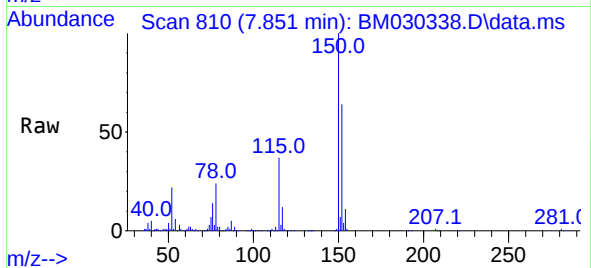

#5
2-Fluorophenol
Concen: 102.120 ng
RT: 5.428 min Scan# 398
Delta R.T. -0.000 min
Lab File: BM030338.D
Acq: 09 Jun 2021 12:24

Tgt Ion:112 Resp: 1047365
Ion Ratio Lower Upper
112 100
64 60.5 47.1 70.7
63 31.4 27.3 40.9


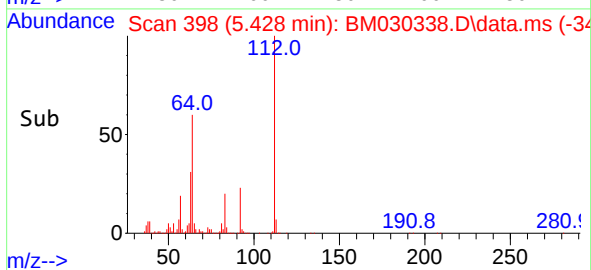
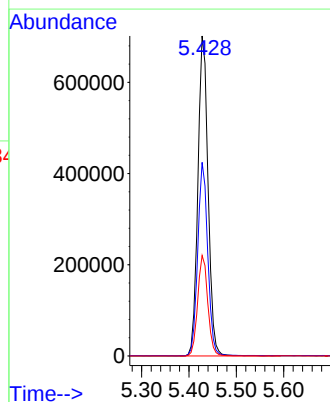





#7
Phenol-d6
Concen: 95.325 ng
RT: 7.010 min Scan# 667
Delta R.T. -0.000 min
Lab File: BM030338.D
Acq: 09 Jun 2021 12:24




Instrument :
BNA_M
ClientSampleId :
13


Tgt Ion: 99 Resp: 1415315
Ion Ratio Lower Upper
99 100
42 20.1 18.0 27.0
71 32.5 30.9 46.3

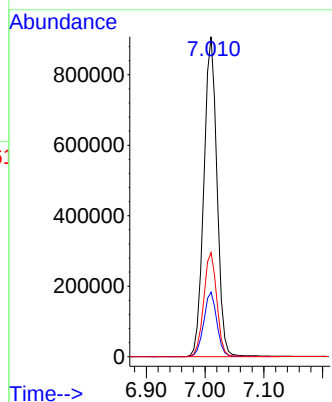

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.639 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BM030338.D
Acq: 09 Jun 2021 12:24

Tgt Ion: 136 Resp: 726864
Ion Ratio Lower Upper
136 100
137 11.2 8.4 12.6
54 8.6 5.5 8.3#
68 6.0 4.2 6.2


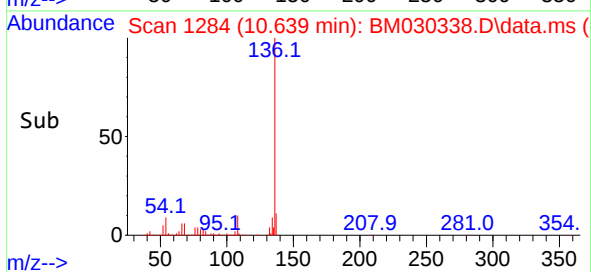
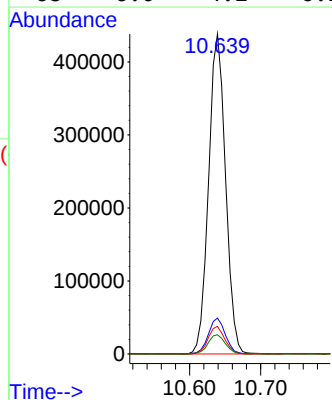





#23
Nitrobenzene-d5
Concen: 58.707 ng
RT: 9.004 min Scan# 1006
Delta R.T. -0.006 min
Lab File: BM030338.D
Acq: 09 Jun 2021 12:24




Instrument :
BNA_M
ClientSampleId :
13


Tgt Ion: 82 Resp: 875904
Ion Ratio Lower Upper
82 100
128 41.8 31.1 46.7
54 52.0 37.3 55.9

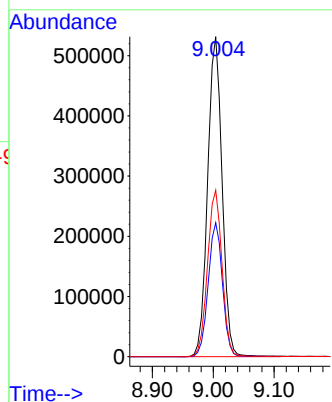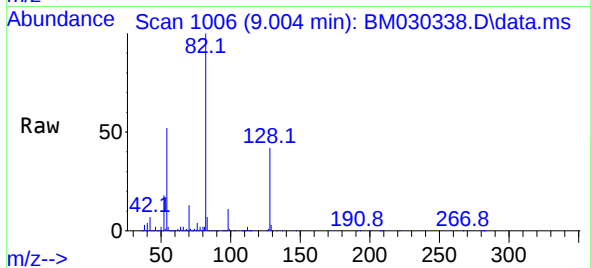

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.474 min Scan# 1936
Delta R.T. 0.000 min
Lab File: BM030338.D
Acq: 09 Jun 2021 12:24

Tgt Ion:164 Resp: 505802
Ion Ratio Lower Upper
164 100
162 101.4 83.4 125.0
160 45.3 37.2 55.8


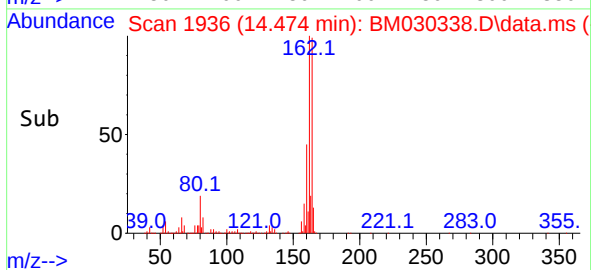
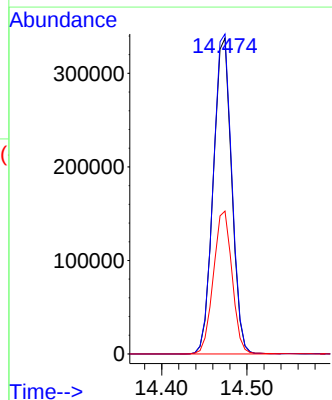





#42
2,4,6-Tribromophenol
Concen: 98.489 ng
RT: 15.956 min Scan# 2188
Delta R.T. -0.000 min
Lab File: BM030338.D
Acq: 09 Jun 2021 12:24




Instrument :
BNA_M
ClientSampleId :
13


Tgt Ion:330 Resp: 626324
Ion Ratio Lower Upper
330 100
332 96.3 77.0 115.4
141 37.1 30.2 45.2

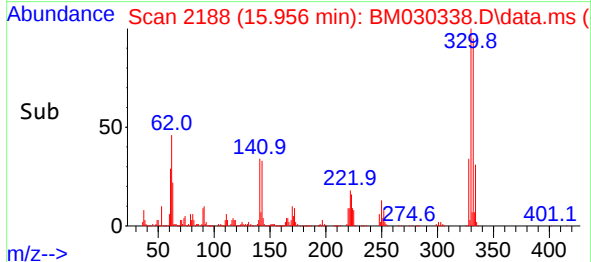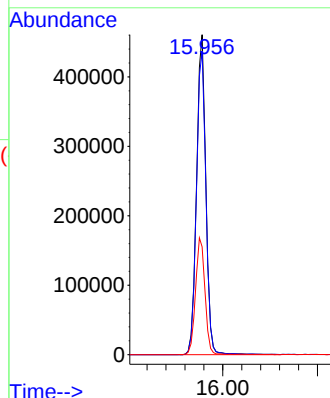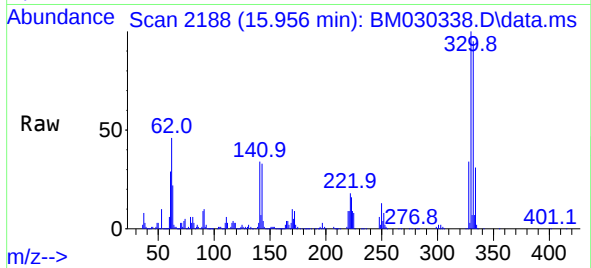

#45
2-Fluorobiphenyl
Concen: 59.867 ng
RT: 13.098 min Scan# 1702
Delta R.T. -0.000 min
Lab File: BM030338.D
Acq: 09 Jun 2021 12:24

Tgt Ion:172 Resp: 2302639
Ion Ratio Lower Upper
172 100
171 35.2 28.6 43.0
170 23.0 18.4 27.6


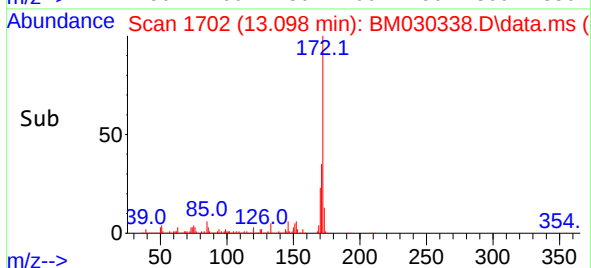
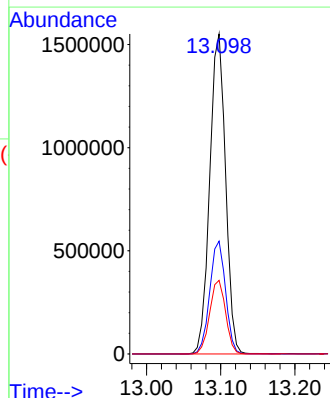





#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.203 min Scan# 2400
Delta R.T. -0.006 min
Lab File: BM030338.D
Acq: 09 Jun 2021 12:24




Instrument :
BNA_M
ClientSampled :
13


Tgt Ion:188 Resp: 1192459
Ion Ratio Lower Upper
188 100
94 9.0 6.0 9.0
80 10.1 6.6 9.8#

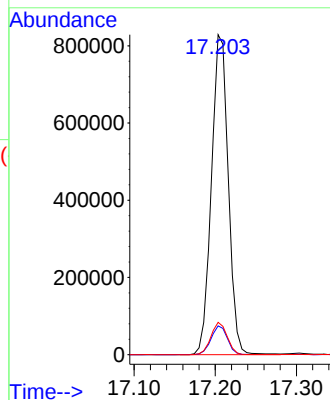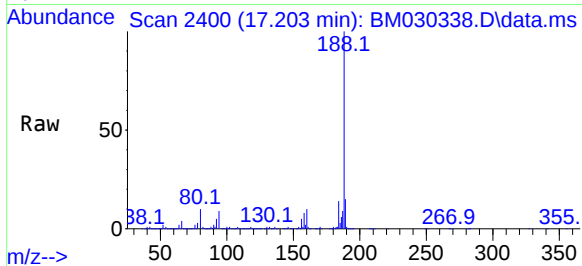

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.368 min Scan# 3108
Delta R.T. -0.000 min
Lab File: BM030338.D
Acq: 09 Jun 2021 12:24

Tgt Ion:240 Resp: 1315131
Ion Ratio Lower Upper
240 100
120 10.2 7.0 10.6
236 26.1 21.0 31.4

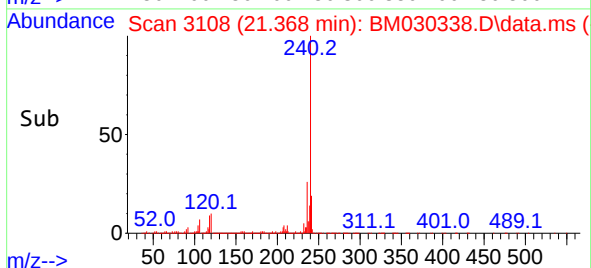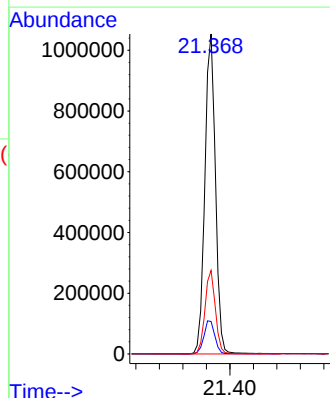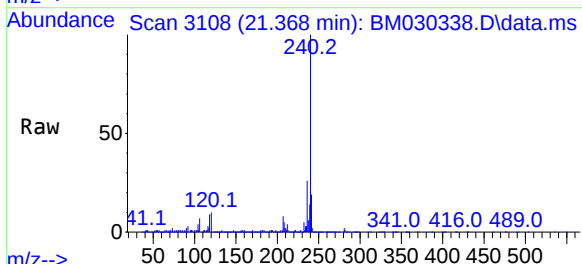







#79
 Terphenyl-d14
 Concen: 59.473 ng
 RT: 19.821 min Scan# 2845
 Delta R.T. -0.000 min
 Lab File: BM030338.D
 Acq: 09 Jun 2021 12:24

Instrument :
 BNA_M
 ClientSampled :
 13

Tgt Ion:244 Resp: 4453014




Ion	Ratio	Lower	Upper
244	100		
212	7.5	6.3	9.5
122	9.9	6.9	10.3

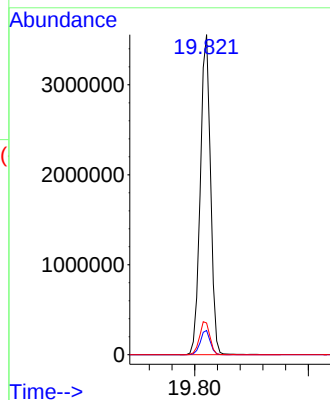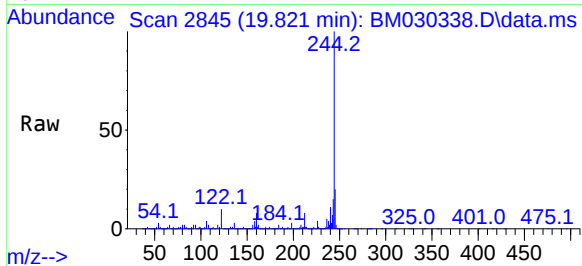


#84
 Bis(2-ethylhexyl)phthalate
 Concen: 4.508 ng
 RT: 21.280 min Scan# 3093
 Delta R.T. -0.000 min
 Lab File: BM030338.D
 Acq: 09 Jun 2021 12:24

Tgt Ion:149 Resp: 15899

Ion	Ratio	Lower	Upper
149	100		
167	28.1	22.6	33.8
279	5.0	3.8	5.8

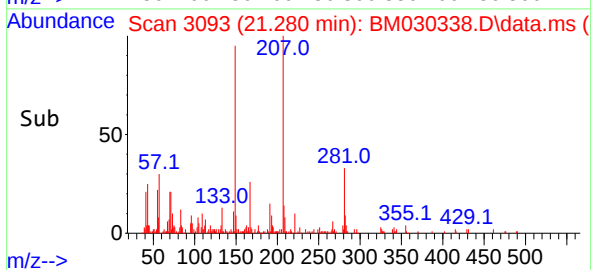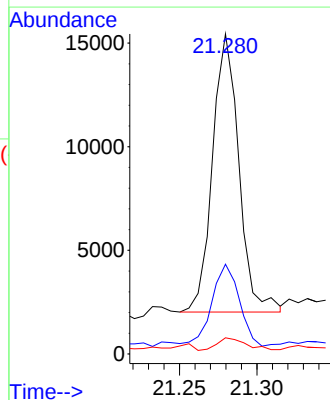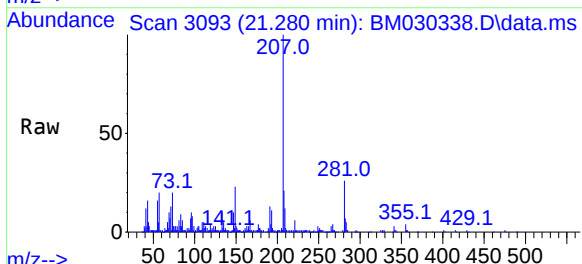

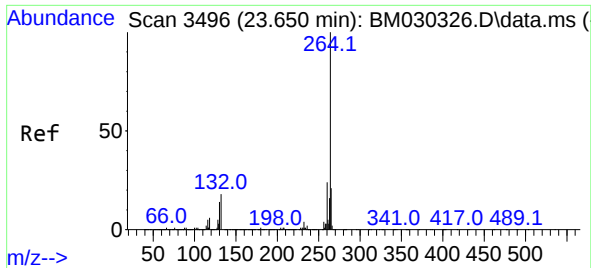

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.650 min Scan# 3496
 Delta R.T. -0.000 min
 Lab File: BM030338.D
 Acq: 09 Jun 2021 12:24

Instrument :
 BNA_M
 ClientSampleId :
 13

Tgt Ion:264 Resp: 1058777

Ion	Ratio	Lower	Upper
264	100		
260	26.7	19.8	29.8
265	21.5	17.7	26.5

