

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
 Data File : BM030348.D
 Acq On : 09 Jun 2021 18:44
 Operator : CG/JU
 Sample : M2612-19
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 18-B12(78-82)

Quant Time: Jun 10 02:27:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 08 20:51:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	195955	20.000	ng	0.00
21) Naphthalene-d8	10.639	136	789018	20.000	ng	# 0.00
39) Acenaphthene-d10	14.474	164	551582	20.000	ng	0.00
64) Phenanthrene-d10	17.204	188	1290892	20.000	ng	# 0.00
76) Chrysene-d12	21.368	240	1371392	20.000	ng	0.00
86) Perylene-d12	23.650	264	1224776	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.428	112	1199425	99.505	ng	0.00
7) Phenol-d6	7.010	99	1591684	91.216	ng	0.00
23) Nitrobenzene-d5	9.004	82	930985	57.483	ng	0.00
42) 2,4,6-Tribromophenol	15.957	330	703547	101.450	ng	0.00
45) 2-Fluorobiphenyl	13.098	172	2171517	51.772	ng	0.00
79) Terphenyl-d14	19.821	244	4138138	53.000	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.927	163	473197	10.780	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030348.D
Acq On : 09 Jun 2021 18:44
Operator : CG/JU
Sample : M2612-19
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
18-B12(78-82)

Quant Time: Jun 10 02:27:15 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 08 20:51:08 2021
Response via : Initial Calibration




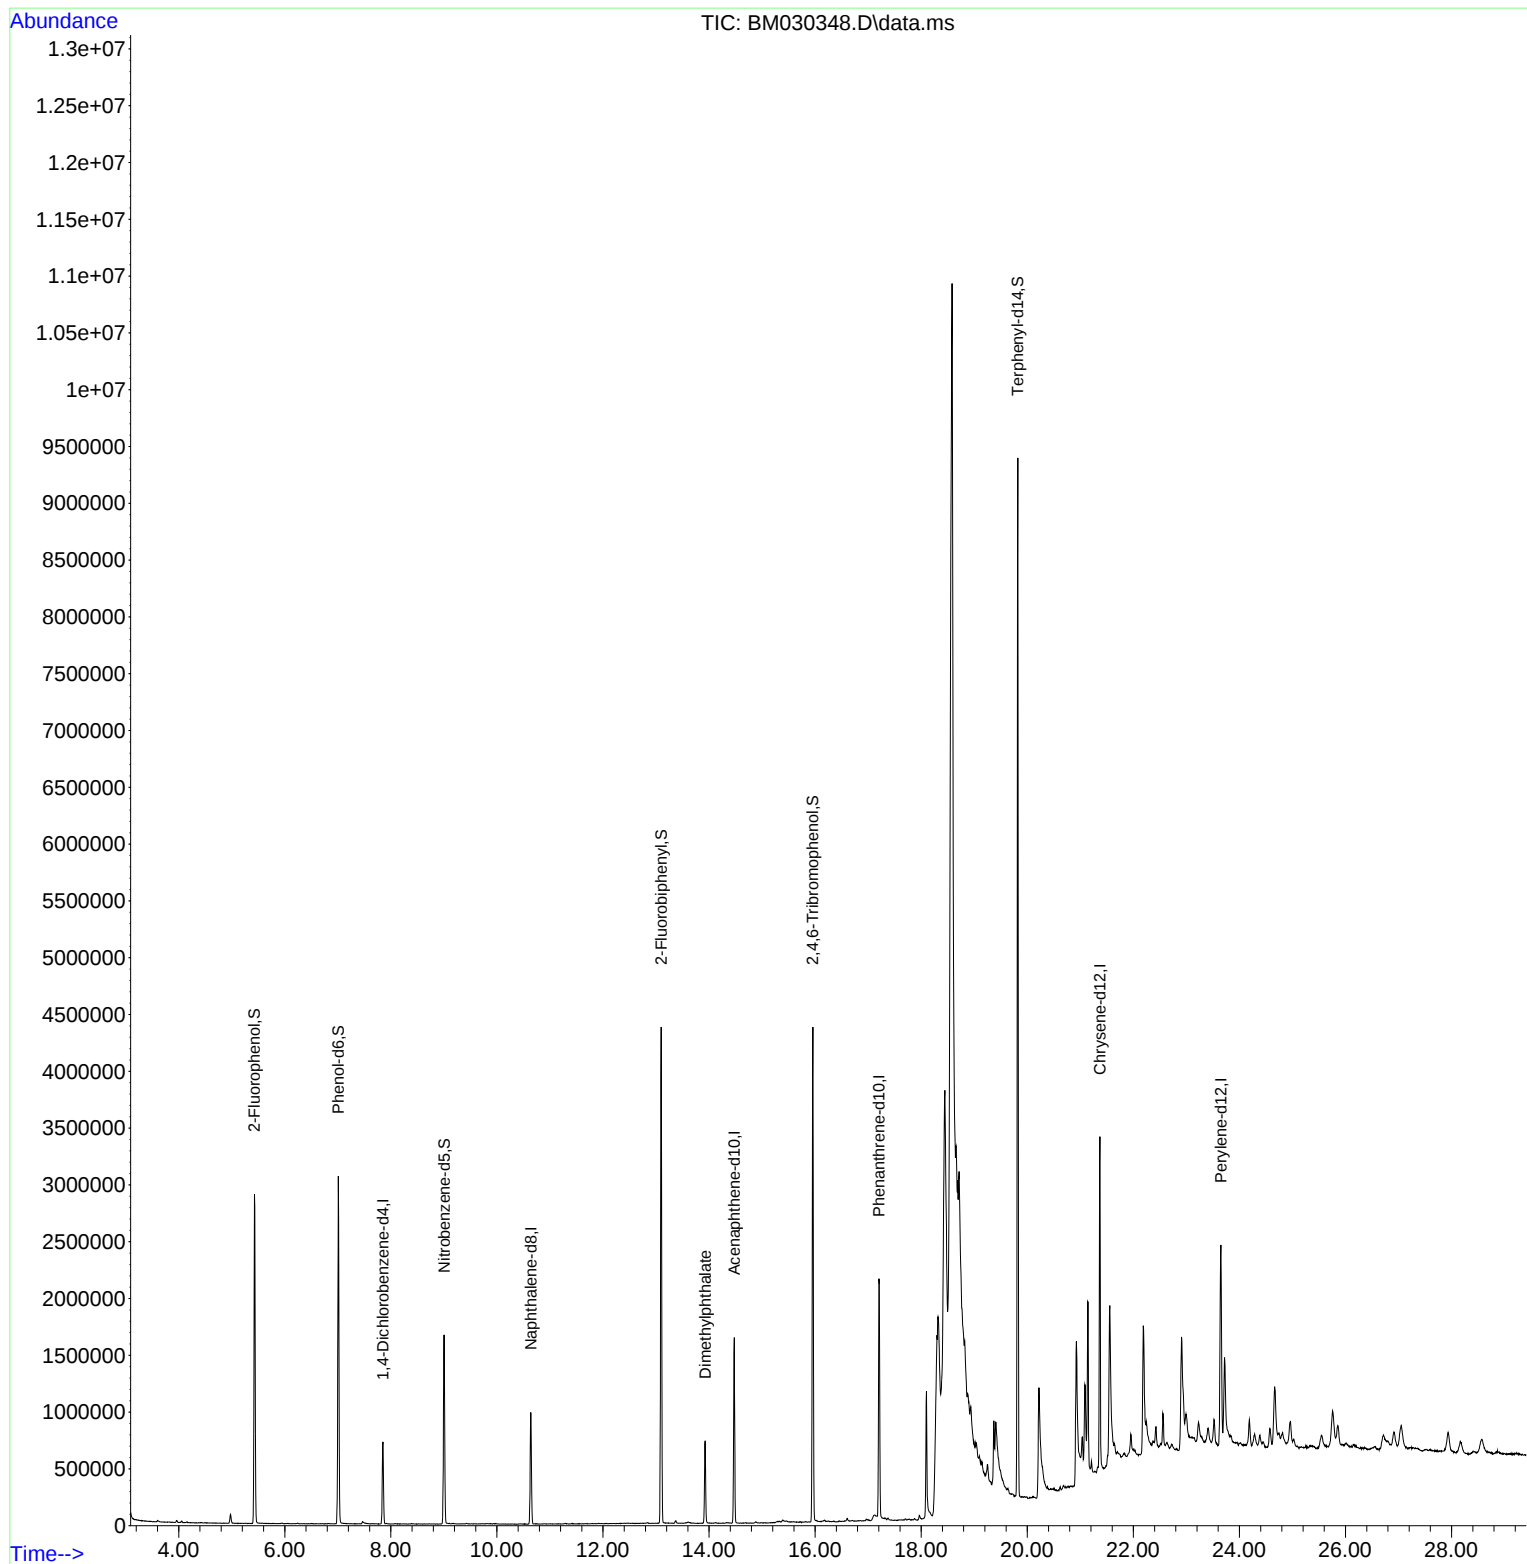




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.851 min Scan# 810
Delta R.T. 0.000 min
Lab File: BM030348.D
Acq: 09 Jun 2021 18:44




Instrument :
BNA_M
ClientSampleId :
18-B12(78-82)


Tgt Ion:152 Resp: 195955
Ion Ratio Lower Upper
152 100
150 155.1 125.9 188.9
115 57.0 44.6 67.0

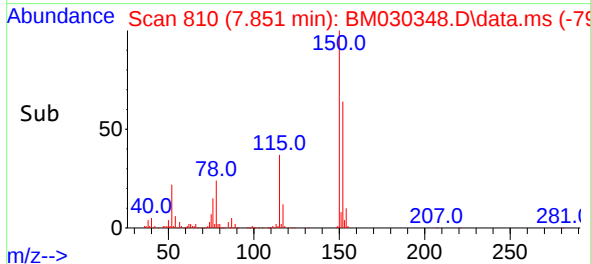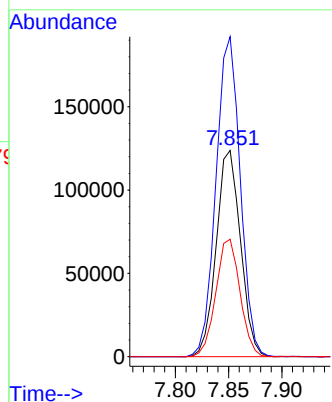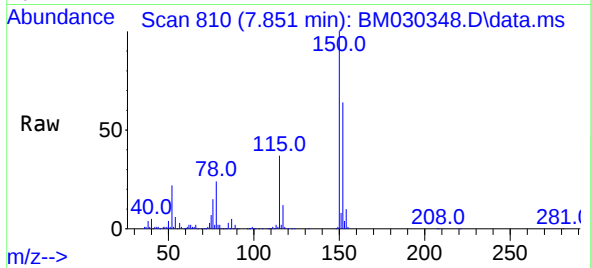

#5
2-Fluorophenol
Concen: 99.505 ng
RT: 5.428 min Scan# 398
Delta R.T. 0.000 min
Lab File: BM030348.D
Acq: 09 Jun 2021 18:44

Tgt Ion:112 Resp: 1199425
Ion Ratio Lower Upper
112 100
64 60.4 47.1 70.7
63 32.8 27.3 40.9

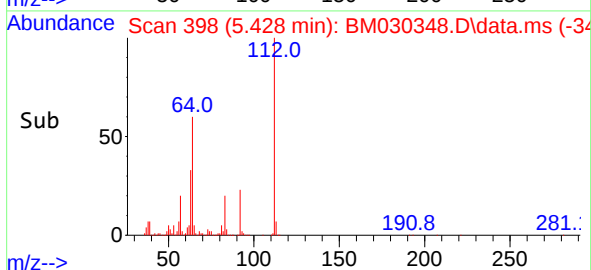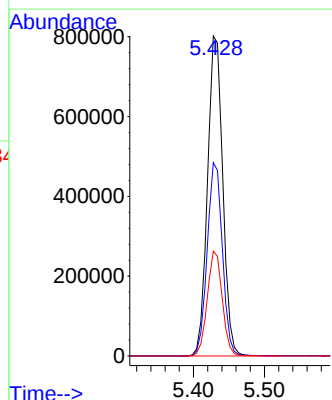







#7
Phenol-d6
Concen: 91.216 ng
RT: 7.010 min Scan# 667
Delta R.T. 0.000 min
Lab File: BM030348.D
Acq: 09 Jun 2021 18:44

Instrument :
BNA_M
ClientSampleId :
18-B12(78-82)

Tgt Ion: 99 Resp: 1591684




Ion	Ratio	Lower	Upper
99	100		
42	20.6	18.0	27.0
71	33.2	30.9	46.3

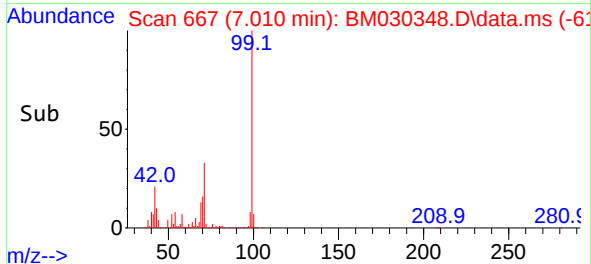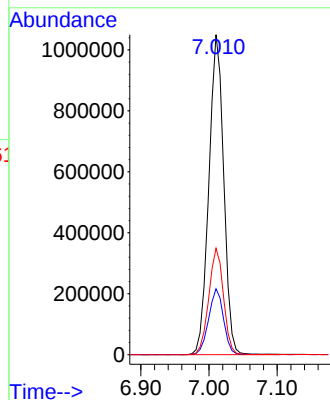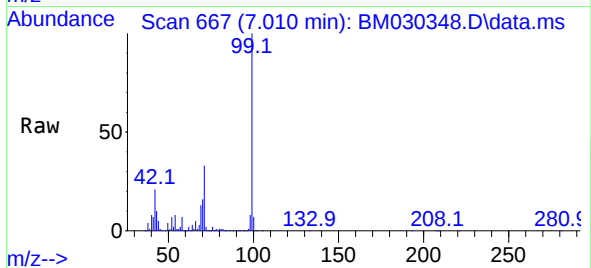


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.639 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BM030348.D
Acq: 09 Jun 2021 18:44

Tgt Ion: 136 Resp: 789018

Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.4	12.6
54	8.8	5.5	8.3#
68	6.2	4.2	6.2


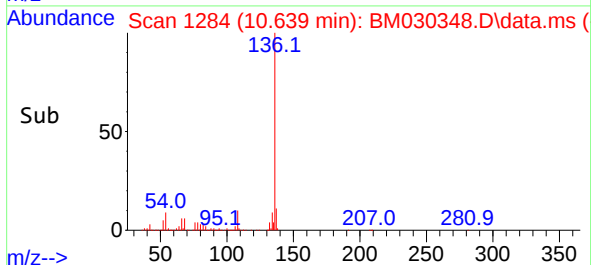
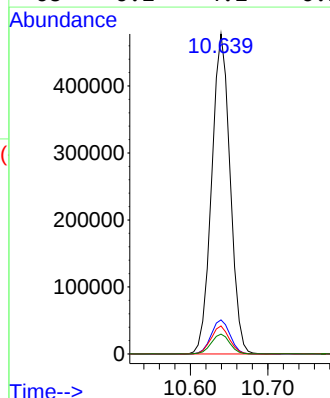
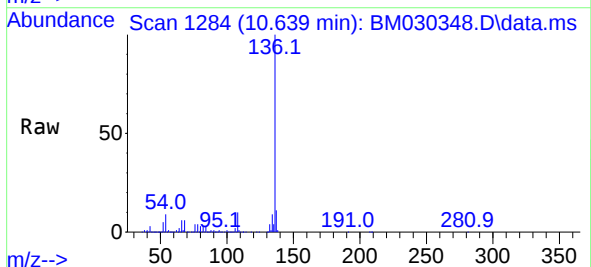




#23
Nitrobenzene-d5
Concen: 57.483 ng
RT: 9.004 min Scan# 1006
Delta R.T. -0.006 min
Lab File: BM030348.D
Acq: 09 Jun 2021 18:44




Instrument :
BNA_M
ClientSampleId :
18-B12(78-82)


Tgt Ion: 82 Resp: 930985
Ion Ratio Lower Upper
82 100
128 41.3 31.1 46.7
54 51.8 37.3 55.9

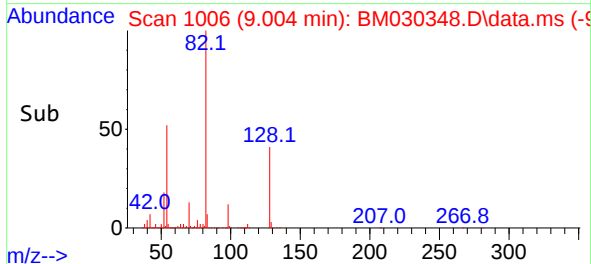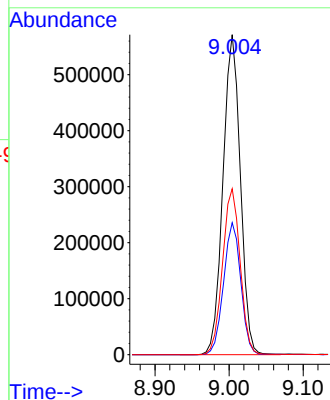

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.474 min Scan# 1936
Delta R.T. 0.000 min
Lab File: BM030348.D
Acq: 09 Jun 2021 18:44

Tgt Ion:164 Resp: 551582
Ion Ratio Lower Upper
164 100
162 102.5 83.4 125.0
160 45.6 37.2 55.8


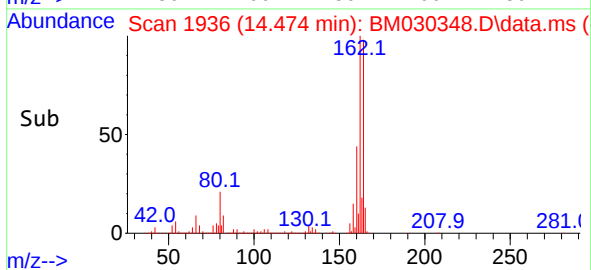
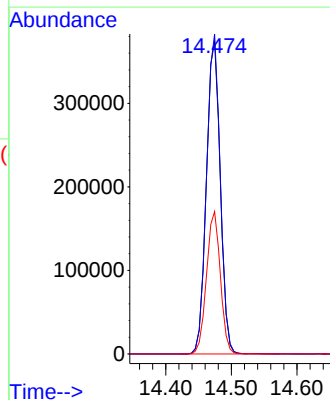
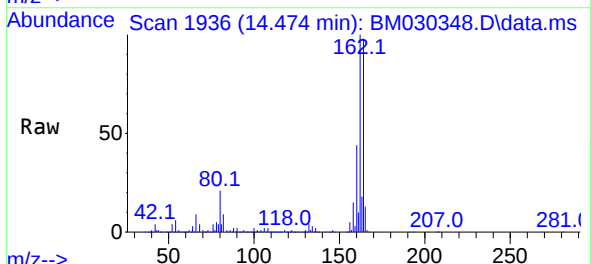




#42
2,4,6-Tribromophenol
Concen: 101.450 ng
RT: 15.957 min Scan# 2188
Delta R.T. 0.000 min
Lab File: BM030348.D
Acq: 09 Jun 2021 18:44




Instrument :
BNA_M
ClientSampleId :
18-B12(78-82)


Tgt Ion:330 Resp: 703547
Ion Ratio Lower Upper
330 100
332 96.2 77.0 115.4
141 38.8 30.2 45.2

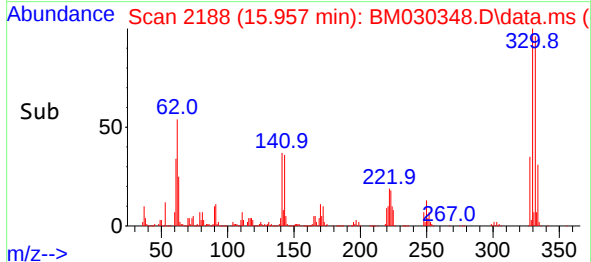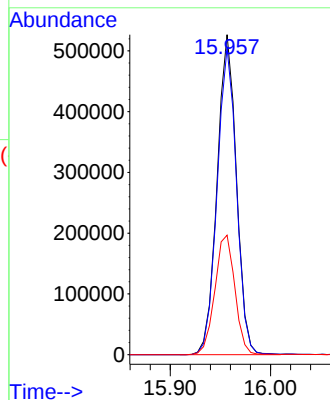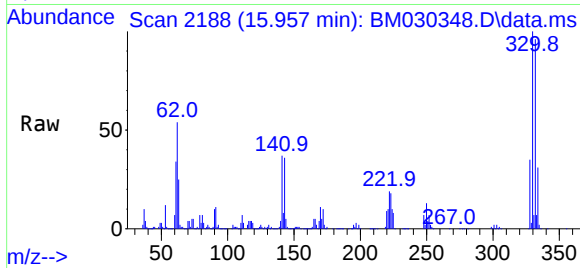

#45
2-Fluorobiphenyl
Concen: 51.772 ng
RT: 13.098 min Scan# 1702
Delta R.T. 0.000 min
Lab File: BM030348.D
Acq: 09 Jun 2021 18:44

Tgt Ion:172 Resp: 2171517
Ion Ratio Lower Upper
172 100
171 35.5 28.6 43.0
170 23.2 18.4 27.6


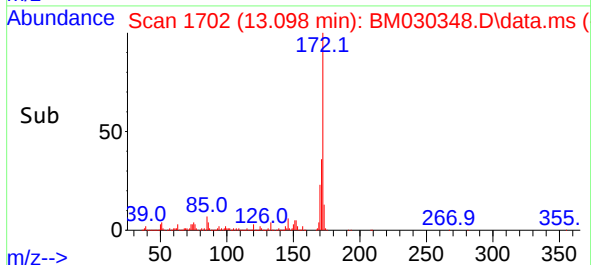
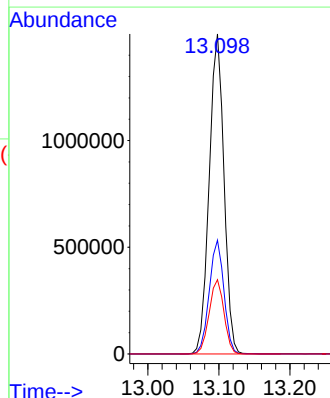
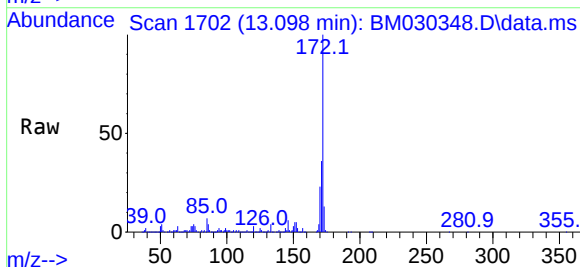




#50
Dimethylphthalate
Concen: 10.780 ng
RT: 13.927 min Scan# 1843
Delta R.T. -0.006 min
Lab File: BM030348.D
Acq: 09 Jun 2021 18:44




Instrument :
BNA_M
ClientSampleId :
18-B12(78-82)


Tgt Ion:163 Resp: 473197
Ion Ratio Lower Upper
163 100
194 4.2 3.3 4.9
164 9.9 7.9 11.9

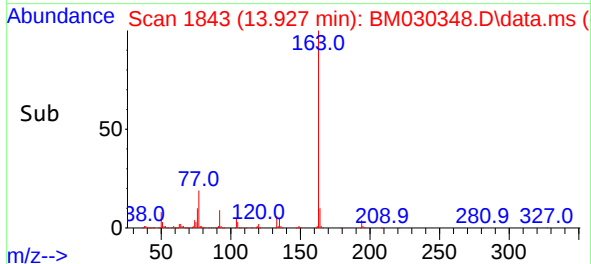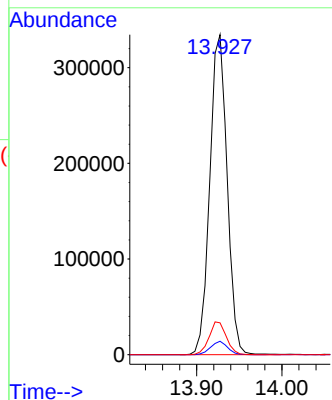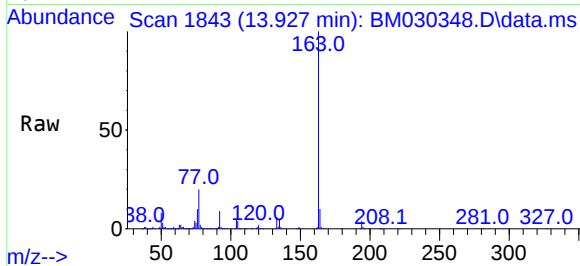

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.204 min Scan# 2400
Delta R.T. -0.005 min
Lab File: BM030348.D
Acq: 09 Jun 2021 18:44

Tgt Ion:188 Resp: 1290892
Ion Ratio Lower Upper
188 100
94 9.4 6.0 9.0#
80 9.8 6.6 9.8#


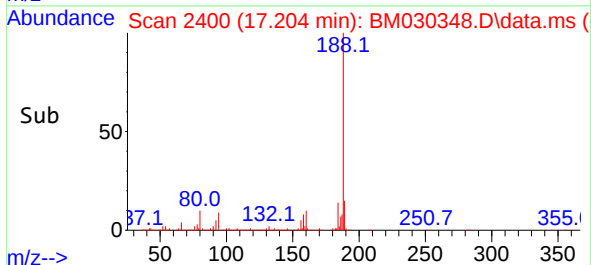
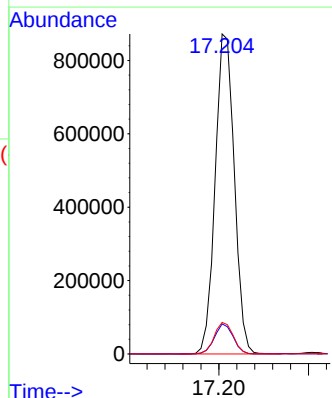
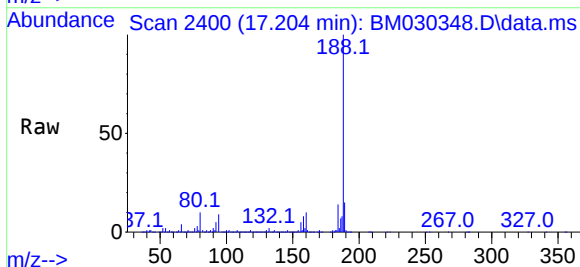




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.368 min Scan# 3108
Delta R.T. 0.000 min
Lab File: BM030348.D
Acq: 09 Jun 2021 18:44




Instrument :
BNA_M
ClientSampleId :
18-B12(78-82)


Tgt Ion:240 Resp: 1371392
Ion Ratio Lower Upper
240 100
120 10.2 7.0 10.6
236 25.6 21.0 31.4

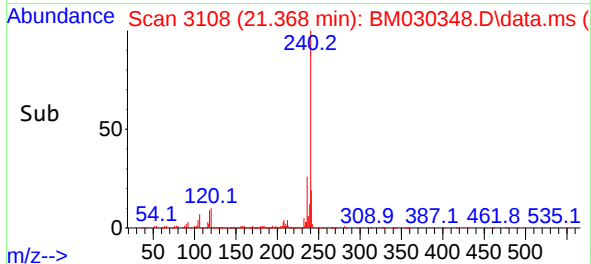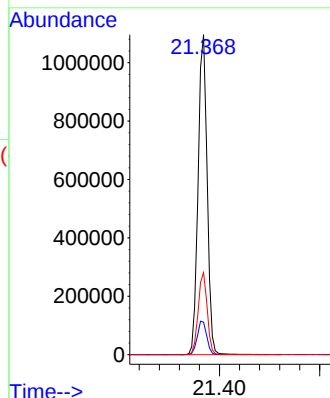

#79
Terphenyl-d14
Concen: 53.000 ng
RT: 19.821 min Scan# 2845
Delta R.T. 0.000 min
Lab File: BM030348.D
Acq: 09 Jun 2021 18:44


Tgt Ion:244 Resp: 4138138
Ion Ratio Lower Upper
244 100
212 7.3 6.3 9.5
122 10.3 6.9 10.3#

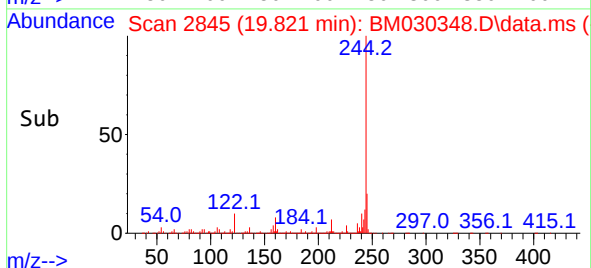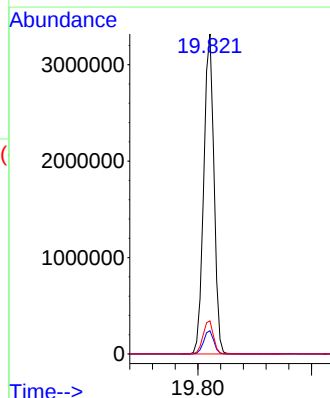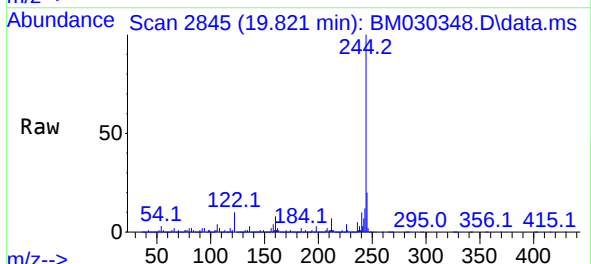

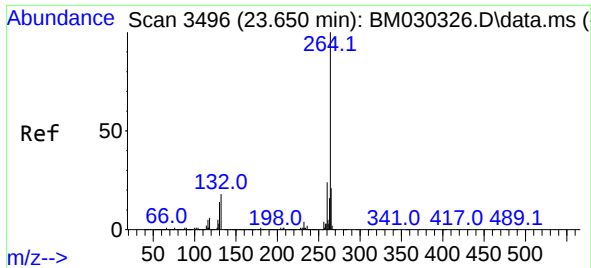

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.650 min Scan# 3496
 Delta R.T. 0.000 min
 Lab File: BM030348.D
 Acq: 09 Jun 2021 18:44

Instrument :
 BNA_M
 ClientSampleId :
 18-B12(78-82)

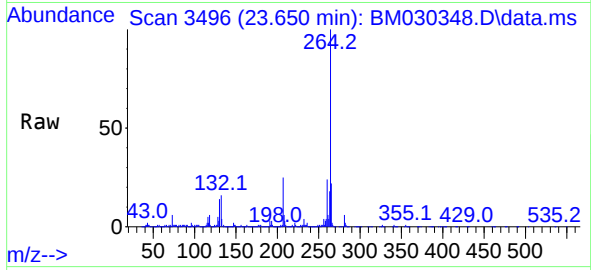

Tgt Ion:264 Resp: 1224776

Ion	Ratio	Lower	Upper
264	100		
260	23.7	19.8	29.8
265	22.1	17.7	26.5

