

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
 Data File : BM030357.D
 Acq On : 10 Jun 2021 00:19
 Operator : CG/JU
 Sample : M2631-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0225-FIELD-BLANK-1

Quant Time: Jun 10 02:29:00 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 08 20:51:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.845	152	219252	20.000	ng	0.00
21) Naphthalene-d8	10.639	136	931226	20.000	ng	# 0.00
39) Acenaphthene-d10	14.468	164	670962	20.000	ng	0.00
64) Phenanthrene-d10	17.203	188	1519558	20.000	ng	# 0.00
76) Chrysene-d12	21.362	240	1571475	20.000	ng	# 0.00
86) Perylene-d12	23.644	264	1402365	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.428	112	708665	52.544	ng	0.00
7) Phenol-d6	7.004	99	540958	27.707	ng	0.00
23) Nitrobenzene-d5	9.004	82	1489599	77.929	ng	0.00
42) 2,4,6-Tribromophenol	15.956	330	1155357	136.958	ng	0.00
45) 2-Fluorobiphenyl	13.098	172	3929975	77.026	ng	0.00
79) Terphenyl-d14	19.821	244	7791910	87.090	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.921	163	371286	6.953	ng	99
84) Bis(2-ethylhexyl)phtha...	21.274	149	9549	4.392	ng	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030357.D
Acq On : 10 Jun 2021 00:19
Operator : CG/JU
Sample : M2631-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0225-FIELD-BLANK-1

Quant Time: Jun 10 02:29:00 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 08 20:51:08 2021
Response via : Initial Calibration




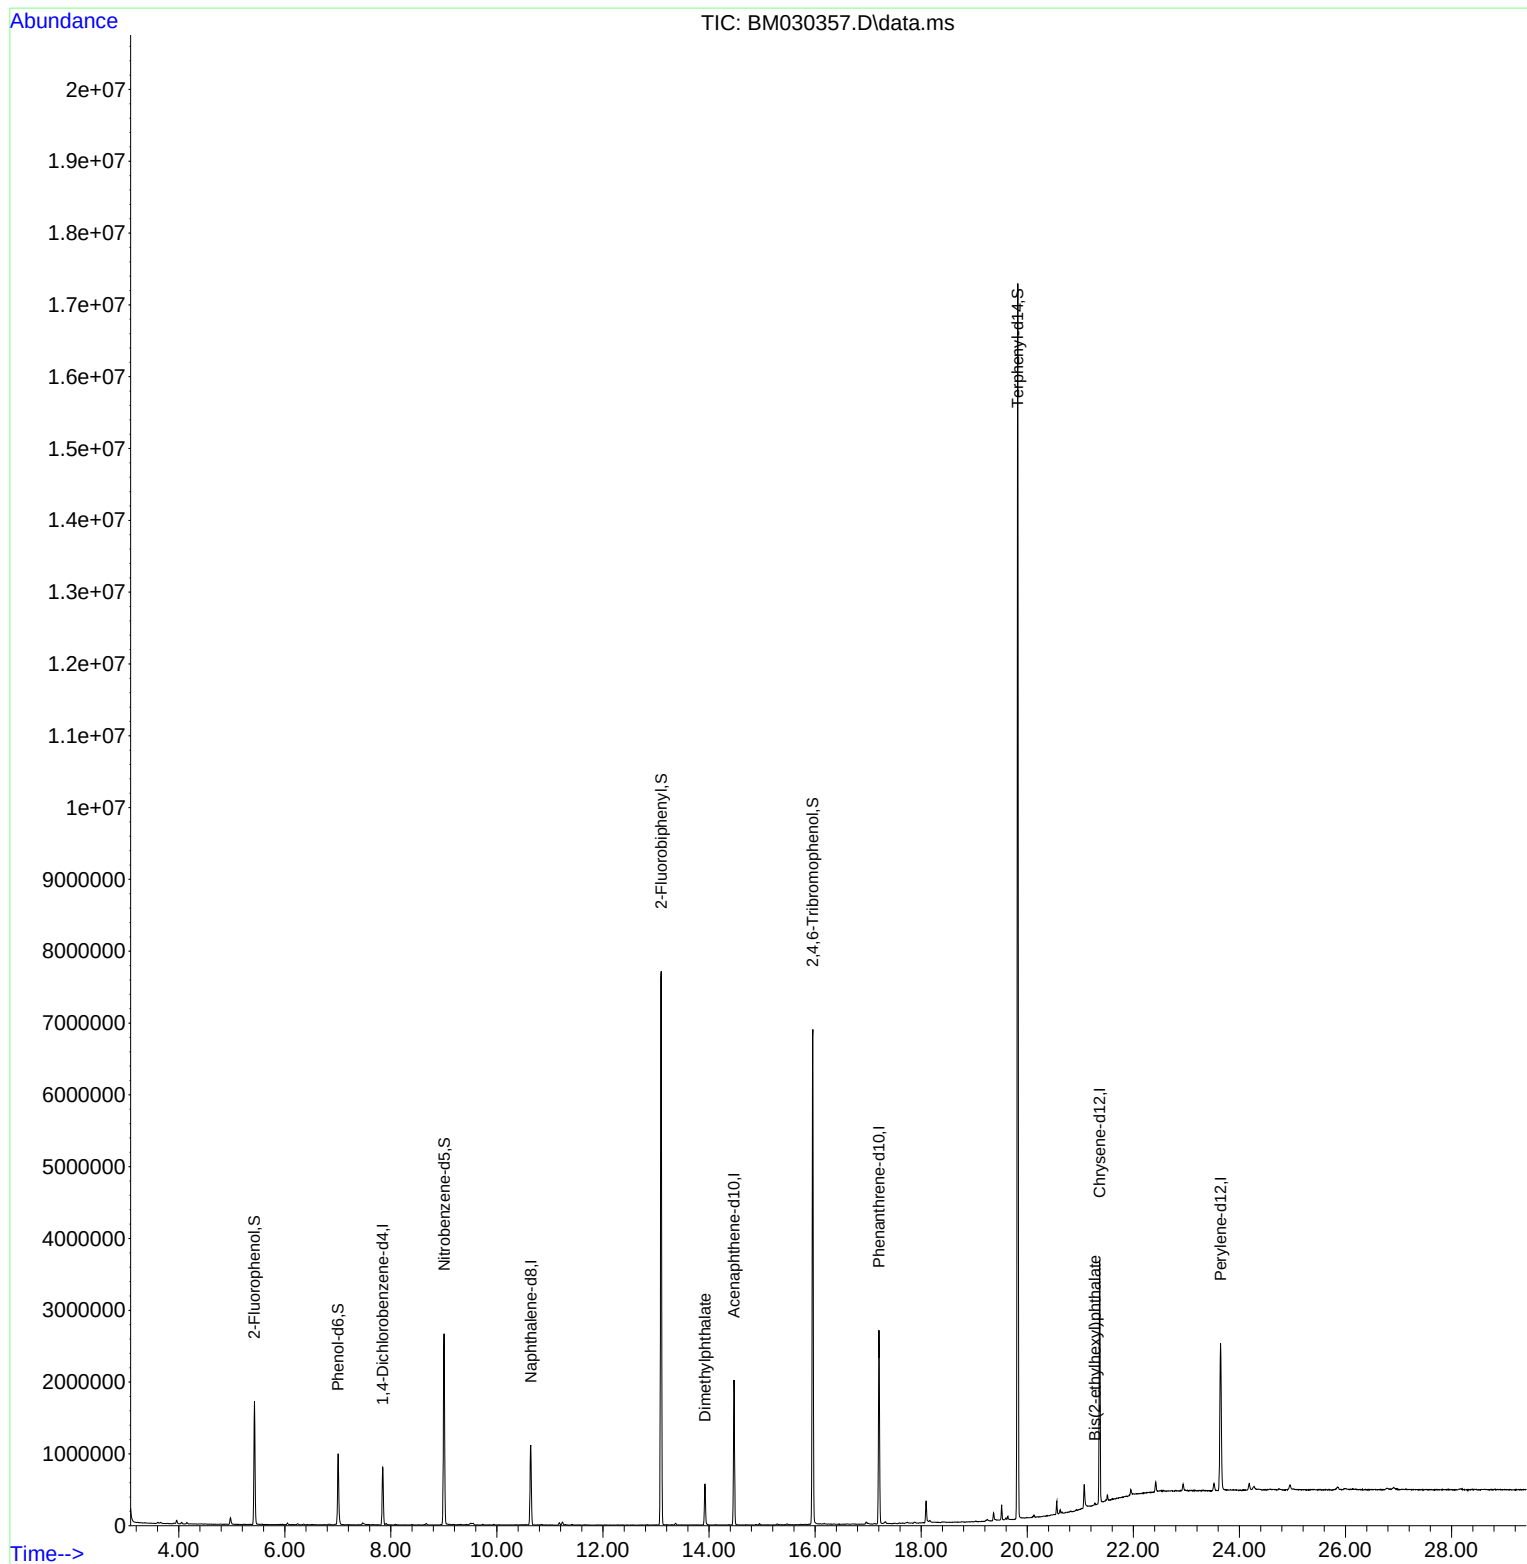




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.845 min Scan# 809
Delta R.T. -0.006 min
Lab File: BM030357.D
Acq: 10 Jun 2021 00:19




Instrument :
BNA_M
ClientSampleId :
0225-FIELD-BLANK-1


Tgt Ion:152 Resp: 219252
Ion Ratio Lower Upper
152 100
150 155.6 125.9 188.9
115 57.4 44.6 67.0

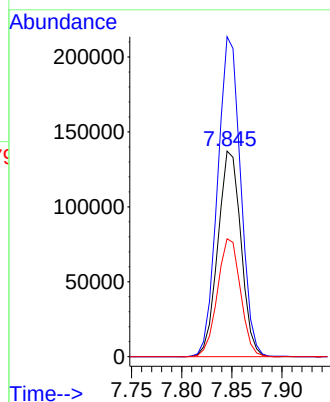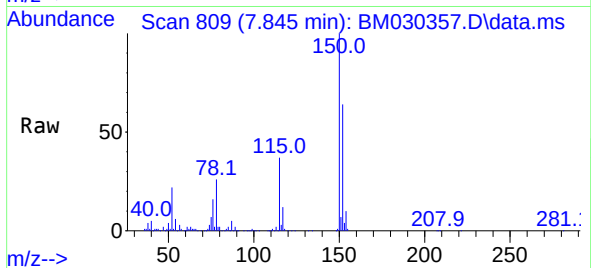

#5
2-Fluorophenol
Concen: 52.544 ng
RT: 5.428 min Scan# 398
Delta R.T. -0.000 min
Lab File: BM030357.D
Acq: 10 Jun 2021 00:19

Tgt Ion:112 Resp: 708665
Ion Ratio Lower Upper
112 100
64 59.2 47.1 70.7
63 31.3 27.3 40.9


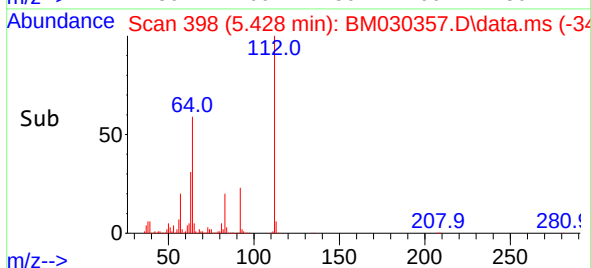
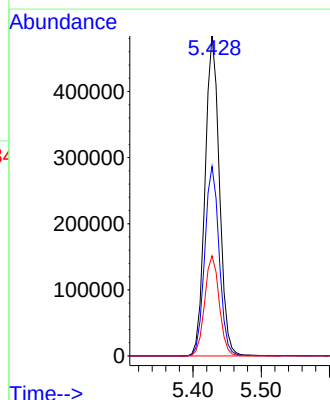





#7
Phenol-d6
Concen: 27.707 ng
RT: 7.004 min Scan# 666
Delta R.T. -0.006 min
Lab File: BM030357.D
Acq: 10 Jun 2021 00:19




Instrument :
BNA_M
ClientSampleId :
0225-FIELD-BLANK-1


Tgt Ion: 99 Resp: 540958
Ion Ratio Lower Upper
99 100
42 20.5 18.0 27.0
71 32.4 30.9 46.3

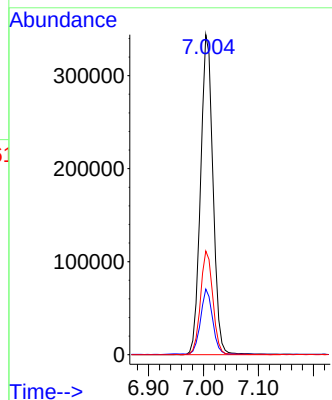

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.639 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BM030357.D
Acq: 10 Jun 2021 00:19

Tgt Ion: 136 Resp: 931226
Ion Ratio Lower Upper
136 100
137 11.0 8.4 12.6
54 9.1 5.5 8.3#
68 6.5 4.2 6.2#


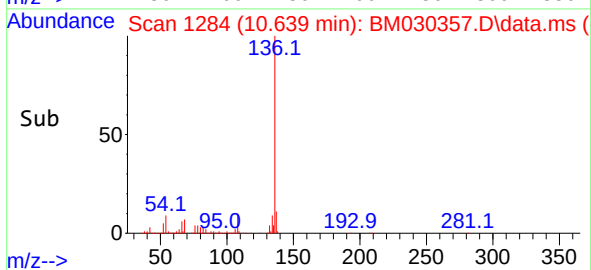
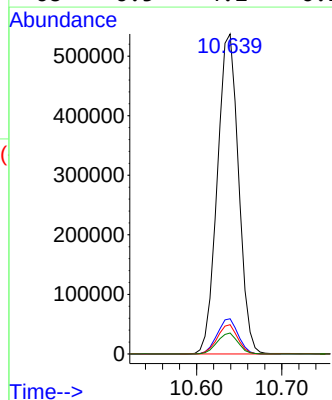





#23
Nitrobenzene-d5
Concen: 77.929 ng
RT: 9.004 min Scan# 1006
Delta R.T. -0.006 min
Lab File: BM030357.D
Acq: 10 Jun 2021 00:19




Instrument :
BNA_M
ClientSampleId :
0225-FIELD-BLANK-1


Tgt Ion: 82 Resp: 1489599
Ion Ratio Lower Upper
82 100
128 40.7 31.1 46.7
54 51.7 37.3 55.9

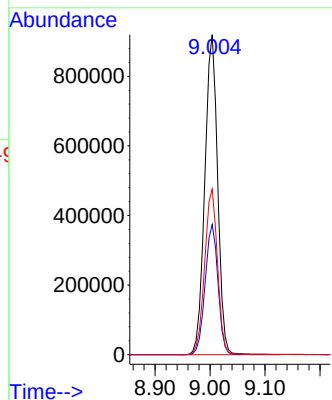

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.468 min Scan# 1935
Delta R.T. -0.006 min
Lab File: BM030357.D
Acq: 10 Jun 2021 00:19

Tgt Ion:164 Resp: 670962
Ion Ratio Lower Upper
164 100
162 103.1 83.4 125.0
160 46.3 37.2 55.8


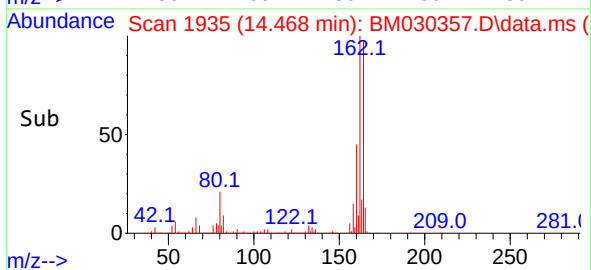
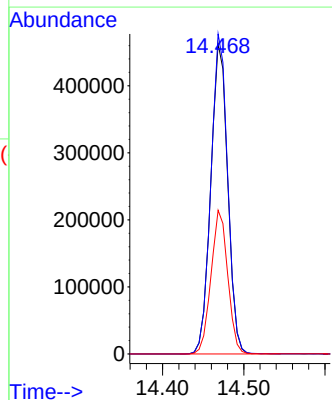





#42
2,4,6-Tribromophenol
Concen: 136.958 ng
RT: 15.956 min Scan# 2188
Delta R.T. -0.000 min
Lab File: BM030357.D
Acq: 10 Jun 2021 00:19




Instrument :
BNA_M
ClientSampleId :
0225-FIELD-BLANK-1


Tgt Ion:330 Resp: 1155357
Ion Ratio Lower Upper
330 100
332 96.1 77.0 115.4
141 37.4 30.2 45.2

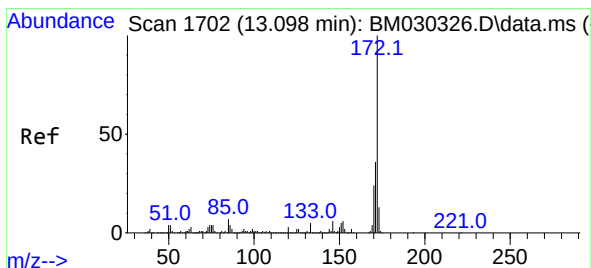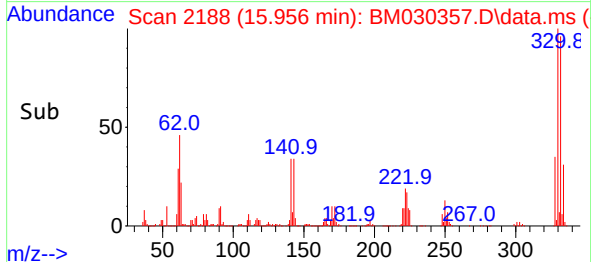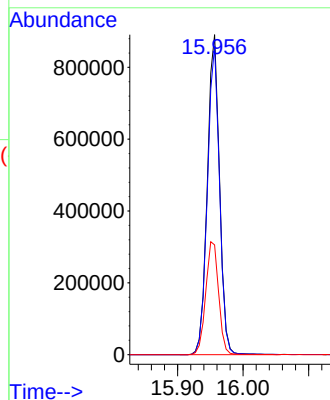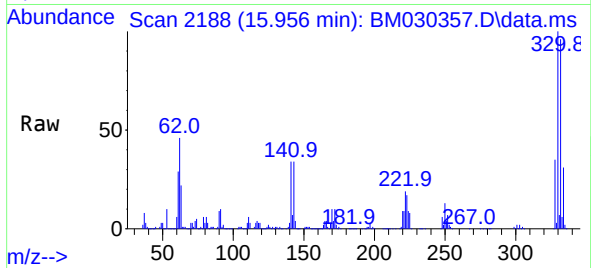

#45
2-Fluorobiphenyl
Concen: 77.026 ng
RT: 13.098 min Scan# 1702
Delta R.T. -0.000 min
Lab File: BM030357.D
Acq: 10 Jun 2021 00:19

Tgt Ion:172 Resp: 3929975
Ion Ratio Lower Upper
172 100
171 35.7 28.6 43.0
170 23.6 18.4 27.6


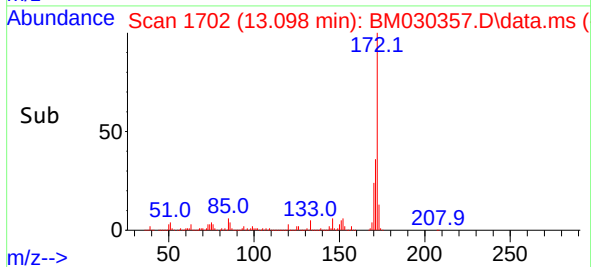
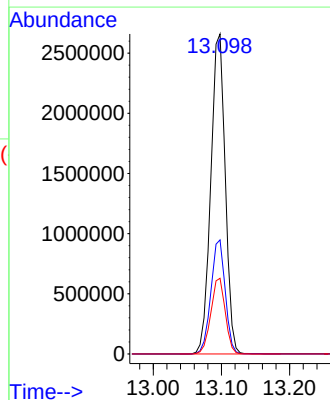
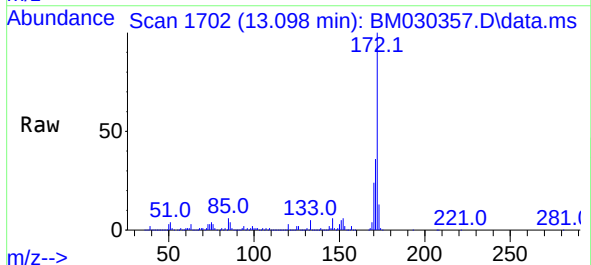




#50
Dimethylphthalate
Concen: 6.953 ng
RT: 13.921 min Scan# 1842
Delta R.T. -0.012 min
Lab File: BM030357.D
Acq: 10 Jun 2021 00:19




Instrument :
BNA_M
ClientSampleId :
0225-FIELD-BLANK-1


Tgt Ion:163 Resp: 371286
Ion Ratio Lower Upper
163 100
194 4.2 3.3 4.9
164 9.6 7.9 11.9

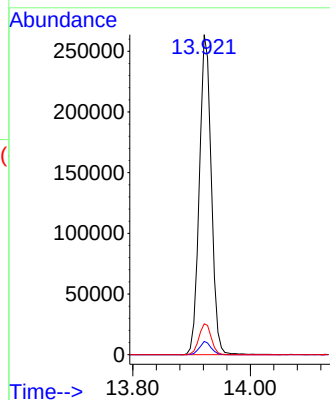

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.203 min Scan# 2400
Delta R.T. -0.006 min
Lab File: BM030357.D
Acq: 10 Jun 2021 00:19

Tgt Ion:188 Resp: 1519558
Ion Ratio Lower Upper
188 100
94 9.2 6.0 9.0#
80 9.8 6.6 9.8


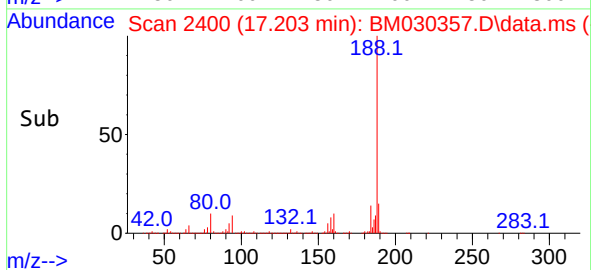
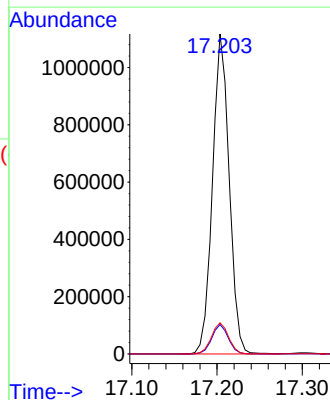





#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.362 min Scan# 3107
Delta R.T. -0.006 min
Lab File: BM030357.D
Acq: 10 Jun 2021 00:19




Instrument :
BNA_M
ClientSampleId :
0225-FIELD-BLANK-1


Tgt Ion:240 Resp: 1571475
Ion Ratio Lower Upper
240 100
120 10.7 7.0 10.6#
236 26.0 21.0 31.4

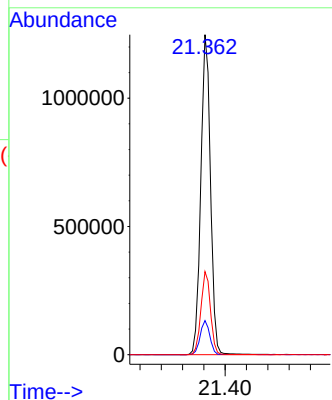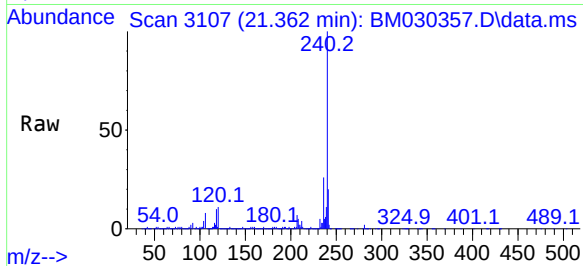

#79
Terphenyl-d14
Concen: 87.090 ng
RT: 19.821 min Scan# 2845
Delta R.T. -0.000 min
Lab File: BM030357.D
Acq: 10 Jun 2021 00:19

Tgt Ion:244 Resp: 7791910
Ion Ratio Lower Upper
244 100
212 8.5 6.3 9.5
122 11.3 6.9 10.3#


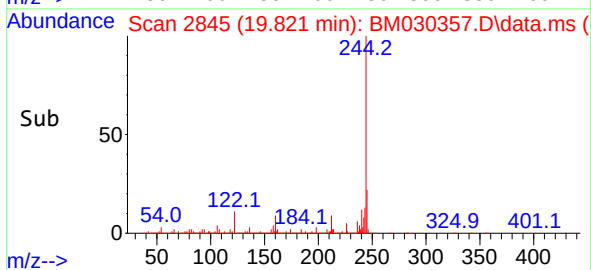
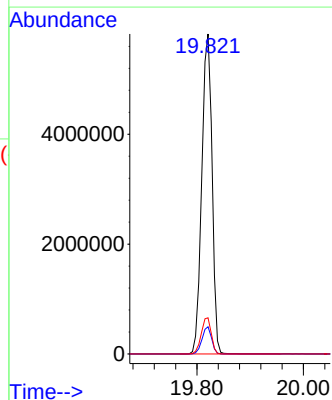
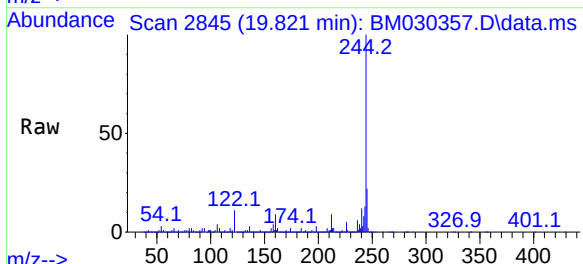




#84
Bis(2-ethylhexyl)phthalate
Concen: 4.392 ng
RT: 21.274 min Scan# 3092
Delta R.T. -0.006 min
Lab File: BM030357.D
Acq: 10 Jun 2021 00:19

Instrument :
BNA_M
ClientSampleId :
0225-FIELD-BLANK-1

Tgt Ion:	149	Resp:	9549
Ion	Ratio	Lower	Upper
149	100		
167	22.7	22.6	33.8
279	3.9	3.8	5.8

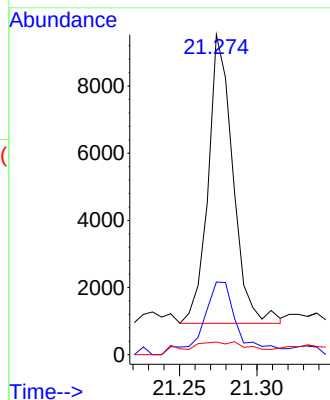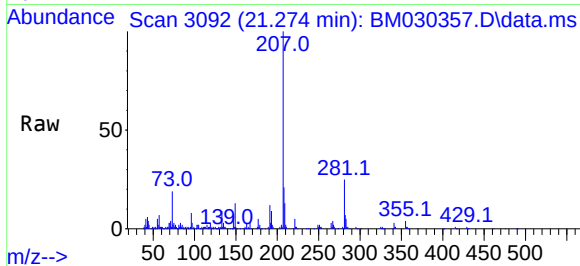

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.644 min Scan# 3495
Delta R.T. -0.006 min
Lab File: BM030357.D
Acq: 10 Jun 2021 00:19

Tgt Ion:	264	Resp:	1402365
Ion	Ratio	Lower	Upper
264	100		
260	23.6	19.8	29.8
265	21.8	17.7	26.5

