

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
 Data File : BM030331.D
 Acq On : 08 Jun 2021 20:39
 Operator : CG/JU
 Sample : PB136847BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB136847BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM030331.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	391	398	412	rBV	4483537	6551214	41.20%	10.180%
2	7.010	659	667	683	rBV	4390898	6841187	43.02%	10.631%
3	7.851	801	810	817	rBV	778209	1215975	7.65%	1.890%
4	9.004	994	1006	1022	rBV	2552187	4138669	26.03%	6.431%
5	10.639	1276	1284	1294	rBV	997563	1662367	10.45%	2.583%
6	13.098	1695	1702	1716	rBV	7078184	10097370	63.50%	15.690%
7	14.474	1928	1936	1943	rBV	1521550	2266269	14.25%	3.522%
8	15.957	2181	2188	2200	rBV	5459204	7489895	47.10%	11.639%
9	17.210	2393	2401	2411	rBV	1904696	2708432	17.03%	4.209%
10	19.821	2839	2845	2850	rBV	13098723	15901980	100.00%	24.710%
11	21.368	3102	3108	3113	rBV	2224171	2845380	17.89%	4.421%
12	23.644	3489	3495	3508	rVB2	1394918	2635578	16.57%	4.095%




Sum of corrected areas: 64354316

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030331.D
Acq On : 08 Jun 2021 20:39
Operator : CG/JU
Sample : PB136847BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136847BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

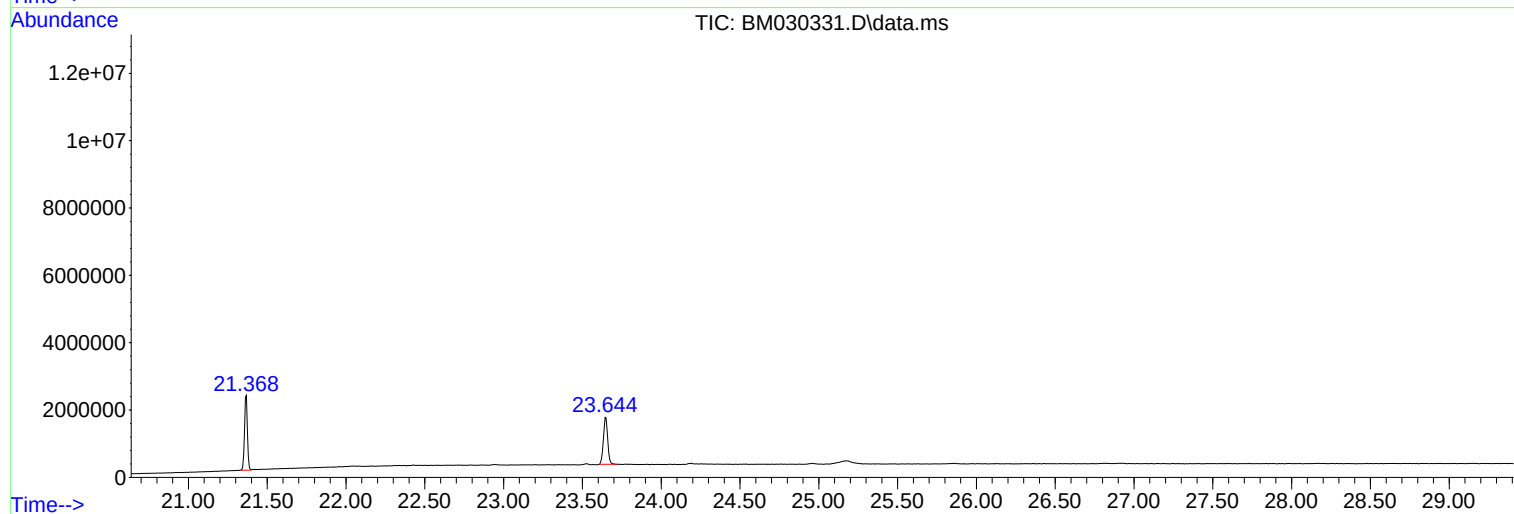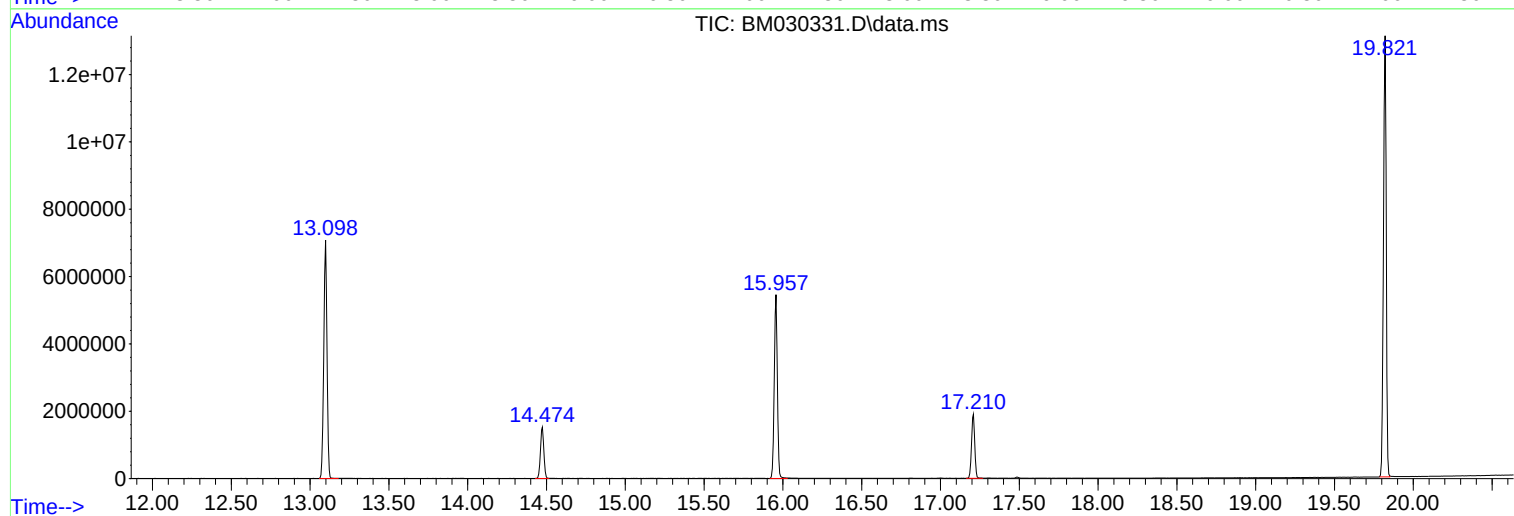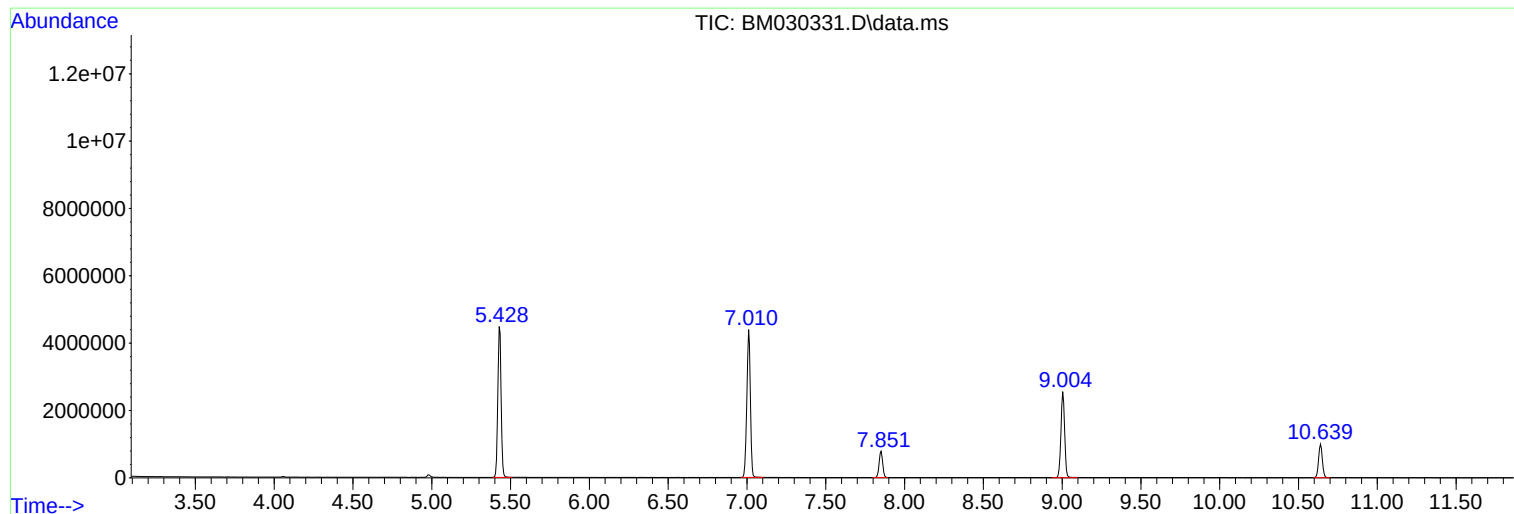

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030331.D
Acq On : 08 Jun 2021 20:39
Operator : CG/JU
Sample : PB136847BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136847BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030331.D
Acq On : 08 Jun 2021 20:39
Operator : CG/JU
Sample : PB136847BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136847BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------