

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
 Data File : BM030342.D
 Acq On : 09 Jun 2021 14:53
 Operator : CG/JU
 Sample : M2613-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 18-B12(118-122)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM030342.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	391	398	409	rBV	3714637	5600246	31.53%	8.433%
2	7.010	659	667	687	rBV	3960240	6285062	35.39%	9.464%
3	7.851	802	810	817	rBV	641794	1038403	5.85%	1.564%
4	9.004	998	1006	1017	rBV	2295705	3770345	21.23%	5.677%
5	10.639	1276	1284	1292	rBV	903046	1533967	8.64%	2.310%
6	13.098	1694	1702	1712	rBV	6552262	9255721	52.12%	13.937%
7	14.474	1929	1936	1944	rVB	1458660	2215250	12.47%	3.336%
8	15.957	2181	2188	2206	rBV	5628086	7733866	43.55%	11.646%
9	17.204	2393	2400	2413	rBV	1999325	2946755	16.59%	4.437%
10	18.092	2545	2551	2561	rBV	146031	239190	1.35%	0.360%
11	19.250	2744	2748	2762	rVB2	112235	260505	1.47%	0.392%
12	19.821	2839	2845	2853	rBV	15345813	17759559	100.00%	26.743%
13	21.086	3056	3060	3069	rBV2	97495	201768	1.14%	0.304%
14	21.368	3103	3108	3116	rBV	2996616	3833951	21.59%	5.773%
15	23.650	3490	3496	3509	rVB2	1869317	3734473	21.03%	5.623%


Sum of corrected areas: 66409061

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030342.D
Acq On : 09 Jun 2021 14:53
Operator : CG/JU
Sample : M2613-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
18-B12(118-122)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

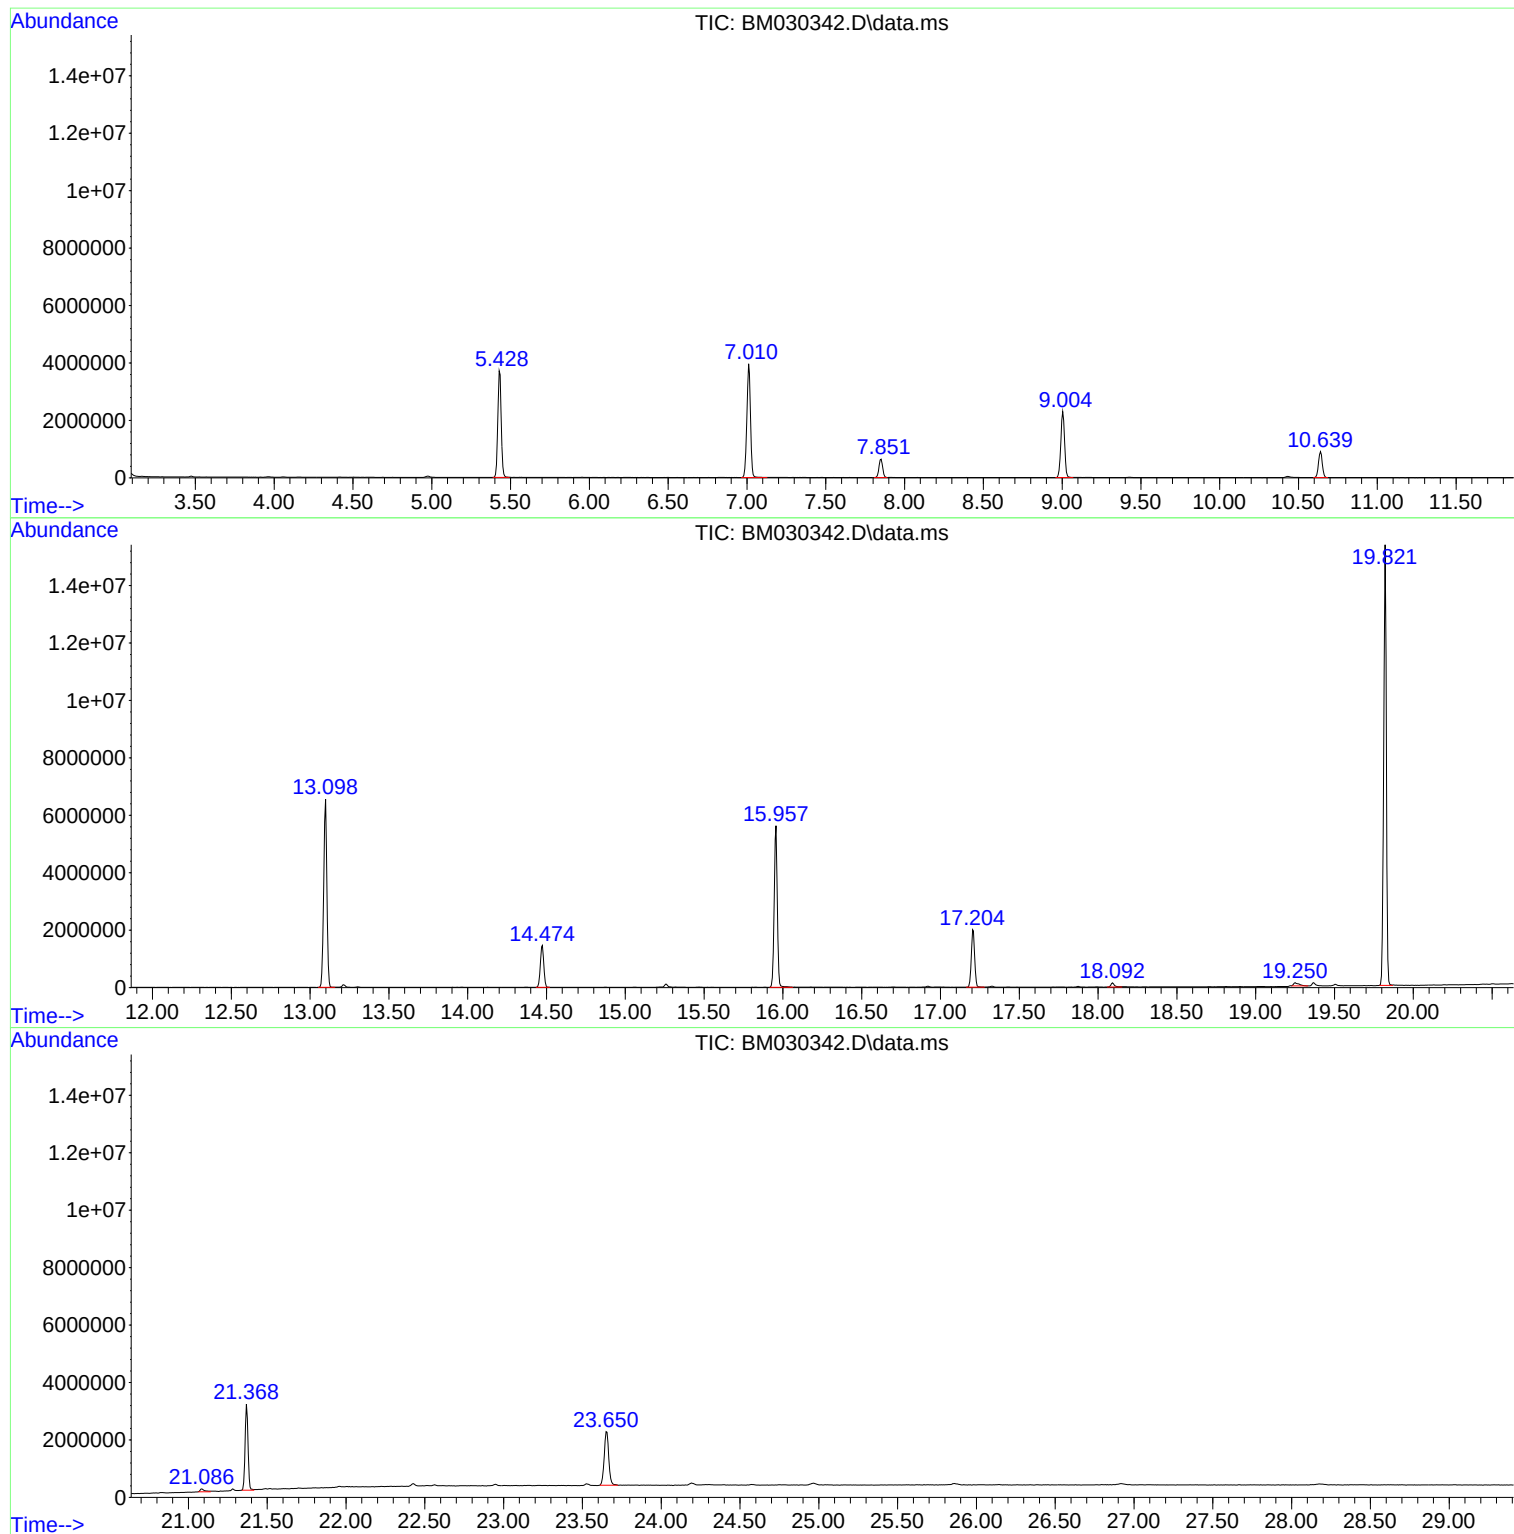

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030342.D
Acq On : 09 Jun 2021 14:53
Operator : CG/JU
Sample : M2613-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
18-B12(118-122)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030342.D
Acq On : 09 Jun 2021 14:53
Operator : CG/JU
Sample : M2613-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
18-B12(118-122)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
