

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
 Data File : BM030347.D
 Acq On : 09 Jun 2021 18:03
 Operator : CG/JU
 Sample : PB136946BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB136946BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM030347.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.434	391	399	413	rBV	4271331	6380162	35.50%	9.557%
2	7.010	657	667	682	rBV	4227693	6678958	37.16%	10.004%
3	7.851	802	810	820	rBV	685785	1106785	6.16%	1.658%
4	9.004	997	1006	1021	rBV	2450290	3958763	22.02%	5.930%
5	10.639	1276	1284	1296	rBV	902268	1540102	8.57%	2.307%
6	13.098	1694	1702	1715	rBV	6496909	9632879	53.59%	14.429%
7	14.468	1928	1935	1944	rBV	1394945	2135157	11.88%	3.198%
8	15.957	2180	2188	2200	rBV	5541412	7660679	42.62%	11.475%
9	17.204	2393	2400	2414	rBV	1837992	2716710	15.11%	4.069%
10	19.821	2839	2845	2854	rBV	14983571	17974744	100.00%	26.924%
11	21.368	3103	3108	3117	rBV	2708965	3382161	18.82%	5.066%
12	23.650	3489	3496	3506	rBV2	1901835	3593419	19.99%	5.383%




Sum of corrected areas: 66760519

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030347.D
Acq On : 09 Jun 2021 18:03
Operator : CG/JU
Sample : PB136946BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136946BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

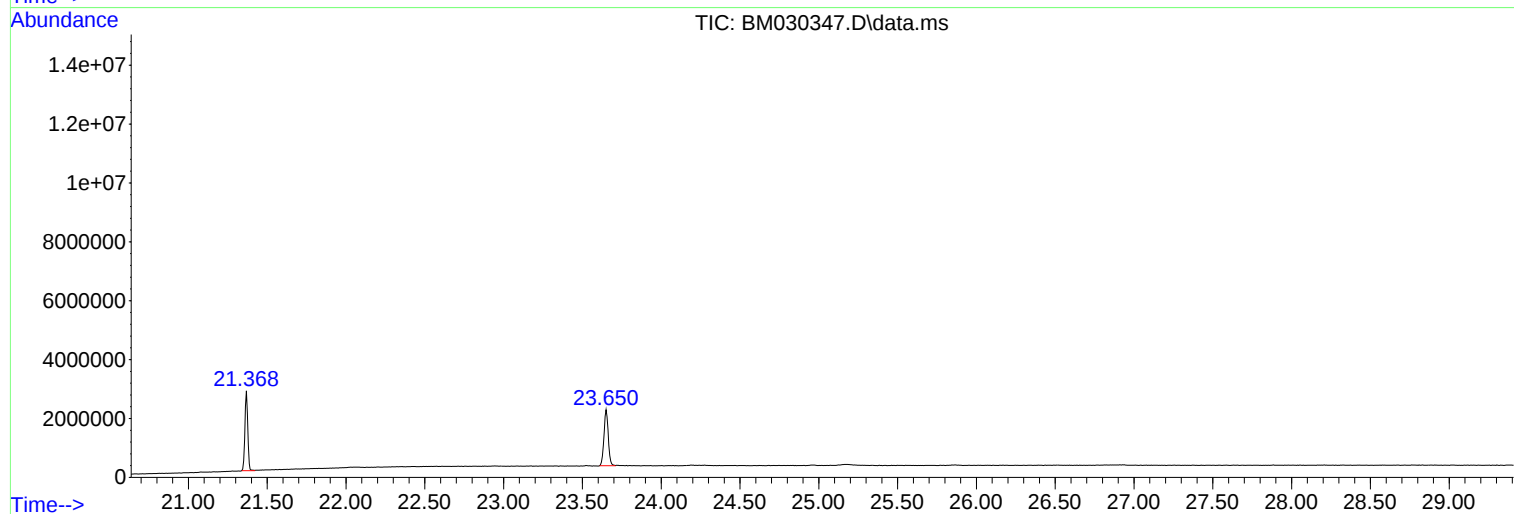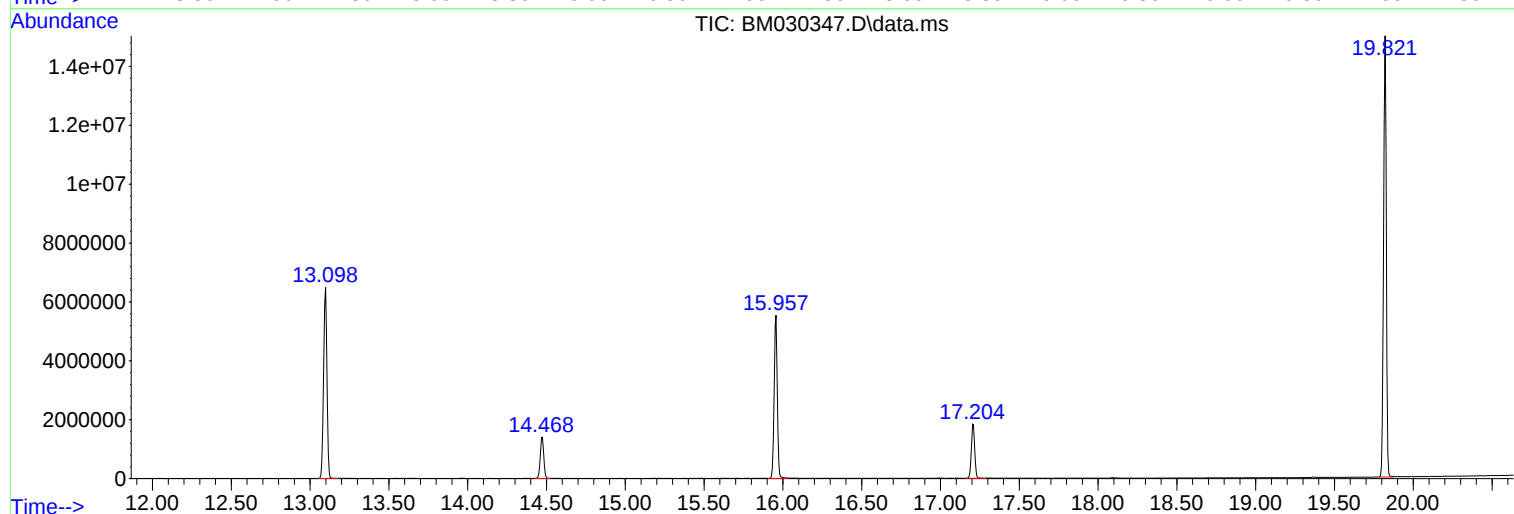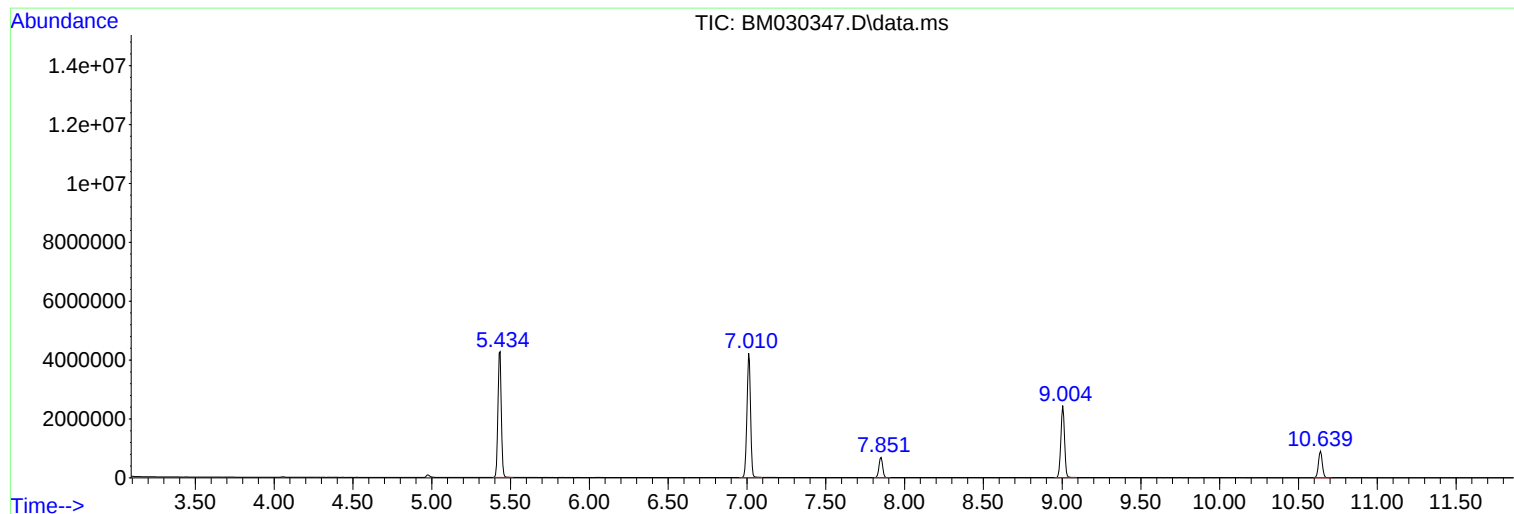

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030347.D
Acq On : 09 Jun 2021 18:03
Operator : CG/JU
Sample : PB136946BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136946BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030347.D
Acq On : 09 Jun 2021 18:03
Operator : CG/JU
Sample : PB136946BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136946BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------