
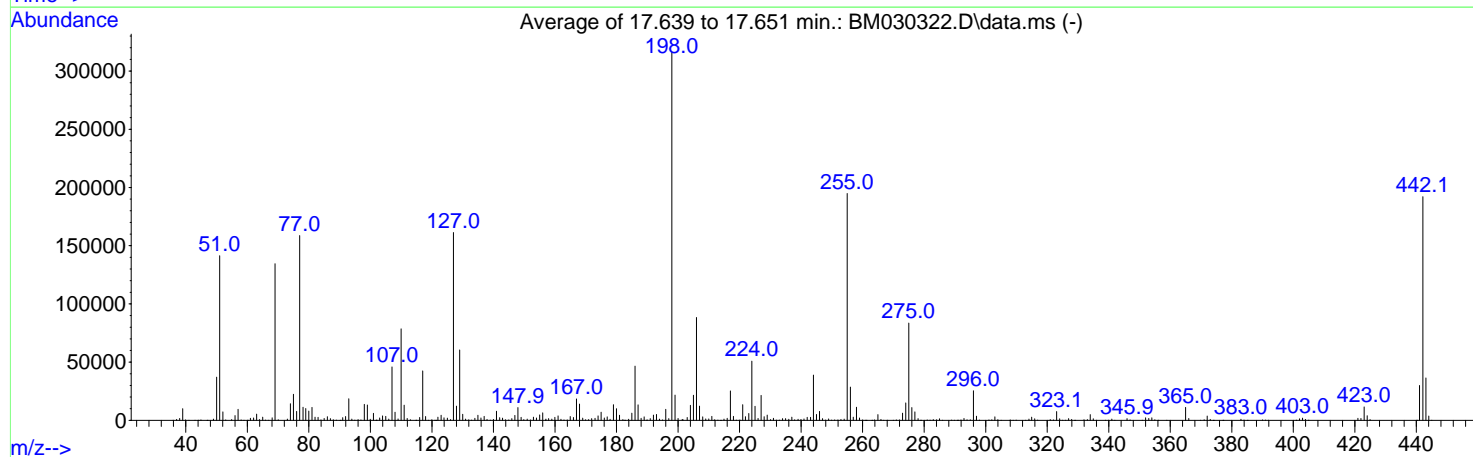


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
 Data File : BM030322.D
 Acq On : 08 Jun 2021 14:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 08 20:51:08 2021

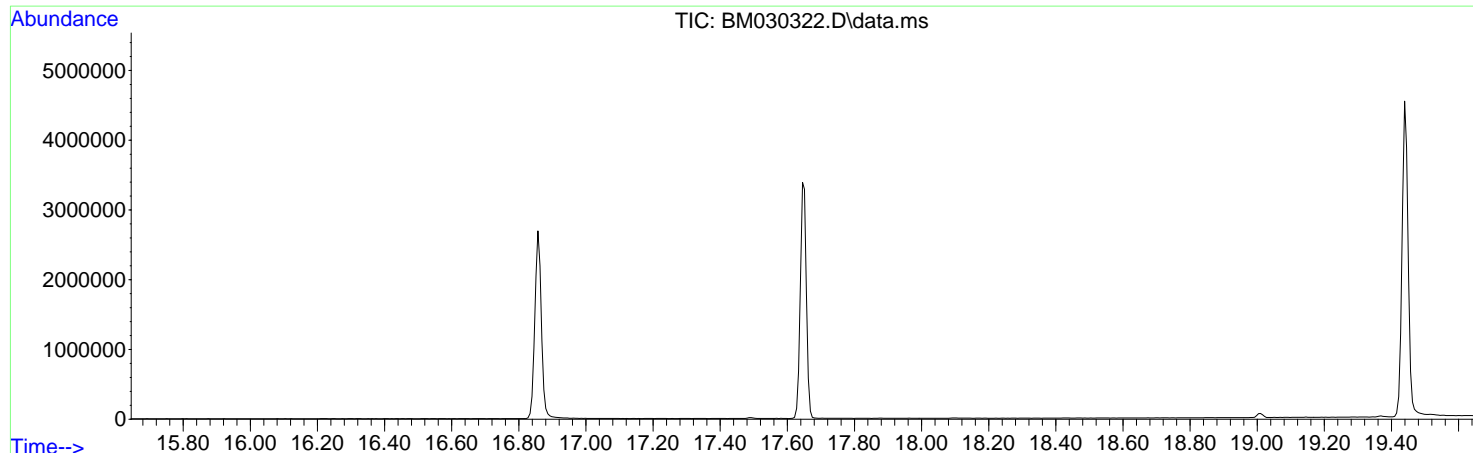




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	141447	PASS
68	69	0.00	2	1.6	2164	PASS
69	198	0.00	100	42.6	134595	PASS
70	69	0.00	2	0.4	574	PASS
127	198	10	80	51.1	161312	PASS
197	198	0.00	2	0.5	1484	PASS
198	198	100	100	100.0	315925	PASS
199	198	5	9	6.9	21711	PASS
275	198	10	60	26.4	83493	PASS
365	198	1	100	3.5	11126	PASS
441	198	0.01	100	9.5	30007	PASS
442	442	50	100	100.0	192104	PASS
443	442	15	24	19.0	36413	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
 Data File : BM030322.D
 Acq On : 08 Jun 2021 14:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampled :
 DFTPP

Quant Time: Jun 08 18:14:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 08 17:34:01 2021
 Response via : Initial Calibration

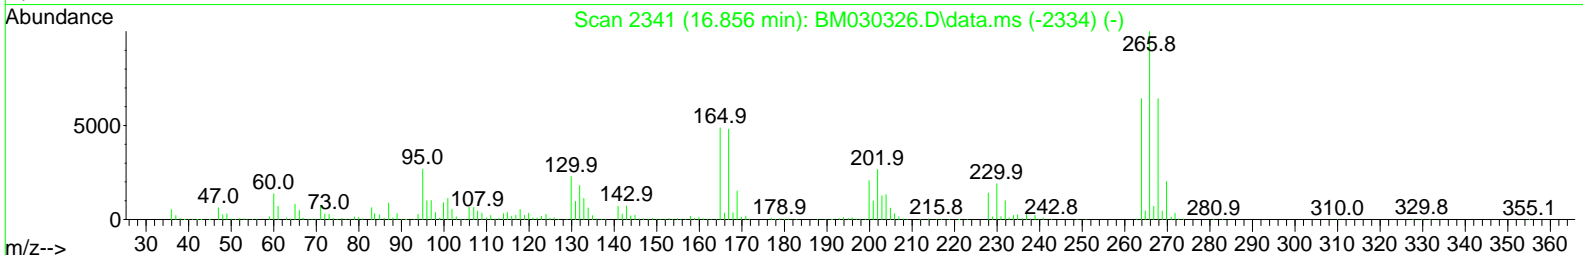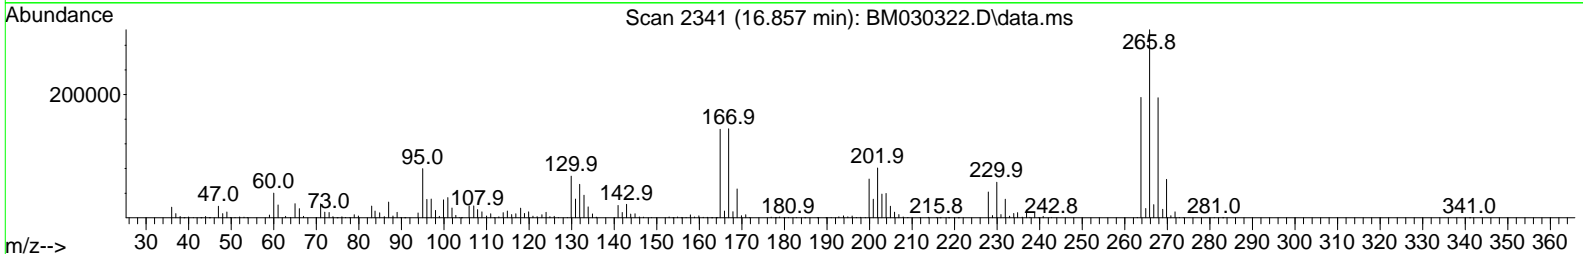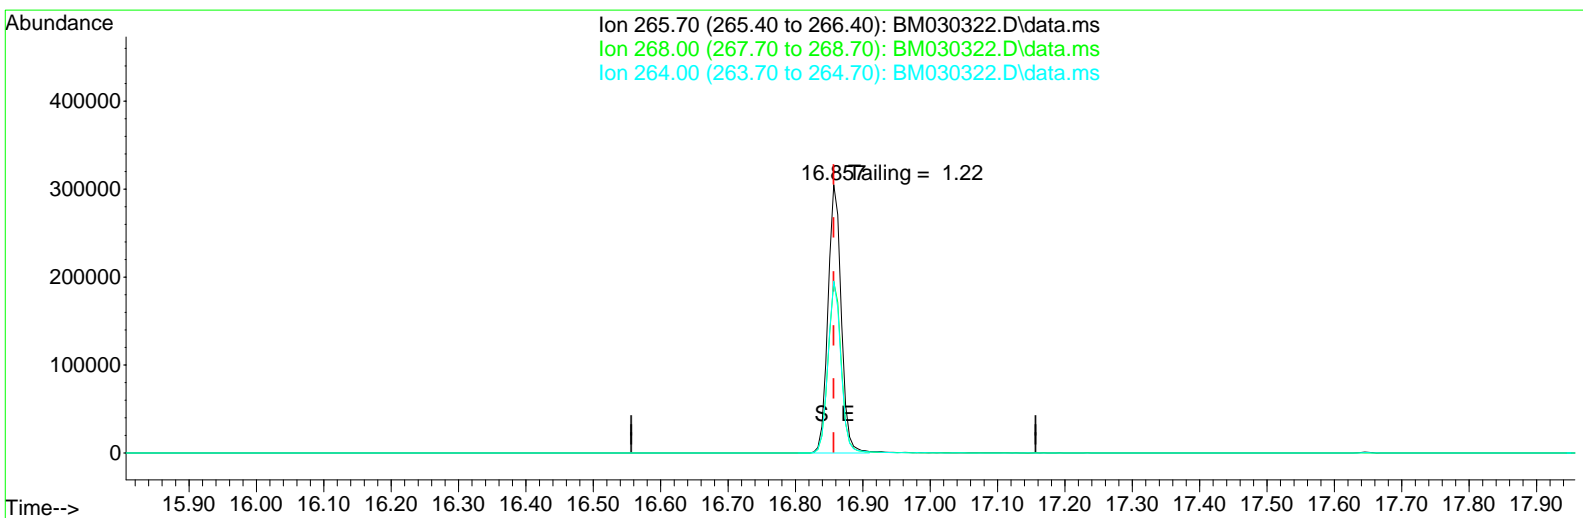

TIC: BM030322.D\data.ms

(70) Pentachlorophenol (C)

16.857min (+ 0.000) 286454.94 ng




response 417476

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	63.88
264.00	64.90	64.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
 Data File : BM030322.D
 Acq On : 08 Jun 2021 14:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 08 18:14:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 08 17:34:01 2021
 Response via : Initial Calibration

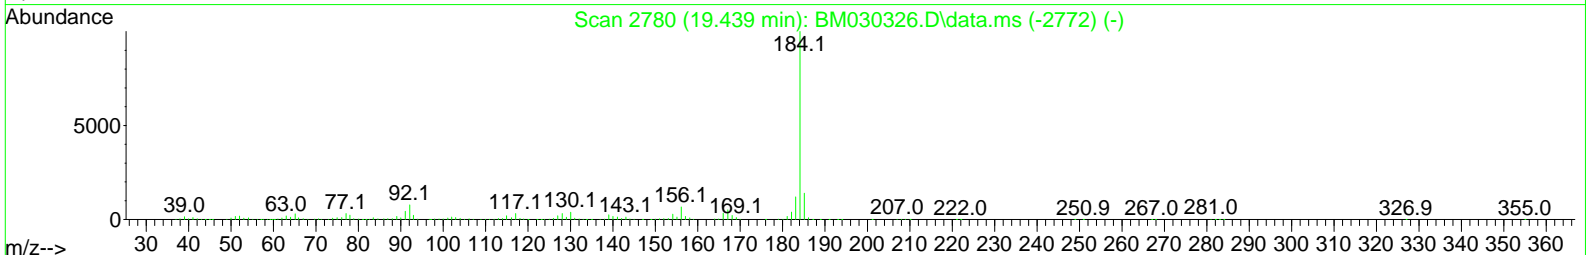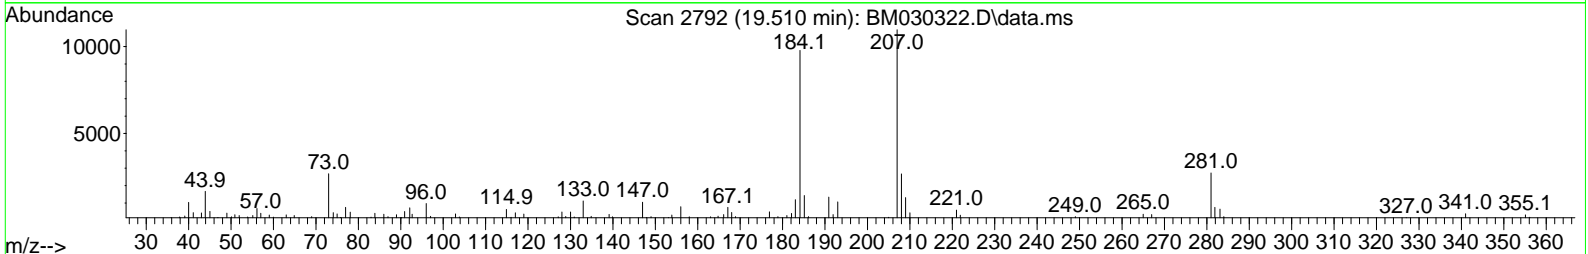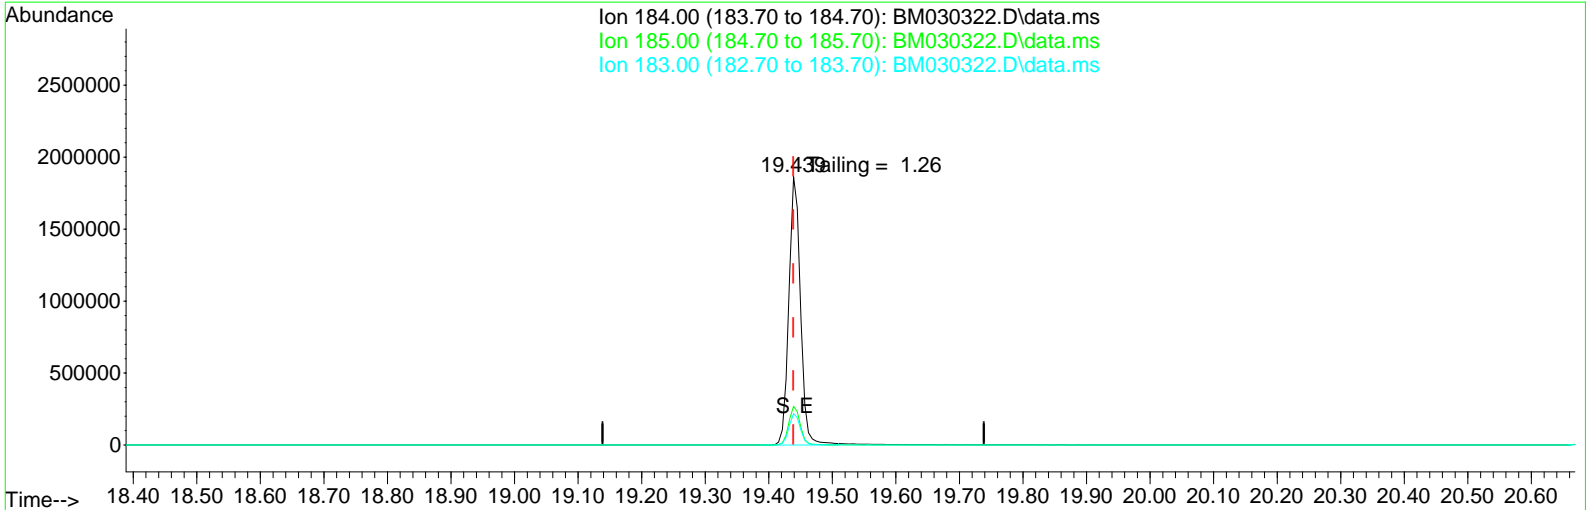

TIC: BM030322.D\data.ms

(77) Benzidine

19.439min (+ 0.000) 358485.93 ng

response 2413633

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.46
183.00	12.30	11.69
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_M
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
6/9/2021	BNA_M	<u>BM030322.D</u>
Compound Name	Response	Retention Time
DDT	1237992	20.67
DDD	5702	20.23
DDE	1121	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6823	1244815	0.55