
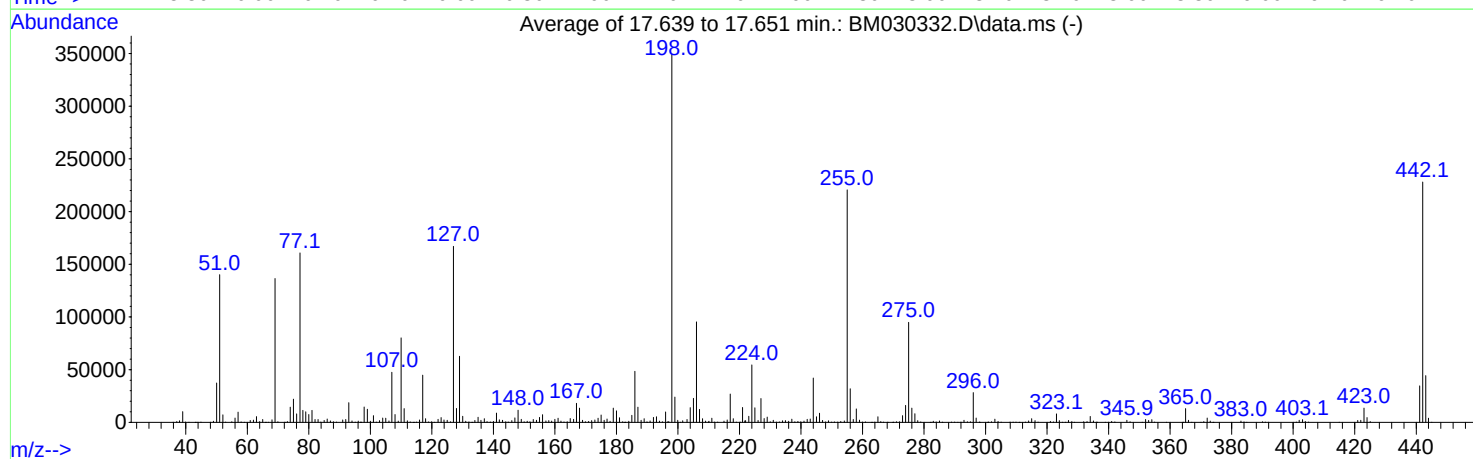


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
 Data File : BM030332.D
 Acq On : 09 Jun 2021 08:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 08 20:51:08 2021

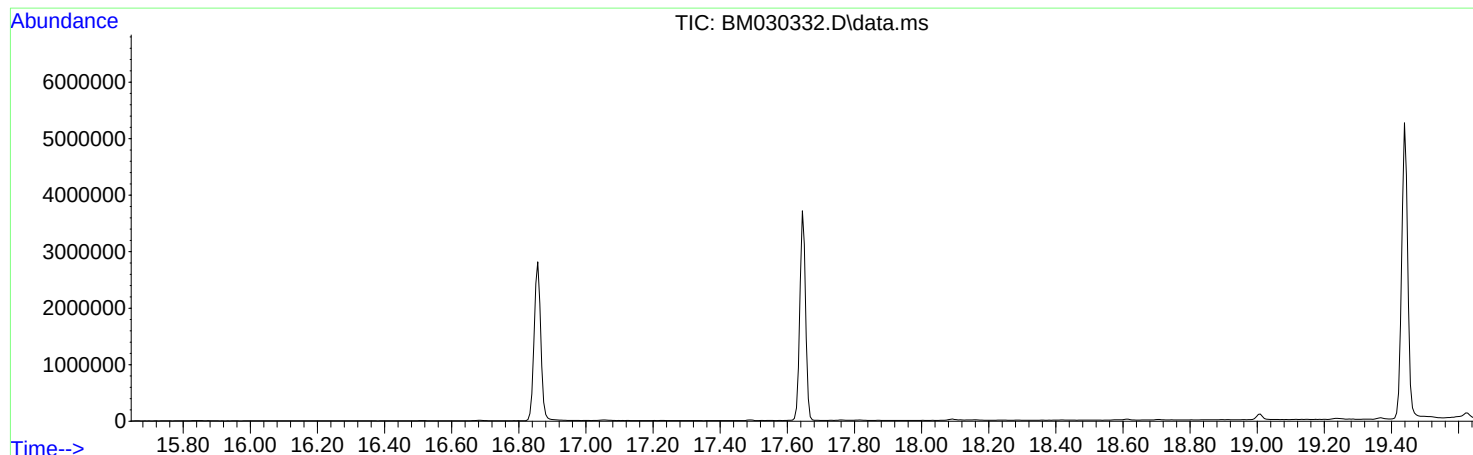




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	140164	PASS
68	69	0.00	2	1.7	2375	PASS
69	198	0.00	100	39.1	136512	PASS
70	69	0.00	2	0.5	624	PASS
127	198	10	80	47.9	167019	PASS
197	198	0.00	2	0.2	765	PASS
198	198	100	100	100.0	349035	PASS
199	198	5	9	6.9	24043	PASS
275	198	10	60	27.2	94896	PASS
365	198	1	100	3.8	13112	PASS
441	198	0.01	100	9.9	34664	PASS
442	442	50	100	100.0	228019	PASS
443	442	15	24	19.5	44405	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
 Data File : BM030332.D
 Acq On : 09 Jun 2021 08:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 09 14:11:04 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 08 20:51:08 2021
 Response via : Initial Calibration

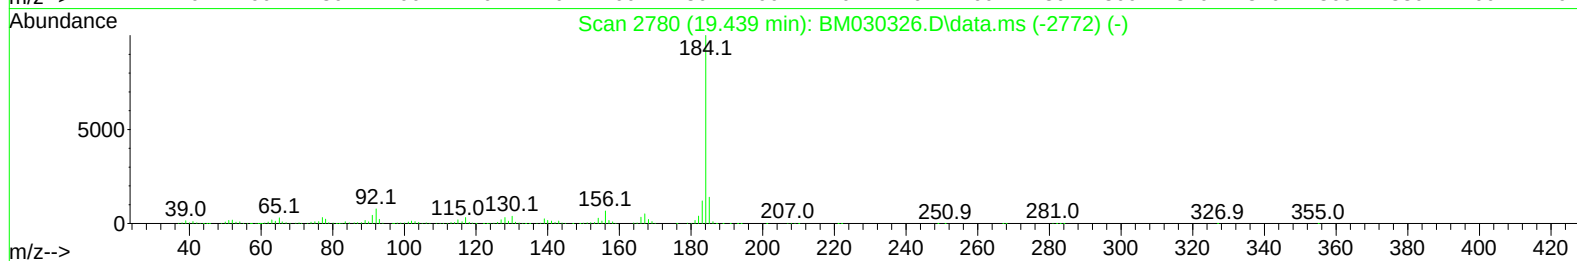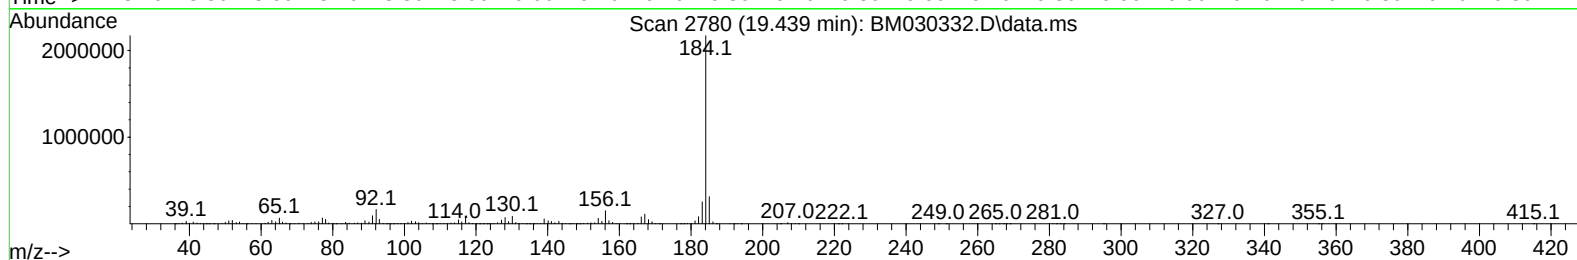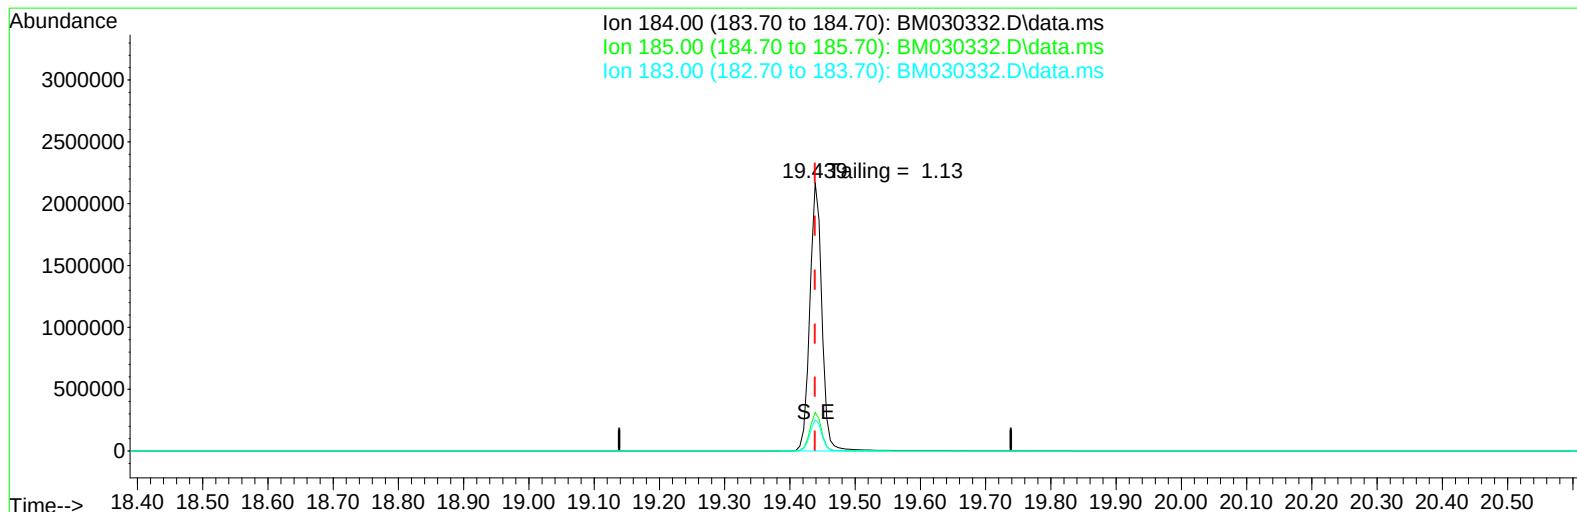

TIC: BM030332.D\data.ms

(77) Benzidine

19.439min (+ 0.000) 11454.42 ng




response 2798455

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.40
183.00	12.30	11.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060921\
Data File : BM030332.D
Acq On : 09 Jun 2021 08:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 09 14:11:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 08 20:51:08 2021
Response via : Initial Calibration

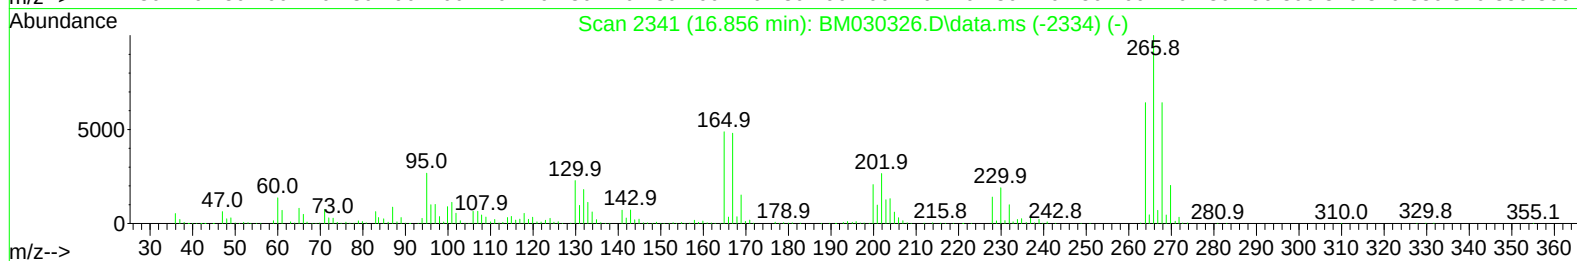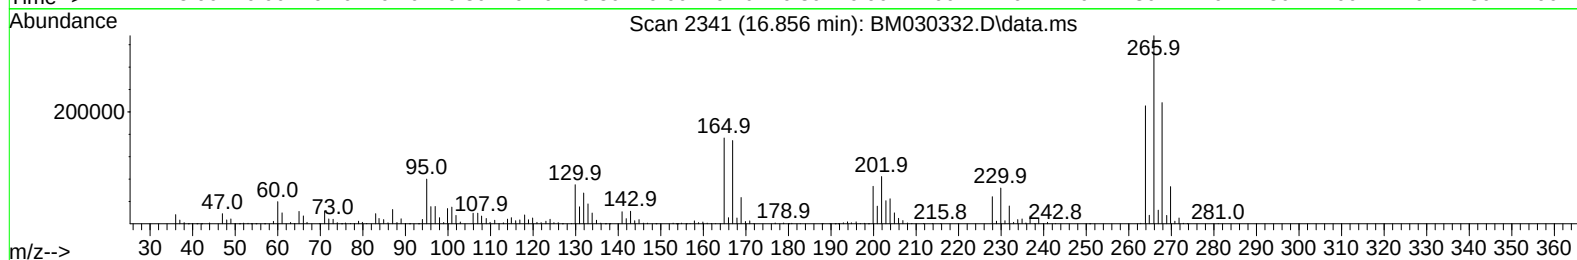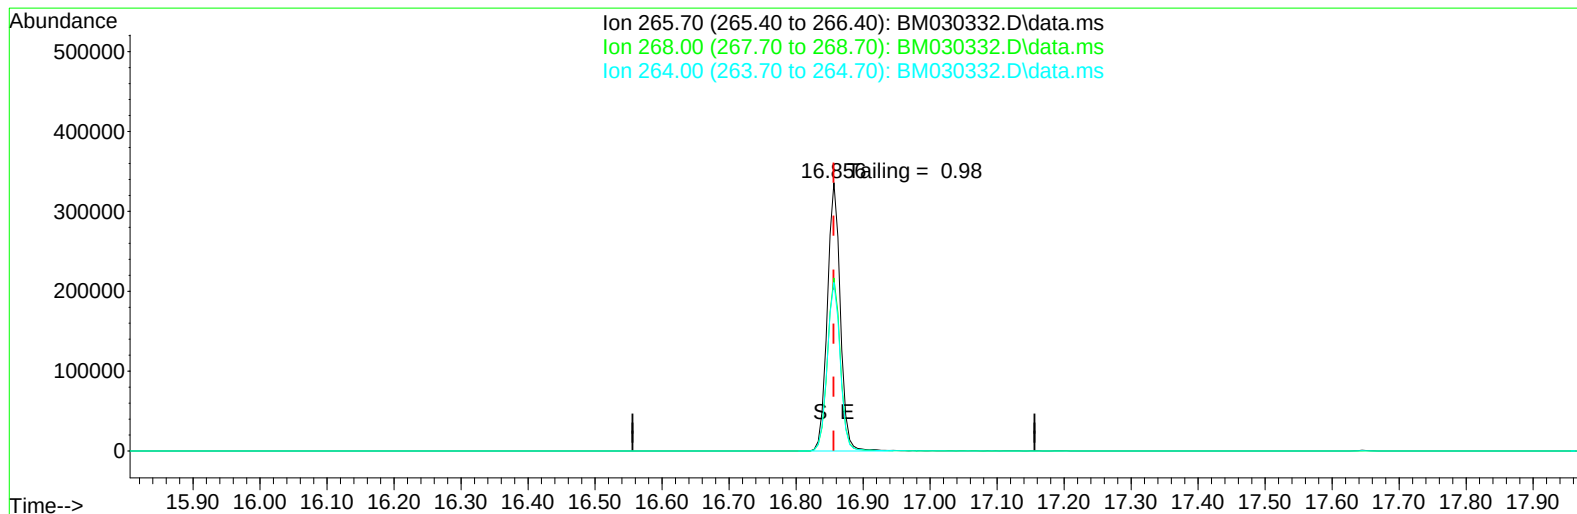

TIC: BM030332.D\data.ms

(70) Pentachlorophenol (C)

16.856min (+ 0.000) 95335.07 ng

response 454185

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	64.48
264.00	64.90	62.76
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_M
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
6/9/2021	BNA_M	<u>BM030332.D</u>
Compound Name	Response	Retention Time
DDT	1525884	20.66
DDD	10062	20.23
DDE	1993	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12055	1537939	0.78