
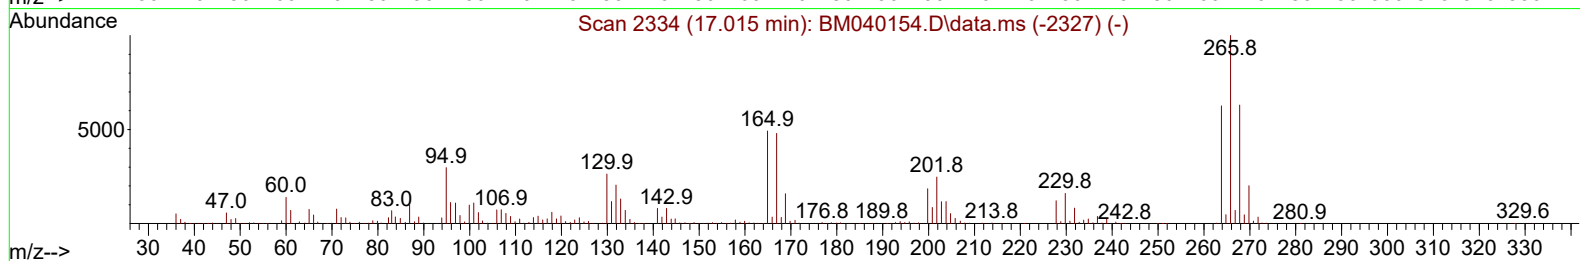
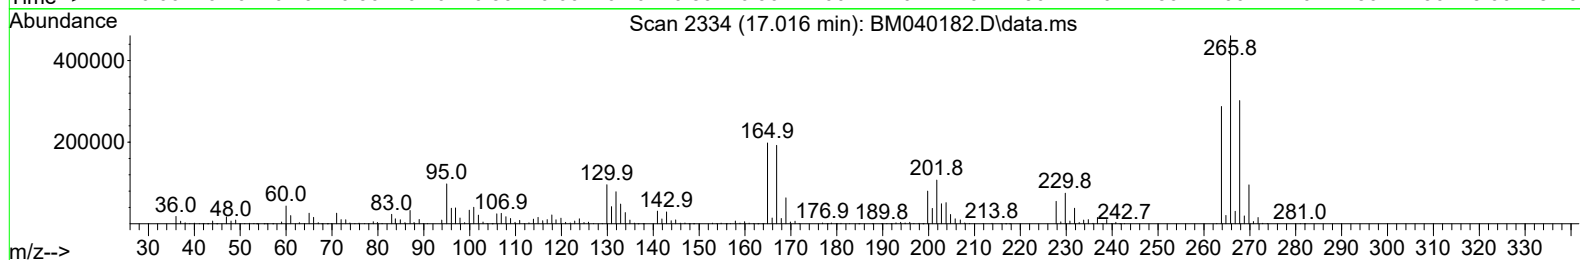


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
 Data File : BM040182.D
 Acq On : 09 Jun 2023 08:49
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 09:20:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 08 23:25:50 2023
 Response via : Initial Calibration

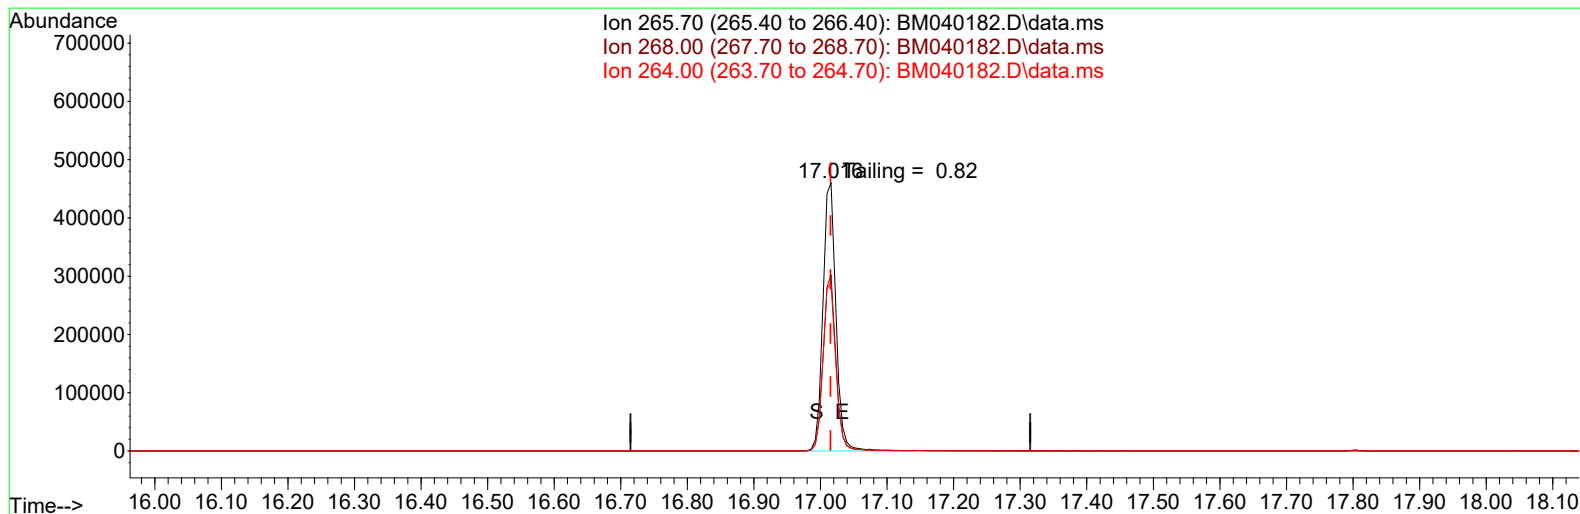

TIC: BM040182.D\data.ms

(70) Pentachlorophenol (C)




17.016min (+ 0.001) 1400717.30 ng

response 627720

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	65.57
264.00	62.60	62.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040182.D
Acq On : 09 Jun 2023 08:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 09:20:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 23:25:50 2023
Response via : Initial Calibration

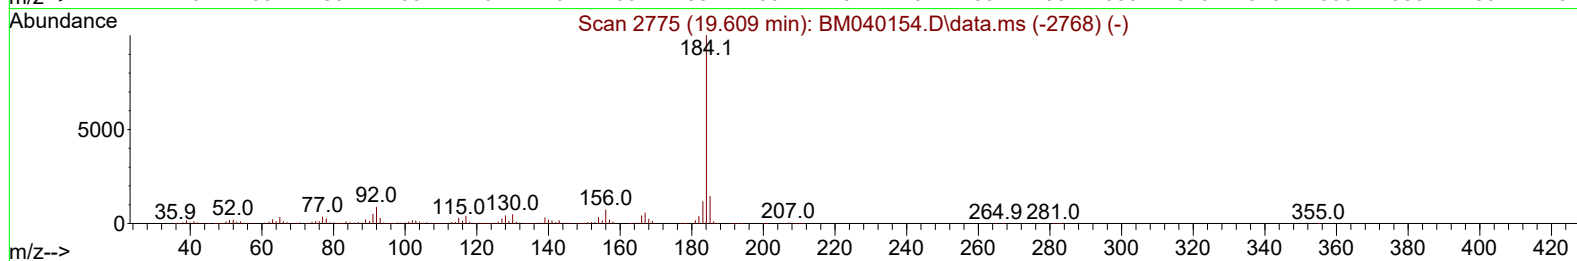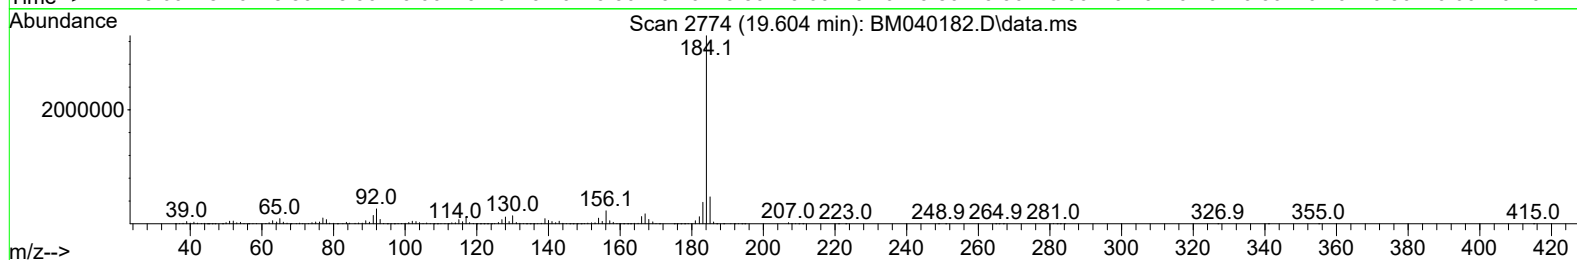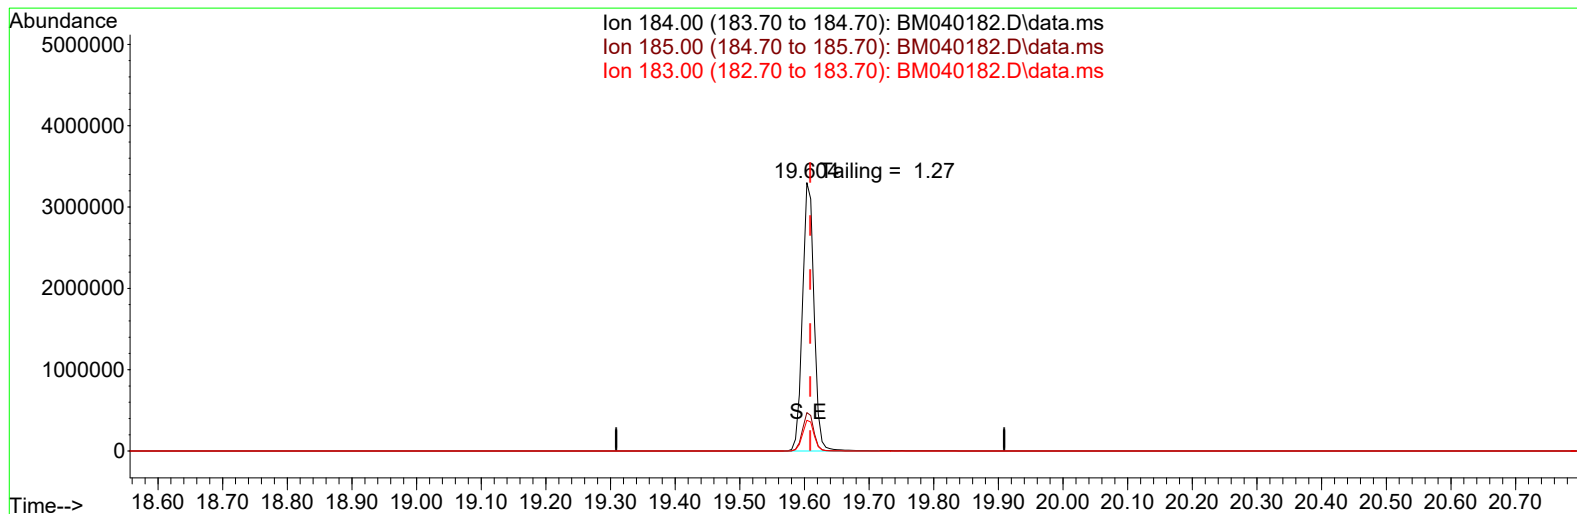

TIC: BM040182.D\data.ms

(77) Benzidine

19.604min (-0.005) 256714.86 ng

response 4112485

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.34
183.00	11.70	11.44
0.00	0.00	0.00