

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
 Data File : BM040184.D
 Acq On : 09 Jun 2023 10:37
 Operator : MA/JU
 Sample : PB153141BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB153141BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040184.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.540	376	383	399	rBV	8279614	11666203	42.72%	10.377%
2	7.145	647	656	671	rBV	7453387	11861319	43.43%	10.551%
3	7.987	792	799	808	rVB	1441577	2186901	8.01%	1.945%
4	9.157	988	998	1008	rBV	4435309	7058458	25.85%	6.279%
5	10.798	1269	1277	1287	rBV	1852415	3079607	11.28%	2.739%
6	13.251	1687	1694	1707	rBV	12516407	17923010	65.63%	15.943%
7	14.621	1920	1927	1941	rBV	2738046	3999910	14.65%	3.558%
8	16.110	2173	2180	2196	rBV	10163473	13685501	50.11%	12.173%
9	17.368	2387	2394	2407	rBV	3361733	4659133	17.06%	4.144%
10	19.986	2833	2839	2844	rBV	23223485	27308880	100.00%	24.291%
11	21.544	3099	3104	3111	rBV	3702847	4530923	16.59%	4.030%
12	23.980	3511	3518	3531	rVB	2312793	4462322	16.34%	3.969%




Sum of corrected areas: 112422167

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040184.D
Acq On : 09 Jun 2023 10:37
Operator : MA/JU
Sample : PB153141BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153141BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

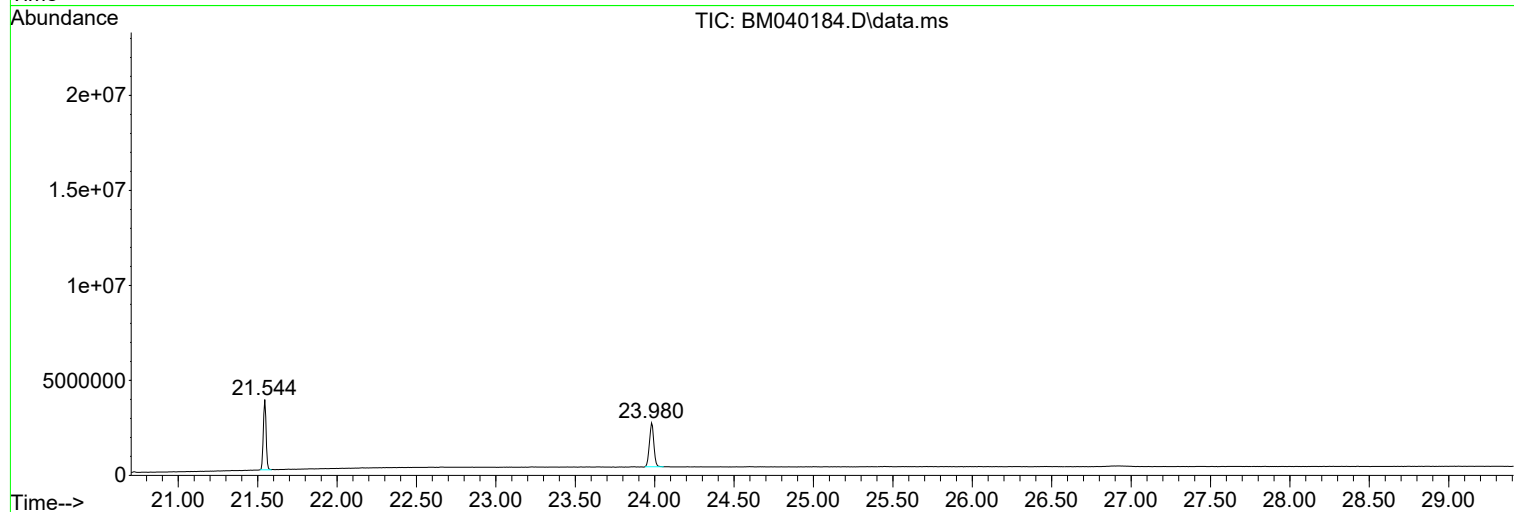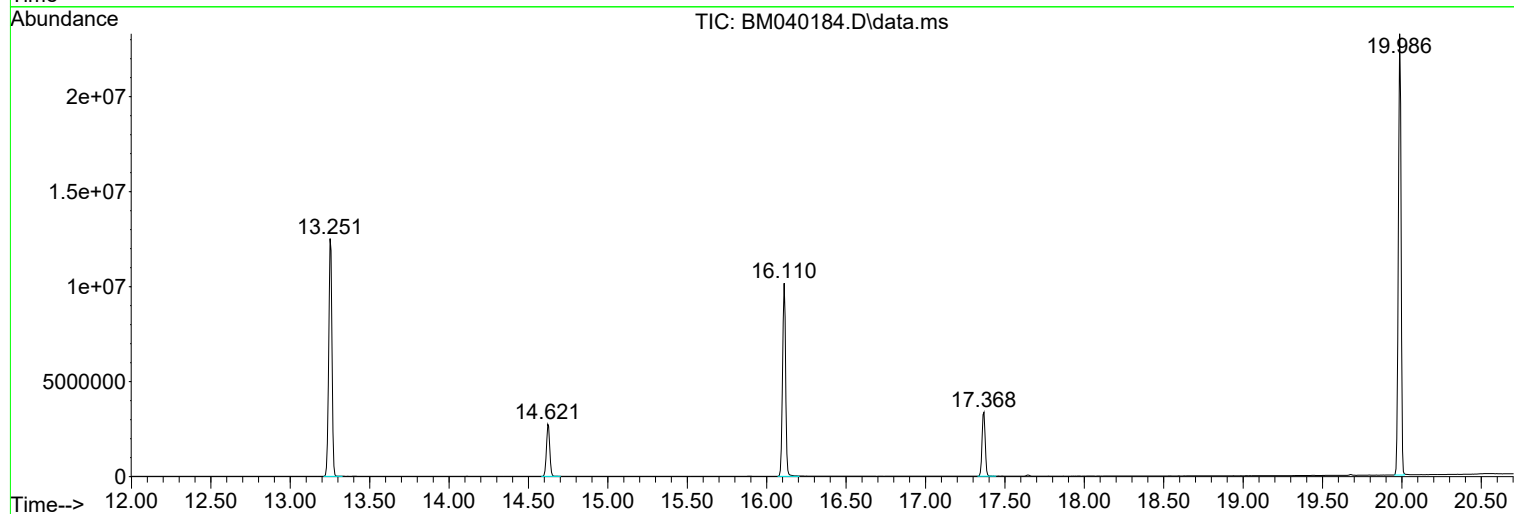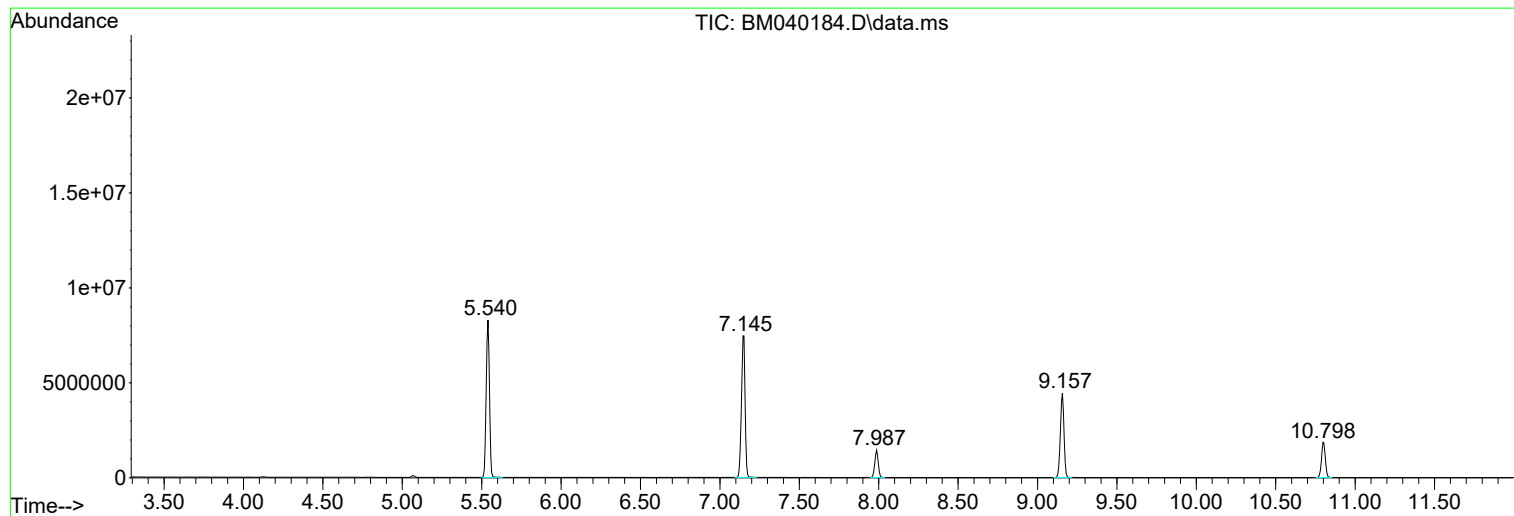

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040184.D
Acq On : 09 Jun 2023 10:37
Operator : MA/JU
Sample : PB153141BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153141BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040184.D
Acq On : 09 Jun 2023 10:37
Operator : MA/JU
Sample : PB153141BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153141BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------