

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
 Data File : BM040201.D
 Acq On : 09 Jun 2023 22:48
 Operator : MA/JU
 Sample : PB153297BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB153297BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.540	376	383	399	rBV	8285374	12004195	35.20%	9.501%
2	7.151	648	657	666	rBV	7713170	12458895	36.53%	9.861%
3	7.987	790	799	806	rBV	1215859	1871001	5.49%	1.481%
4	9.157	986	998	1009	rBV	4700879	7520813	22.05%	5.953%
5	10.798	1268	1277	1288	rBV	1711805	2768013	8.12%	2.191%
6	13.251	1687	1694	1708	rBV	13839433	19826890	58.14%	15.693%
7	14.622	1920	1927	1944	rBV	2642125	3902225	11.44%	3.089%
8	16.110	2173	2180	2198	rBV	12525559	17127733	50.22%	13.556%
9	17.368	2387	2394	2406	rBV	3441634	4883347	14.32%	3.865%
10	19.986	2833	2839	2844	rBV	26729795	34103128	100.00%	26.992%
11	21.545	3098	3104	3114	rBV	4114354	5237765	15.36%	4.146%
12	23.980	3511	3518	3528	rVB	2302454	4639328	13.60%	3.672%




Sum of corrected areas: 126343333

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040201.D
Acq On : 09 Jun 2023 22:48
Operator : MA/JU
Sample : PB153297BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153297BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

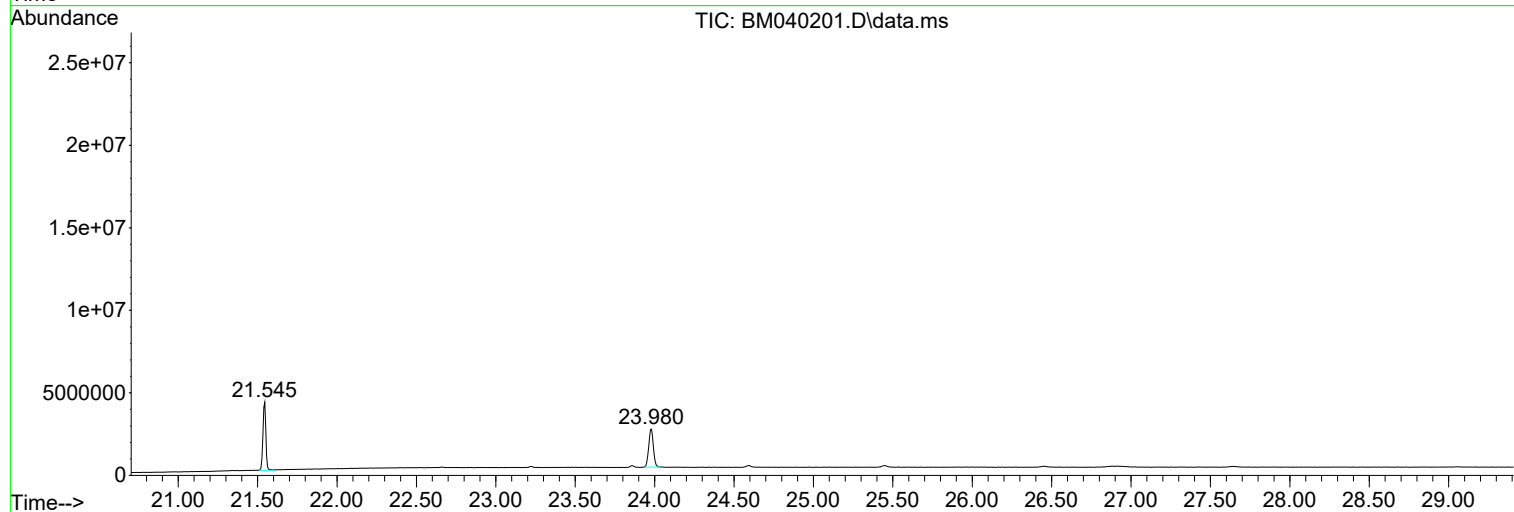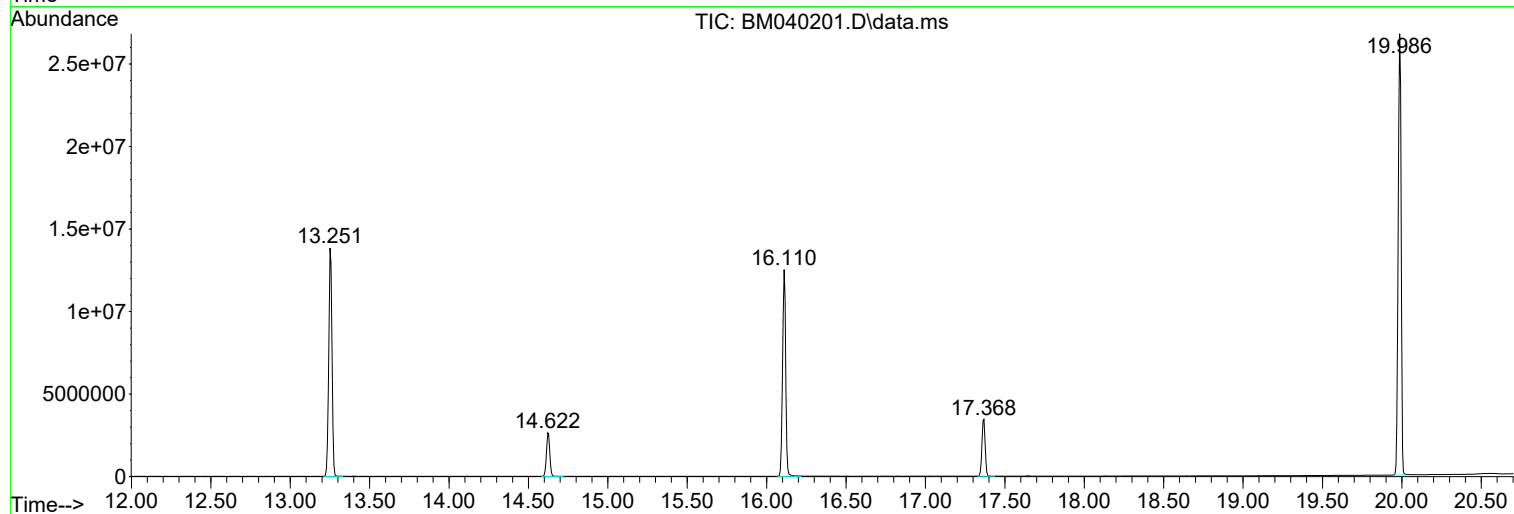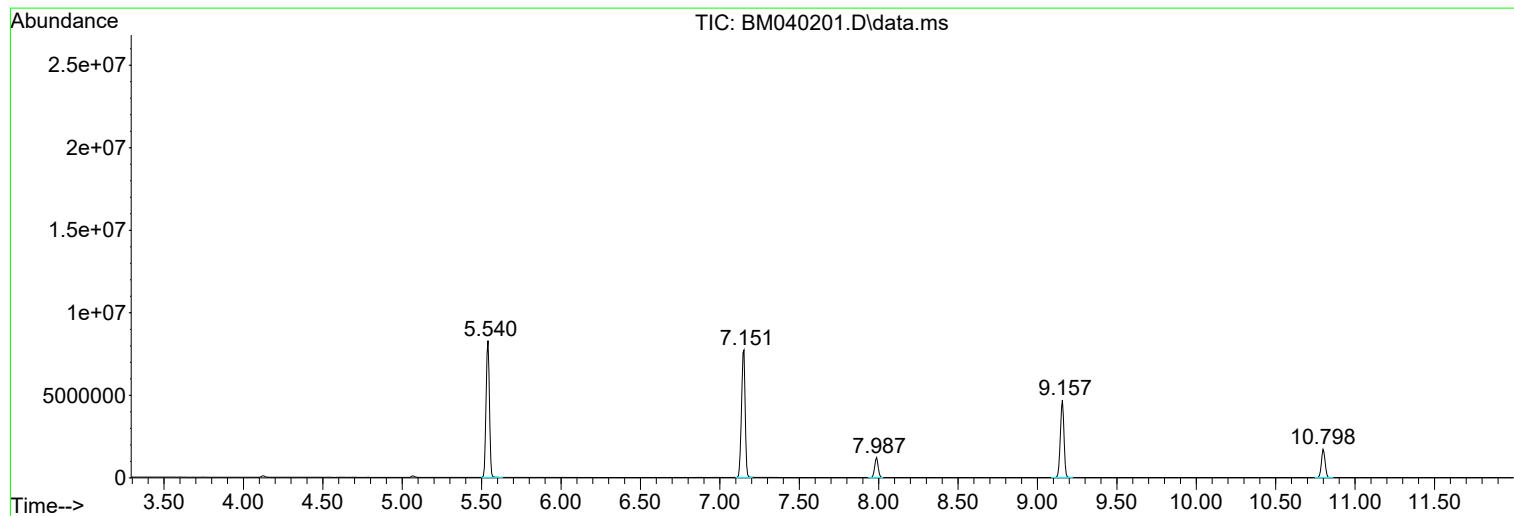

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040201.D
Acq On : 09 Jun 2023 22:48
Operator : MA/JU
Sample : PB153297BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153297BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040201.D
Acq On : 09 Jun 2023 22:48
Operator : MA/JU
Sample : PB153297BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153297BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------