

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM060923\  
 Data File : BM040202.D  
 Acq On : 09 Jun 2023 23:25  
 Operator : MA/JU  
 Sample : PB153261BL  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 PB153261BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM060823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040202.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.540       | 376           | 383         | 395          | rBV      | 5957904        | 8678061       | 33.58%          | 8.869%        |
| 2         | 7.145       | 648           | 656         | 666          | rBV      | 5851339        | 9040975       | 34.98%          | 9.240%        |
| 3         | 7.987       | 791           | 799         | 806          | rBV      | 1115039        | 1719884       | 6.65%           | 1.758%        |
| 4         | 9.151       | 987           | 997         | 1009         | rBV      | 3226281        | 5289991       | 20.47%          | 5.406%        |
| 5         | 10.798      | 1269          | 1277        | 1290         | rBV      | 1548765        | 2577692       | 9.97%           | 2.634%        |
| 6         | 13.251      | 1687          | 1694        | 1703         | rBV      | 9930164        | 14164315      | 54.80%          | 14.476%       |
| 7         | 14.621      | 1919          | 1927        | 1938         | rBV      | 2422568        | 3609625       | 13.97%          | 3.689%        |
| 8         | 16.110      | 2173          | 2180        | 2199         | rBV      | 9289698        | 12173532      | 47.10%          | 12.442%       |
| 9         | 17.368      | 2387          | 2394        | 2403         | rBV      | 3405435        | 4674870       | 18.09%          | 4.778%        |
| 10        | 19.986      | 2833          | 2839        | 2844         | rBV      | 22083135       | 25846282      | 100.00%         | 26.415%       |
| 11        | 21.545      | 3098          | 3104        | 3111         | rBV      | 4180432        | 5199870       | 20.12%          | 5.314%        |
| 12        | 23.980      | 3511          | 3518        | 3529         | rVB      | 2509312        | 4870484       | 18.84%          | 4.978%        |




Sum of corrected areas: 97845581

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM060923\  
Data File : BM040202.D  
Acq On : 09 Jun 2023 23:25  
Operator : MA/JU  
Sample : PB153261BL  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB153261BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM060823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

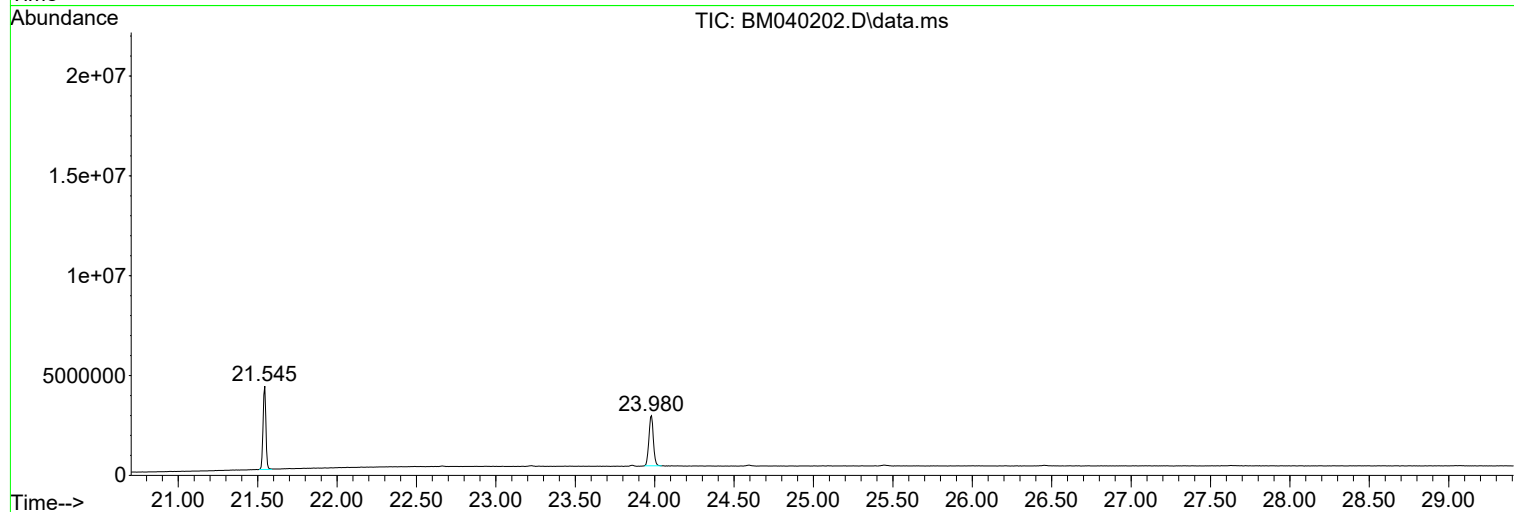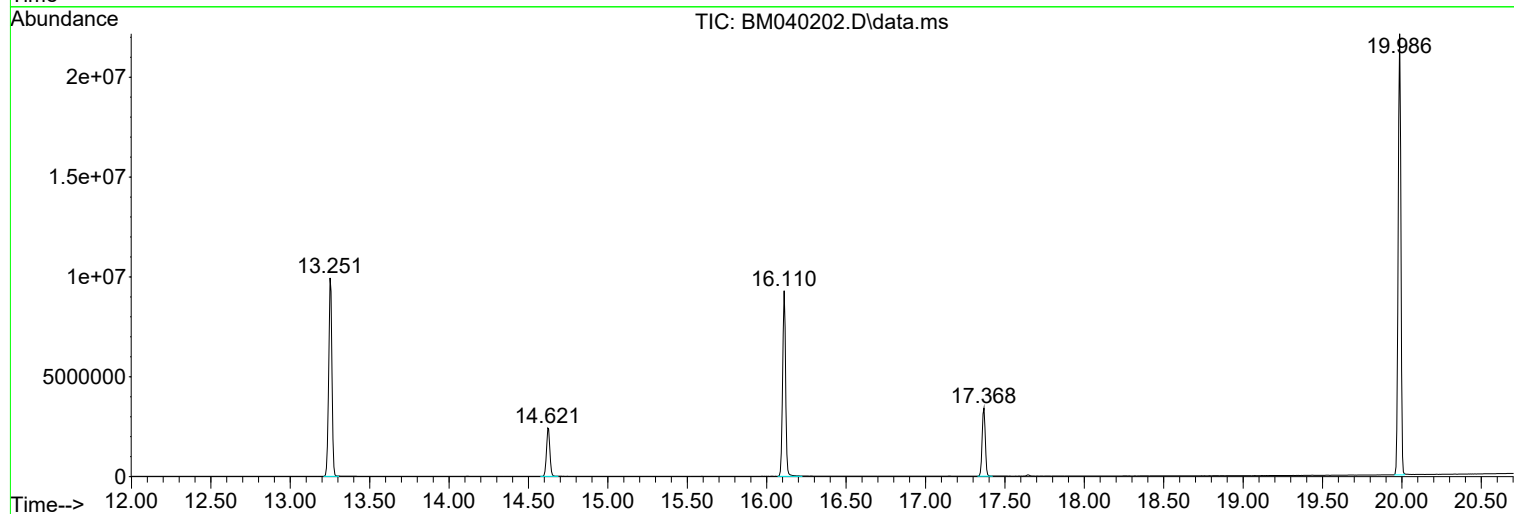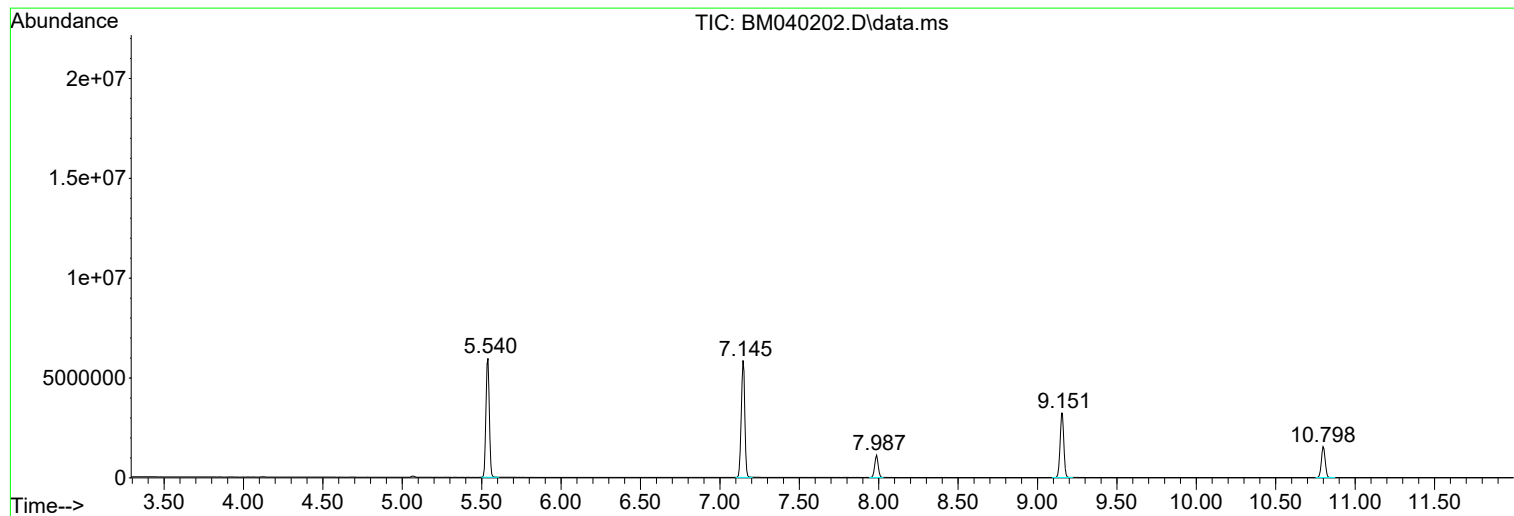

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM060923\  
Data File : BM040202.D  
Acq On : 09 Jun 2023 23:25  
Operator : MA/JU  
Sample : PB153261BL  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB153261BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM060823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM060923\  
Data File : BM040202.D  
Acq On : 09 Jun 2023 23:25  
Operator : MA/JU  
Sample : PB153261BL  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB153261BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM060823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|