

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
 Data File : BM040203.D
 Acq On : 10 Jun 2023 00:01
 Operator : MA/JU
 Sample : PB153277BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB153277BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040203.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.540	376	383	396	rBV	5693693	8322290	33.34%	8.998%
2	7.146	648	656	675	rBV	5706252	8692381	34.82%	9.398%
3	7.987	791	799	808	rBV	1007406	1573157	6.30%	1.701%
4	9.152	990	997	1012	rBV	3130969	5013507	20.08%	5.420%
5	10.799	1269	1277	1288	rBV	1431311	2338681	9.37%	2.529%
6	13.251	1687	1694	1709	rBV	9668132	13485989	54.02%	14.581%
7	14.622	1920	1927	1942	rBV	2273814	3266603	13.09%	3.532%
8	16.110	2173	2180	2199	rBV	8542040	11476556	45.97%	12.408%
9	17.369	2387	2394	2406	rBV	2907042	4208605	16.86%	4.550%
10	19.986	2833	2839	2850	rBV	22017632	24963426	100.00%	26.990%
11	21.539	3098	3103	3112	rBV	3676526	4757974	19.06%	5.144%
12	23.980	3511	3518	3531	rVB	2175015	4392661	17.60%	4.749%




Sum of corrected areas: 92491830

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040203.D
Acq On : 10 Jun 2023 00:01
Operator : MA/JU
Sample : PB153277BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153277BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

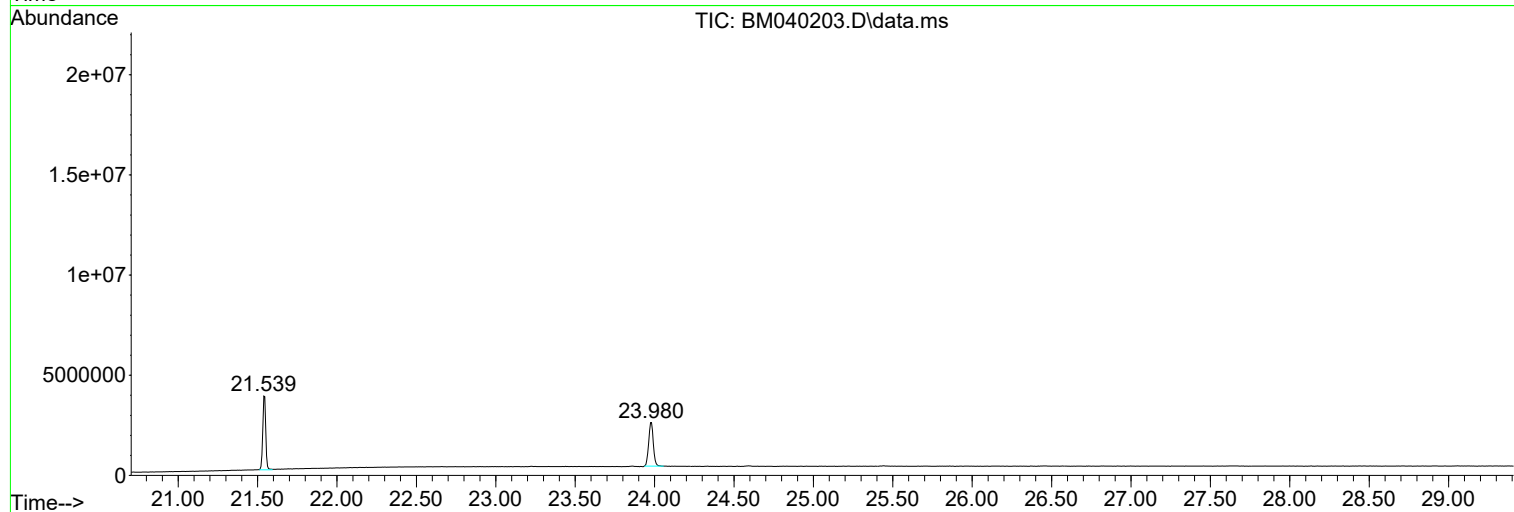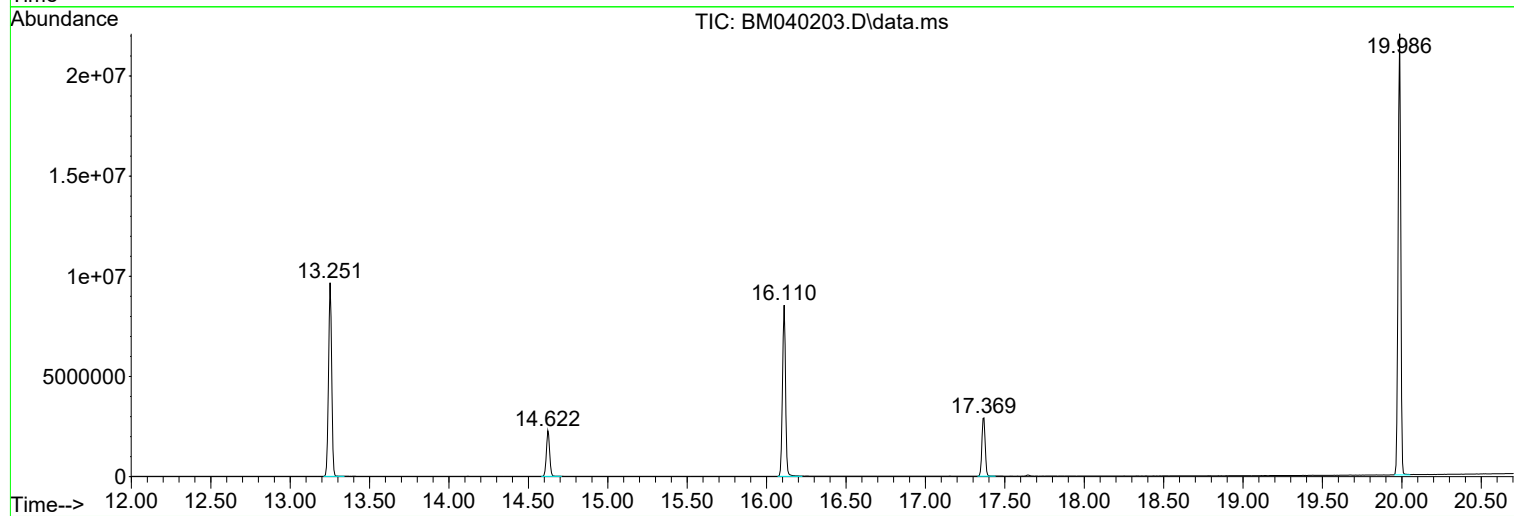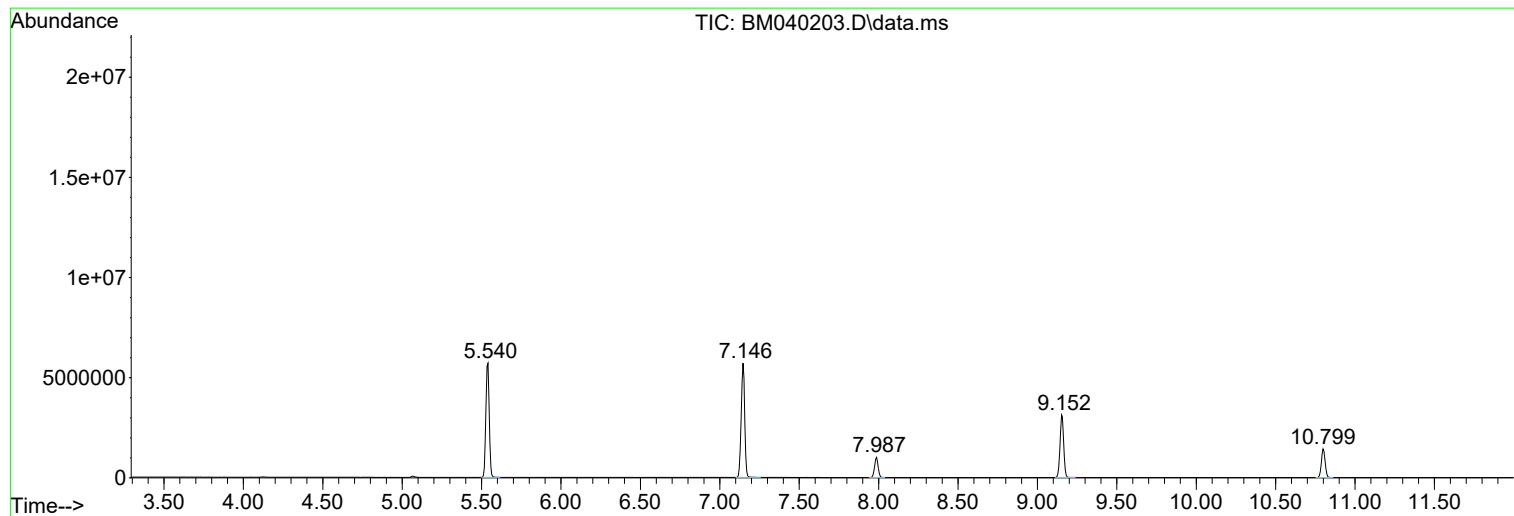

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040203.D
Acq On : 10 Jun 2023 00:01
Operator : MA/JU
Sample : PB153277BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153277BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040203.D
Acq On : 10 Jun 2023 00:01
Operator : MA/JU
Sample : PB153277BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB153277BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------