

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
 Data File : BM040206.D
 Acq On : 10 Jun 2023 01:51
 Operator : MA/JU
 Sample : 03047-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SB33B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040206.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.534	375	382	395	rBV	2832935	4146395	32.10%	6.811%
2	7.140	648	655	668	rBV	2950435	4598379	35.60%	7.554%
3	7.987	792	799	807	rBV	1030180	1597023	12.36%	2.623%
4	9.151	989	997	1010	rBV	1657107	2628110	20.35%	4.317%
5	10.798	1268	1277	1287	rBV	1490226	2432827	18.84%	3.996%
6	13.251	1687	1694	1706	rBV	5139925	7199187	55.74%	11.826%
7	14.621	1919	1927	1939	rBV	2376586	3417352	26.46%	5.614%
8	15.974	2151	2157	2163	rBV	202846	289301	2.24%	0.475%
9	16.110	2173	2180	2204	rBV	4522398	6273096	48.57%	10.305%
10	17.362	2387	2393	2404	rBV	3065994	4371226	33.84%	7.181%
11	18.251	2539	2544	2552	rBV	186534	291682	2.26%	0.479%
12	19.980	2833	2838	2851	rBV	11181811	12915677	100.00%	21.217%
13	21.239	3048	3052	3062	rBV	330695	496778	3.85%	0.816%
14	21.539	3098	3103	3112	rBV	3986020	5068359	39.24%	8.326%
15	23.974	3510	3517	3531	rVB	2638108	5149135	39.87%	8.459%




Sum of corrected areas: 60874527

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040206.D
Acq On : 10 Jun 2023 01:51
Operator : MA/JU
Sample : 03047-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB33B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

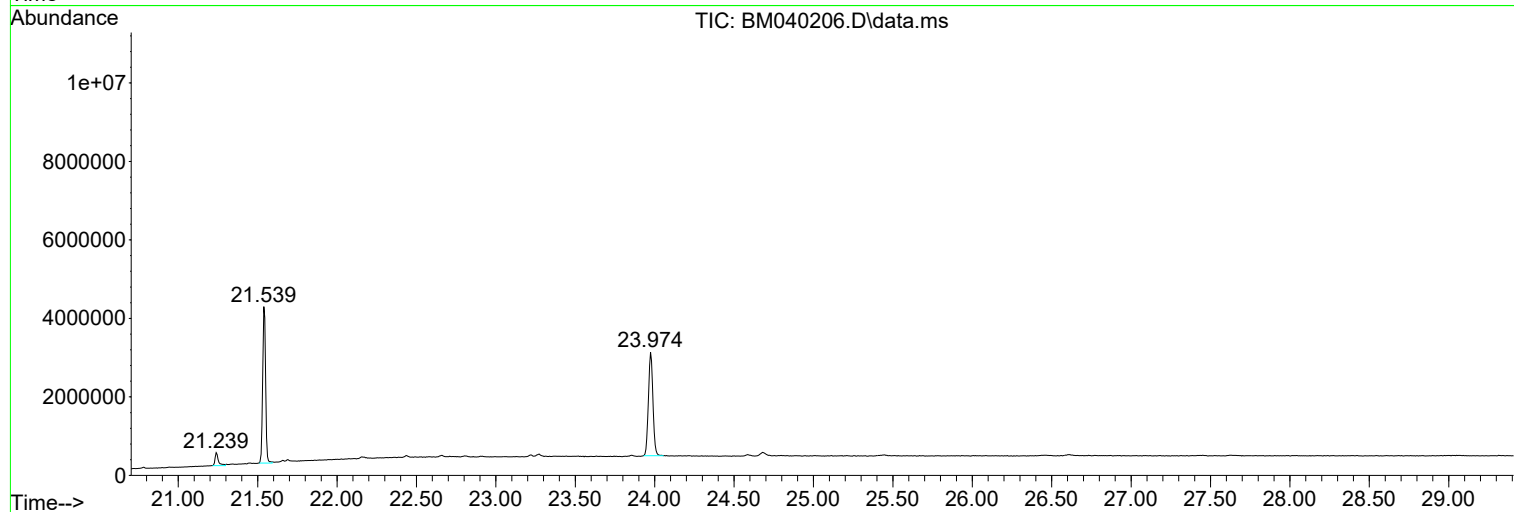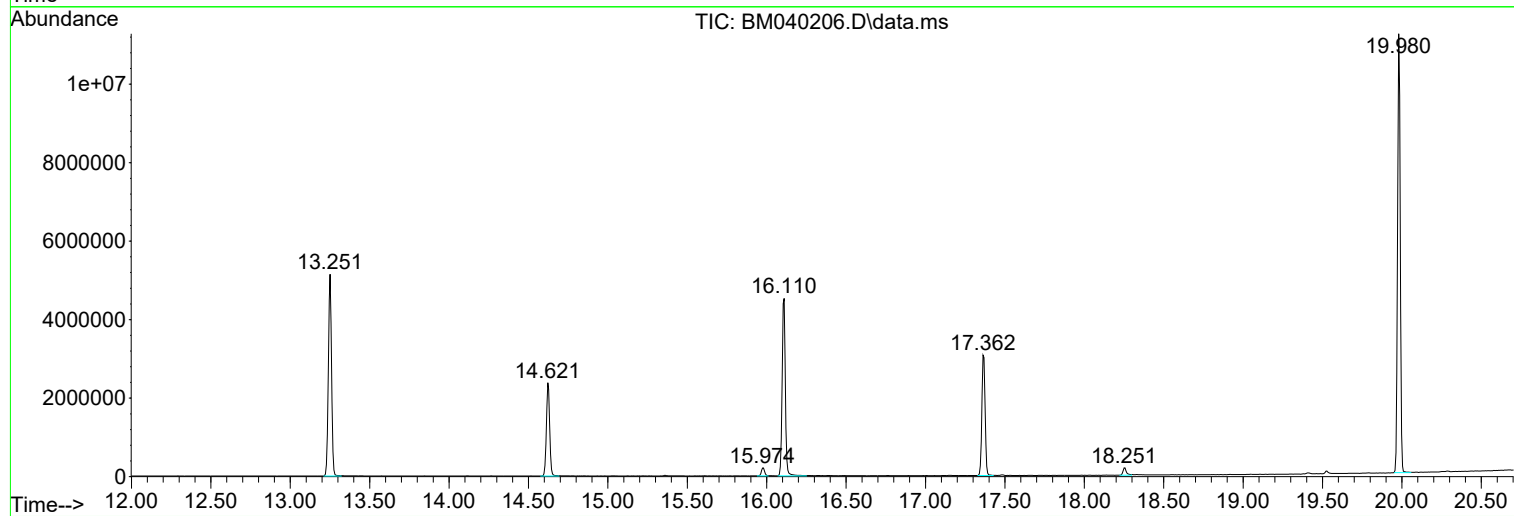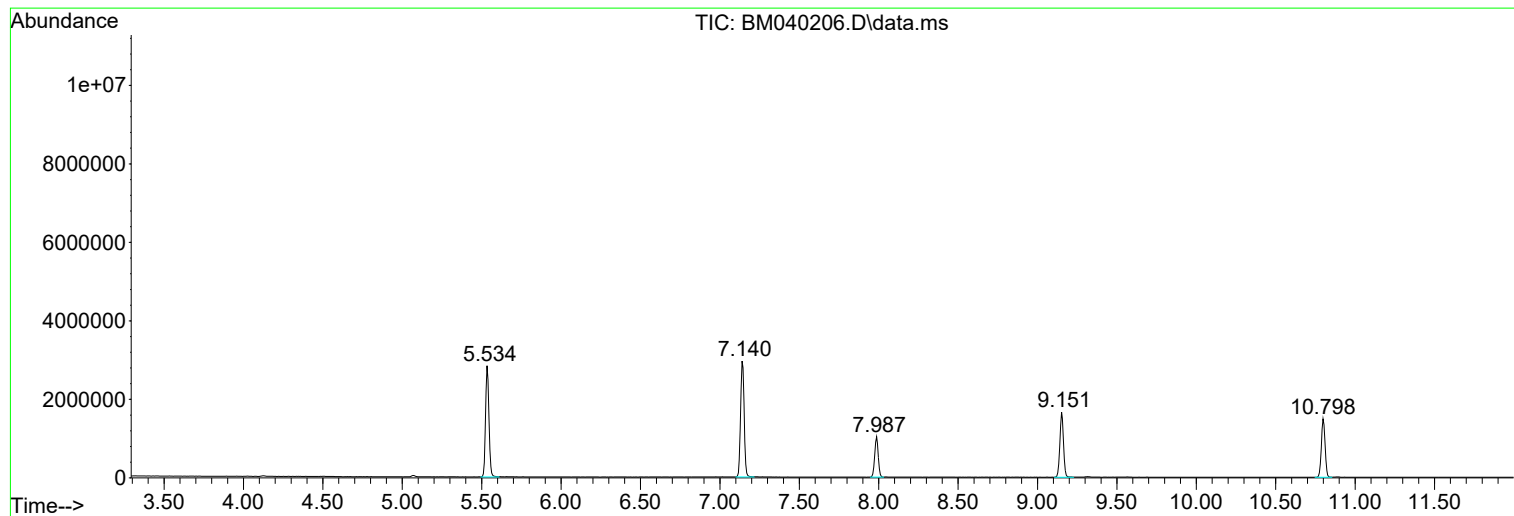

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040206.D
Acq On : 10 Jun 2023 01:51
Operator : MA/JU
Sample : 03047-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB33B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040206.D
Acq On : 10 Jun 2023 01:51
Operator : MA/JU
Sample : 03047-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB33B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------