

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
 Data File : BM040212.D
 Acq On : 10 Jun 2023 05:29
 Operator : MA/JU
 Sample : 03096-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TP-24-0A

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM040212.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.534	375	382	396	rBV	4239588	6181071	35.85%	7.578%
2	7.145	646	656	669	rBV	4238691	6645287	38.54%	8.148%
3	7.986	792	799	806	rBV	1241947	1950717	11.31%	2.392%
4	9.151	988	997	1014	rBV	2470640	3906730	22.66%	4.790%
5	10.798	1269	1277	1288	rBV	1832528	2956380	17.15%	3.625%
6	13.251	1686	1694	1705	rBV	7251334	10196346	59.14%	12.501%
7	14.621	1919	1927	1940	rBV	2960731	4185817	24.28%	5.132%
8	15.974	2151	2157	2164	rBV	310936	442354	2.57%	0.542%
9	16.109	2173	2180	2199	rBV	6409764	8945014	51.88%	10.967%
10	17.362	2387	2393	2406	rBV	3880292	5316037	30.83%	6.518%
11	18.251	2539	2544	2552	rBV	200704	310179	1.80%	0.380%
12	19.980	2833	2838	2844	rBV	14517634	17241209	100.00%	21.139%
13	20.739	2963	2967	2971	rBV	558838	551010	3.20%	0.676%
14	21.239	3048	3052	3062	rBV	539148	745450	4.32%	0.914%
15	21.539	3098	3103	3112	rBV	4794058	5901508	34.23%	7.236%
16	22.656	3290	3293	3300	rVB3	152463	204160	1.18%	0.250%
17	23.974	3510	3517	3527	rVB	3145340	5882585	34.12%	7.212%




Sum of corrected areas: 81561854

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040212.D
Acq On : 10 Jun 2023 05:29
Operator : MA/JU
Sample : 03096-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-24-0A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

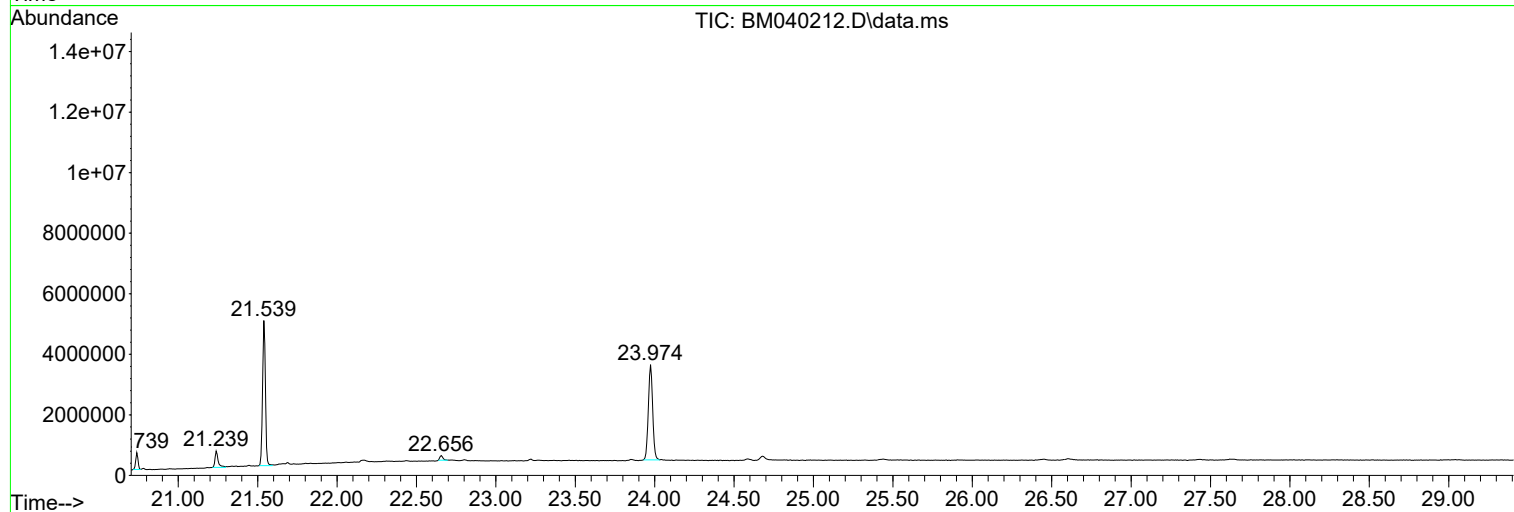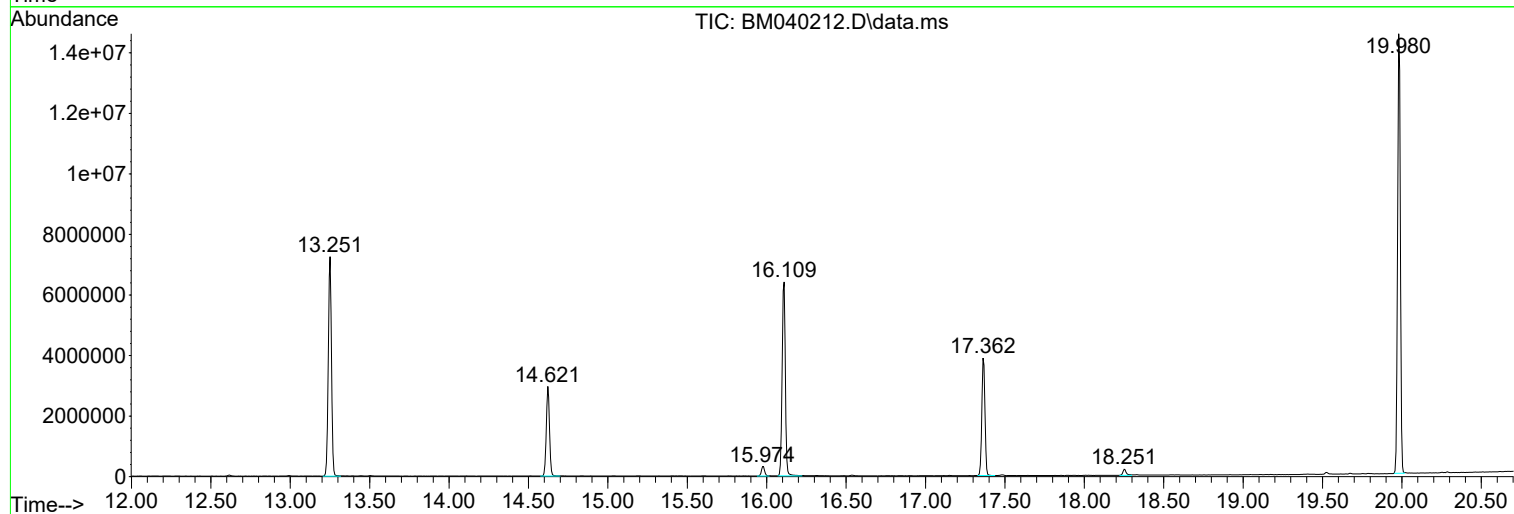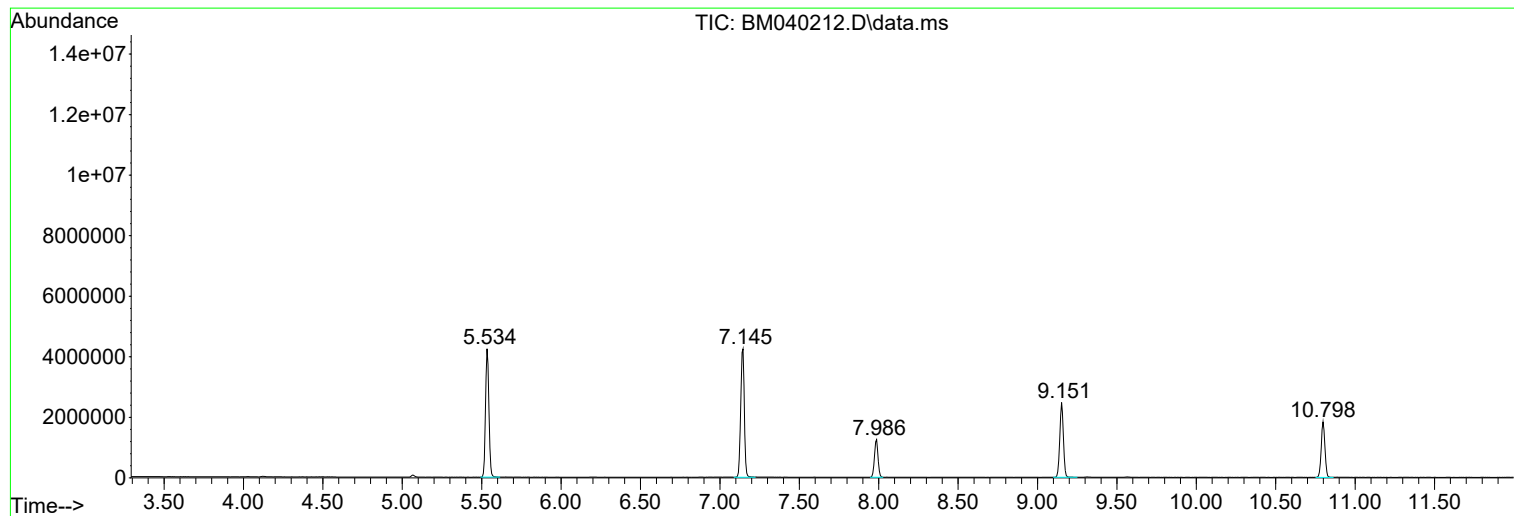

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040212.D
Acq On : 10 Jun 2023 05:29
Operator : MA/JU
Sample : 03096-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-24-0A










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.974	2.11 ng	442354	Acenaphthene-d10	14.621

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			2-Chloro-1-phenyl-1-propanone	168	C9H9ClO	006084-17-9	47
3			Benzenecarbothioic acid, S-methy...	152	C8H8OS	005925-68-8	47
4			1-Propanone, 2-bromo-1-phenyl-	212	C9H9BrO	002114-00-3	47
5			Benzeneacetic acid, .alpha.-oxo-...	164	C9H8O3	015206-55-0	47

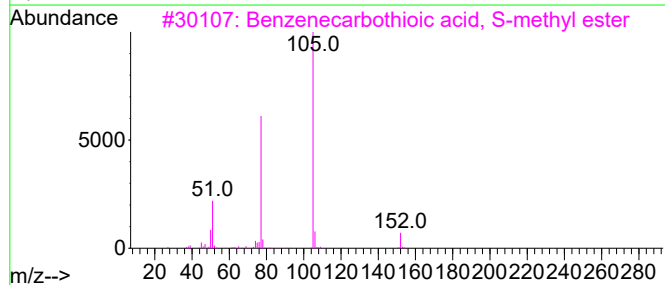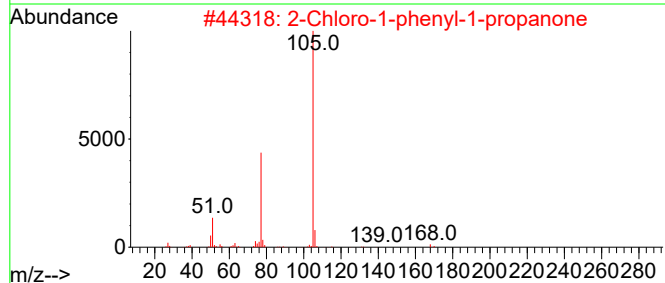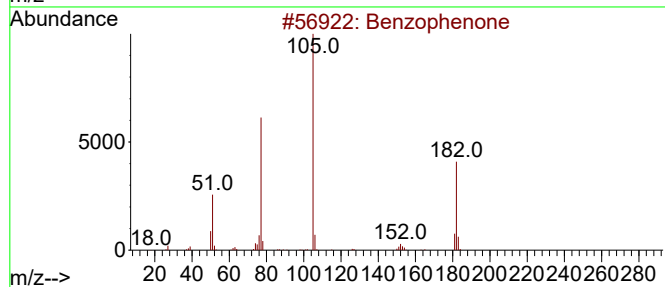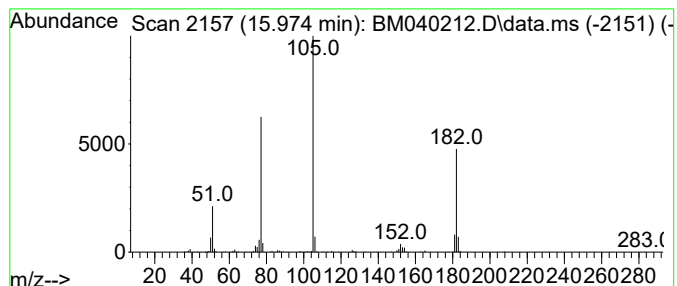

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040212.D
Acq On : 10 Jun 2023 05:29
Operator : MA/JU
Sample : 03096-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-24-0A










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Dichloroacetic acid, heptad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.238	2.53 ng	745450	Chrysene-d12	21.538

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	94
2			1-Hexacosene	364	C26H52	018835-33-1	94
3			Nonacos-1-ene	406	C29H58	018835-35-3	94
4			1-Heneicosanol	312	C21H44O	015594-90-8	93
5			Behenic alcohol	326	C22H46O	000661-19-8	93

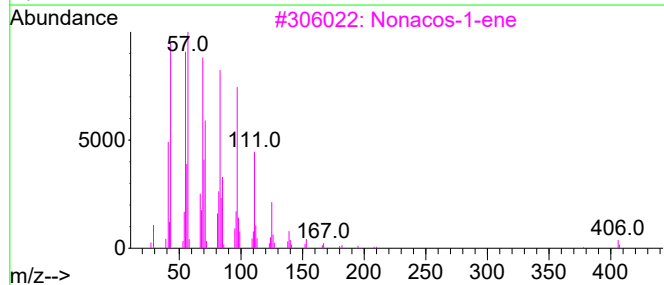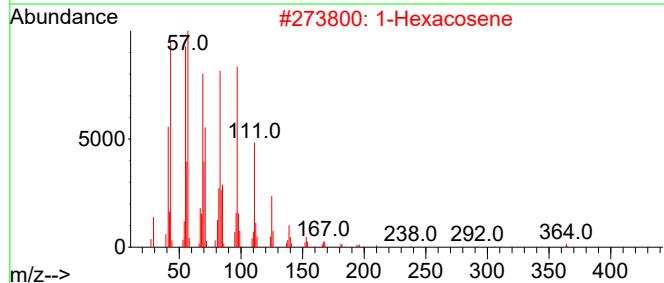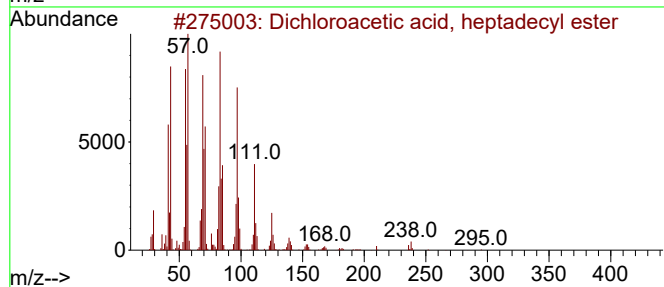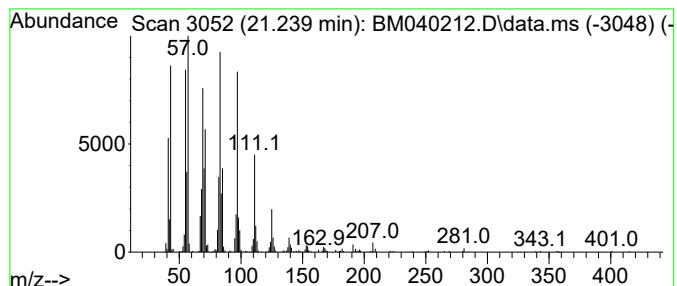

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
Data File : BM040212.D
Acq On : 10 Jun 2023 05:29
Operator : MA/JU
Sample : 03096-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TP-24-0A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.974	2.1	ng	442354	3	14.621	4185820	20.0
Dichloroacetic ...	21.238	2.5	ng	745450	5	21.538	5901510	20.0