
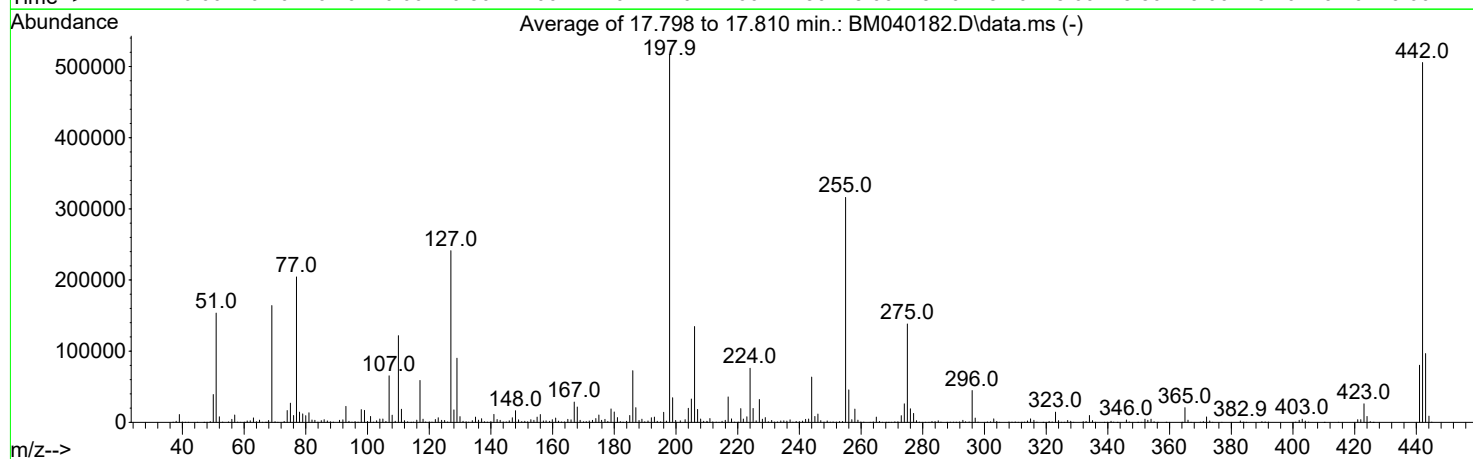


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM060923\  
Data File : BM040182.D  
Acq On : 09 Jun 2023 08:49  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM060823.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Jun 08 23:25:50 2023

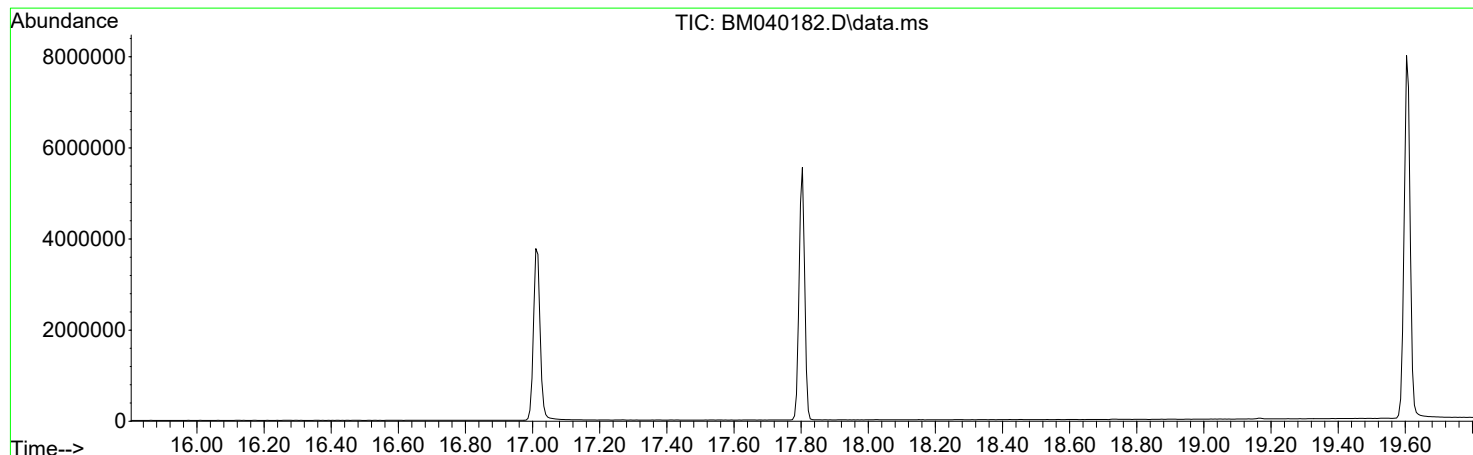

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 29.7         | 153482     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 2668       | PASS                |
| 69             | 198             | 0.00            | 100             | 31.7         | 164032     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 923        | PASS                |
| 127            | 198             | 10              | 80              | 46.7         | 241365     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 1850       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 516928     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 34592      | PASS                |
| 275            | 198             | 10              | 60              | 26.8         | 138384     | PASS                |
| 365            | 198             | 1               | 100             | 4.0          | 20704      | PASS                |
| 441            | 198             | 0.01            | 100             | 15.6         | 80403      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 505621     | PASS                |
| 443            | 442             | 15              | 24              | 19.1         | 96685      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 6/9/2023      | BNA_M            | <u>BM040182.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1732551          | 20.839             |
| DDD           | 24899            | 20.398             |
| DDE           | 1731             | 19.886             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 26630         | 1759181          | 1.51               |
|               |                  |                    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM060923\  
 Data File : BM040182.D  
 Acq On : 09 Jun 2023 08:49  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Quant Time: Jun 09 09:20:40 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM060823.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 08 23:25:50 2023  
 Response via : Initial Calibration

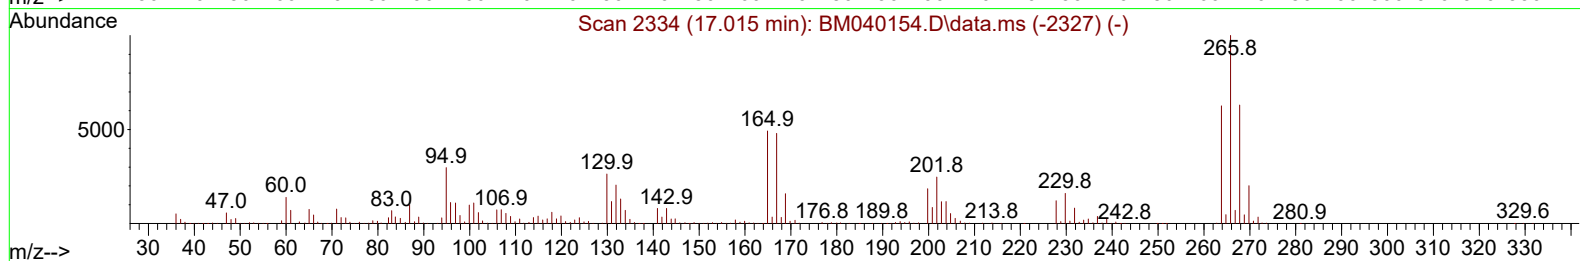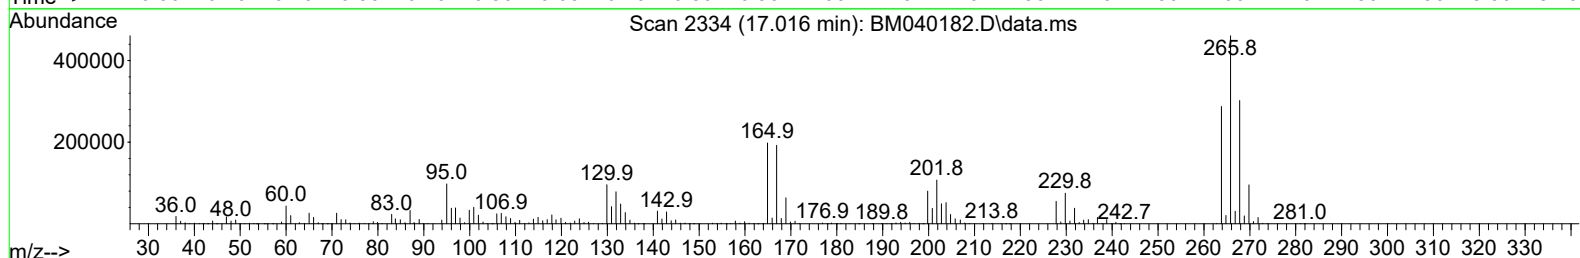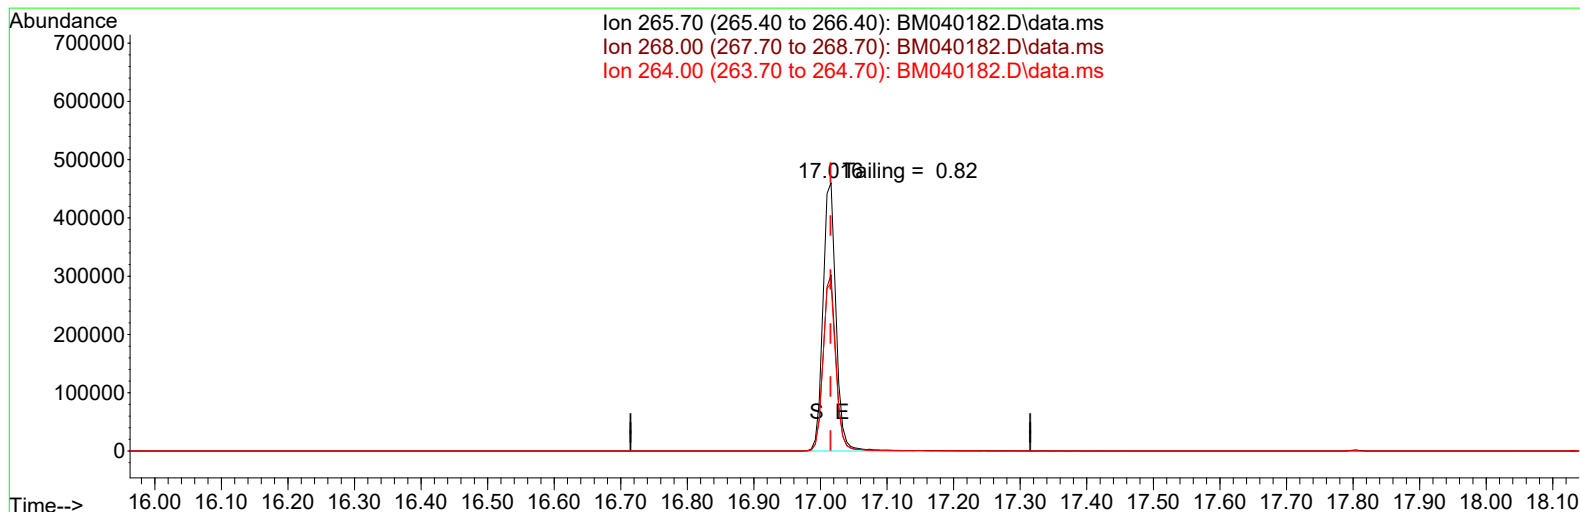

TIC: BM040182.D\data.ms

**(70) Pentachlorophenol (C)**

17.016min (+ 0.001) 1400717.30 ng




response 627720

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.00  | 65.57  |
| 264.00 | 62.60  | 62.41  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM060923\  
Data File : BM040182.D  
Acq On : 09 Jun 2023 08:49  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Jun 09 09:20:40 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM060823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jun 08 23:25:50 2023  
Response via : Initial Calibration

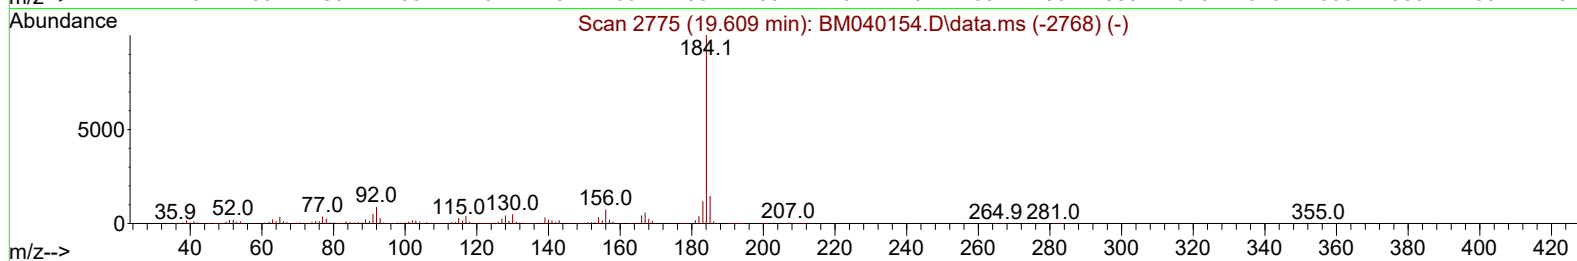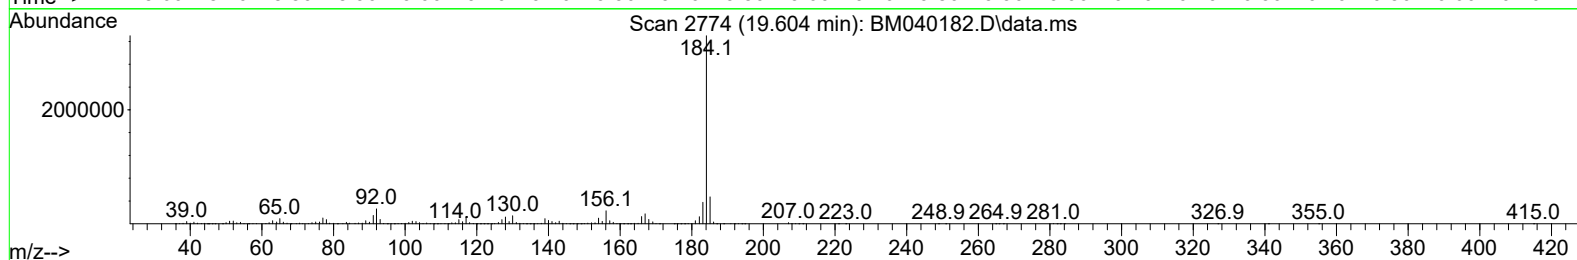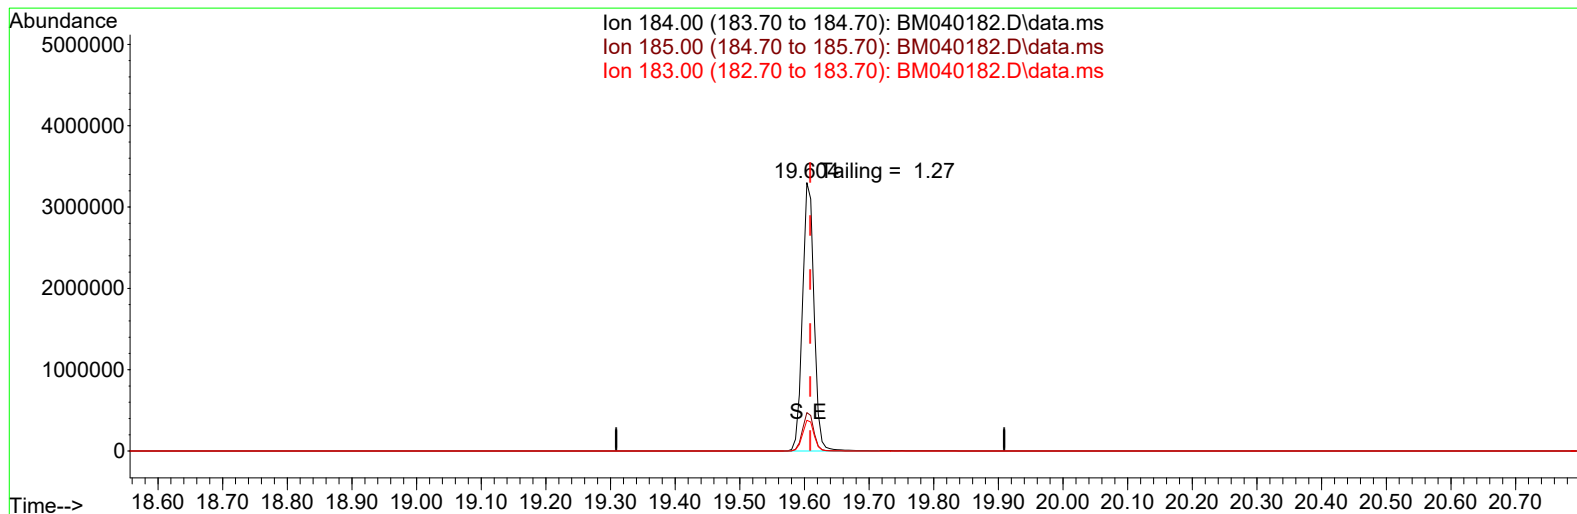

TIC: BM040182.D\data.ms

(77) Benzidine

19.604min (-0.005) 256714.86 ng

response 4112485

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.50  | 14.34  |
| 183.00 | 11.70  | 11.44  |
| 0.00   | 0.00   | 0.00   |