
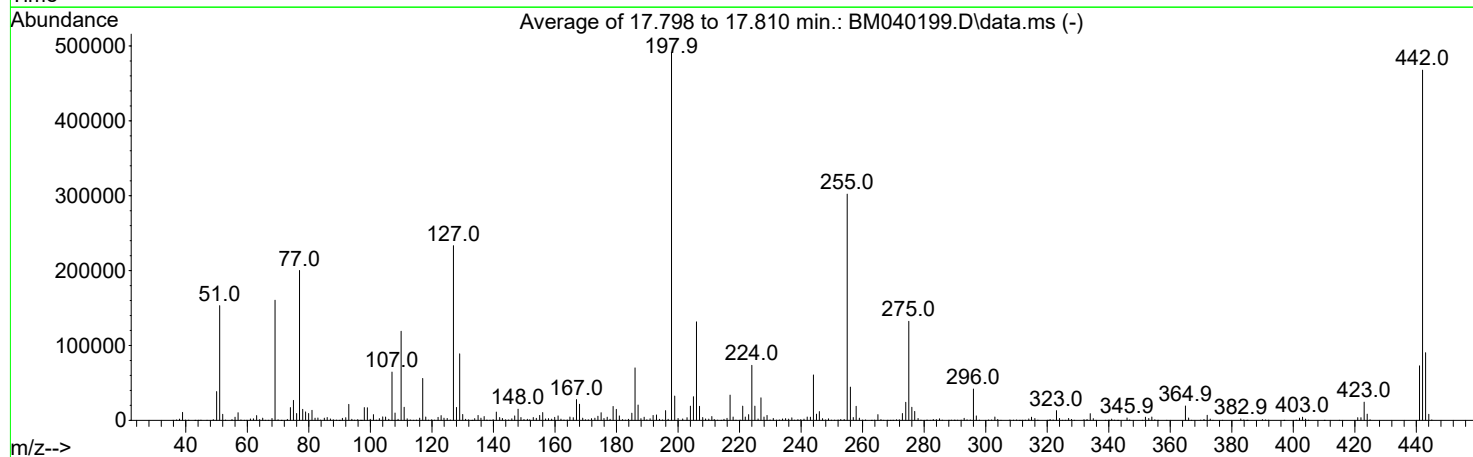


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
 Data File : BM040199.D
 Acq On : 09 Jun 2023 20:22
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 08 23:25:50 2023

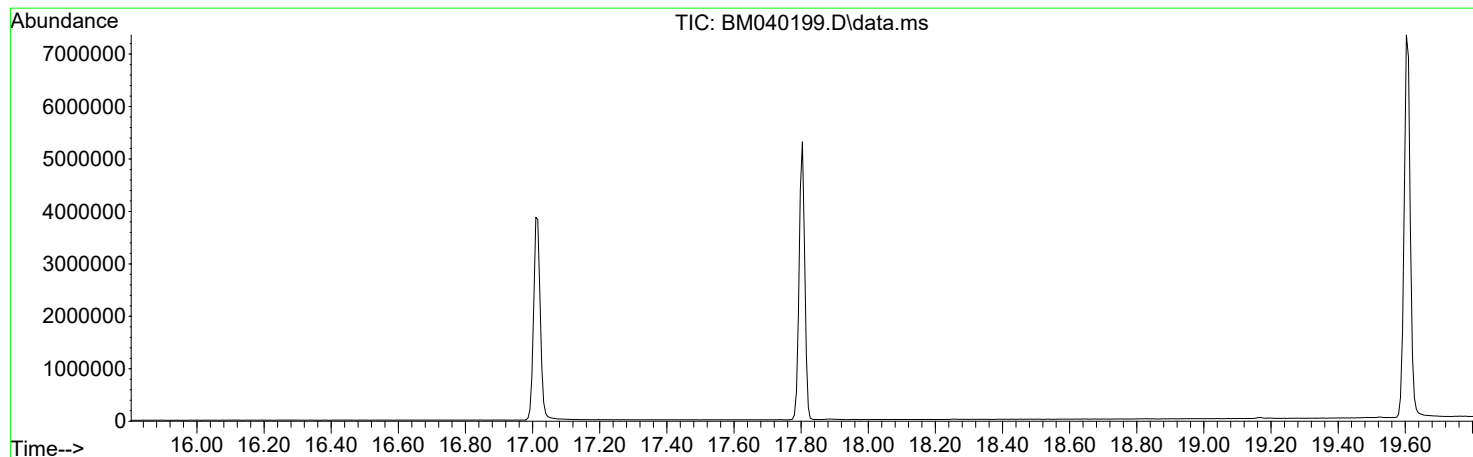

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	153176	PASS
68	69	0.00	2	1.6	2609	PASS
69	198	0.00	100	32.7	160581	PASS
70	69	0.00	2	0.6	916	PASS
127	198	10	80	47.5	233280	PASS
197	198	0.00	2	0.3	1506	PASS
198	198	100	100	100.0	491307	PASS
199	198	5	9	6.6	32515	PASS
275	198	10	60	26.9	132389	PASS
365	198	1	100	3.9	19283	PASS
441	198	0.01	100	14.9	72968	PASS
442	442	50	100	100.0	467712	PASS
443	442	15	24	19.3	90464	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/9/2023	BNA_M	<u>BM040199.D</u>
Compound Name	Response	Retention Time
DDT	1156594	20.839
DDD	245452	20.398
DDE	3997	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
249449	1406043	17.74

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
 Data File : BM040199.D
 Acq On : 09 Jun 2023 20:22
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 10 06:05:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 08 23:25:50 2023
 Response via : Initial Calibration

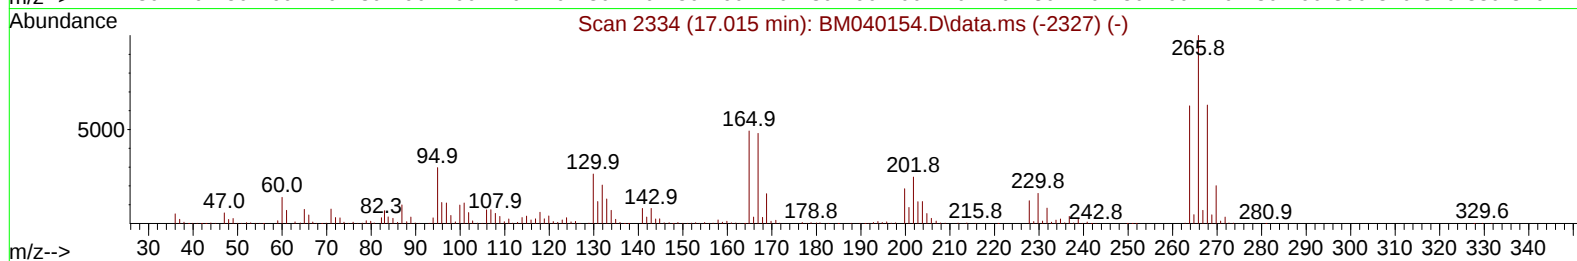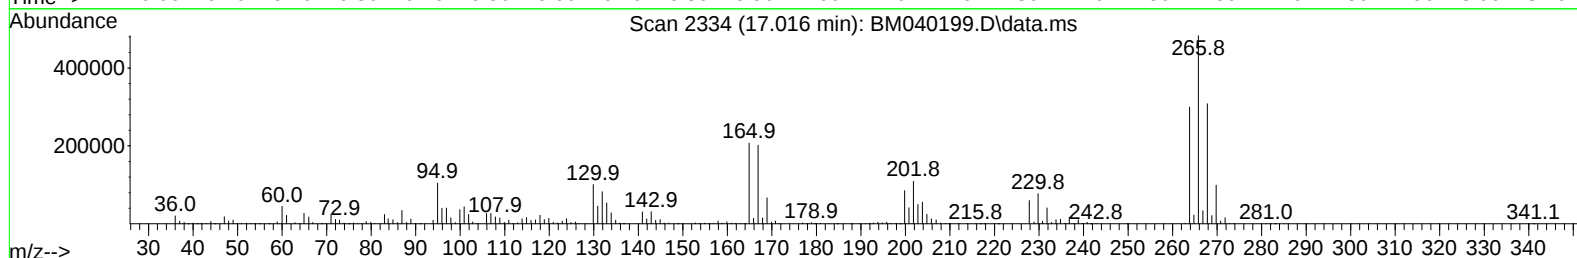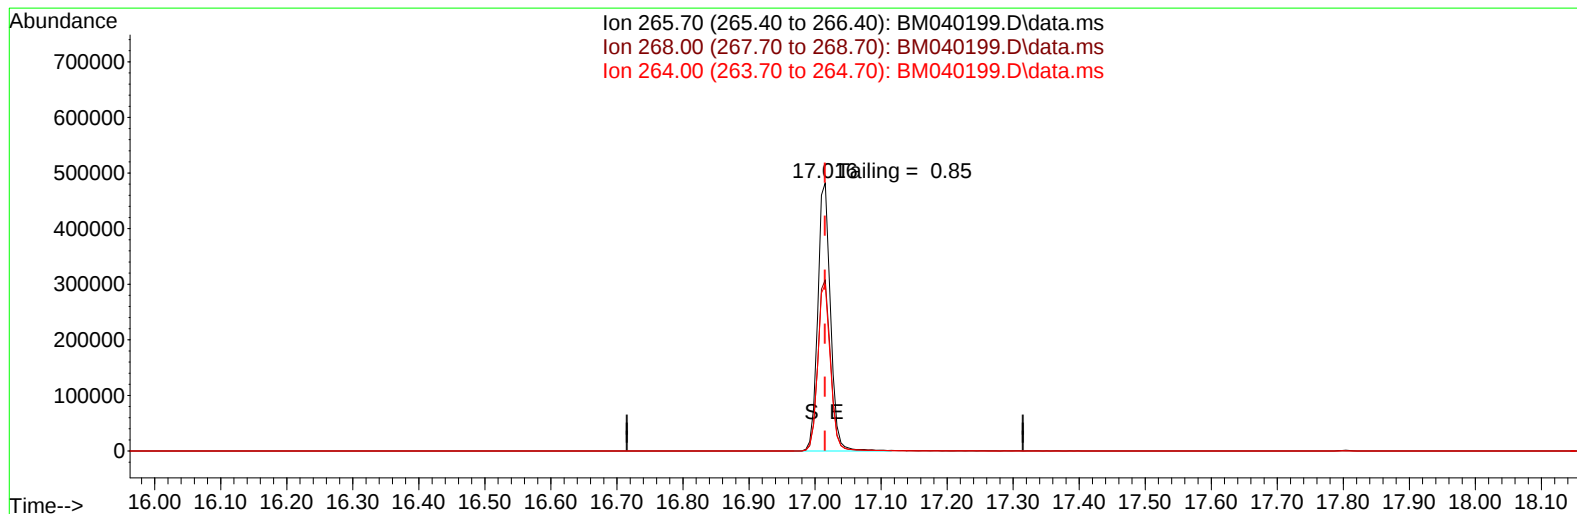

TIC: BM040199.D\data.ms

(70) Pentachlorophenol (C)

17.016min (+ 0.001) 272962.02 ng




response 648557

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.82
264.00	62.60	62.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060923\
 Data File : BM040199.D
 Acq On : 09 Jun 2023 20:22
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 10 06:05:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 08 23:25:50 2023
 Response via : Initial Calibration

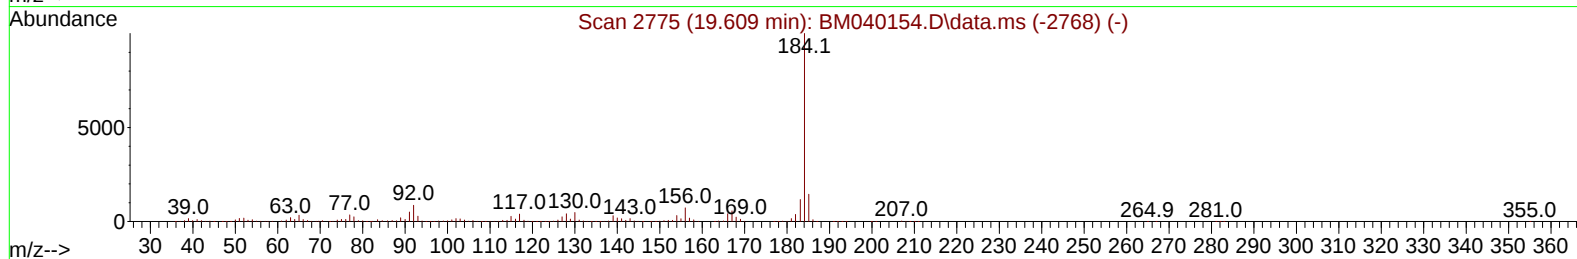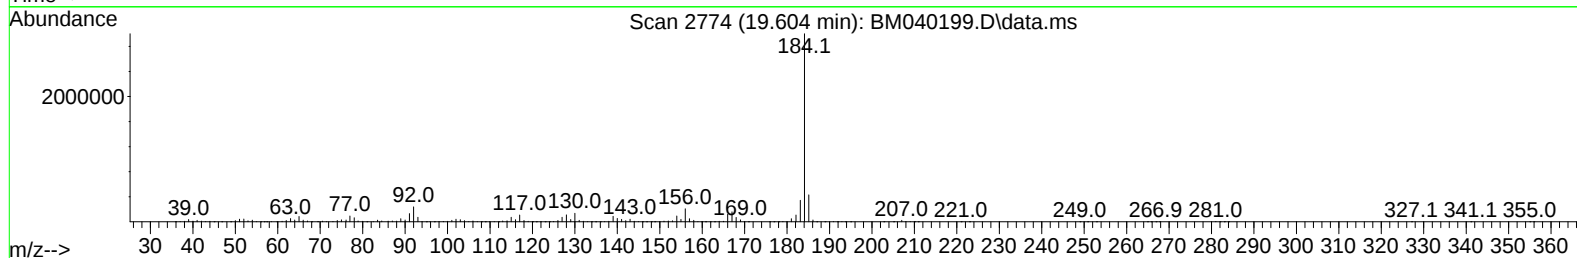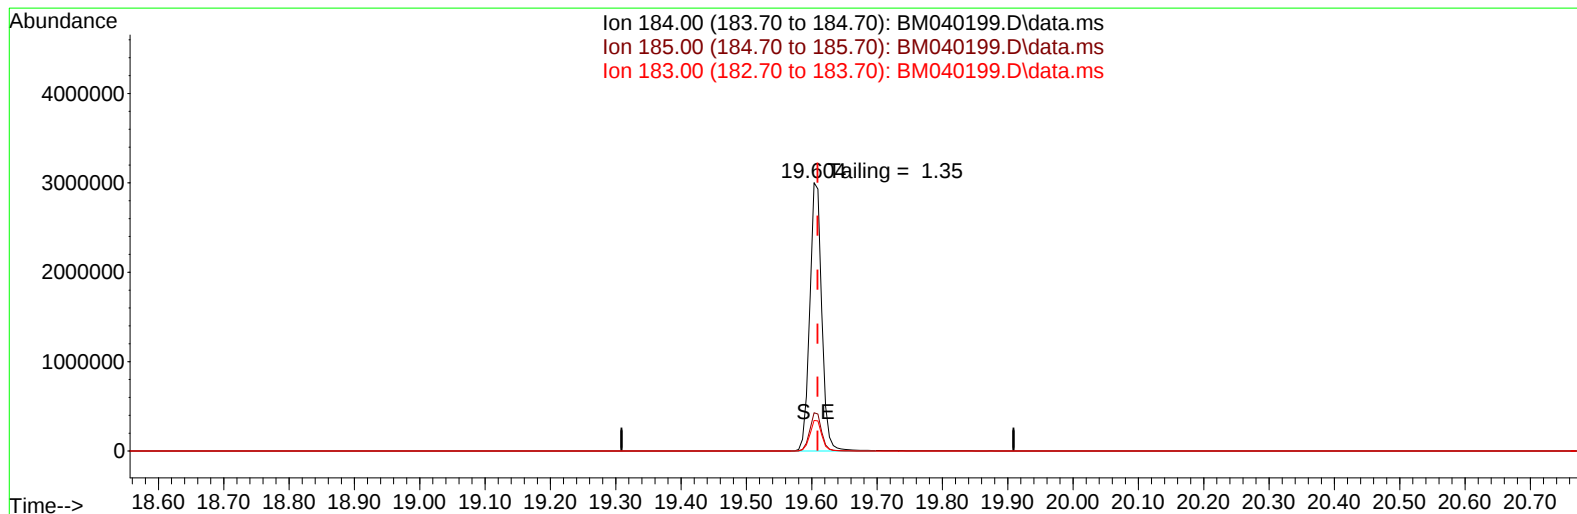

TIC: BM040199.D\data.ms

(77) Benzidine

19.604min (-0.005) 187516.66 ng

response 3852667

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.26
183.00	11.70	11.40
0.00	0.00	0.00