

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061019\
 Data File : BM020828.D
 Acq On : 10 Jun 2019 10:19
 Operator : HP/JU
 Sample : K3017-02
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 11 00:22:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jun 09 01:02:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	315444	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	1275948	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	728750	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	1645773	20.00	ng/ul	0.00
77) Chrysene-d12	21.37	240	1537370	20.00	ng/ul	0.00
85) Perylene-d12	23.65	264	1741980	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	25883	3.91	ng/uL	0.00
5) Phenol-d5	6.97	99	453797	18.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	295549	20.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	390209	20.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	302871	15.60	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	190678	21.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	196767	21.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	384709	20.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	418573	18.59	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	1211230	22.47	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	1454264	21.28	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	128647	13.91	ng/ul	0.00
57) Fluorene-d10	15.44	176	1018928	22.24	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	90195	10.72	ng/ul	0.00
70) Anthracene-d10	17.29	188	1468489	20.43	ng/ul	0.00
78) Pyrene-d10	19.58	212	1596039	21.48	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.50	264	1638563	20.70	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.90	163	117592	2.179	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061019\
Data File : BM020828.D
Acq On : 10 Jun 2019 10:19
Operator : HP/JU
Sample : K3017-02
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 11 00:22:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jun 09 01:02:58 2019
Response via : Initial Calibration

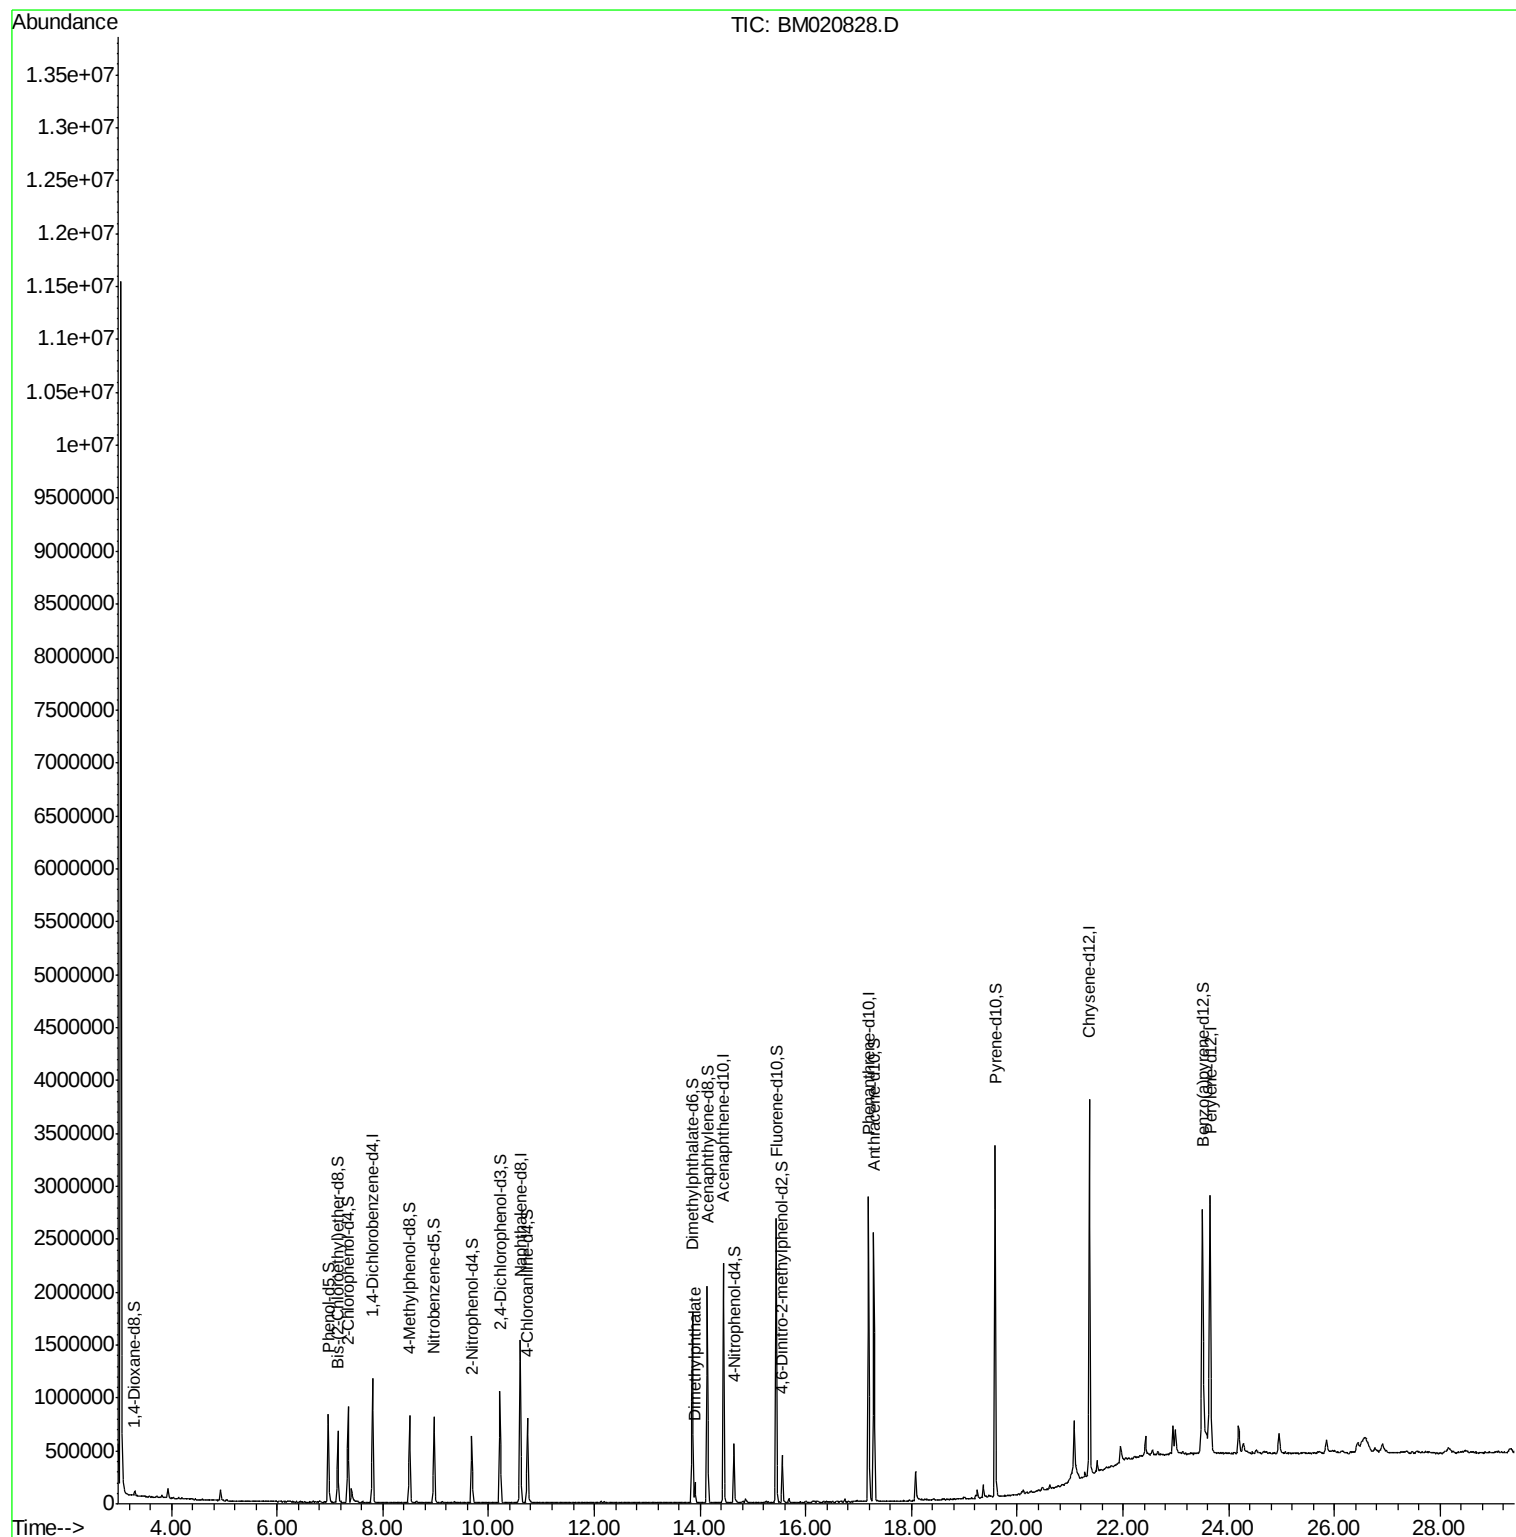

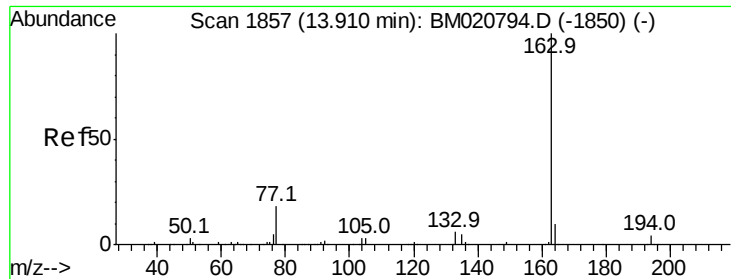

#44

Dimethylphthalate

Concen: 2.179 ng/ul

RT: 13.90 min Scan# 1856

Delta R.T. -0.01 min

Lab File: BM020828.D

Acq: 10 Jun 2019 10:19

Instrument :

BNA_M

ClientSampleId :

Tot Ion:163 Resp: 117592

Ion Ratio Lower Upper

163 100

194 4.8 3.2 4.8#

164 11.5 8.0 12.0

