

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061019\
 Data File : BM020848.D
 Acq On : 10 Jun 2019 22:23
 Operator : HP/JU
 Sample : K3006-19
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 11 00:24:22 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jun 09 01:02:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	279920	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	1166804	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	690106	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	1611121	20.00	ng/ul	0.00
77) Chrysene-d12	21.37	240	1565840	20.00	ng/ul	0.00
85) Perylene-d12	23.65	264	1779089	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	26160	4.46	ng/uL	0.00
5) Phenol-d5	6.97	99	479716	22.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	304798	23.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	415483	24.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	378596	21.97	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	204695	25.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	221670	27.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	418448	24.47	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	522946	25.40	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	1414742	27.71	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	1566386	24.20	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	150367	17.17	ng/ul	0.00
57) Fluorene-d10	15.44	176	1171931	27.01	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	98576	11.96	ng/ul	0.00
70) Anthracene-d10	17.29	188	1764521	25.07	ng/ul	0.00
78) Pyrene-d10	19.58	212	1934039	25.55	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.50	264	2028906	25.09	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.90	163	508016	9.939	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061019\
Data File : BM020848.D
Acq On : 10 Jun 2019 22:23
Operator : HP/JU
Sample : K3006-19
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 11 00:24:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jun 09 01:02:58 2019
Response via : Initial Calibration

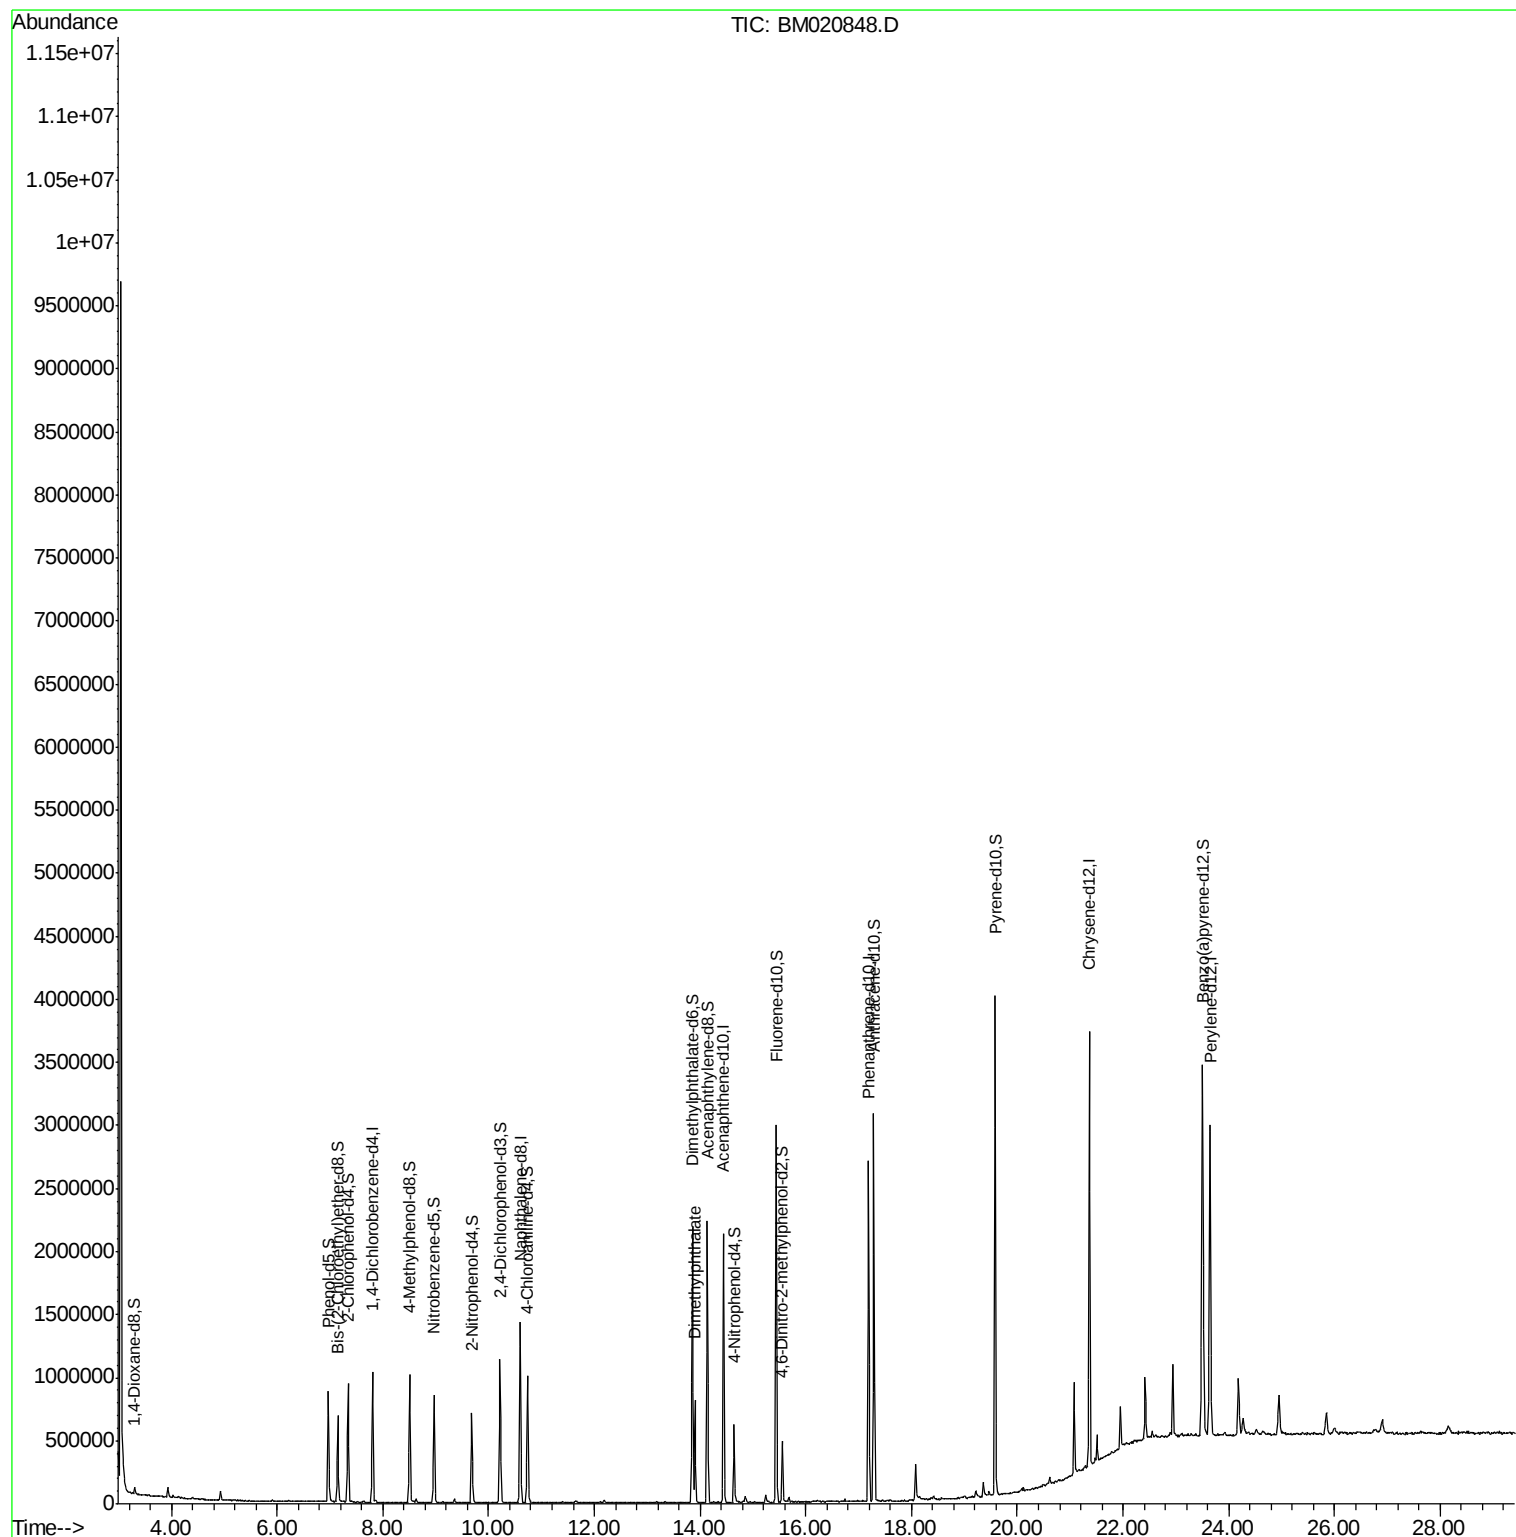

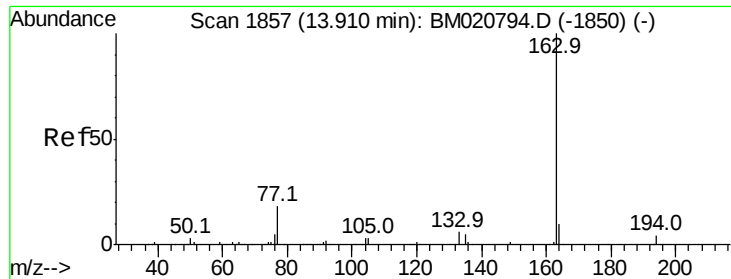

#44

Dimethylphthalate

Concen: 9.939 ng/ul

RT: 13.90 min Scan# 1856

Delta R.T. -0.01 min

Lab File: BM020848.D

Acq: 10 Jun 2019 22:23

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 508016

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 10.0 8.0 12.0

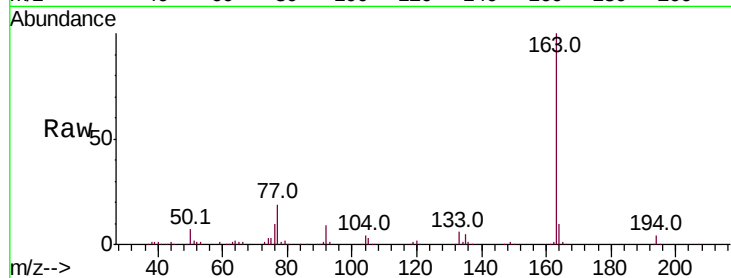

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

