

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061019\  
 Data File : BM020855.D  
 Acq On : 11 Jun 2019 03:13  
 Operator : HP/JU  
 Sample : K3017-18  
 Misc :  
 ALS Vial : 28 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :

Quant Time: Jun 11 05:41:50 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM060619MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sun Jun 09 01:02:58 2019  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.81  | 152  | 385478   | 20.00 | ng/ul | 0.00     |
| 18) Naphthalene-d8        | 10.60 | 136  | 1505432  | 20.00 | ng/ul | 0.00     |
| 35) Acenaphthene-d10      | 14.45 | 164  | 830655   | 20.00 | ng/ul | 0.00     |
| 61) Phenanthrene-d10      | 17.19 | 188  | 1775644  | 20.00 | ng/ul | 0.00     |
| 77) Chrysene-d12          | 21.37 | 240  | 1678860  | 20.00 | ng/ul | 0.00     |
| 85) Perylene-d12          | 23.66 | 264  | 1981437  | 20.00 | ng/ul | 0.00     |

## System Monitoring Compounds

|                                |       |     |         |       |       |      |
|--------------------------------|-------|-----|---------|-------|-------|------|
| 3) 1,4-Dioxane-d8              | 3.31  | 96  | 26923   | 3.33  | ng/uL | 0.00 |
| 5) Phenol-d5                   | 6.97  | 99  | 566595  | 19.21 | ng/ul | 0.00 |
| 7) Bis-(2-Chloroethyl)ether-d  | 7.15  | 67  | 331867  | 18.77 | ng/ul | 0.00 |
| 9) 2-Chlorophenol-d4           | 7.34  | 132 | 481115  | 20.48 | ng/ul | 0.00 |
| 13) 4-Methylphenol-d8          | 8.51  | 113 | 463231  | 19.52 | ng/ul | 0.00 |
| 19) Nitrobenzene-d5            | 8.97  | 128 | 224287  | 21.83 | ng/ul | 0.00 |
| 22) 2-Nitrophenol-d4           | 9.69  | 143 | 251457  | 23.77 | ng/ul | 0.00 |
| 26) 2,4-Dichlorophenol-d3      | 10.22 | 165 | 493742  | 22.38 | ng/ul | 0.00 |
| 29) 4-Chloroaniline-d4         | 10.75 | 131 | 172432  | 6.49  | ng/ul | 0.00 |
| 43) Dimethylphthalate-d6       | 13.86 | 166 | 1440302 | 23.44 | ng/ul | 0.00 |
| 46) Acenaphthylene-d8          | 14.14 | 160 | 1748826 | 22.45 | ng/ul | 0.00 |
| 51) 4-Nitrophenol-d4           | 14.65 | 143 | 201326  | 19.09 | ng/ul | 0.00 |
| 57) Fluorene-d10               | 15.44 | 176 | 1195280 | 22.89 | ng/ul | 0.00 |
| 62) 4,6-Dinitro-2-methylphenol | 15.56 | 200 | 82603   | 9.10  | ng/ul | 0.00 |
| 70) Anthracene-d10             | 17.29 | 188 | 1792951 | 23.12 | ng/ul | 0.00 |
| 78) Pyrene-d10                 | 19.59 | 212 | 1866631 | 23.00 | ng/ul | 0.00 |
| 89) Benzo(a)pyrene-d12         | 23.52 | 264 | 2048133 | 22.74 | ng/ul | 0.00 |

## Target Compounds

|                                |       |     |          |         | Ovalue    |
|--------------------------------|-------|-----|----------|---------|-----------|
| 6) Phenol                      | 7.00  | 94  | 617034   | 20.323  | ng/ul 99  |
| 10) 2-Chlorophenol             | 7.37  | 128 | 482029   | 19.949  | ng/ul 95  |
| 14) Acetophenone               | 8.63  | 105 | 65010    | 1.773   | ng/ul 96  |
| 15) N-Nitroso-di-n-propylamine | 8.62  | 70  | 383546   | 19.870  | ng/ul 96  |
| 33) 4-Chloro-3-methylphenol    | 11.88 | 107 | 486436   | 21.605  | ng/ul 98  |
| 44) Dimethylphthalate          | 13.90 | 163 | 576858   | 9.376   | ng/ul 99  |
| 47) Acenaphthylene             | 14.17 | 152 | 92683    | 1.230   | ng/ul 98  |
| 49) Acenaphthene               | 14.51 | 153 | 1224856  | 23.278  | ng/ul 98  |
| 52) 4-Nitrophenol              | 14.66 | 109 | 173211   | 20.038  | ng/ul 95  |
| 54) 2,4-Dinitrotoluene         | 14.82 | 165 | 392484   | 23.525  | ng/ul 98  |
| 58) Fluorene                   | 15.50 | 166 | 65856    | 1.102   | ng/ul 100 |
| 68) Pentachlorophenol          | 16.84 | 266 | 277064   | 22.335  | ng/ul 99  |
| 69) Phenanthrene               | 17.23 | 178 | 3790994  | 42.422  | ng/ul 99  |
| 71) Anthracene                 | 17.33 | 178 | 338301   | 3.693   | ng/ul 98  |
| 74) Carbazole                  | 17.60 | 167 | 726999   | 9.126   | ng/ul 98  |
| 76) Fluoranthene               | 19.25 | 202 | 13108065 | 127.997 | ng/ul 98  |
| 79) Pyrene                     | 19.62 | 202 | 12701208 | 122.559 | ng/ul 100 |
| 82) Benzo(a)anthracene         | 21.36 | 228 | 4472163  | 42.702  | ng/ul 96  |
| 84) Chrysene                   | 21.41 | 228 | 7307506  | 75.196  | ng/ul 98  |
| 87) Benzo(b)fluoranthene       | 22.98 | 252 | 11606698 | 100.695 | ng/ul 98  |
| 88) Benzo(k)fluoranthene       | 22.98 | 252 | 11606698 | 105.348 | ng/ul 98  |
| 90) Benzo(a)pyrene             | 23.57 | 252 | 6531637  | 59.562  | ng/ul 95  |
| 91) Indeno(1,2,3-cd)pyrene     | 25.99 | 276 | 6516190  | 50.310  | ng/ul# 94 |

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061019\  
Data File : BM020855.D  
Acq On : 11 Jun 2019 03:13  
Operator : HP/JU  
Sample : K3017-18  
Misc :  
ALS Vial : 28 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :

Quant Time: Jun 11 05:41:50 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM060619MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sun Jun 09 01:02:58 2019  
Response via : Initial Calibration


| Internal Standards         | R.T.  | QIon | Response | Conc   | Units  | Dev(Min) |
|----------------------------|-------|------|----------|--------|--------|----------|
| 92) Dibenzo(a,h)anthracene | 25.99 | 278  | 1417574  | 12.917 | ng/ul# | 82       |
| 93) Benzo(g,h,i)perylene   | 26.71 | 276  | 6069574  | 57.762 | ng/ul  | 96       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061019\  
Data File : BM020855.D  
Acq On : 11 Jun 2019 03:13  
Operator : HP/JU  
Sample : K3017-18  
Misc :  
ALS Vial : 28 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :

Quant Time: Jun 11 05:41:50 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM060619MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sun Jun 09 01:02:58 2019  
Response via : Initial Calibration

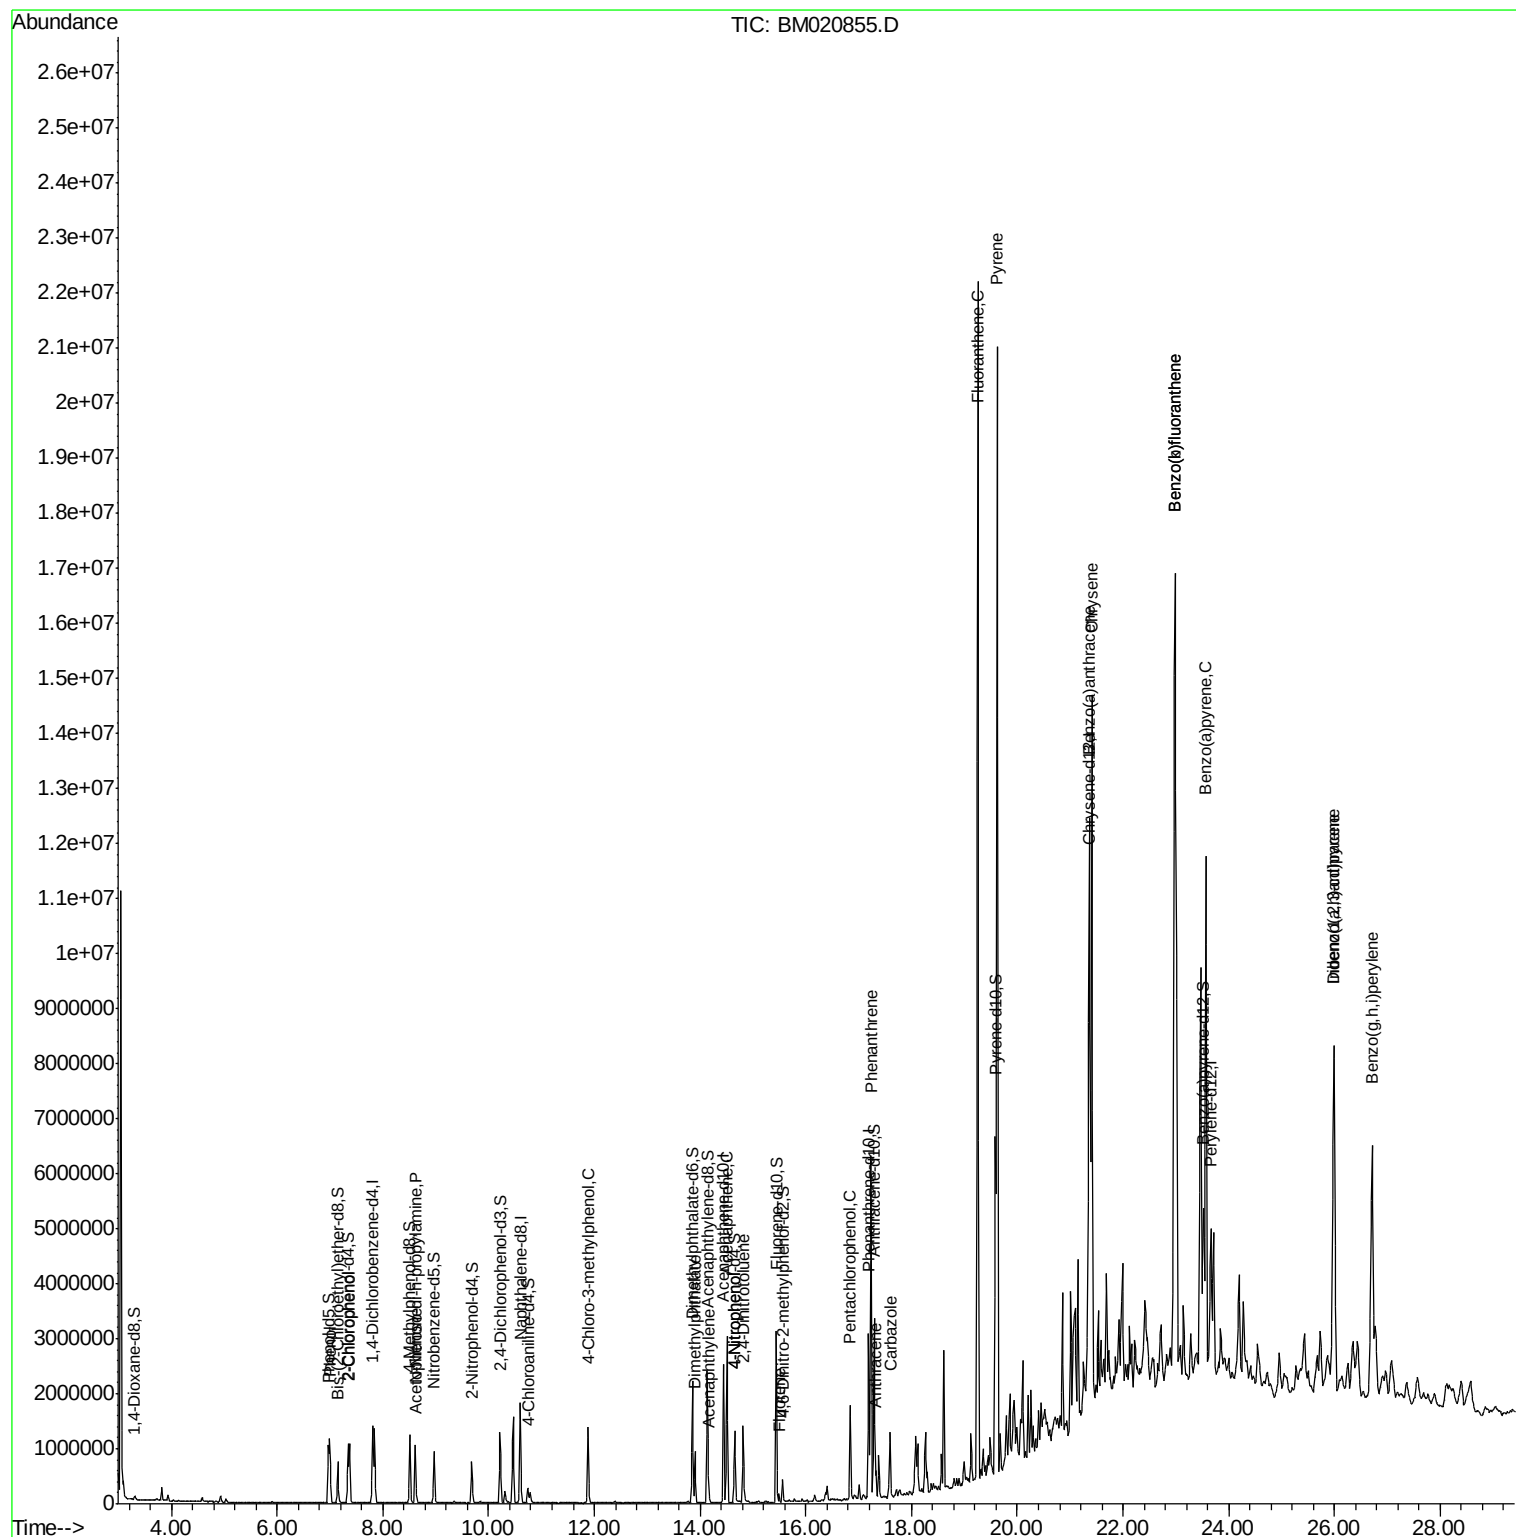

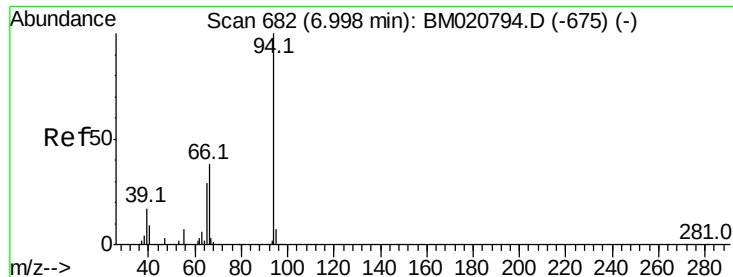





#6

Phenol

Concen: 20.323 ng/ul  
RT: 7.00 min Scan# 682  
Delta R.T. 0.00 min  
Lab File: BM020855.D  
Acq: 11 Jun 2019 03:13

Instrument :  
BNA\_M  
ClientSampleId :

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 94      | 100   |       |       |
| 65      | 28.4  | 23.3  | 34.9  |
| 66      | 39.5  | 32.1  | 48.1  |

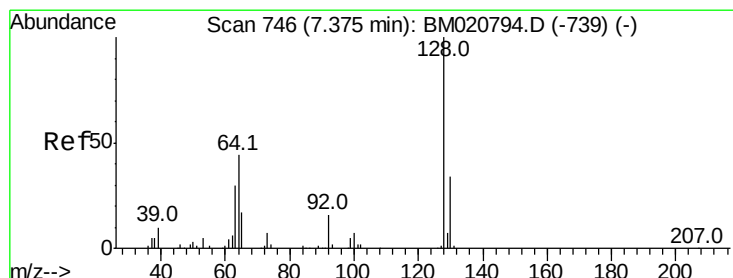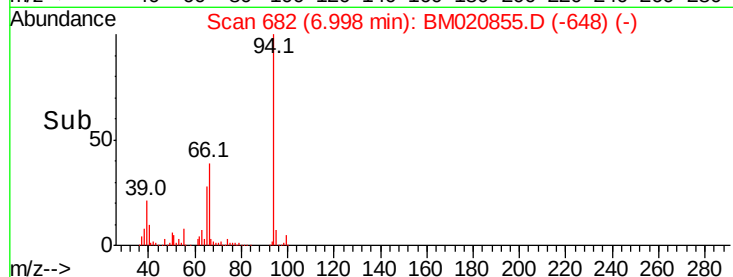
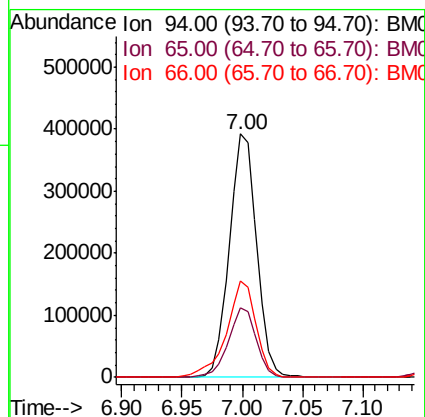
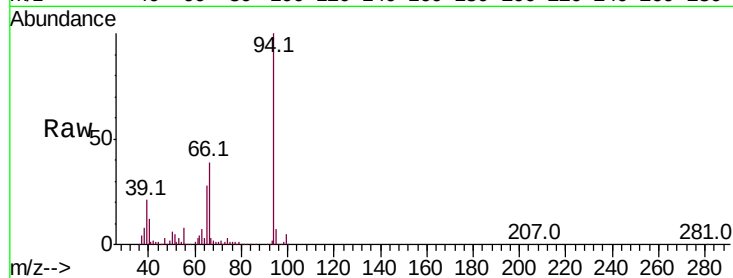



#10

2-Chlorophenol

Concen: 19.949 ng/ul  
RT: 7.37 min Scan# 746  
Delta R.T. 0.00 min  
Lab File: BM020855.D  
Acq: 11 Jun 2019 03:13

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 128     | 100   |       |       |
| 64      | 44.5  | 39.0  | 58.4  |
| 130     | 33.1  | 27.5  | 41.3  |

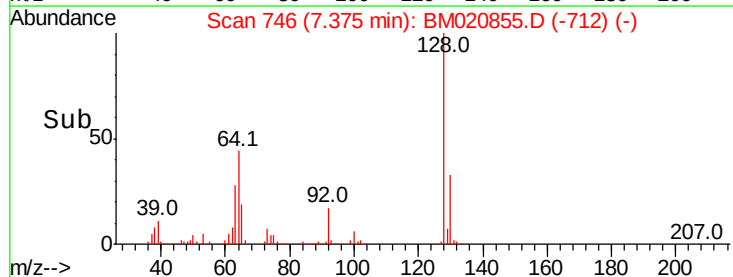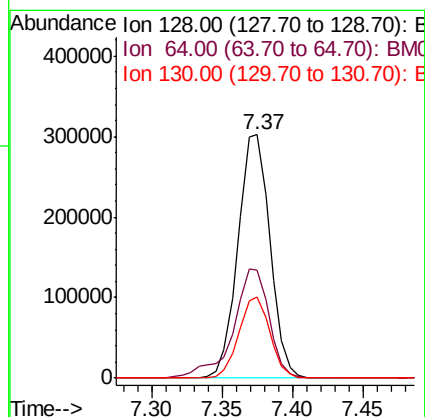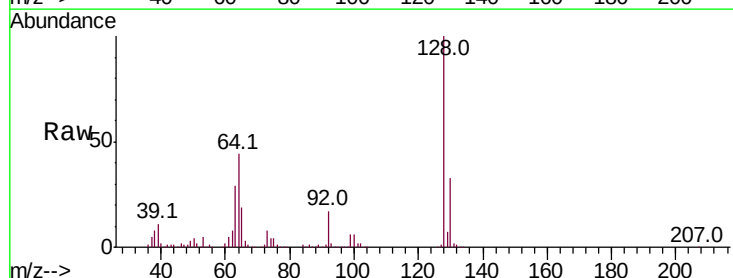

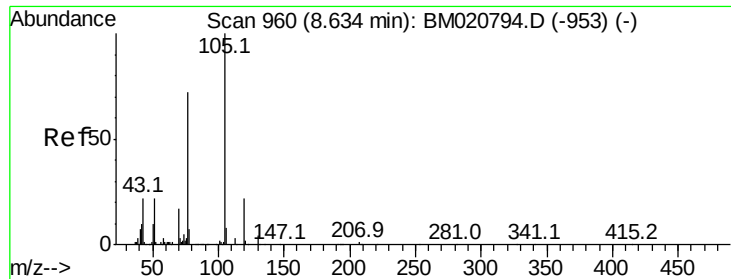

#14

Acetophenone

Concen: 1.773 ng/ul

RT: 8.63 min Scan# 960

Delta R.T. 0.00 min

Lab File: BM020855.D

Acq: 11 Jun 2019 03:13

Instrument :

BNA\_M

ClientSampled :


Tot Ion:105 Resp: 65010

Ion Ratio Lower Upper

105 100

77 77.5 64.6 97.0




51 24.2 21.4 32.2

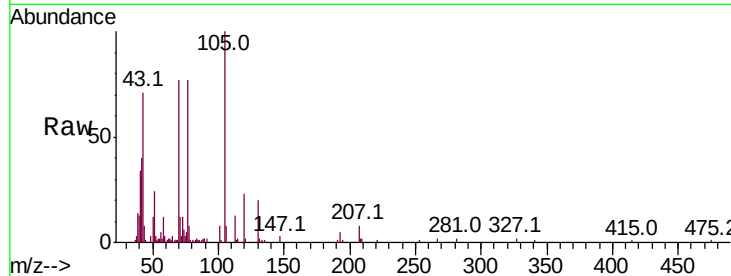

Abundance Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BM0

Ion 51.00 (50.70 to 51.70): BM0

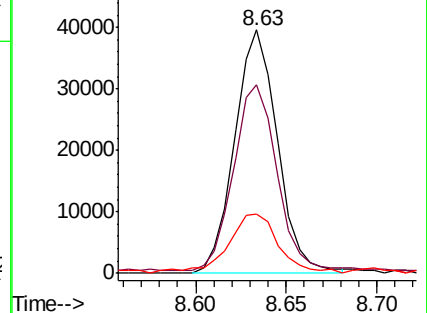

#15

N-Nitroso-di-n-propylamine

Concen: 19.870 ng/ul

RT: 8.62 min Scan# 957

Delta R.T. 0.00 min

Lab File: BM020855.D

Acq: 11 Jun 2019 03:13

Tgt Ion: 70 Resp: 383546


Ion Ratio Lower Upper

70 100

42 51.3 43.6 65.4

101 9.9 8.2 12.2

130 22.1 15.8 23.8






Abundance Ion 70.00 (69.70 to 70.70): BM0

Ion 42.00 (41.70 to 42.70): BM0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

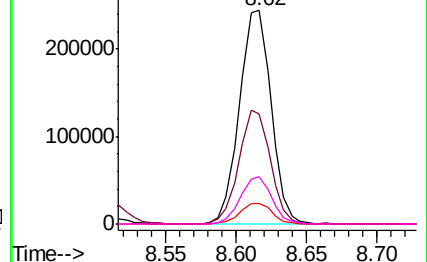







#33  
 4-Chloro-3-methylphenol  
 Concen: 21.605 ng/ul  
 RT: 11.88 min Scan# 1512  
 Delta R.T. -0.01 min  
 Lab File: BM020855.D  
 Acq: 11 Jun 2019 03:13

Instrument :  
 BNA\_M  
 ClientSampleId :

Tot Ion:107 Resp: 486436  
 Ion Ratio Lower Upper  
 107 100  
 144 26.4 21.3 31.9  
 142 80.7 63.2 94.8

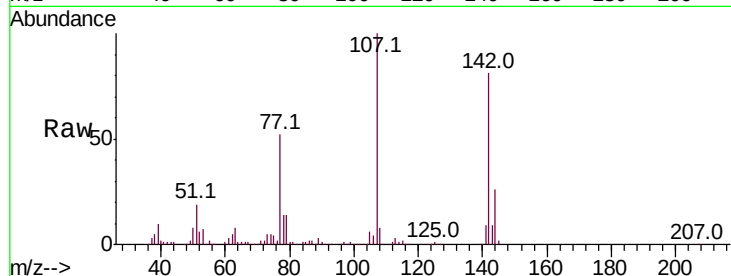


Abundance Ion 107.00 (106.70 to 107.70): E  
 Ion 144.00 (143.70 to 144.70): E  
 Ion 142.00 (141.70 to 142.70): E


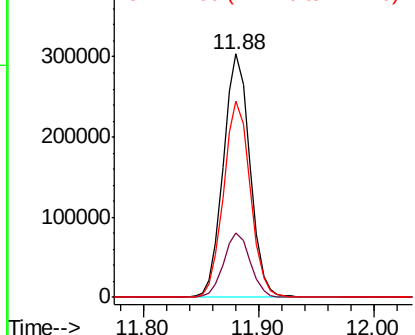



#44  
 Dimethylphthalate  
 Concen: 9.376 ng/ul  
 RT: 13.90 min Scan# 1856  
 Delta R.T. -0.01 min  
 Lab File: BM020855.D  
 Acq: 11 Jun 2019 03:13

Tgt Ion:163 Resp: 576858  
 Ion Ratio Lower Upper  
 163 100  
 194 3.9 3.2 4.8  
 164 10.3 8.0 12.0



Abundance Ion 163.00 (162.70 to 163.70): E  
 Ion 194.00 (193.70 to 194.70): E  
 Ion 164.00 (163.70 to 164.70): E




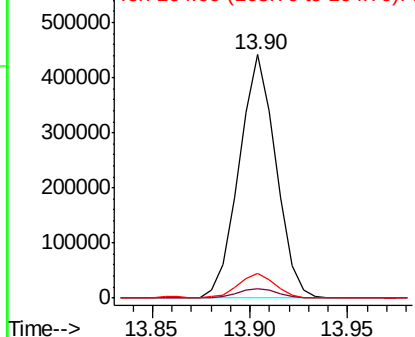


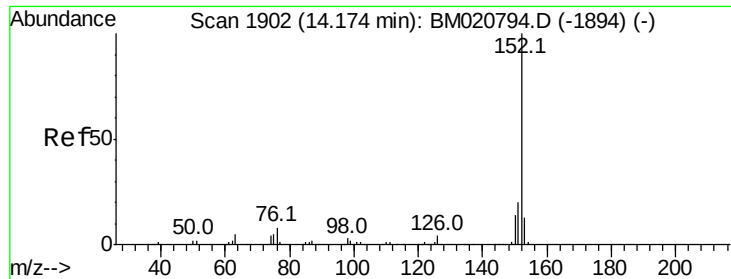

#47  
Acenaphthylene  
Concen: 1.230 ng/ul  
RT: 14.17 min Scan# 1901  
Delta R.T. 0.00 min  
Lab File: BM020855.D  
Acq: 11 Jun 2019 03:13




Instrument :  
BNA\_M  
ClientSampleId :


Tot Ion:152 Resp: 92683  
Ion Ratio Lower Upper  
152 100  
151 21.2 16.2 24.2  
153 13.8 10.6 15.8

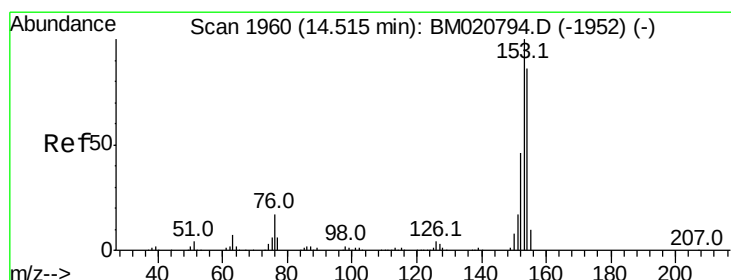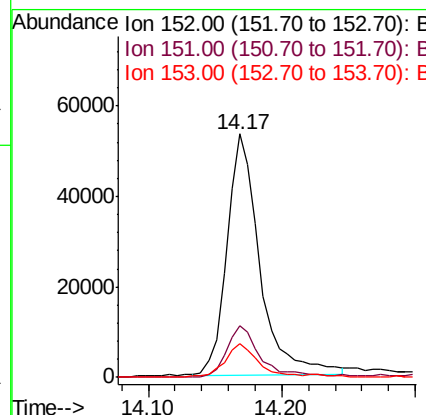

#49  
Acenaphthene  
Concen: 23.278 ng/ul  
RT: 14.51 min Scan# 1959  
Delta R.T. -0.01 min  
Lab File: BM020855.D  
Acq: 11 Jun 2019 03:13

Tgt Ion:153 Resp: 1224856  
Ion Ratio Lower Upper  
153 100  
152 46.5 37.3 55.9  
154 88.7 68.7 103.1

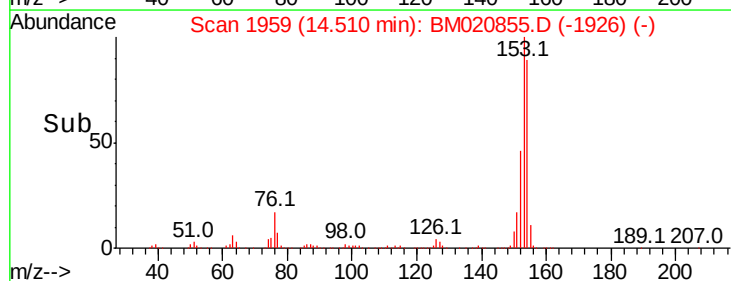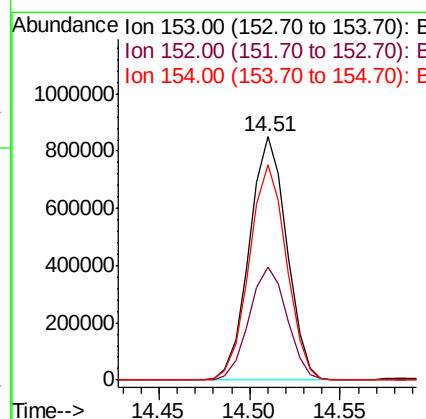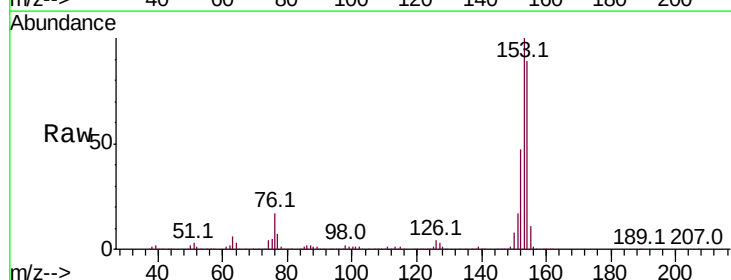

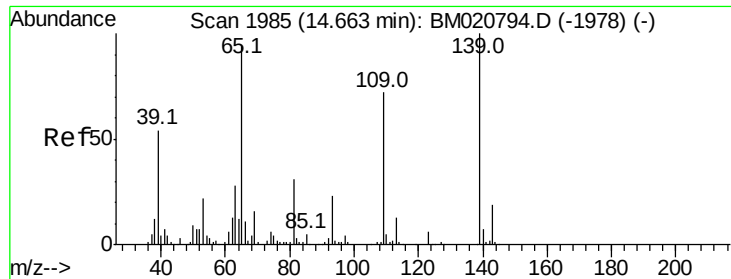

#52

4-Nitrophenol

Concen: 20.038 ng/ul

RT: 14.66 min Scan# 1985

Delta R.T. 0.00 min

Lab File: BM020855.D

Acq: 11 Jun 2019 03:13

Instrument :

BNA\_M

ClientSampleId :


Tot Ion:109 Resp: 173211

Ion Ratio Lower Upper

109 100

139 129.1 105.9 158.9




65 124.2 106.2 159.4

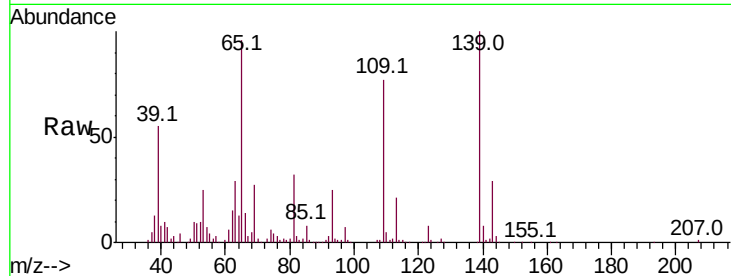

Abundance Ion 109.00 (108.70 to 109.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 65.00 (64.70 to 65.70): BM

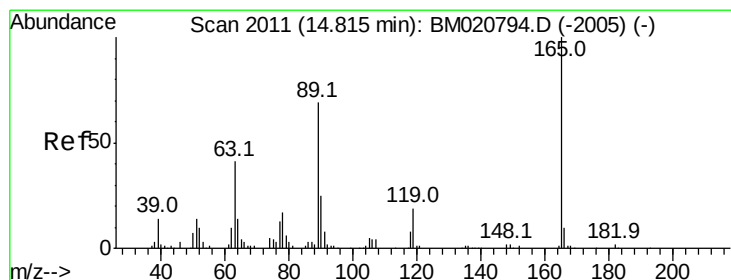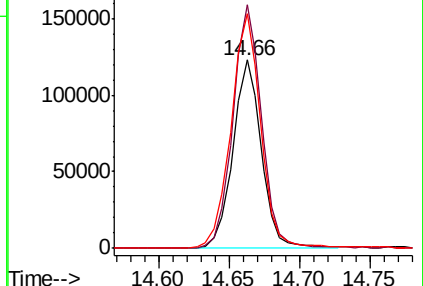

#54

2,4-Dinitrotoluene

Concen: 23.525 ng/ul

RT: 14.82 min Scan# 2011

Delta R.T. 0.00 min

Lab File: BM020855.D

Acq: 11 Jun 2019 03:13


Tgt Ion:165 Resp: 392484

Ion Ratio Lower Upper

165 100

63 38.0 31.7 47.5



182 2.9 2.2 3.4




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BM

Ion 182.00 (181.70 to 182.70): E

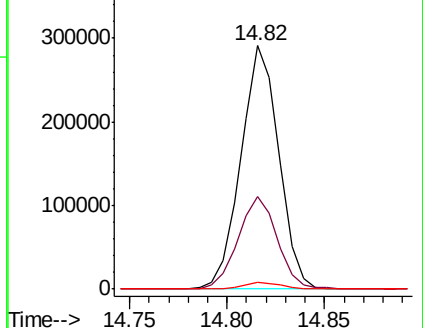









#58  
 Fluorene  
 Concen: 1.102 ng/ul  
 RT: 15.50 min Scan# 2127  
 Delta R.T. 0.00 min  
 Lab File: BM020855.D  
 Acq: 11 Jun 2019 03:13

Instrument :  
 BNA\_M  
 ClientSampleId :

Tot Ion:166 Resp: 65856  
 Ion Ratio Lower Upper  
 166 100  
 165 98.5 78.6 117.8  
 167 12.9 10.8 16.2

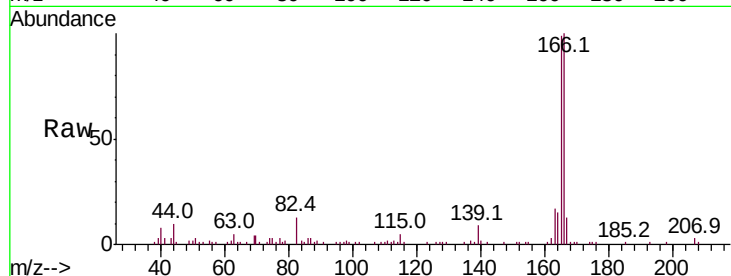


Abundance Ion 166.00 (165.70 to 166.70): E  
 Ion 165.00 (164.70 to 165.70): E  
 Ion 167.00 (166.70 to 167.70): E


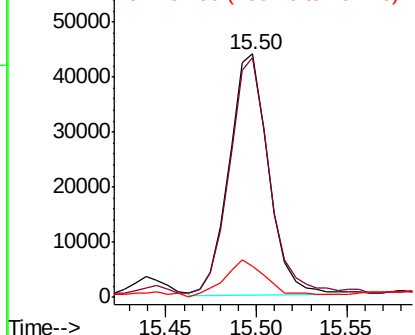



#68  
 Pentachlorophenol  
 Concen: 22.335 ng/ul  
 RT: 16.84 min Scan# 2355  
 Delta R.T. 0.00 min  
 Lab File: BM020855.D  
 Acq: 11 Jun 2019 03:13

Tgt Ion:266 Resp: 277064  
 Ion Ratio Lower Upper  
 266 100  
 264 63.7 50.3 75.5  
 268 63.0 51.2 76.8



Abundance Ion 265.70 (265.40 to 266.40): E  
 Ion 264.00 (263.70 to 264.70): E  
 Ion 268.00 (267.70 to 268.70): E

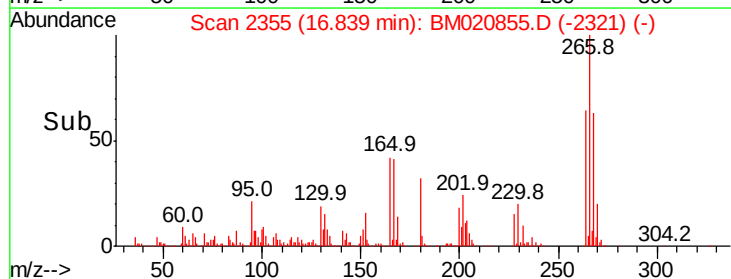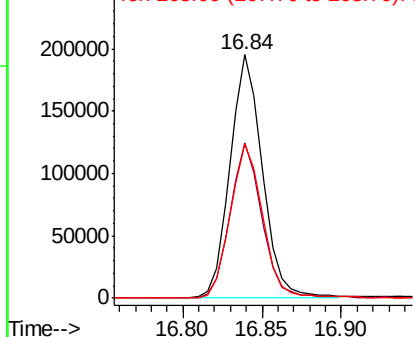

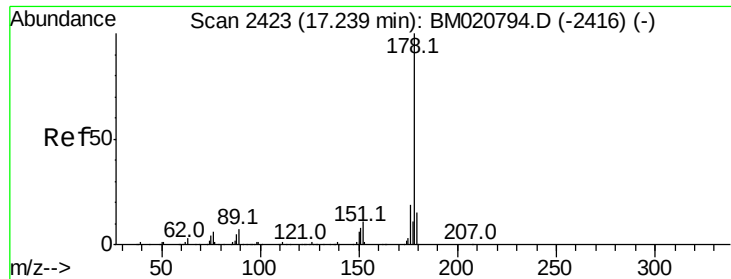

#69

Phenanthrene

Concen: 42.422 ng/ul

RT: 17.23 min Scan# 2422

Delta R.T. -0.01 min

Lab File: BM020855.D

Acq: 11 Jun 2019 03:13

Instrument :

BNA\_M

ClientSampleId :


Tot Ion:178 Resp: 3790994

Ion Ratio Lower Upper

178 100

179 15.7 12.3 18.5




176 19.4 14.8 22.2



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

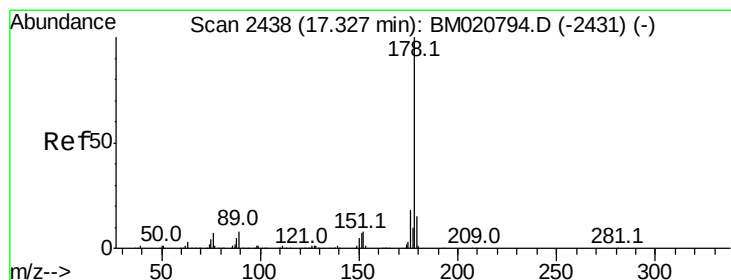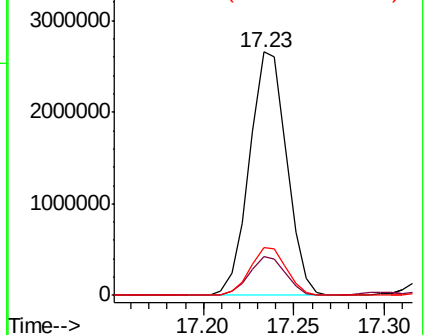

#71

Anthracene

Concen: 3.693 ng/ul

RT: 17.33 min Scan# 2438

Delta R.T. 0.00 min

Lab File: BM020855.D

Acq: 11 Jun 2019 03:13


Tgt Ion:178 Resp: 338301

Ion Ratio Lower Upper

178 100

179 15.2 12.1 18.1



176 17.2 14.9 22.3




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E




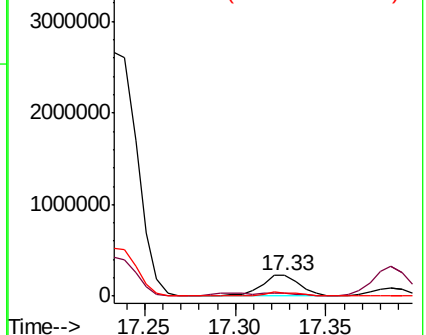


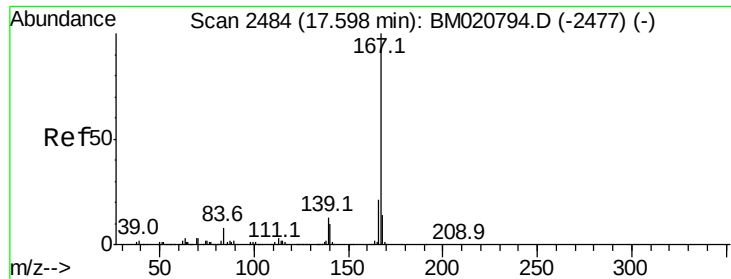

#74  
 Carbazole  
 Concen: 9.126 ng/ul  
 RT: 17.60 min Scan# 2484  
 Delta R.T. 0.00 min  
 Lab File: BM020855.D  
 Acq: 11 Jun 2019 03:13




Instrument :  
 BNA\_M  
 ClientSampleId :


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 167     | 100   |       |       |
| 166     | 22.1  | 17.0  | 25.6  |
| 139     | 12.4  | 10.5  | 15.7  |

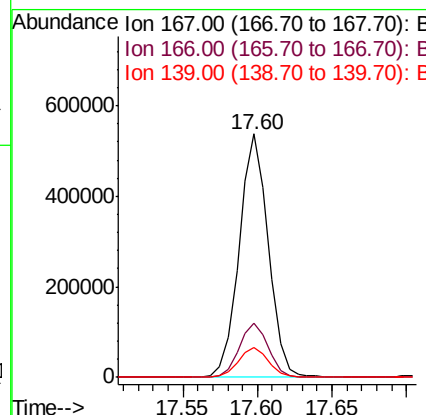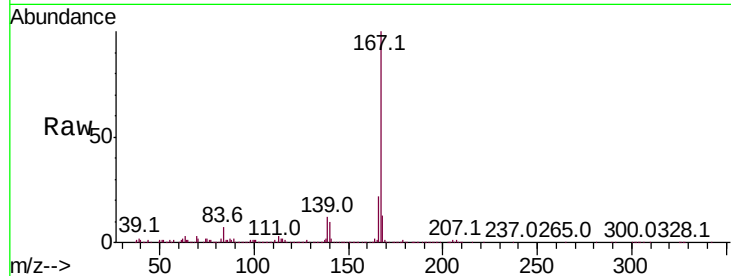

#76  
 Fluoranthene  
 Concen: 127.997 ng/ul  
 RT: 19.25 min Scan# 2765  
 Delta R.T. 0.00 min  
 Lab File: BM020855.D  
 Acq: 11 Jun 2019 03:13

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 202     | 100   |       |       |
| 101     | 10.6  | 7.9   | 11.9  |
| 100     | 8.2   | 6.2   | 9.4   |

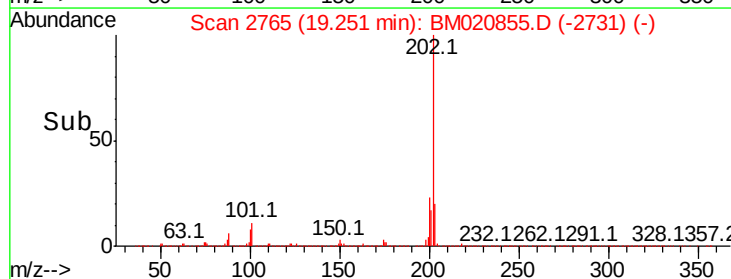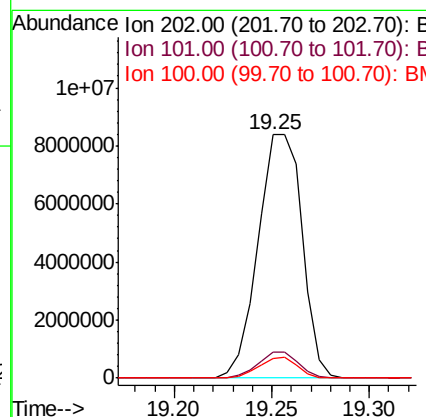







#79  
Pvrene  
Concen: 122.559 ng/ul  
RT: 19.62 min Scan# 2828  
Delta R.T. 0.01 min  
Lab File: BM020855.D  
Acq: 11 Jun 2019 03:13

Instrument :  
BNA\_M  
ClientSampleId :

Tot Ion:202 Resp:12701208  
Ion Ratio Lower Upper  
202 100  
101 11.9 9.8 14.6  
100 10.0 8.0 12.0




Abundance Ion 202.00 (201.70 to 202.70): E  
Ion 101.00 (100.70 to 101.70): E  
Ion 100.00 (99.70 to 100.70): B


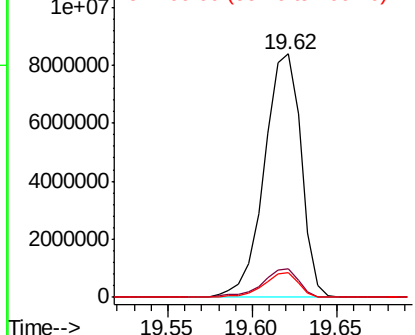



#82  
Benzo(a)anthracene  
Concen: 42.702 ng/ul  
RT: 21.36 min Scan# 3123  
Delta R.T. 0.00 min  
Lab File: BM020855.D  
Acq: 11 Jun 2019 03:13

Tgt Ion:228 Resp: 4472163  
Ion Ratio Lower Upper  
228 100  
229 20.8 15.6 23.4  
226 29.2 21.4 32.2



Abundance Ion 228.00 (227.70 to 228.70): E  
Ion 229.00 (228.70 to 229.70): E  
Ion 226.00 (225.70 to 226.70): E

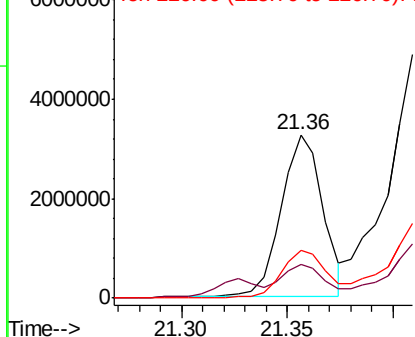



#84

Chrysene

Concen: 75.196 ng/ul

RT: 21.41 min Scan# 3132

Delta R.T. 0.00 min

Lab File: BM020855.D

Acq: 11 Jun 2019 03:13


Instrument :

BNA\_M

ClientSampleId :

Tot Ion:228 Resp: 7307506




| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 228 | 100   |       |       |
| 226 | 30.9  | 24.4  | 36.6  |
| 229 | 22.1  | 16.2  | 24.2  |



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

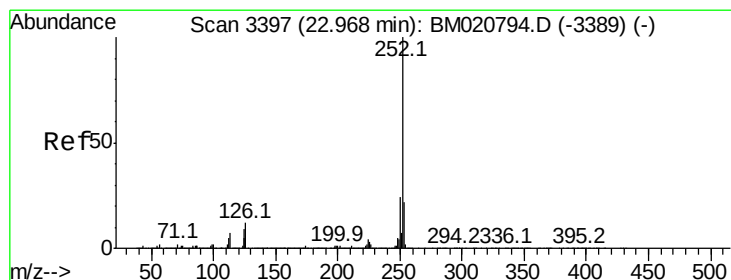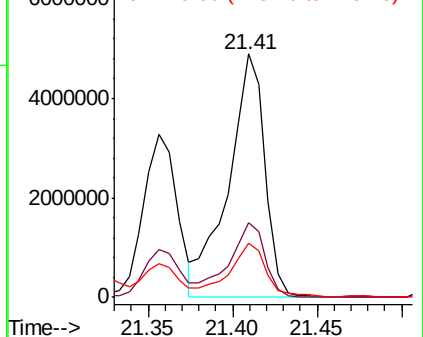

#87

Benzo(b)fluoranthene

Concen: 100.695 ng/ul

RT: 22.98 min Scan# 3399


Delta R.T. 0.01 min

Lab File: BM020855.D

Acq: 11 Jun 2019 03:13

Tgt Ion:252 Resp:11606698



| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 252 | 100   |       |       |
| 253 | 23.2  | 17.6  | 26.4  |
| 125 | 8.9   | 7.3   | 10.9  |




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

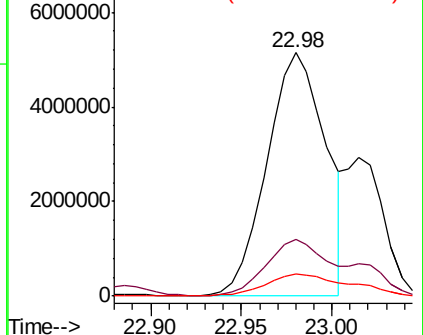

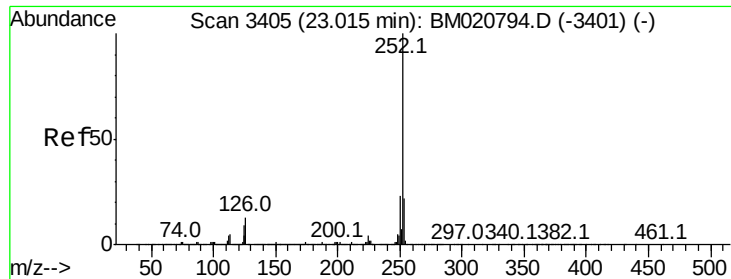

#88

Benzo(k)fluoranthene

Concen: 105.348 ng/ul

RT: 22.98 min Scan# 3399

Delta R.T. -0.04 min

Lab File: BM020855.D

Acq: 11 Jun 2019 03:13

Instrument :

BNA\_M

ClientSampleId :


Tot Ion:252 Resp:11606698

Ion Ratio Lower Upper




252 100

253 23.2 17.6 26.4

125 8.9 7.3 10.9



Abundance Ion 252.00 (251.70 to 252.70): E  
Ion 253.00 (252.70 to 253.70): E  
Ion 125.00 (124.70 to 125.70): E

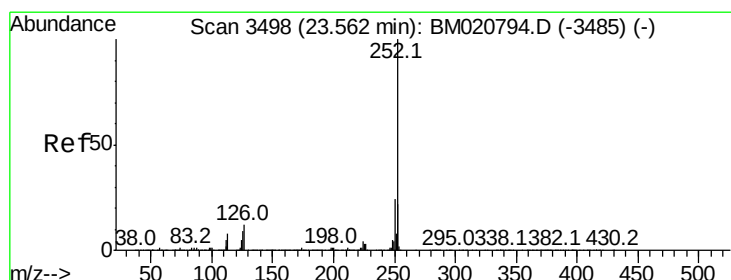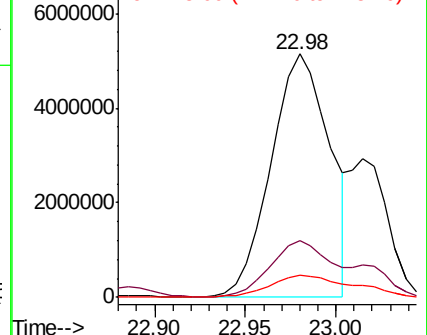

#90

Benzo(a)pyrene

Concen: 59.562 ng/ul

RT: 23.57 min Scan# 3499

Delta R.T. 0.01 min

Lab File: BM020855.D

Acq: 11 Jun 2019 03:13


Tgt Ion:252 Resp: 6531637

Ion Ratio Lower Upper



252 100


253 23.7 17.0 25.6

125 9.0 8.2 12.4



Abundance Ion 252.00 (251.70 to 252.70): E  
Ion 253.00 (252.70 to 253.70): E  
Ion 125.00 (124.70 to 125.70): E




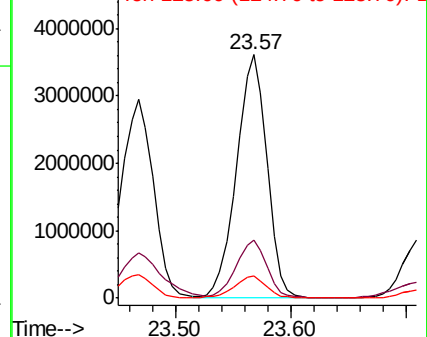




#91  
 Indeno(1,2,3-cd)pyrene  
 Concen: 50.310 ng/ul  
 RT: 25.99 min Scan# 3911  
 Delta R.T. 0.02 min  
 Lab File: BM020855.D  
 Acq: 11 Jun 2019 03:13




Instrument :  
 BNA\_M  
 ClientSampleId :


Tot Ion:276 Resp: 6516190  
 Ion Ratio Lower Upper  
 276 100  
 138 16.9 17.8 26.8#  
 277 24.8 20.0 30.0

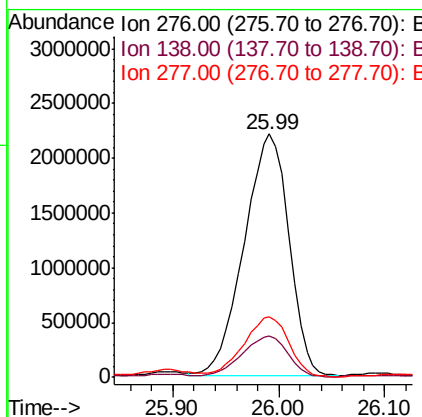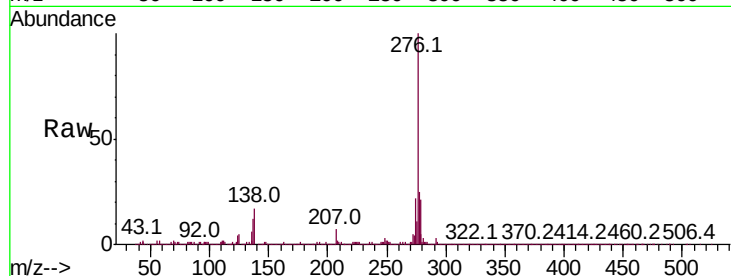

#92  
 Dibenzo(a,h)anthracene  
 Concen: 12.917 ng/ul  
 RT: 25.99 min Scan# 3911  
 Delta R.T. 0.01 min  
 Lab File: BM020855.D  
 Acq: 11 Jun 2019 03:13

Tgt Ion:278 Resp: 1417574  
 Ion Ratio Lower Upper  
 278 100  
 139 0.0 11.6 17.4#  
 279 26.7 18.6 28.0

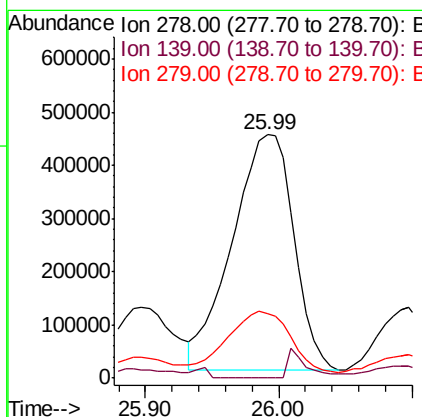

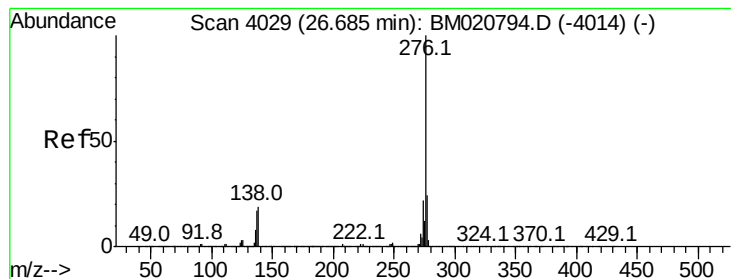

#93

Benzo(a,h,i)perylene

Concen: 57.762 ng/ul

RT: 26.71 min Scan# 4033

Delta R.T. 0.02 min

Lab File: BM020855.D

Acq: 11 Jun 2019 03:13

Instrument :

BNA\_M

ClientSampleId :


Tot Ion:276 Resp: 6069574

Ion Ratio Lower Upper

276 100

138 17.3 16.6 25.0

277 24.3 19.6 29.4



Abundance Ion 276.00 (275.70 to 276.70): E

2500000 Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

