

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061019\
 Data File : BM020849.D
 Acq On : 10 Jun 2019 23:00
 Operator : HP/JU
 Sample : K3006-20
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFHC7

Quant Time: Jun 11 00:24:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jun 09 01:02:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	277760	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	1179404	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	680280	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	1444477	20.00	ng/ul	0.00
77) Chrysene-d12	21.37	240	1230976	20.00	ng/ul	0.00
85) Perylene-d12	23.65	264	1377451	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	17690	3.04	ng/uL	0.00
5) Phenol-d5	6.97	99	303330	14.27	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	205963	16.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	265532	15.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	239656	14.02	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	133690	16.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	140370	16.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	264564	15.31	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	333921	16.04	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	898092	17.85	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	1005633	15.76	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	65471	7.58	ng/ul	0.00
57) Fluorene-d10	15.44	176	716377	16.75	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	44280	5.99	ng/ul	0.00
70) Anthracene-d10	17.29	188	1008562	15.98	ng/ul	0.00
78) Pyrene-d10	19.58	212	1028919	17.29	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.50	264	1006050	16.07	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.90	163	323292	6.416	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061019\
Data File : BM020849.D
Acq On : 10 Jun 2019 23:00
Operator : HP/JU
Sample : K3006-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFHC7

Quant Time: Jun 11 00:24:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jun 09 01:02:58 2019
Response via : Initial Calibration

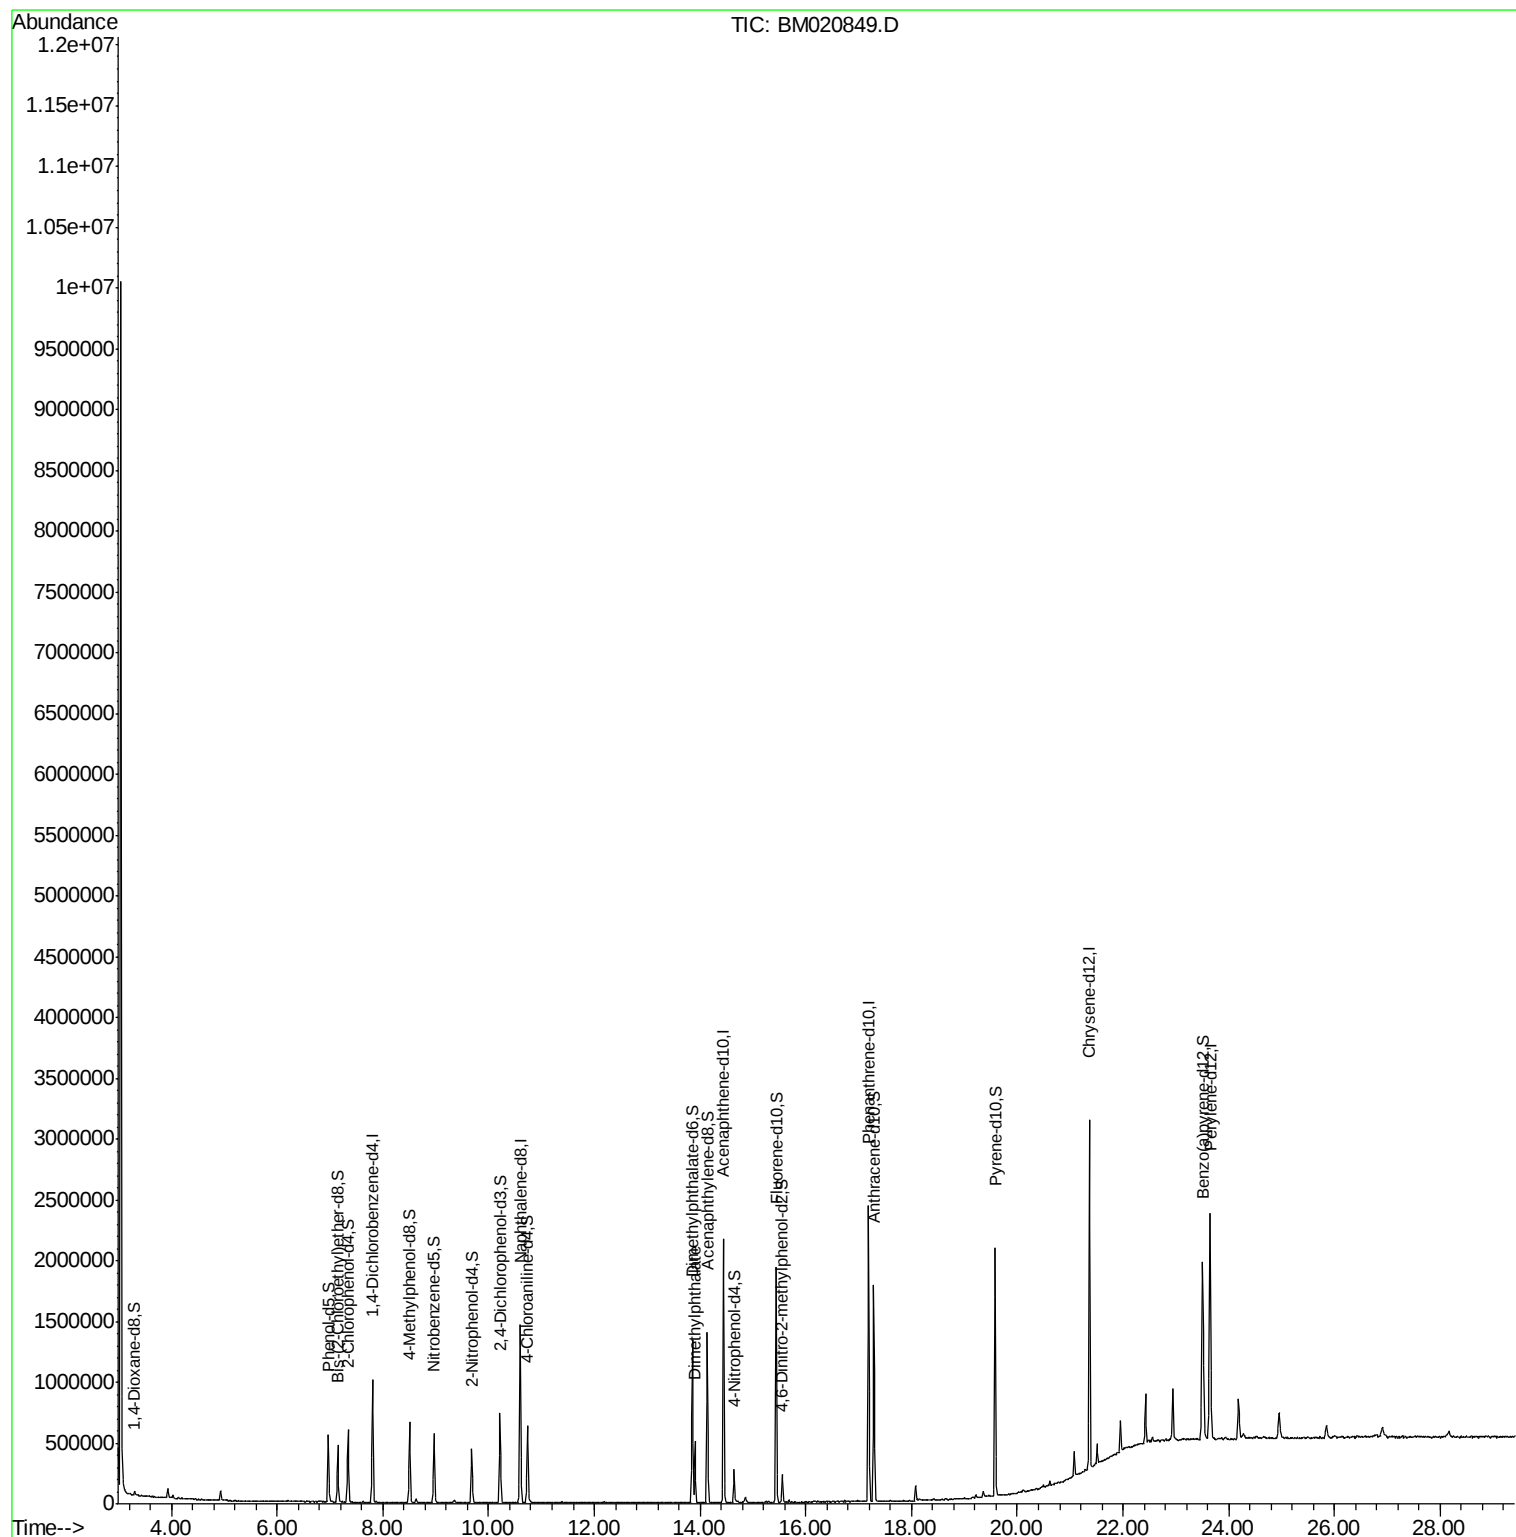

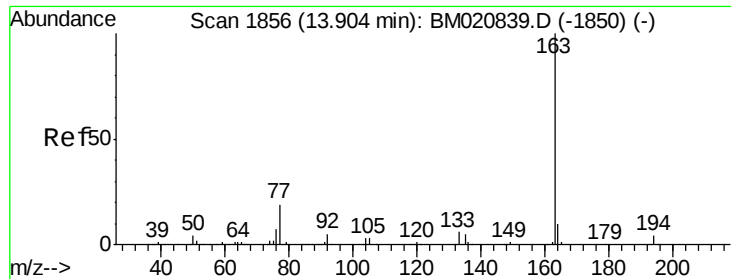

#44

Dimethylphthalate

Concen: 6.416 ng/ul

RT: 13.90 min Scan# 1856

Delta R.T. -0.01 min

Lab File: BM020849.D

Acq: 10 Jun 2019 23:00

Instrument :

BNA_M

ClientSampleId :

BFHC7


Tot Ion:163 Resp: 323292

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 10.4 8.0 12.0

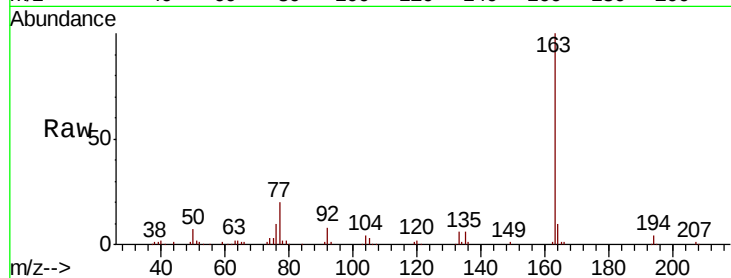

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

