

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061118\
 Data File : BM015610.D
 Acq On : 11 Jun 2018 18:41
 Operator : SJ/JU
 Sample : J3346-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 12 03:11:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 12 03:10:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.34	152	72185	20.00	ng/ul	0.00
18) Naphthalene-d8	11.17	136	354424	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	223469	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.68	188	554159	20.00	ng/ul	0.00
77) Chrysene-d12	21.79	240	709338	20.00	ng/ul	0.00
85) Perylene-d12	24.20	264	825446	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.55	96	7797	5.25	ng/uL	0.00
5) Phenol-d5	7.48	99	163716	24.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.66	67	114070	28.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.86	132	141726	28.28	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	124601	22.07	ng/ul	0.00
19) Nitrobenzene-d5	9.53	128	68630	28.80	ng/ul	0.00
22) 2-Nitrophenol-d4	10.25	143	75633	29.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.79	165	150100	28.28	ng/ul	0.00
29) 4-Chloroaniline-d4	11.31	131	112196	18.97	ng/ul	0.00
43) Dimethylphthalate-d6	14.36	166	542156	29.30	ng/ul	0.00
46) Acenaphthylene-d8	14.66	160	636802	31.91	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	74790	20.94	ng/ul	0.00
57) Fluorene-d10	15.94	176	480501	30.69	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	65453	19.61	ng/ul	0.00
70) Anthracene-d10	17.78	188	747179	29.58	ng/ul	0.00
78) Pyrene-d10	20.03	212	928897	30.44	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.04	264	1243198	30.05	ng/ul	0.00

Target Compounds


					Ovalue	
6) Phenol	7.51	94	19429	2.854	ng/ul#	84
44) Dimethylphthalate	14.40	163	194385	10.289	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061118\
Data File : BM015610.D
Acq On : 11 Jun 2018 18:41
Operator : SJ/JU
Sample : J3346-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 12 03:11:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 12 03:10:28 2018
Response via : Initial Calibration

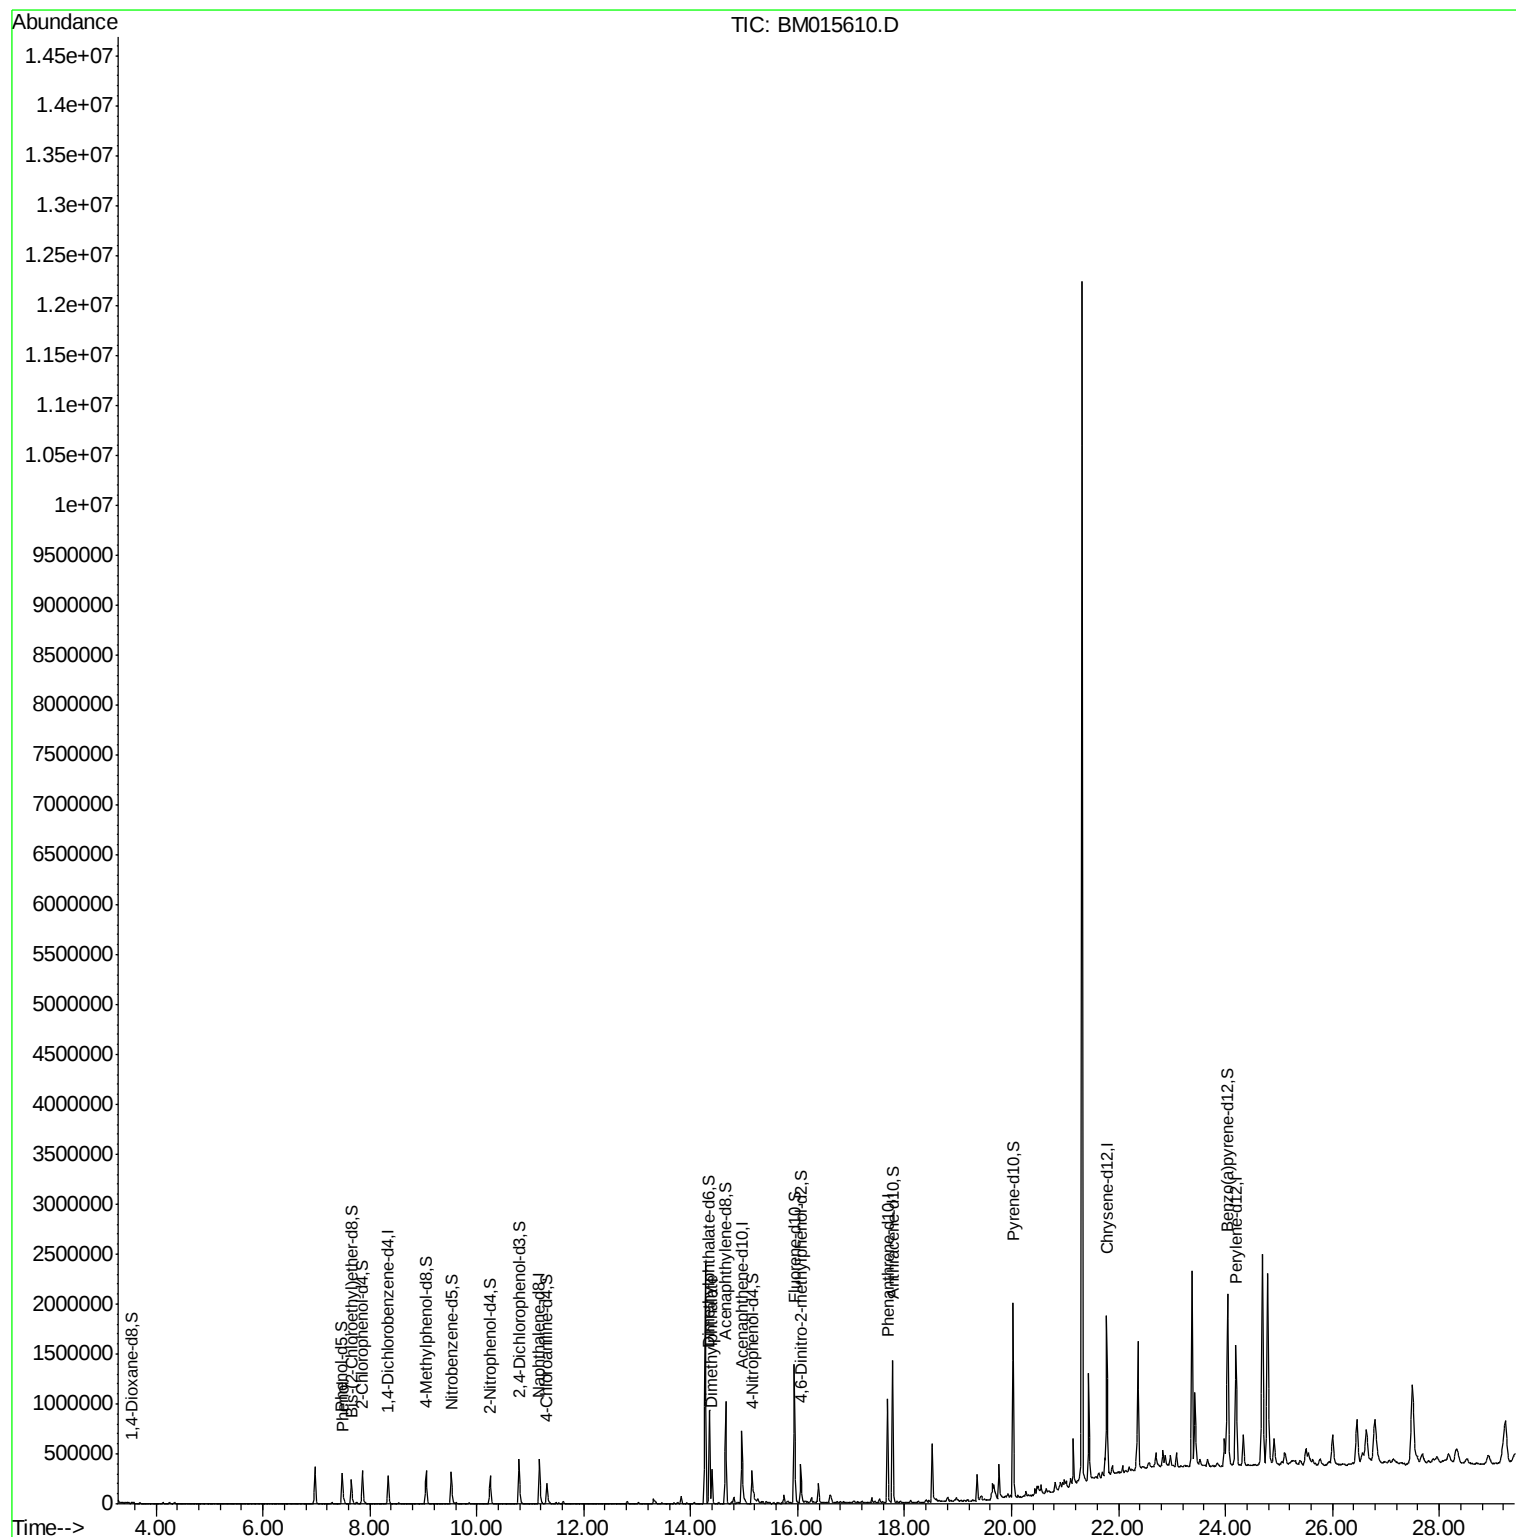

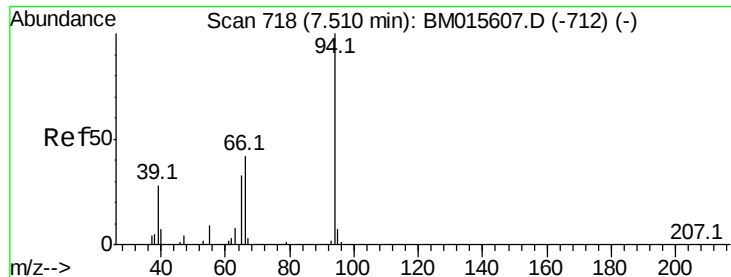

#6

Phenol

Concen: 2.854 ng/ul

RT: 7.51 min Scan# 718

Delta R.T. 0.00 min

Lab File: BM015610.D

Acq: 11 Jun 2018 18:41

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 94 Resp: 19429

Ion Ratio Lower Upper




94 100

65 31.2 21.0 31.6

66 48.9 29.3 43.9#

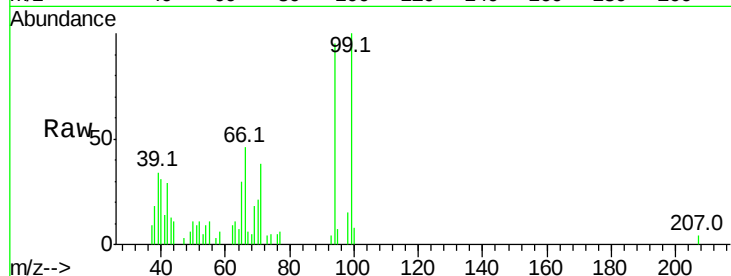

Abundance Ion 94.00 (93.70 to 94.70): BM015610.D (-684) (-)

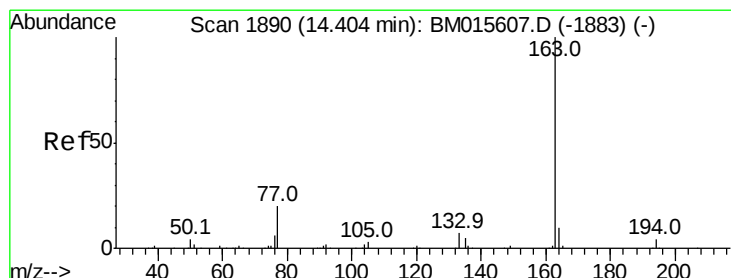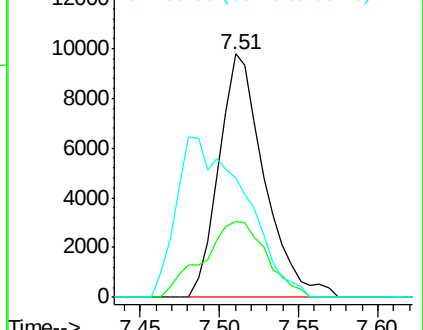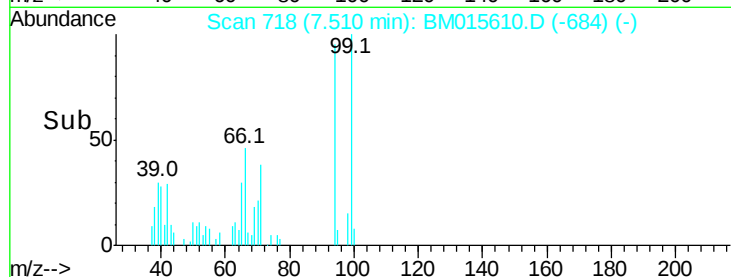

#44

Dimethylphthalate

Concen: 10.289 ng/ul

RT: 14.40 min Scan# 1890

Delta R.T. 0.00 min

Lab File: BM015610.D

Acq: 11 Jun 2018 18:41


Tgt Ion:163 Resp: 194385

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 10.2 7.8 11.8

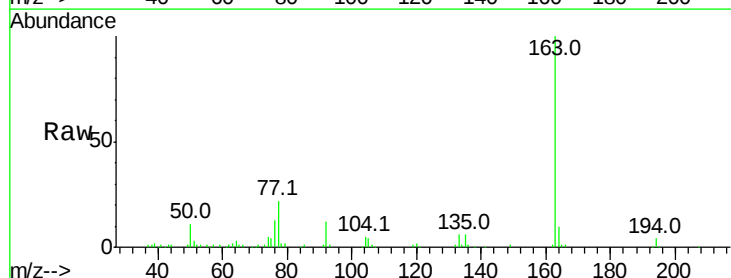

Abundance Ion 163.00 (162.70 to 163.70): BM015610.D (-1856) (-)

