

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061118\
 Data File : BM015611.D
 Acq On : 11 Jun 2018 19:19
 Operator : SJ/JU
 Sample : J3346-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 12 03:12:03 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 12 03:10:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.34	152	32825	20.00	ng/ul	0.00
18) Naphthalene-d8	11.17	136	155226	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	106006	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.68	188	282054	20.00	ng/ul	0.00
77) Chrysene-d12	21.79	240	409941	20.00	ng/ul	0.00
85) Perylene-d12	24.20	264	526374	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.55	96	3272	4.84	ng/uL	0.00
5) Phenol-d5	7.49	99	62700	21.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.66	67	43417	24.12	ng/ul	0.00
9) 2-Chlorophenol-d4	7.86	132	53061	23.29	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	54855	21.37	ng/ul	0.00
19) Nitrobenzene-d5	9.53	128	24794	23.76	ng/ul	0.00
22) 2-Nitrophenol-d4	10.25	143	26941	24.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.79	165	53284	22.92	ng/ul	0.00
29) 4-Chloroaniline-d4	11.31	131	77666	29.98	ng/ul	0.00
43) Dimethylphthalate-d6	14.36	166	238043	27.12	ng/ul	0.00
46) Acenaphthylene-d8	14.66	160	253786	26.81	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	33994	20.07	ng/ul	0.00
57) Fluorene-d10	15.94	176	206653	27.83	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	24421	14.37	ng/ul	0.00
70) Anthracene-d10	17.77	188	349681	27.19	ng/ul	0.00
78) Pyrene-d10	20.03	212	446696	25.33	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.04	264	725611	27.50	ng/ul	0.00
Target Compounds						
6) Phenol	7.51	94	6807	2.199	ng/ul#	75
44) Dimethylphthalate	14.40	163	78309	8.738	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061118\
Data File : BM015611.D
Acq On : 11 Jun 2018 19:19
Operator : SJ/JU
Sample : J3346-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 12 03:12:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 12 03:10:28 2018
Response via : Initial Calibration

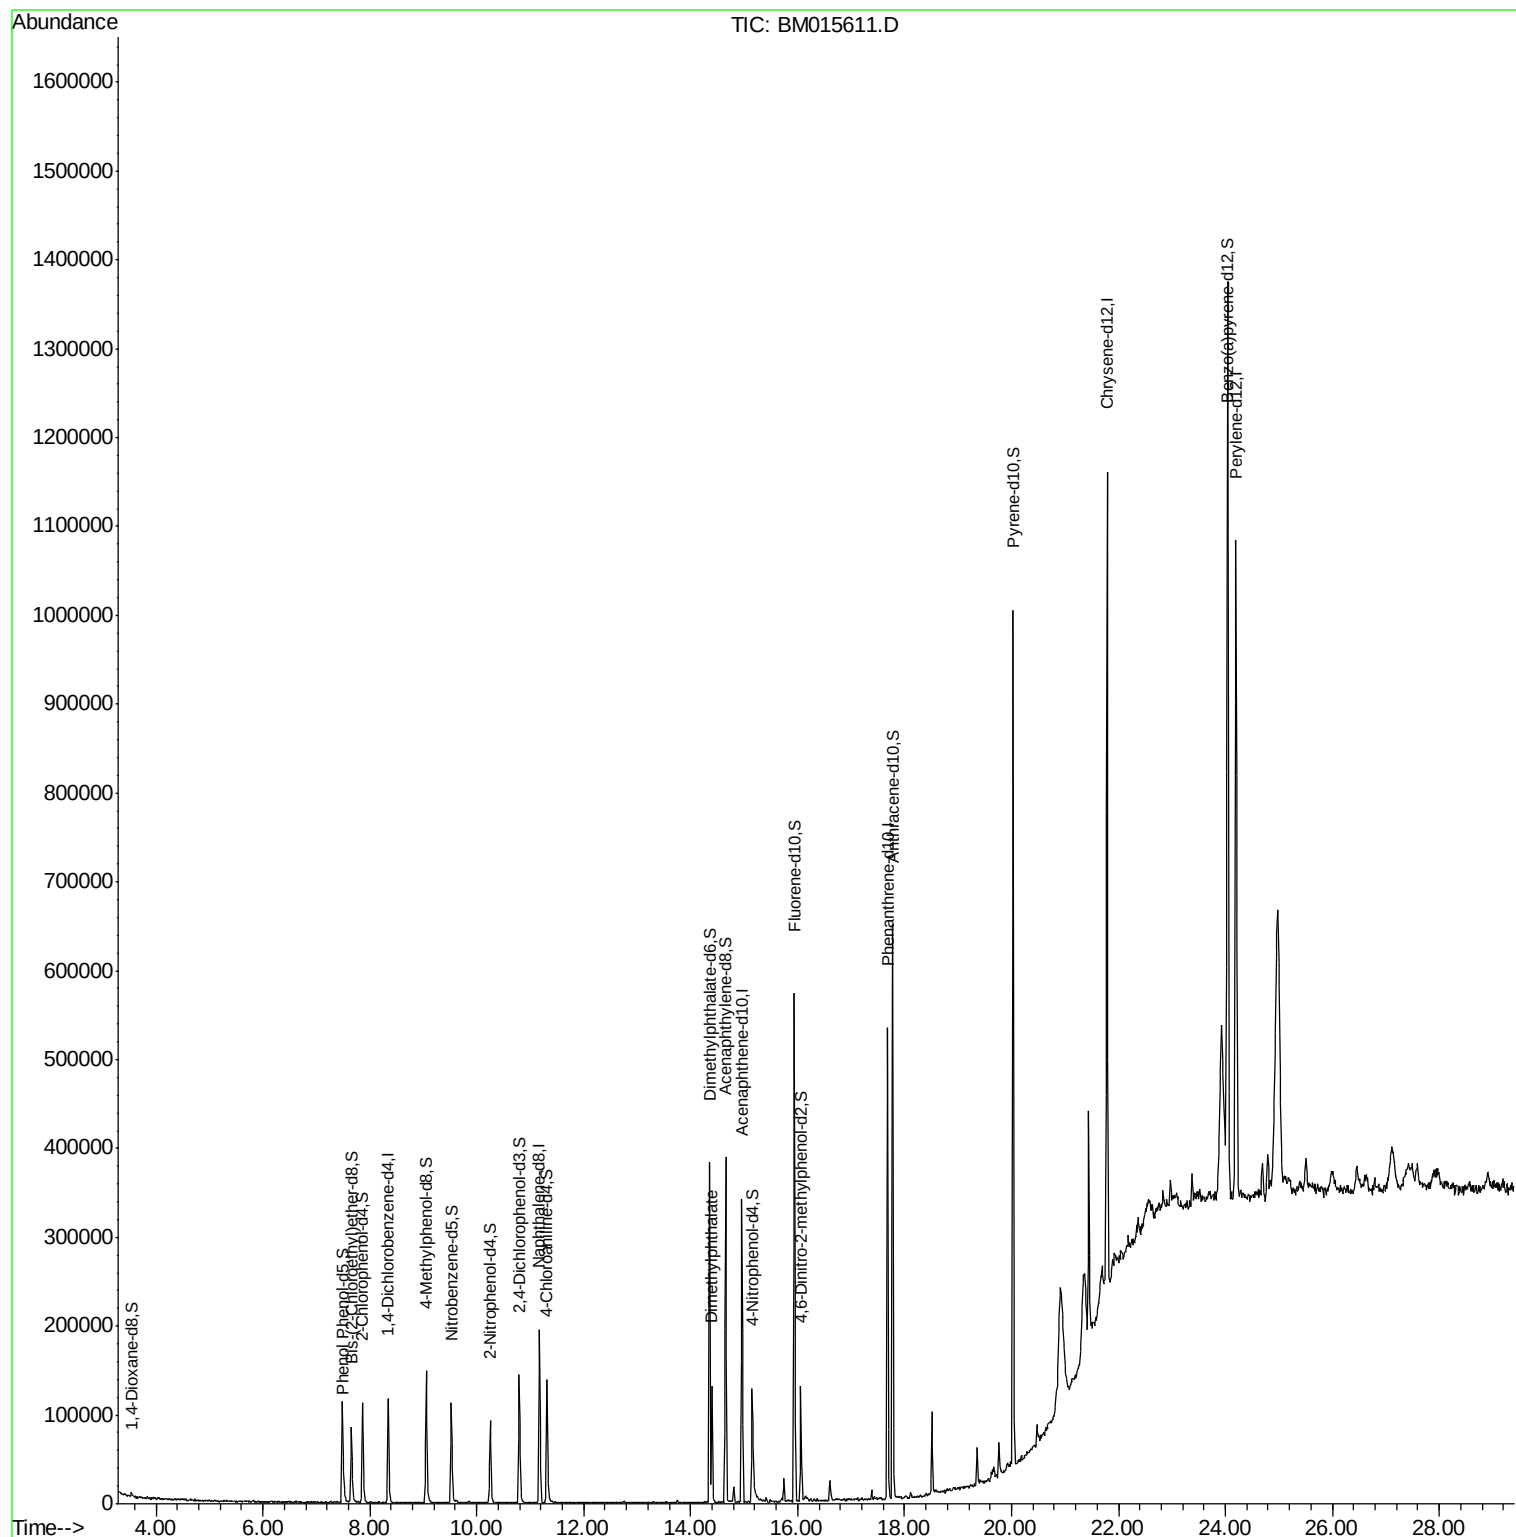

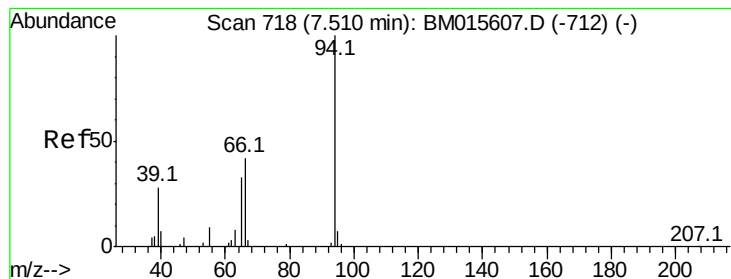

#6

Phenol

Concen: 2.199 ng/ul

RT: 7.51 min Scan# 718

Delta R.T. 0.00 min

Lab File: BM015611.D

Acq: 11 Jun 2018 19:19

Instrument :

BNA_M

ClientSampleId :





Tot Ion: 94 Resp: 6807

Ion Ratio Lower Upper

94 100

65 36.1 21.0 31.6#

66 54.1 29.3 43.9#

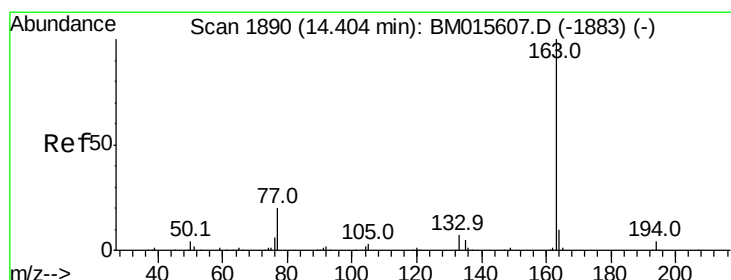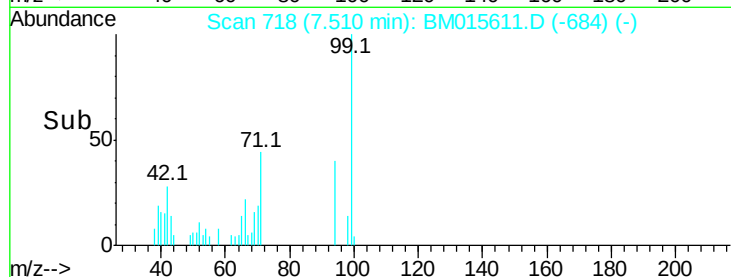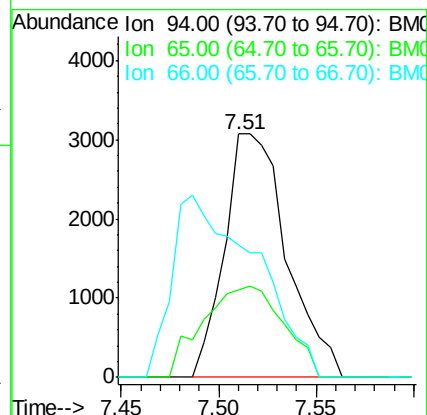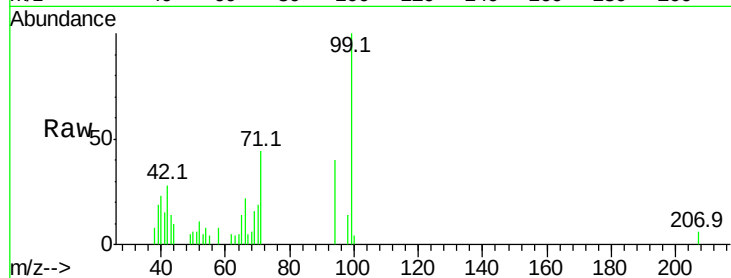

#44

Dimethylphthalate

Concen: 8.738 ng/ul

RT: 14.40 min Scan# 1889

Delta R.T. -0.01 min

Lab File: BM015611.D

Acq: 11 Jun 2018 19:19

Tgt Ion:163 Resp: 78309

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 10.0 7.8 11.8

