

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061118\
 Data File : BM015620.D
 Acq On : 12 Jun 2018 00:51
 Operator : SJ/JU
 Sample : PB110111BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 12 04:38:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 12 03:10:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.34	152	59779	20.00	ng/ul	0.00
18) Naphthalene-d8	11.17	136	311980	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	208732	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.68	188	526041	20.00	ng/ul	0.00
77) Chrysene-d12	21.78	240	650286	20.00	ng/ul	0.00
85) Perylene-d12	24.19	264	734572	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.54	96	9136	7.43	ng/uL	0.00
5) Phenol-d5	7.48	99	189372	34.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.65	67	130633	39.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.86	132	160161	38.60	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	170890	36.55	ng/ul	0.00
19) Nitrobenzene-d5	9.52	128	83285	39.70	ng/ul	0.00
22) 2-Nitrophenol-d4	10.25	143	95221	42.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.79	165	178281	38.16	ng/ul	0.00
29) 4-Chloroaniline-d4	11.30	131	287654	55.25	ng/ul	0.00
43) Dimethylphthalate-d6	14.35	166	791364	45.79	ng/ul	0.00
46) Acenaphthylene-d8	14.66	160	864483	46.38	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	126727	37.99	ng/ul	0.00
57) Fluorene-d10	15.94	176	668594	45.72	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	102102	32.22	ng/ul	0.00
70) Anthracene-d10	17.77	188	1126979	46.99	ng/ul	0.00
78) Pyrene-d10	20.03	212	1323281	47.31	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.04	264	1731166	47.01	ng/ul	0.00


Target Compounds				Ovalue		
15) N-Nitroso-di-n-propylamine	9.05	70	4692	1.212	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061118\
Data File : BM015620.D
Acq On : 12 Jun 2018 00:51
Operator : SJ/JU
Sample : PB110111BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 12 04:38:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 12 03:10:28 2018
Response via : Initial Calibration

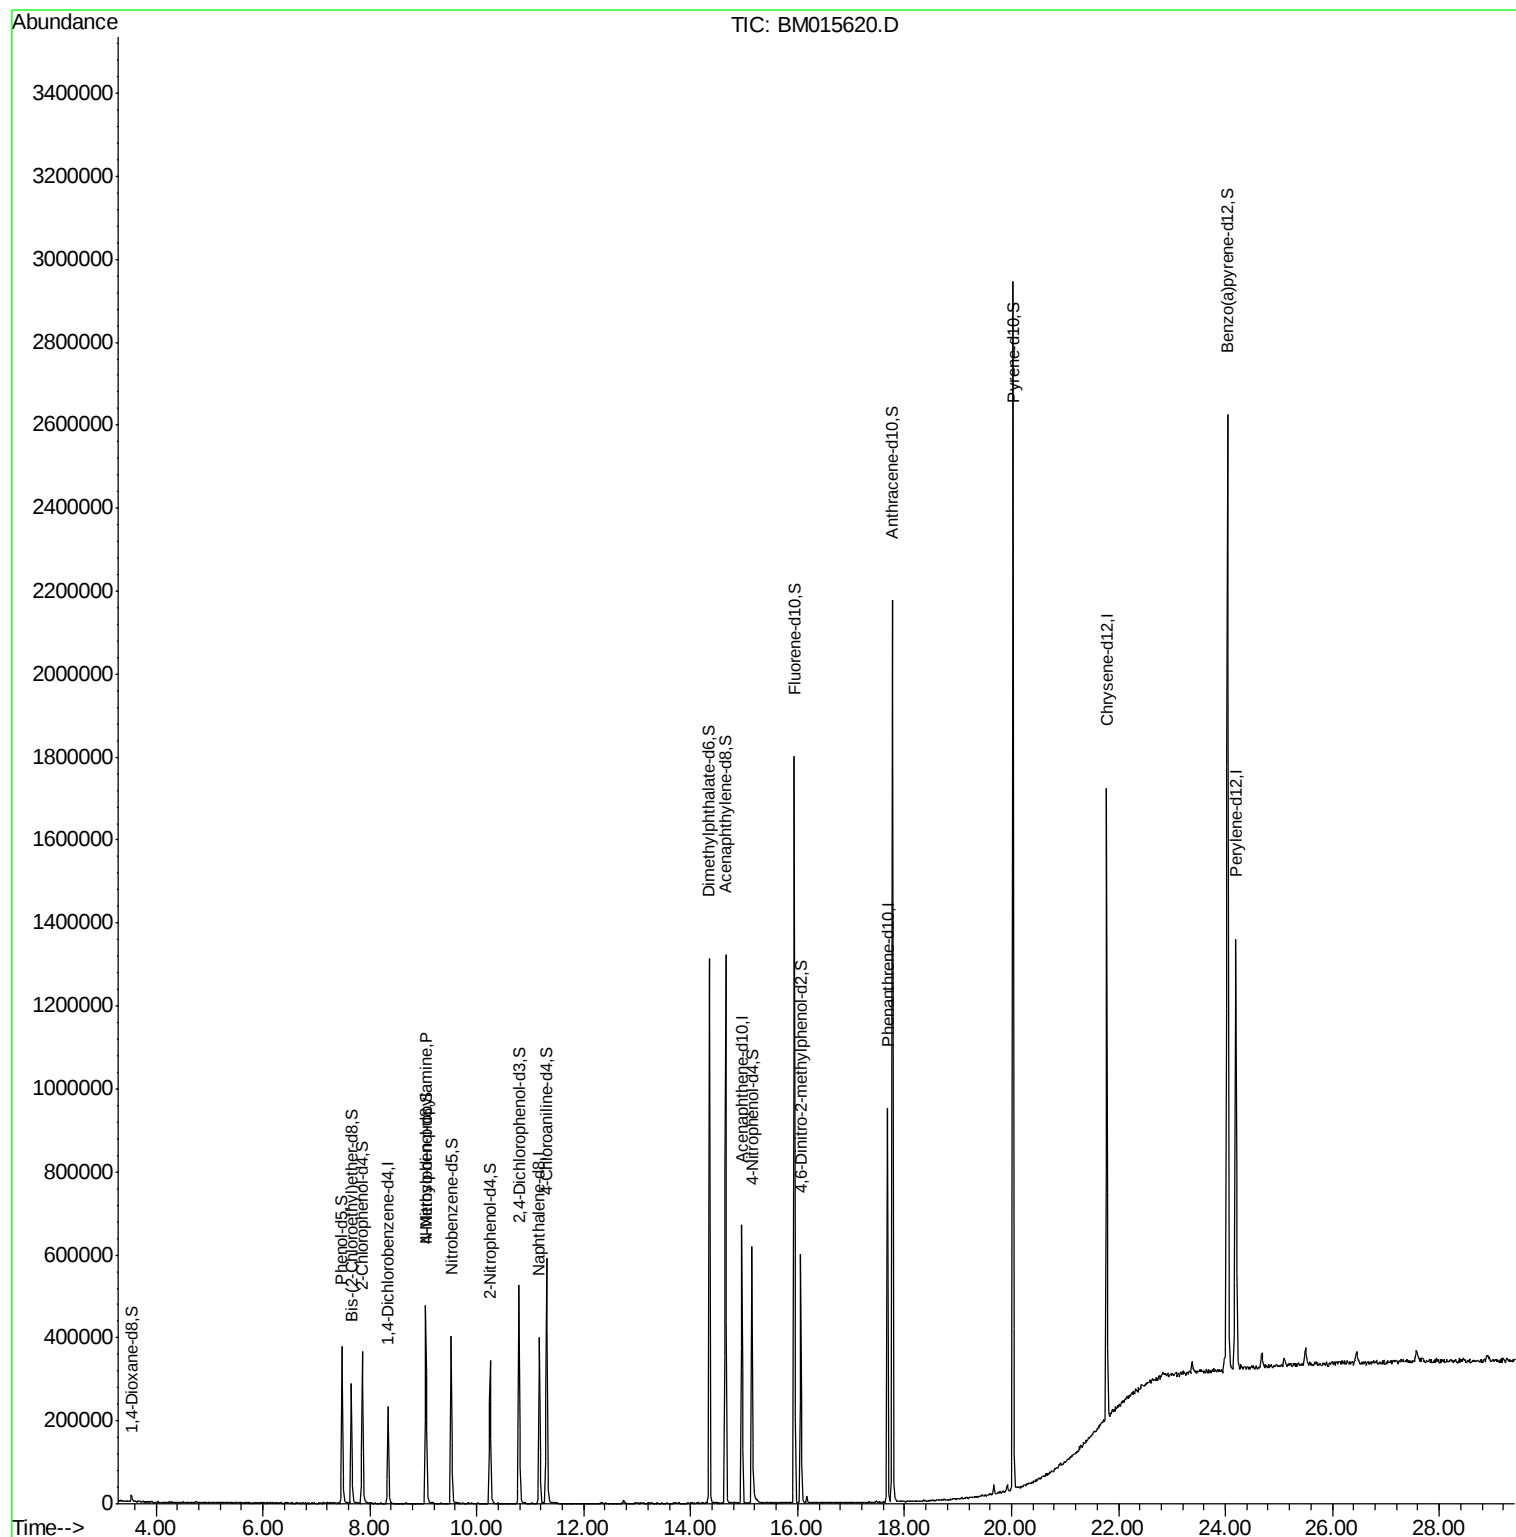

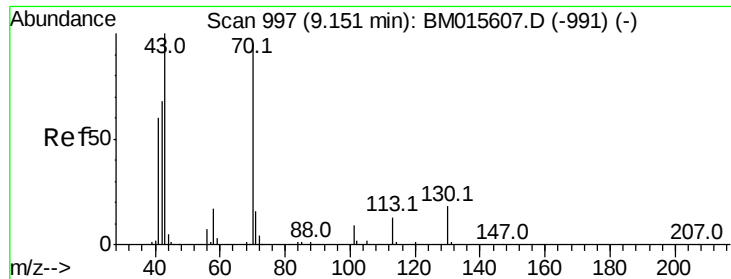

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.212 ng/ul
 RT: 9.05 min Scan# 979
 Delta R.T. -0.11 min
 Lab File: BM015620.D
 Acq: 12 Jun 2018 00:51

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 70 Resp: 4692
 Ion Ratio Lower Upper
 70 100
 42 520.7 35.4 53.0#
 101 0.0 8.4 12.6#
 130 0.0 18.2 27.4#

