

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061119\
 Data File : BM020892.D
 Acq On : 12 Jun 2019 01:55
 Operator : HP/JU
 Sample : K3199-17
 Misc : GCMS CONFIRMATION
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 12 04:04:21 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jun 09 01:02:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	348187	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	1486874	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.45	164	918659	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	1852033	20.00	ng/ul	0.00
77) Chrysene-d12	21.36	240	1280205	20.00	ng/ul	-0.01
85) Perylene-d12	23.64	264	1512287	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	251	0.03	ng/uL	0.00
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	10.60	131	2353	0.09	ng/ul	-0.14
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
46) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.43	176	4026	0.07	ng/ul	-0.01
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.29	188	5323	0.07	ng/ul	0.00
78) Pyrene-d10	19.58	212	434	0.01	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.64	264	1490662	21.69	ng/ul	0.14


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
76) Fluoranthene	19.24	202	124196	1.163	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061119\
Data File : BM020892.D
Acq On : 12 Jun 2019 01:55
Operator : HP/JU
Sample : K3199-17
Misc : GCMS CONFIRMATION
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 12 04:04:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jun 09 01:02:58 2019
Response via : Initial Calibration

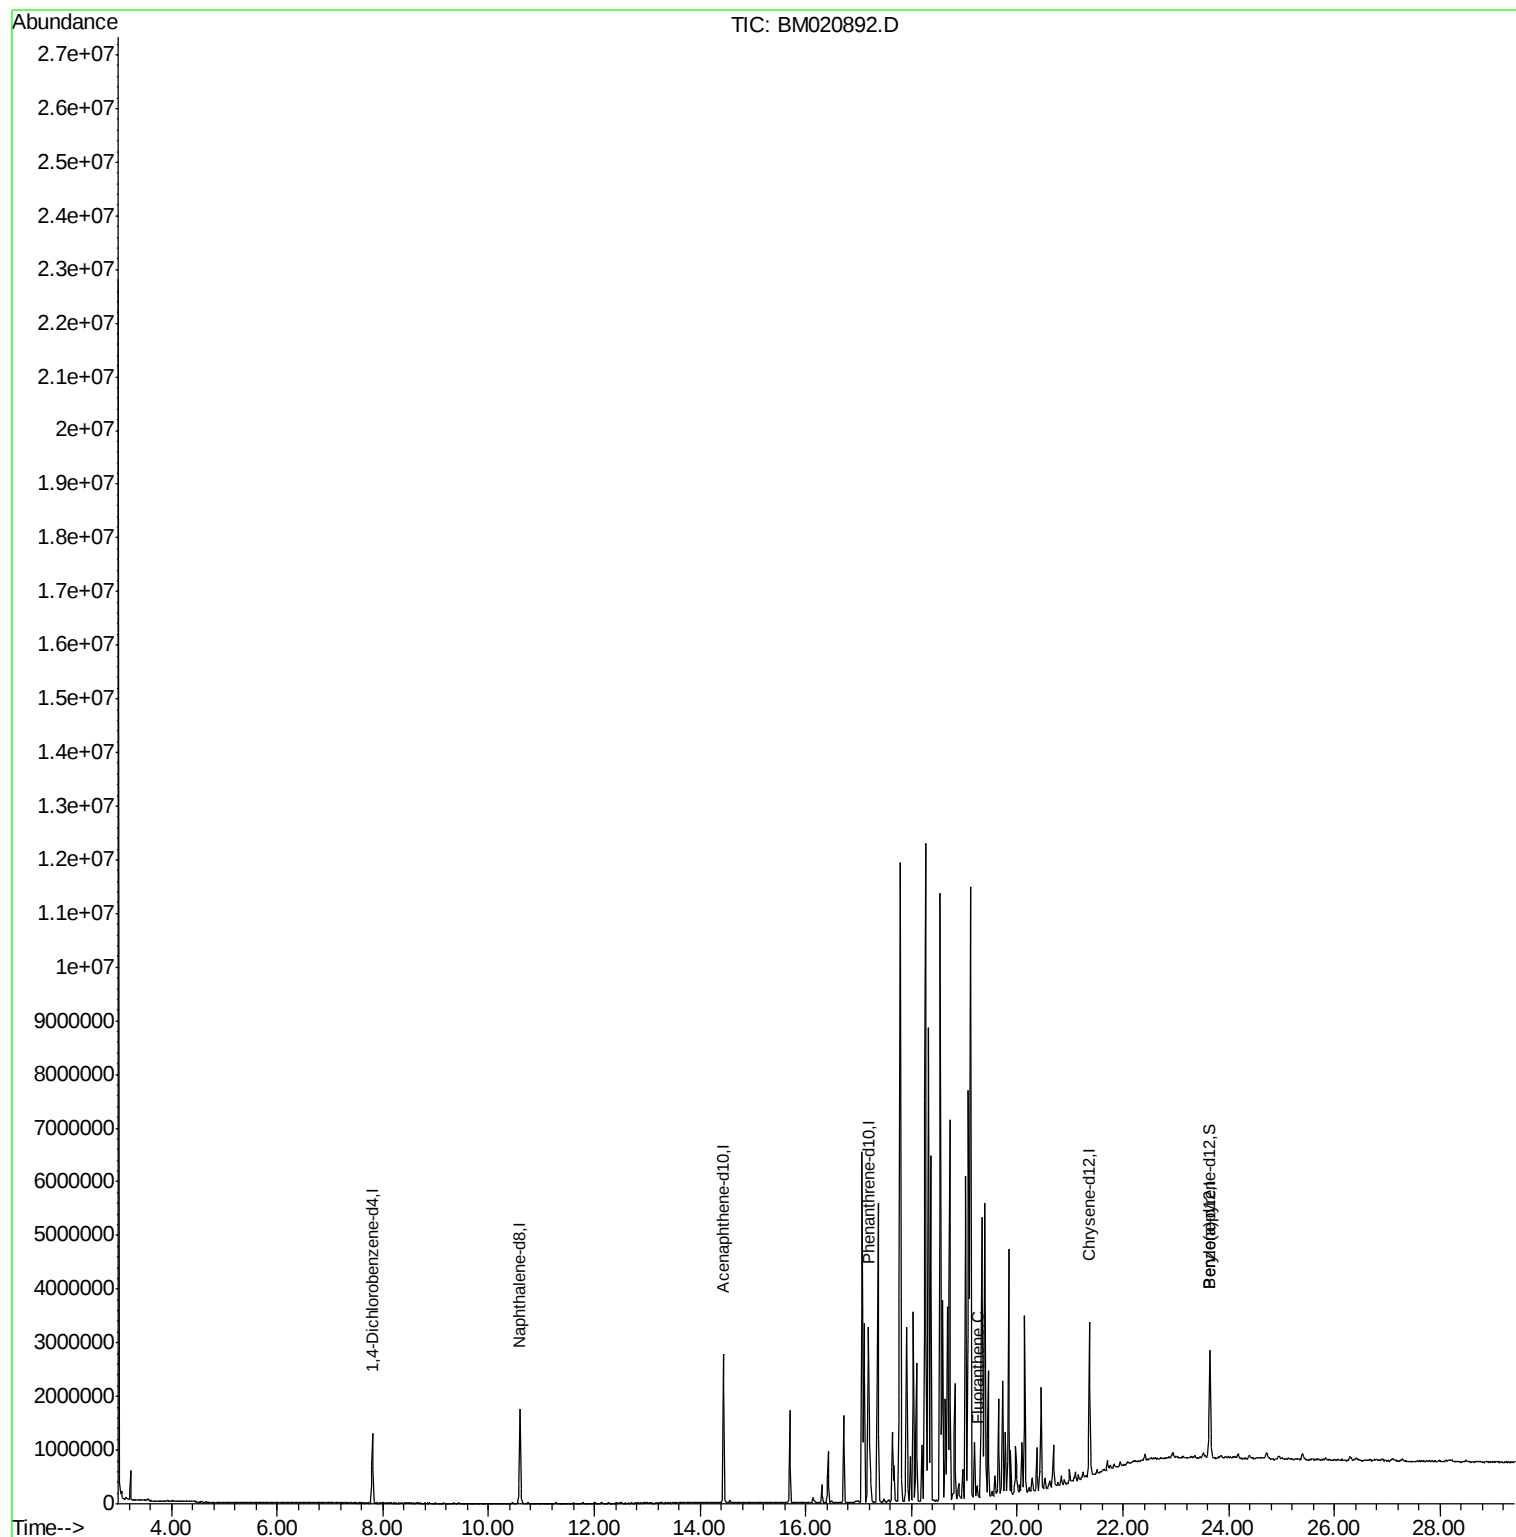


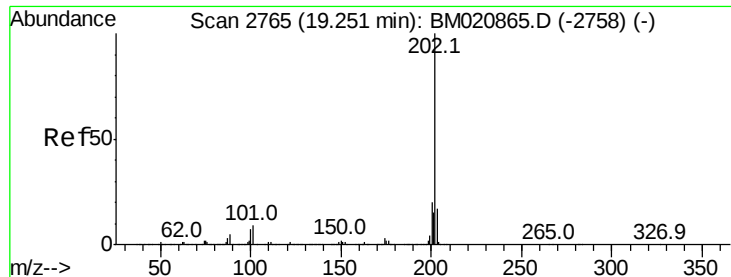

#76
 Fluoranthene
 Concen: 1.163 ng/ul
 RT: 19.24 min Scan# 2764
 Delta R.T. -0.01 min
 Lab File: BM020892.D
 Acq: 12 Jun 2019 01:55

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:	202	Resp:	124196
Ion	Ratio	Lower	Upper
202	100		
101	10.3	7.9	11.9
100	8.8	6.2	9.4

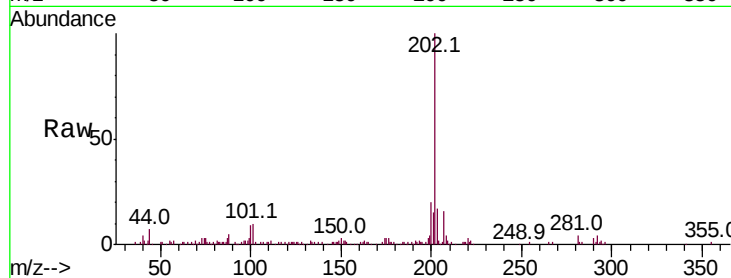

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

