

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061119\
 Data File : BM020892.D
 Acq On : 12 Jun 2019 01:55
 Operator : HP/JU
 Sample : K3199-17
 Misc : GCMS CONFIRMATION
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETND9

Quant Time: Jun 12 04:52:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jun 09 01:02:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	348187	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	1486874	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.45	164	918659	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	1852033	20.00	ng/ul	0.00
77) Chrysene-d12	21.36	240	1280205	20.00	ng/ul	-0.01
85) Perylene-d12	23.64	264	1512287	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL
5) Phenol-d5	0.00	99	0	0.00	ng/ul
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul
46) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
57) Fluorene-d10	0.00	176	0d	0.00	ng/ul
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul
70) Anthracene-d10	0.00	188	0d	0.00	ng/ul
78) Pyrene-d10	0.00	212	0d	0.00	ng/ul
89) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul


Target Compounds				Qvalue
76) Fluoranthene	19.24	202	124196	1.163 ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061119\
 Data File : BM020892.D
 Acq On : 12 Jun 2019 01:55
 Operator : HP/JU
 Sample : K3199-17
 Misc : GCMS CONFIRMATION
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETND9

Quant Time: Jun 12 04:52:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jun 09 01:02:58 2019
 Response via : Initial Calibration

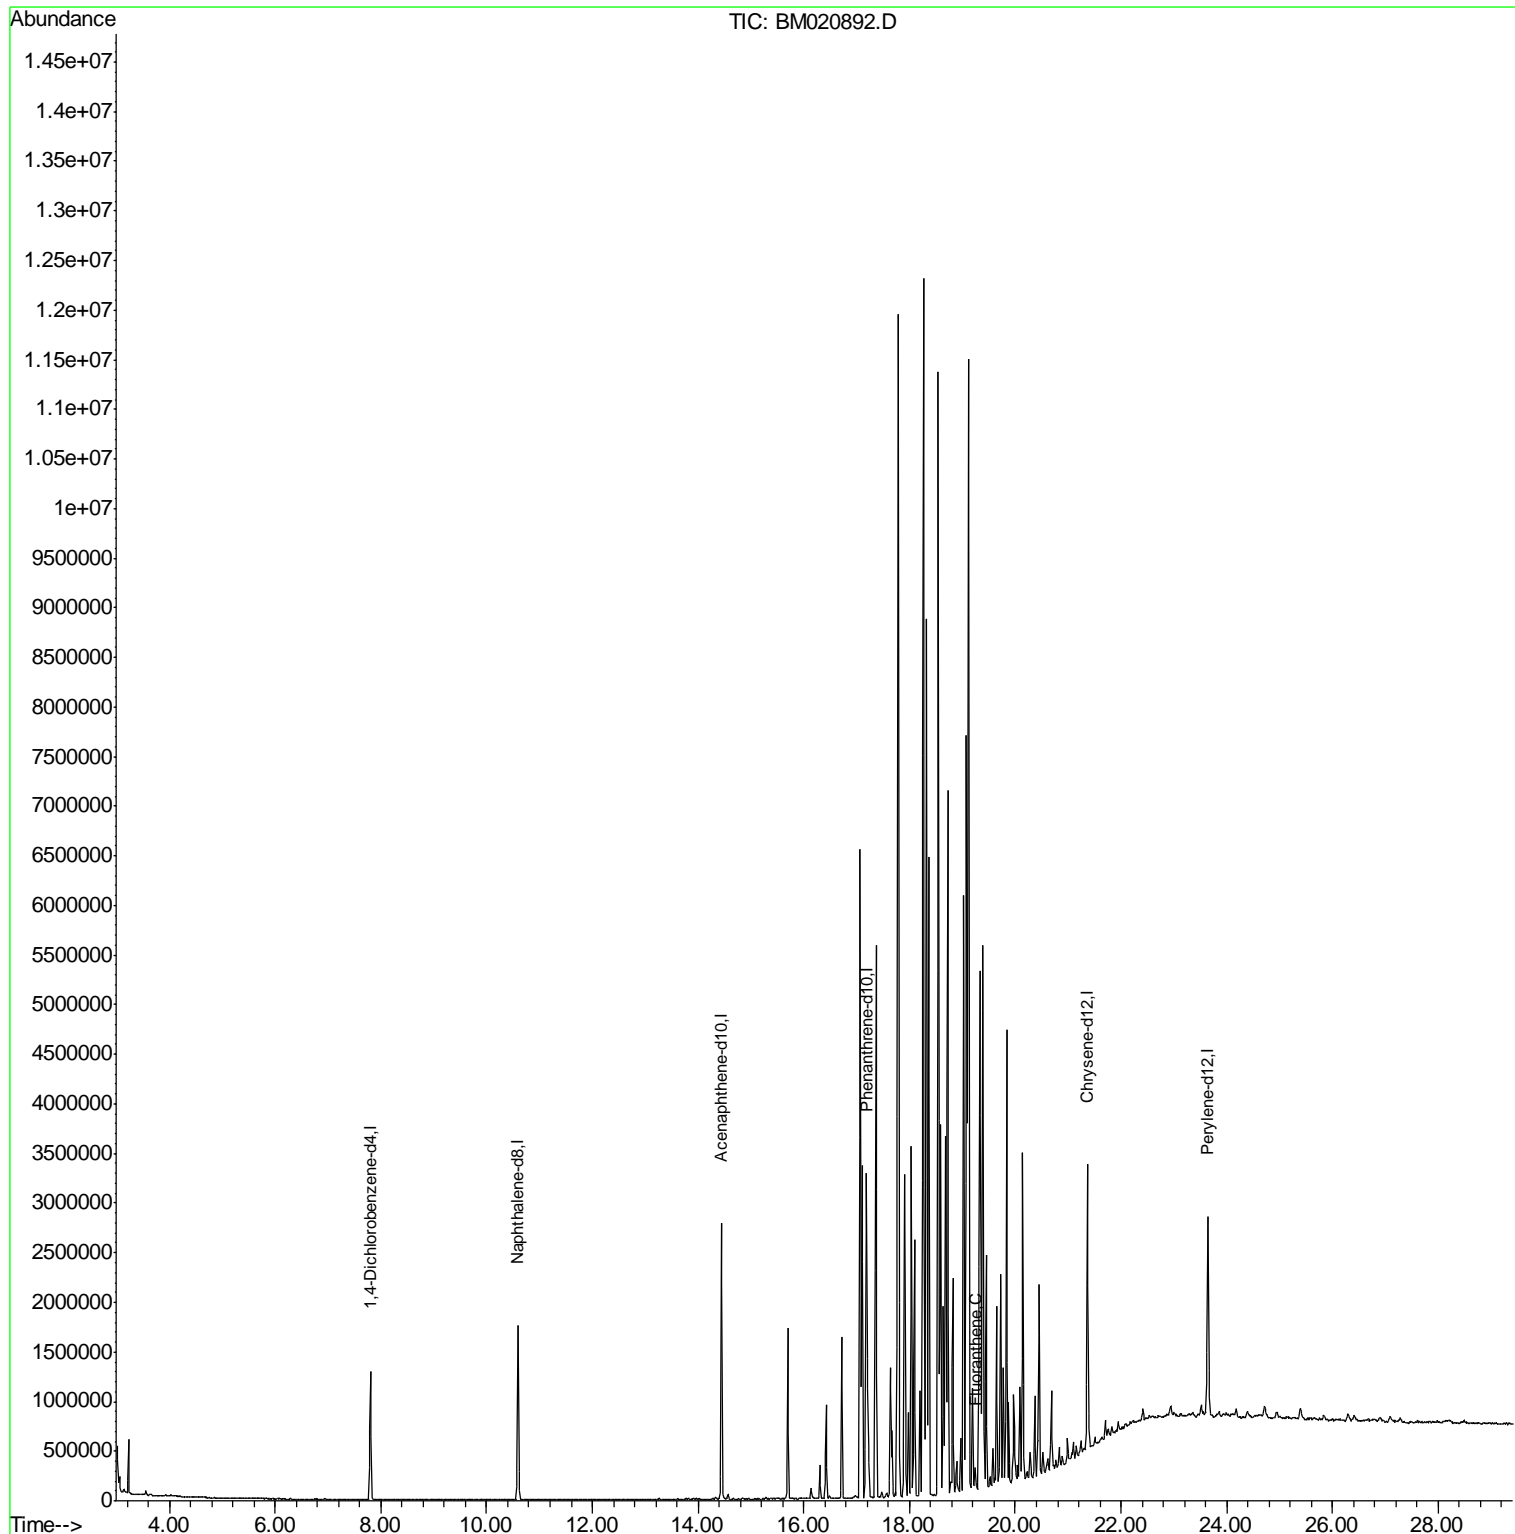

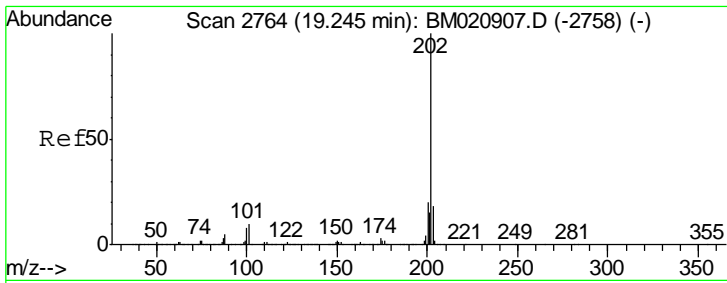

#76
 Fluoranthene
 Concen: 1.163 ng/ul
 RT: 19.24 min Scan# 2764
 Delta R.T. -0.01 min
 Lab File: BM020892.D
 Acq: 12 Jun 2019 01:55

Instrument :
 BNA_M
 ClientSampled :
 ETND9

Tgt Ion	Resp	Lower	Upper
202	124196		
101	10.3	7.9	11.9
100	8.8	6.2	9.4

