

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061119\
 Data File : BM020889.D
 Acq On : 12 Jun 2019 00:06
 Operator : HP/JU
 Sample : K3199-14
 Misc : GCMS CONFIRMATION
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETND5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.057	10	12	18	rVB	169946	180708	4.29%	0.743%
2	3.140	22	26	28	rBV2	39675	42647	1.01%	0.175%
3	3.222	37	40	51	rVB	641238	664473	15.77%	2.732%
4	3.557	94	97	101	rVB2	41062	51359	1.22%	0.211%
5	7.804	811	819	827	rVB	1475478	2269902	53.88%	9.334%
6	10.598	1286	1294	1305	rVB	1826298	3140119	74.54%	12.913%
7	14.445	1941	1948	1961	rVB2	2752223	4212663	100.00%	17.324%
8	17.068	2389	2394	2397	rBV2	41205	55052	1.31%	0.226%
9	17.192	2408	2415	2426	rVB2	2883199	4194162	99.56%	17.247%
10	17.362	2440	2444	2450	rVB	67889	91706	2.18%	0.377%
11	17.792	2510	2517	2523	rVB	145841	256619	6.09%	1.055%
12	17.903	2531	2536	2544	rBV6	41571	67104	1.59%	0.276%
13	18.086	2562	2567	2574	rVB6	29468	52964	1.26%	0.218%
14	18.256	2591	2596	2602	rBV	144156	180520	4.29%	0.742%
15	18.315	2602	2606	2610	rVV	105157	135888	3.23%	0.559%
16	18.356	2610	2613	2619	rVB3	81868	108669	2.58%	0.447%
17	18.545	2640	2645	2649	rBV	112732	160664	3.81%	0.661%
18	18.586	2649	2652	2659	rVB6	35517	47475	1.13%	0.195%
19	18.680	2665	2668	2671	rBV2	47216	51643	1.23%	0.212%
20	18.715	2671	2674	2680	rVB	80958	95835	2.27%	0.394%
21	19.027	2722	2727	2731	rVB	72229	88048	2.09%	0.362%
22	19.080	2731	2736	2738	rBV	60242	86428	2.05%	0.355%
23	19.115	2738	2742	2747	rVB2	126456	188585	4.48%	0.776%
24	19.327	2773	2778	2781	rBV6	57661	93046	2.21%	0.383%
25	19.386	2784	2788	2792	rVB2	64112	83556	1.98%	0.344%
26	19.833	2860	2864	2868	rBV3	53539	63884	1.52%	0.263%
27	20.144	2914	2917	2922	rVB5	42304	52326	1.24%	0.215%
28	21.368	3120	3125	3131	rBV	2919282	3634526	86.28%	14.946%
29	23.650	3506	3513	3523	rVB	2125757	3967030	94.17%	16.313%


Sum of corrected areas: 24317601

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061119\
Data File : BM020889.D
Acq On : 12 Jun 2019 00:06
Operator : HP/JU
Sample : K3199-14
Misc : GCMS CONFIRMATION
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETND5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

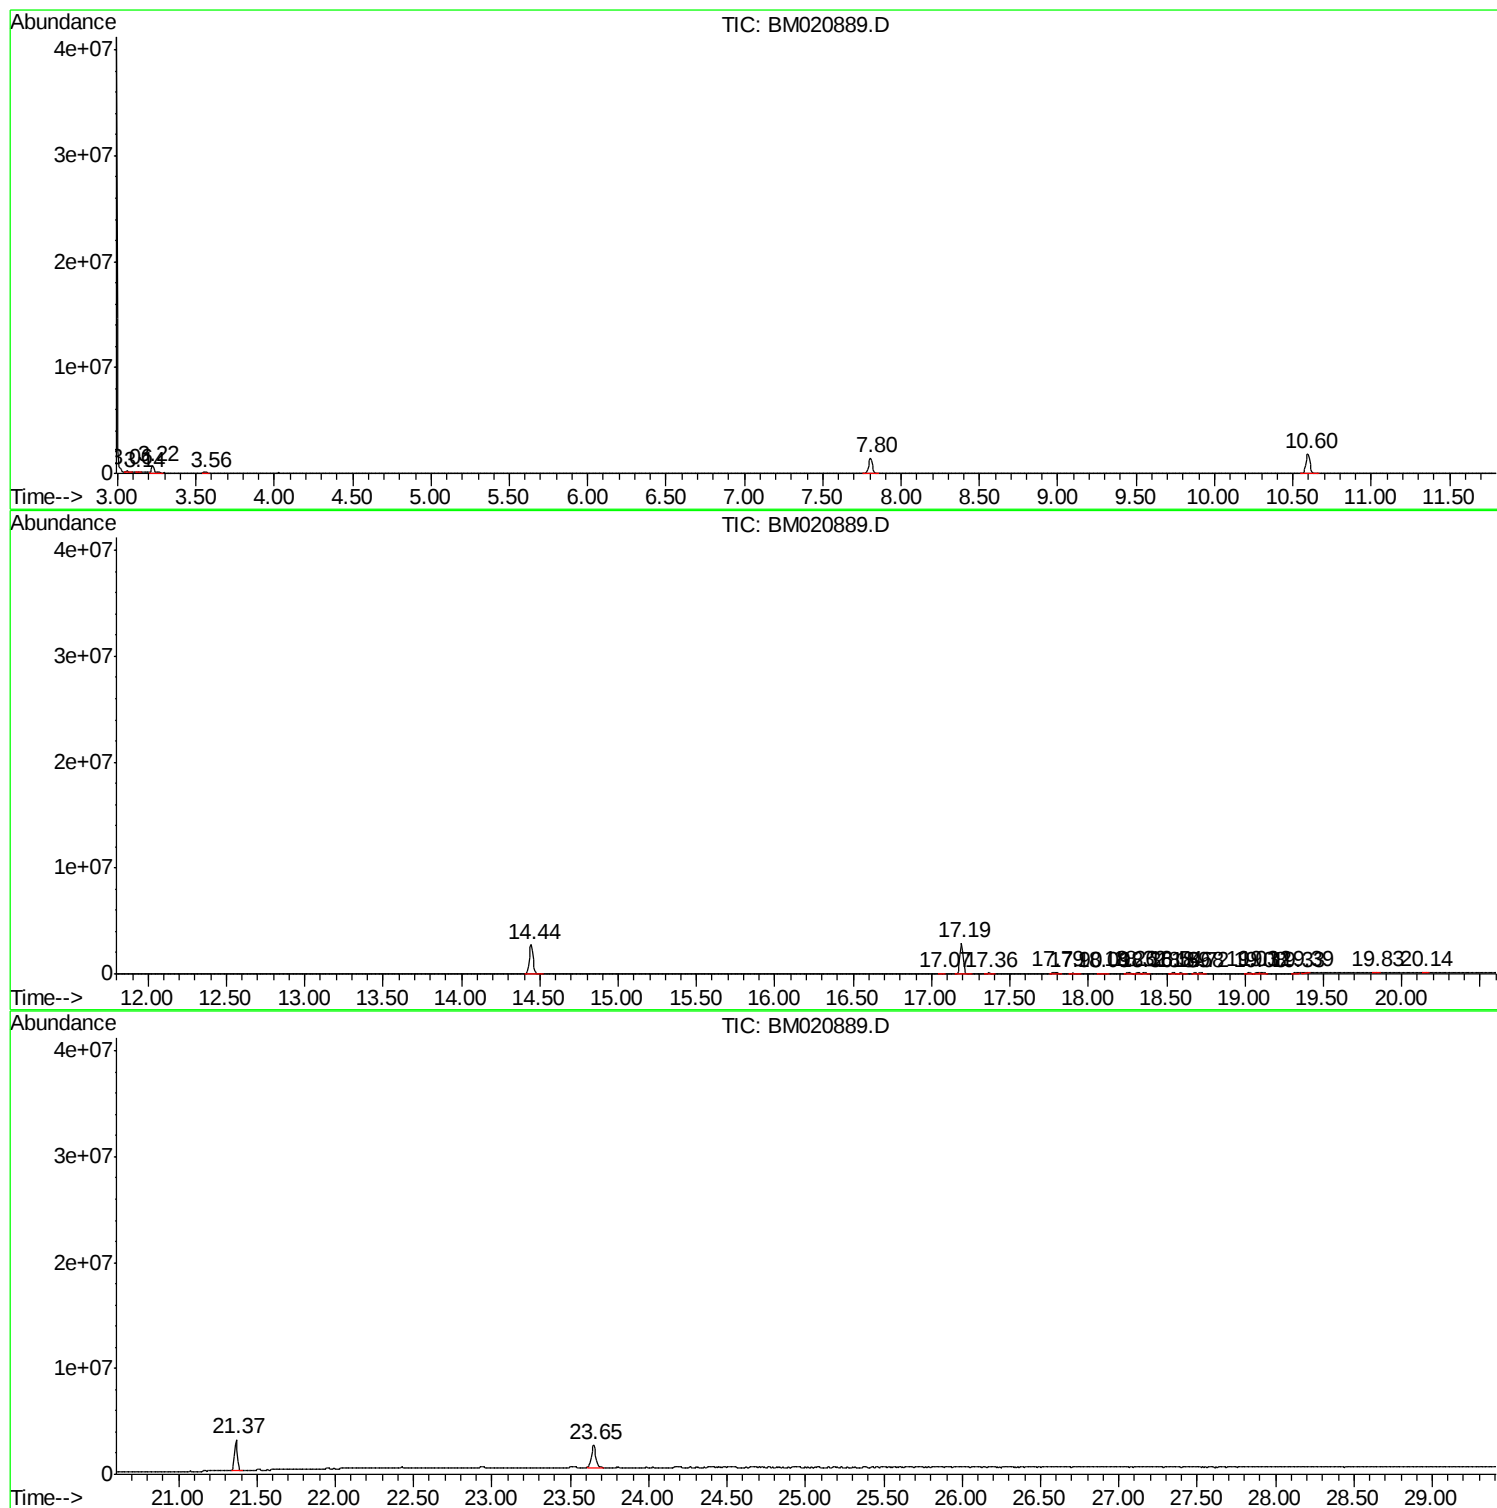

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061119\
Data File : BM020889.D
Acq On : 12 Jun 2019 00:06
Operator : HP/JU
Sample : K3199-14
Misc : GCMS CONFIRMATION
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETND5










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.22	5.85 ng/ul	664473	1,4-Dichlorobenzene-d4	7.80

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptane	100	C7H16	000142-82-5	94
2		Heptane	100	C7H16	000142-82-5	91
3		Heptane	100	C7H16	000142-82-5	90
4		Heptane	100	C7H16	000142-82-5	87
5		Hexane, 3-methyl-	100	C7H16	000589-34-4	42

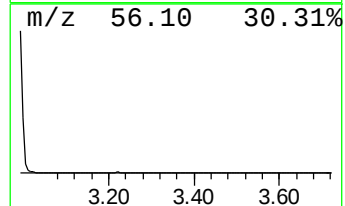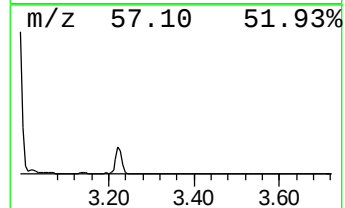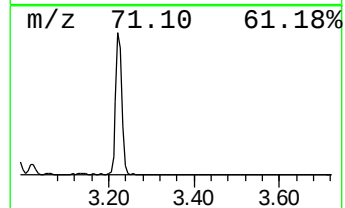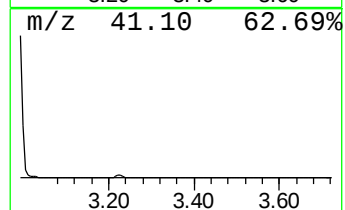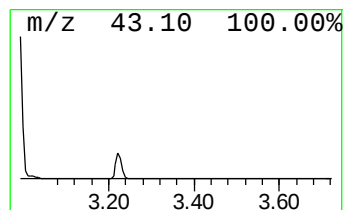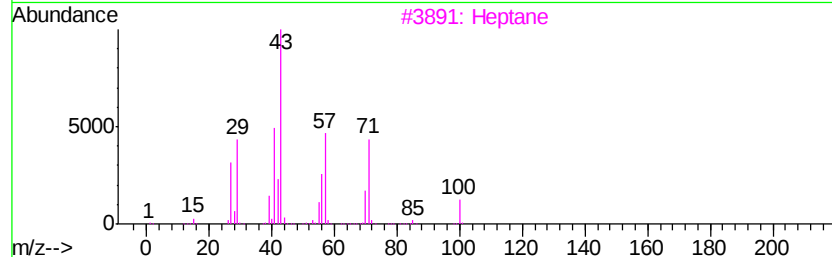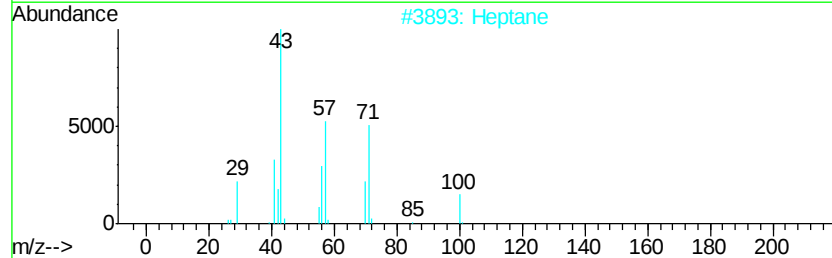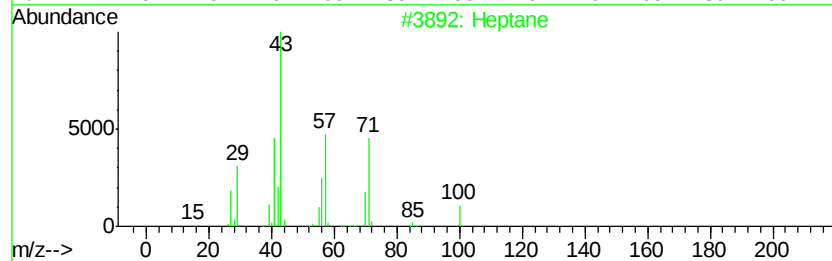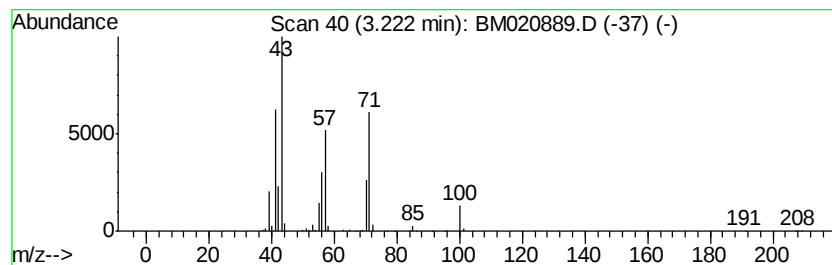

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061119\
Data File : BM020889.D
Acq On : 12 Jun 2019 00:06
Operator : HP/JU
Sample : K3199-14
Misc : GCMS CONFIRMATION
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETND5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	3.22	5.8	ng/ul	664473	1	7.80	2269900	20.0