

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061121\
 Data File : BM030408.D
 Acq On : 11 Jun 2021 17:16
 Operator : CG/JU
 Sample : M2625-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 18-B12(206-210)

Quant Time: Jun 11 18:15:00 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 13:16:52 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	158174	20.000	ng	0.00
21) Naphthalene-d8	10.622	136	561073	20.000	ng	# 0.00
39) Acenaphthene-d10	14.457	164	314639	20.000	ng	0.00
64) Phenanthrene-d10	17.192	188	613978	20.000	ng	# 0.00
76) Chrysene-d12	21.356	240	661319	20.000	ng	0.00
86) Perylene-d12	23.633	264	780931	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.416	112	893732	91.855	ng	0.00
7) Phenol-d6	6.999	99	1119122	79.453	ng	0.00
23) Nitrobenzene-d5	8.987	82	632594	54.928	ng	0.00
42) 2,4,6-Tribromophenol	15.939	330	320993	81.143	ng	0.00
45) 2-Fluorobiphenyl	13.081	172	1351597	56.491	ng	0.00
79) Terphenyl-d14	19.804	244	1905158	50.600	ng	0.00
Target Compounds						
57) 2,4-Dinitrotoluene	15.033	165	185	3.017	ng	# 24
80) Butylbenzylphthalate	20.480	149	116	4.311	ng	# 69
84) Bis(2-ethylhexyl)phtha...	21.274	149	2871	4.358	ng	# 80
85) Di-n-octyl phthalate	22.156	149	231	4.169	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061121\
Data File : BM030408.D
Acq On : 11 Jun 2021 17:16
Operator : CG/JU
Sample : M2625-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
18-B12(206-210)

Quant Time: Jun 11 18:15:00 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 13:16:52 2021
Response via : Initial Calibration




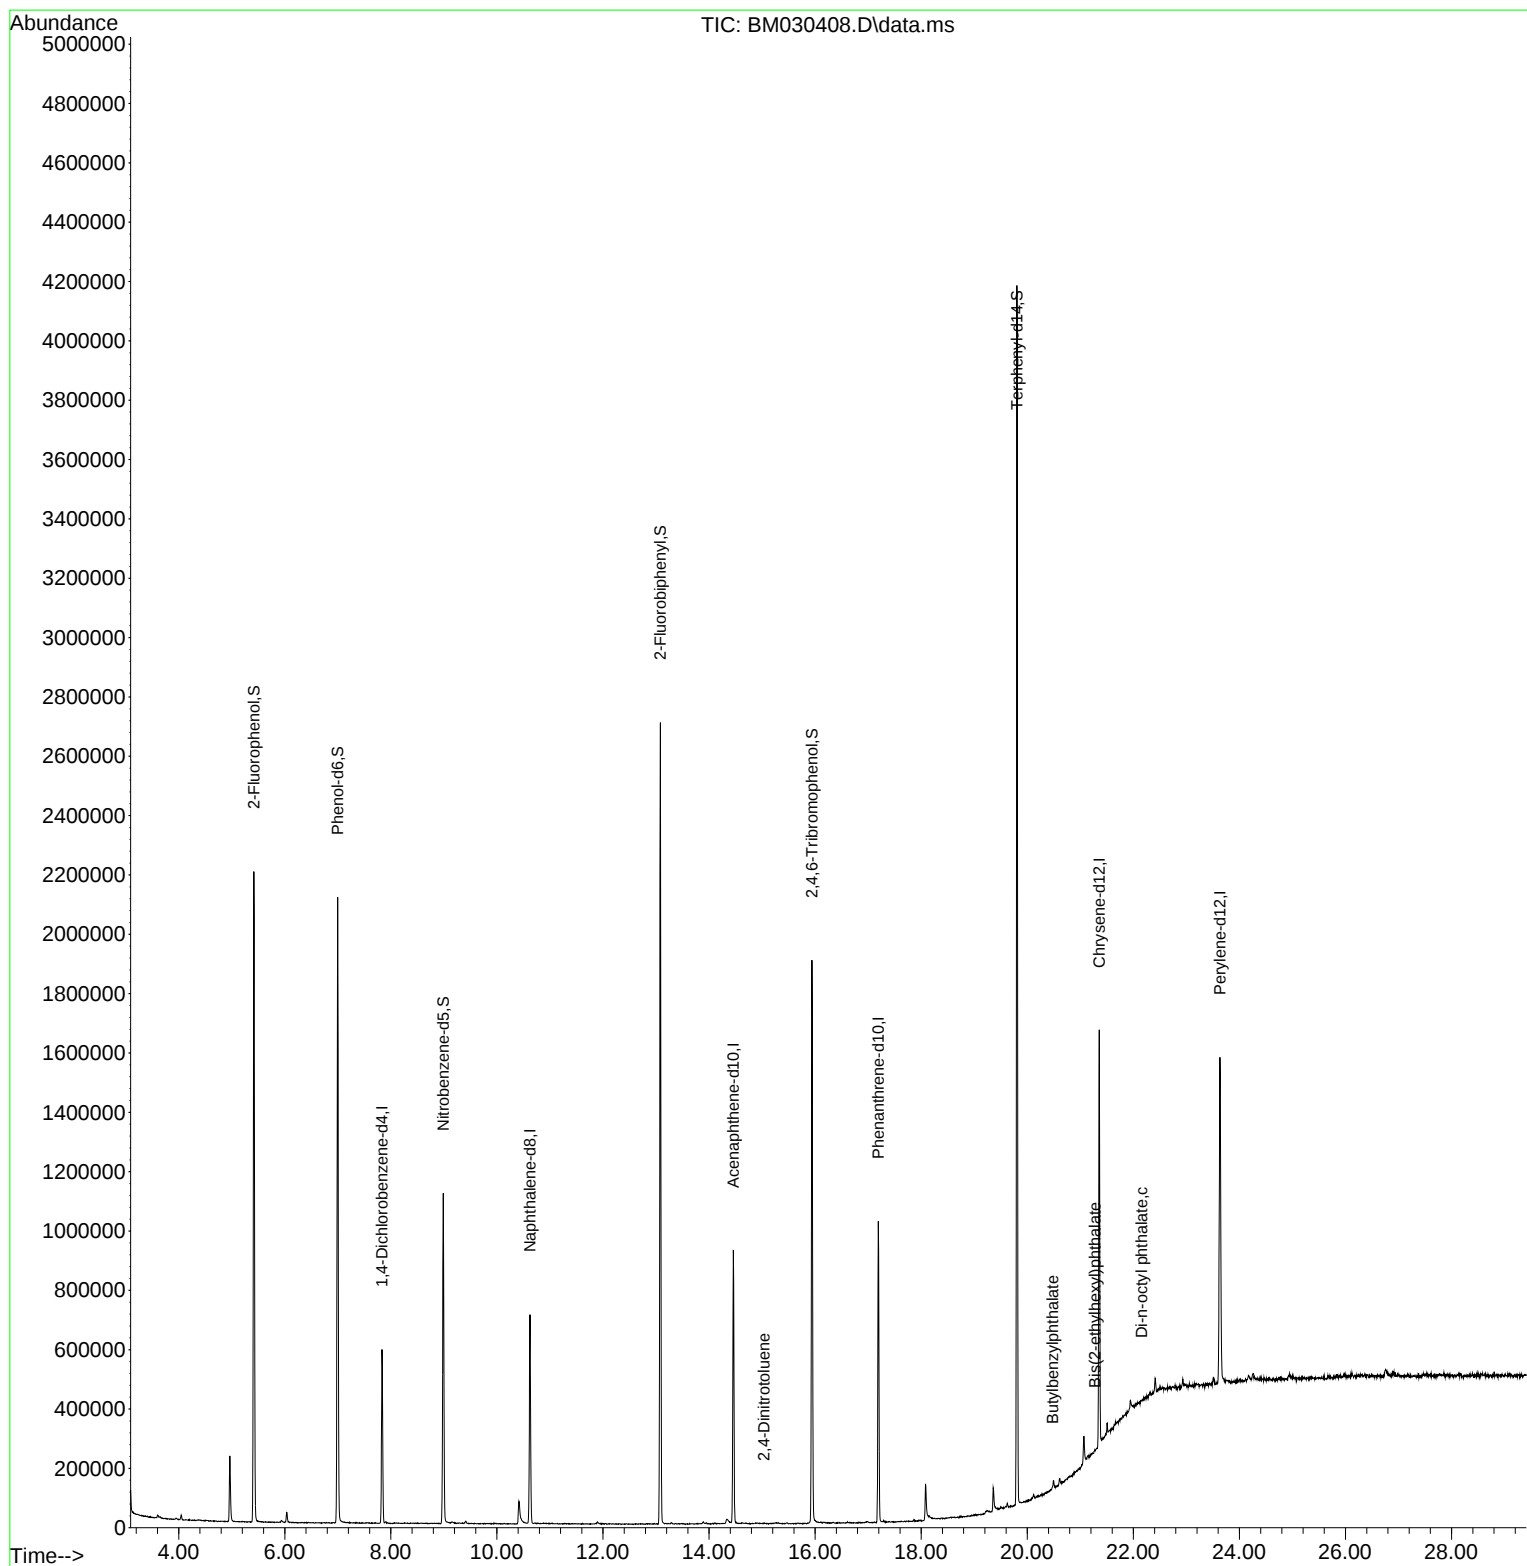




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.834 min Scan# 807
Delta R.T. -0.000 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16




Instrument :
BNA_M
ClientSampleId :
18-B12(206-210)


Tgt Ion:152 Resp: 158174
Ion Ratio Lower Upper
152 100
150 152.3 125.9 188.9
115 57.3 44.6 67.0

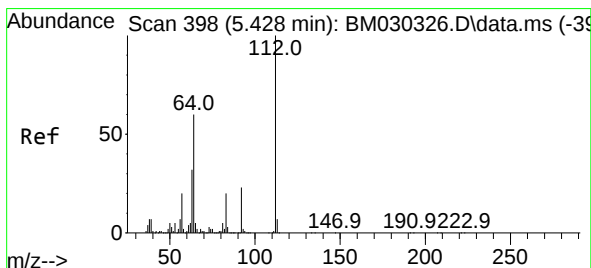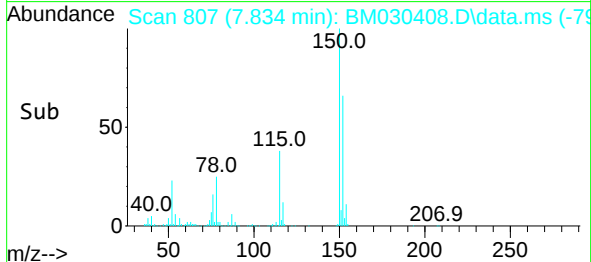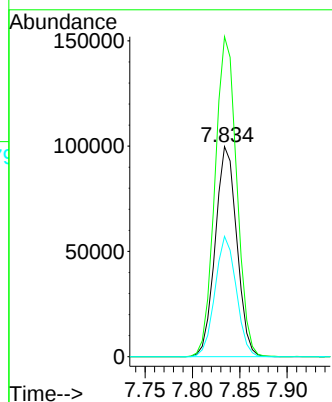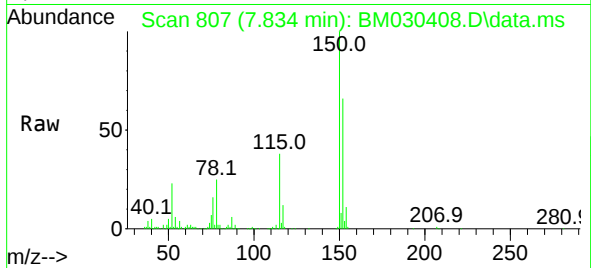

#5
2-Fluorophenol
Concen: 91.855 ng
RT: 5.416 min Scan# 396
Delta R.T. 0.000 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16

Tgt Ion:112 Resp: 893732
Ion Ratio Lower Upper
112 100
64 61.3 47.1 70.7
63 32.8 27.3 40.9


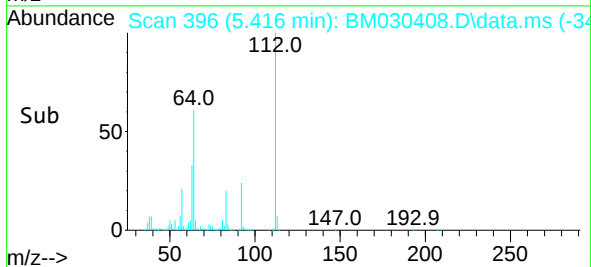
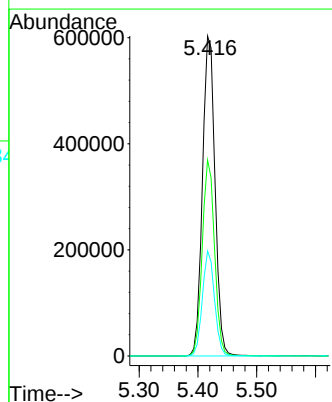
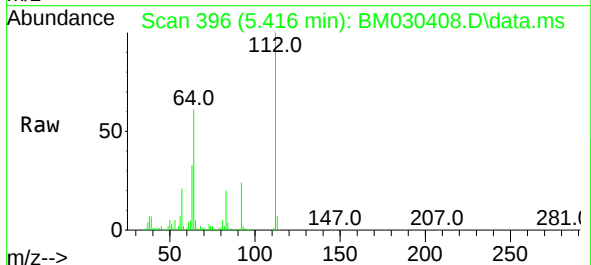


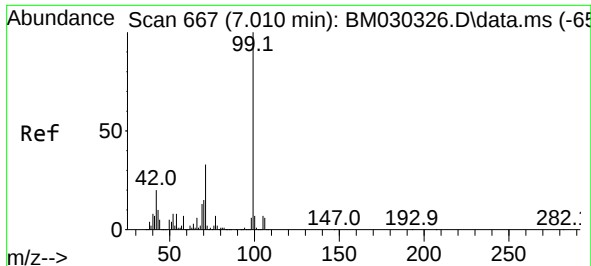

#7
Phenol-d6
Concen: 79.453 ng
RT: 6.999 min Scan# 665
Delta R.T. 0.000 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16




Instrument :
BNA_M
ClientSampleId :
18-B12(206-210)


Tgt Ion: 99 Resp: 1119122
Ion Ratio Lower Upper
99 100
42 20.0 18.0 27.0
71 32.2 30.9 46.3

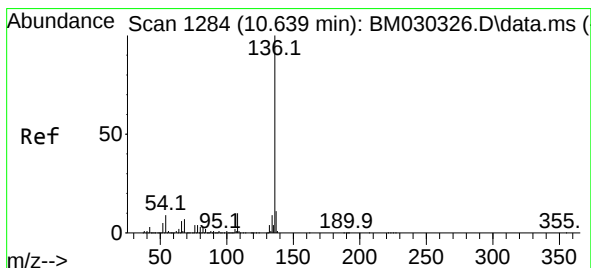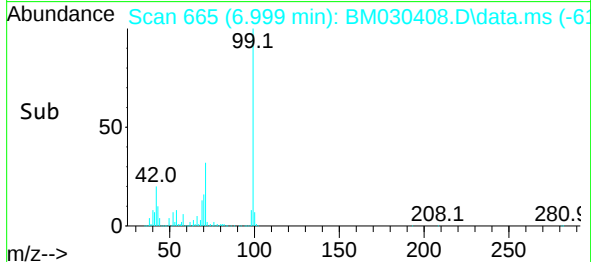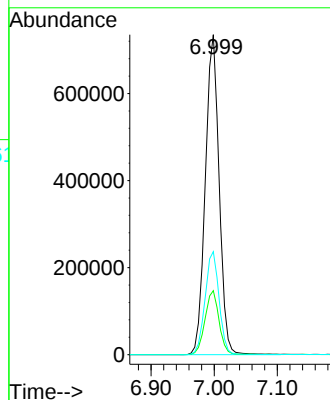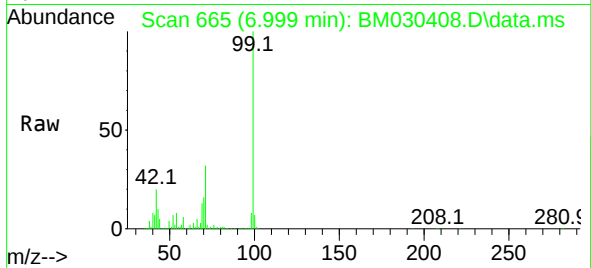

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.622 min Scan# 1281
Delta R.T. -0.006 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16

Tgt Ion: 136 Resp: 561073
Ion Ratio Lower Upper
136 100
137 10.5 8.4 12.6
54 9.1 5.5 8.3#
68 5.9 4.2 6.2


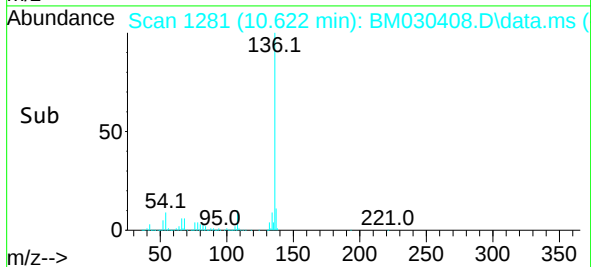
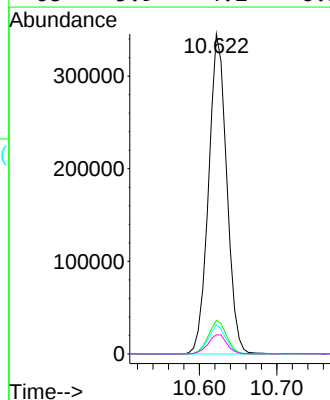
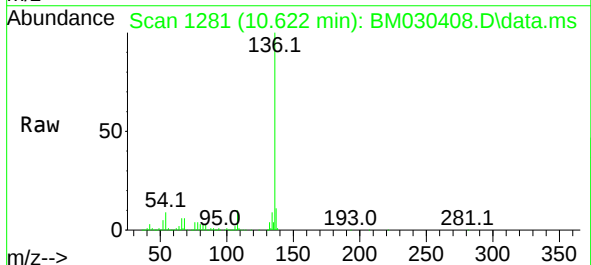


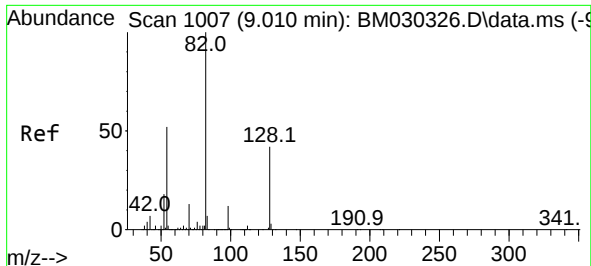

#23
Nitrobenzene-d5
Concen: 54.928 ng
RT: 8.987 min Scan# 1003
Delta R.T. -0.006 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16




Instrument :
BNA_M
ClientSampleId :
18-B12(206-210)


Tgt Ion: 82 Resp: 632594
Ion Ratio Lower Upper
82 100
128 40.0 31.1 46.7
54 52.1 37.3 55.9

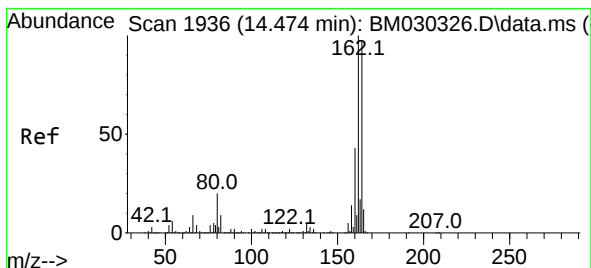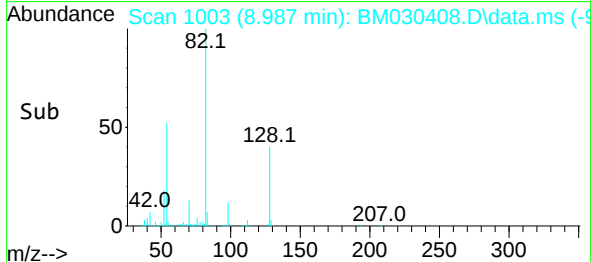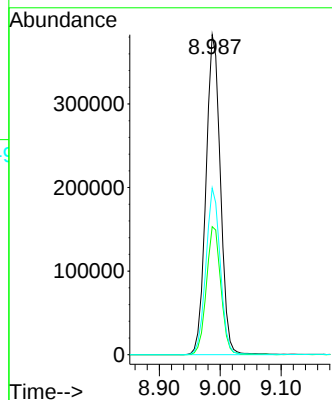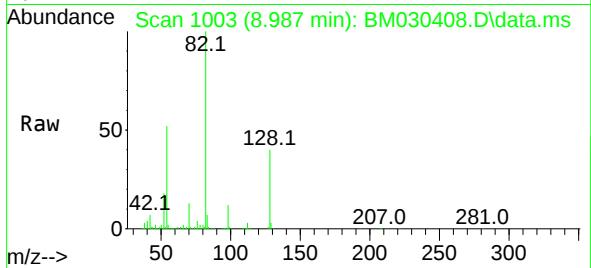

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.457 min Scan# 1933
Delta R.T. -0.006 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16


Tgt Ion:164 Resp: 314639
Ion Ratio Lower Upper
164 100
162 100.8 83.4 125.0
160 45.0 37.2 55.8

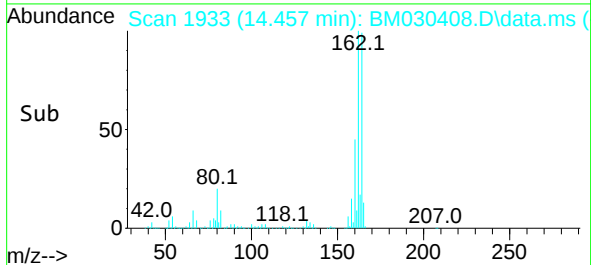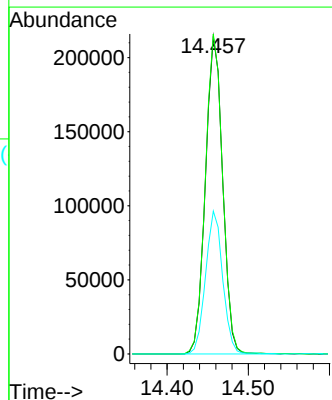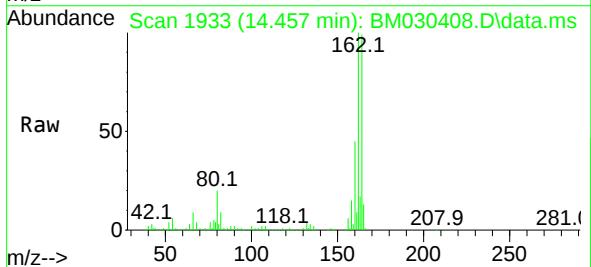



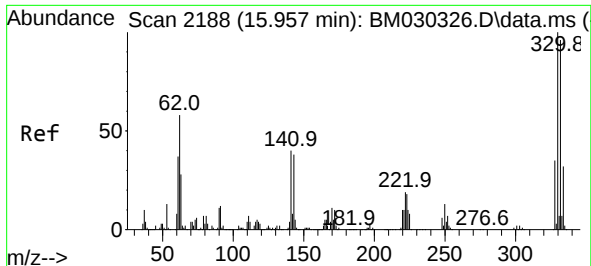


#42
2,4,6-Tribromophenol
Concen: 81.143 ng
RT: 15.939 min Scan# 2185
Delta R.T. -0.006 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16


Instrument :
BNA_M
ClientSampleId :
18-B12(206-210)

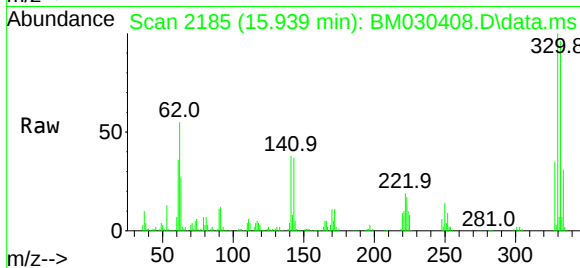



Tgt Ion:330 Resp: 320993
Ion Ratio Lower Upper
330 100
332 95.7 77.0 115.4
141 36.7 30.2 45.2

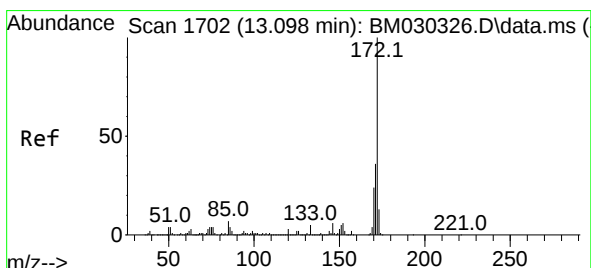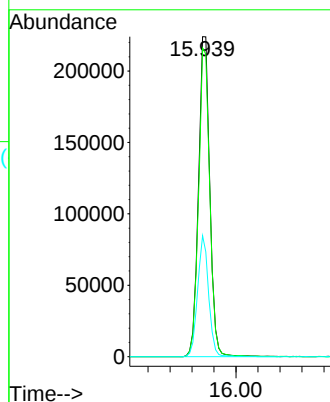


#45
2-Fluorobiphenyl
Concen: 56.491 ng
RT: 13.081 min Scan# 1699
Delta R.T. -0.006 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16

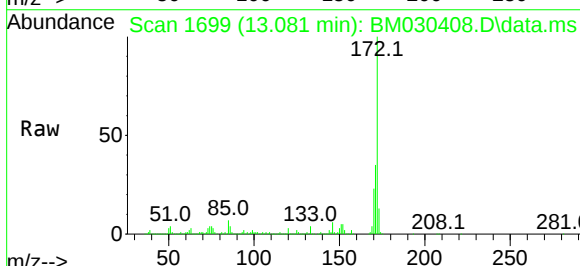

Tgt Ion:172 Resp: 1351597
Ion Ratio Lower Upper
172 100
171 35.3 28.6 43.0
170 23.2 18.4 27.6



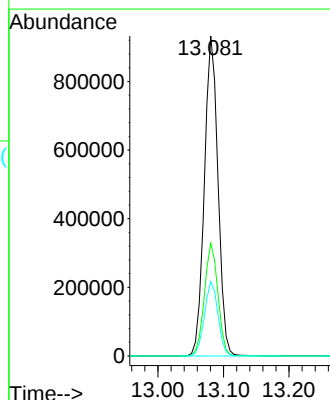
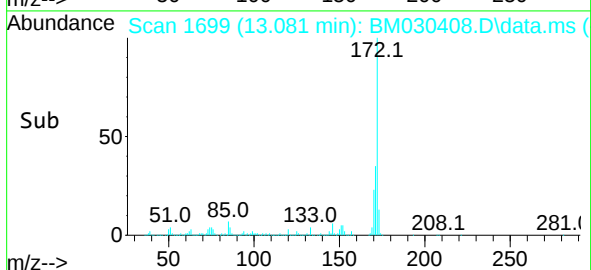




#57
2,4-Dinitrotoluene
Concen: 3.017 ng
RT: 15.033 min Scan# 2031
Delta R.T. 0.212 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16




Instrument :
BNA_M
ClientSampleId :
18-B12(206-210)


Tgt Ion:165 Resp: 185
Ion Ratio Lower Upper
165 100
63 0.0 35.0 52.4#
89 0.0 55.2 82.8#
182 0.0 2.6 3.8#

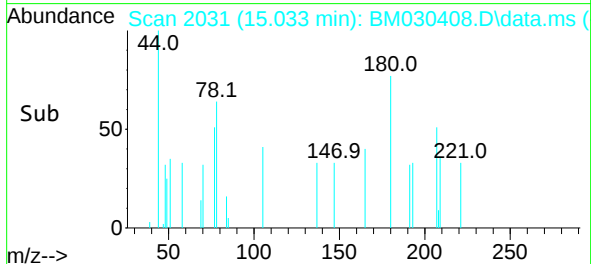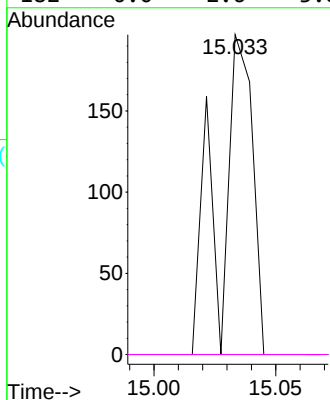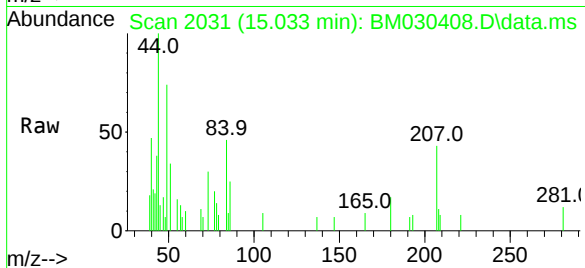

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.192 min Scan# 2398
Delta R.T. -0.006 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16

Tgt Ion:188 Resp: 613978
Ion Ratio Lower Upper
188 100
94 9.2 6.0 9.0#
80 9.5 6.6 9.8


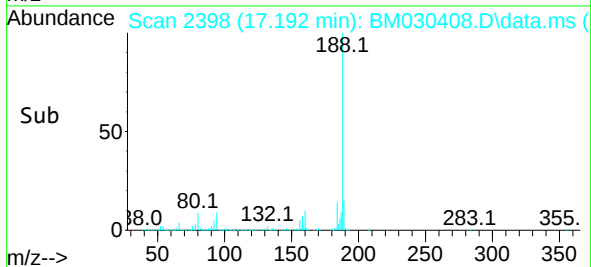
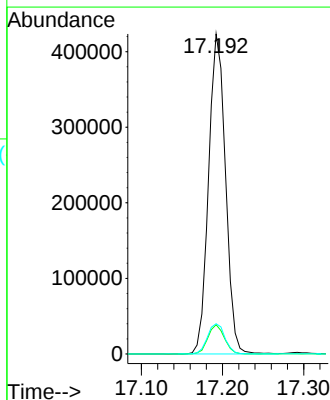
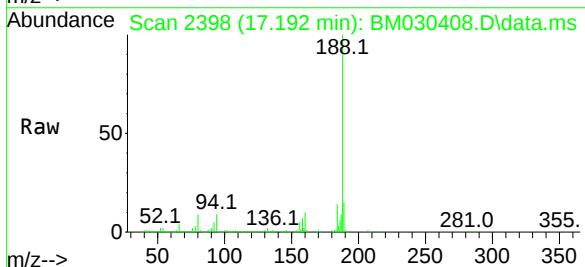




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.356 min Scan# 3106
Delta R.T. 0.000 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16




Instrument :
BNA_M
ClientSampleId :
18-B12(206-210)


Tgt Ion:240 Resp: 661319
Ion Ratio Lower Upper
240 100
120 10.0 7.0 10.6
236 25.1 21.0 31.4

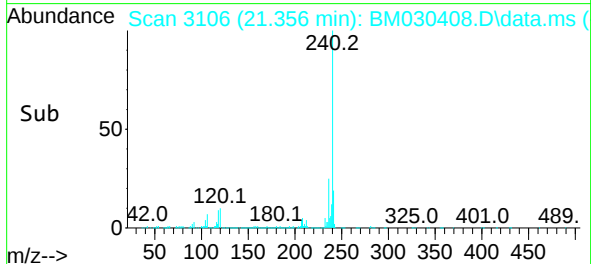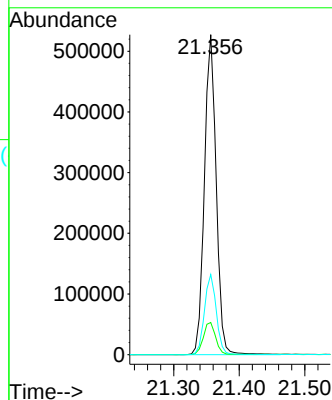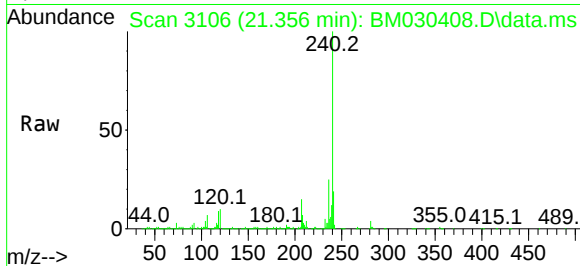

#79
Terphenyl-d14
Concen: 50.600 ng
RT: 19.804 min Scan# 2842
Delta R.T. -0.006 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16

Tgt Ion:244 Resp: 1905158
Ion Ratio Lower Upper
244 100
212 7.2 6.3 9.5
122 10.8 6.9 10.3#


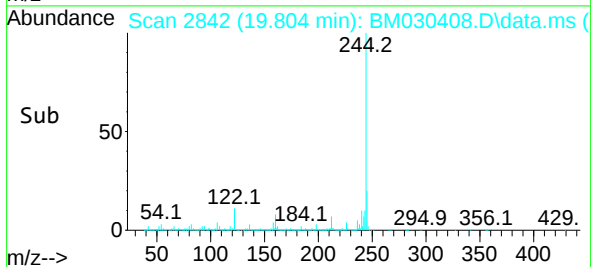
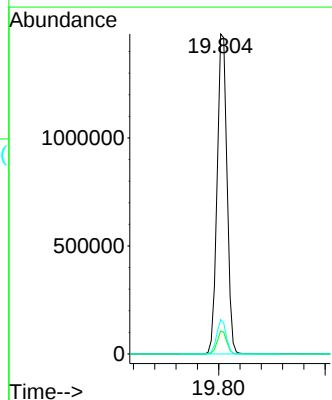
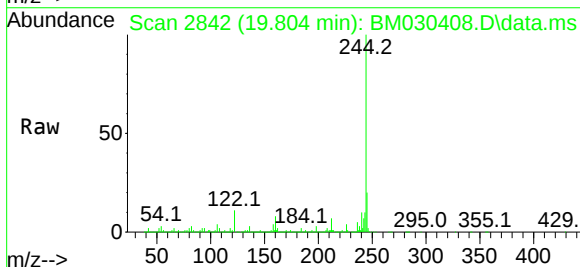


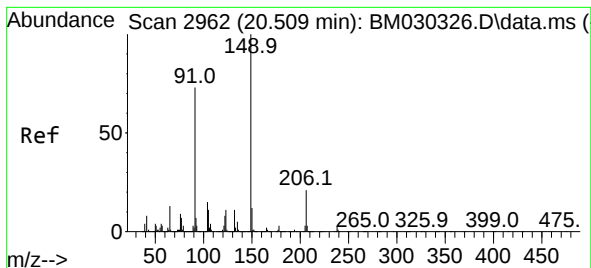

#80
Butylbenzylphthalate
Concen: 4.311 ng
RT: 20.480 min Scan# 2957
Delta R.T. -0.018 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16




Instrument :
BNA_M
ClientSampleId :
18-B12(206-210)


Tgt Ion:149 Resp: 116
Ion Ratio Lower Upper
149 100
91 49.7 57.4 86.0#
206 0.0 16.6 25.0#

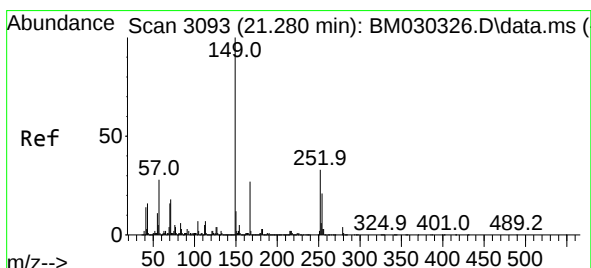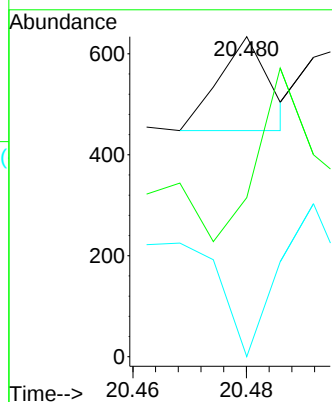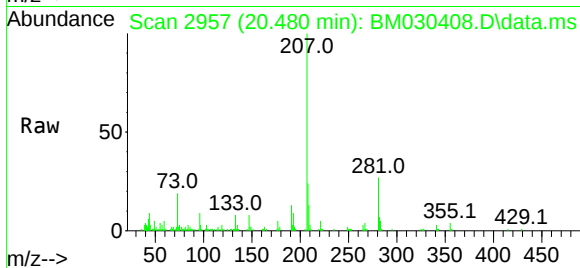

#84
Bis(2-ethylhexyl)phthalate
Concen: 4.358 ng
RT: 21.274 min Scan# 3092
Delta R.T. 0.000 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16

Tgt Ion:149 Resp: 2871
Ion Ratio Lower Upper
149 100
167 16.6 22.6 33.8#
279 8.8 3.8 5.8#


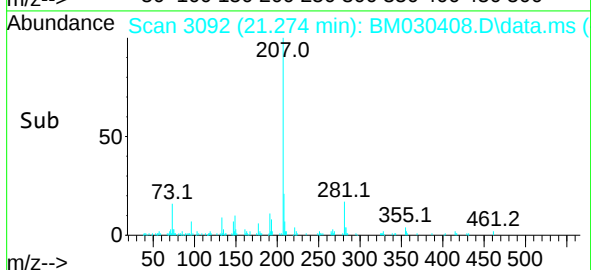
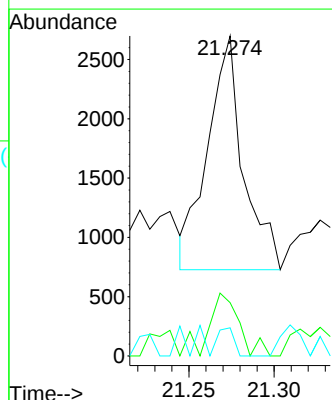
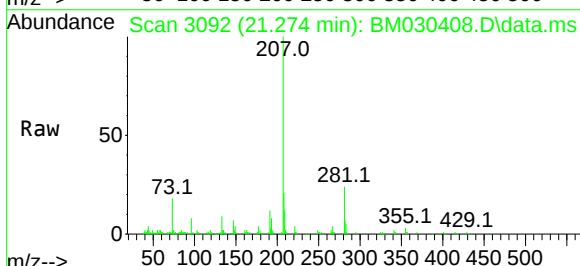




#85
Di-n-octyl phthalate
Concen: 4.169 ng
RT: 22.156 min Scan# 3242
Delta R.T. 0.000 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16

Instrument :
BNA_M
ClientSampleId :
18-B12(206-210)

Tgt Ion:149 Resp: 231
Ion Ratio Lower Upper
149 100
167 0.0 1.3 1.9#
43 155.4 7.4 11.0#

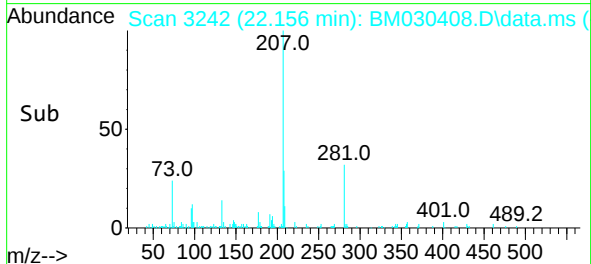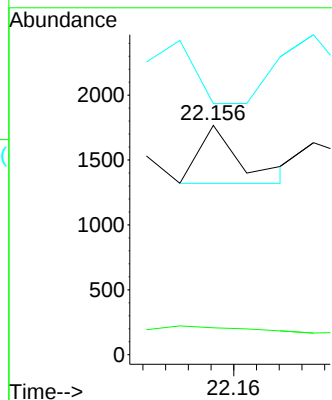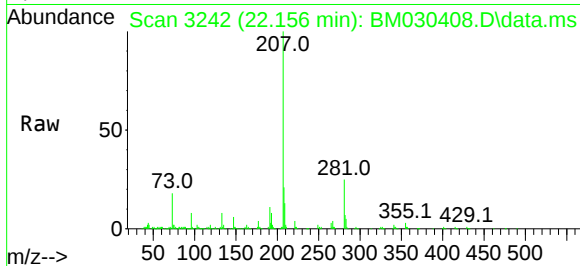

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.633 min Scan# 3493
Delta R.T. 0.000 min
Lab File: BM030408.D
Acq: 11 Jun 2021 17:16

Tgt Ion:264 Resp: 780931
Ion Ratio Lower Upper
264 100
260 23.2 19.8 29.8
265 22.4 17.7 26.5

