


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061121\
 Data File : BM030399.D
 Acq On : 11 Jun 2021 11:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 11 14:10:50 2021

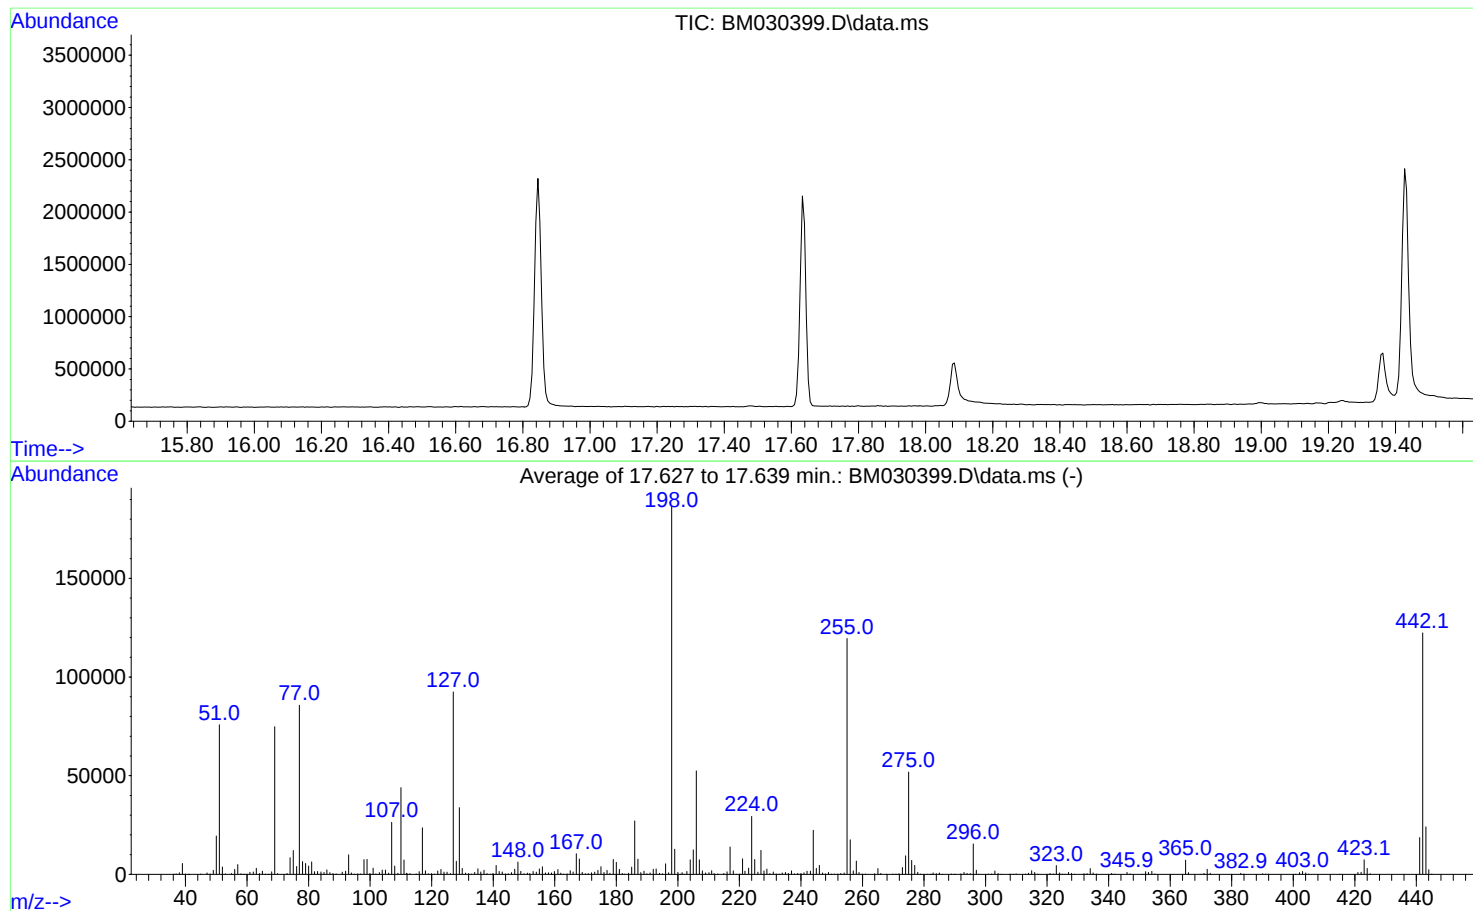

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	75807	PASS
68	69	0.00	2	1.7	1295	PASS
69	198	0.00	100	40.1	74812	PASS
70	69	0.00	2	0.6	442	PASS
127	198	10	80	49.6	92477	PASS
197	198	0.00	2	0.5	840	PASS
198	198	100	100	100.0	186411	PASS
199	198	5	9	6.8	12748	PASS
275	198	10	60	27.8	51824	PASS
365	198	1	100	3.9	7237	PASS
441	198	0.01	100	10.0	18634	PASS
442	442	50	100	100.0	122339	PASS
443	442	15	24	19.7	24121	PASS