

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061219\
 Data File : BM020898.D
 Acq On : 12 Jun 2019 11:10
 Operator : HP/JU
 Sample : K3006-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFHC0

Quant Time: Jun 12 16:18:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jun 09 01:02:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	293202	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	1204614	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.44	164	673012	20.00	ng/ul	-0.01
61) Phenanthrene-d10	17.19	188	1353835	20.00	ng/ul	0.00
77) Chrysene-d12	21.37	240	1159382	20.00	ng/ul	0.00
85) Perylene-d12	23.65	264	1347789	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	40258	6.55	ng/uL	0.00
5) Phenol-d5	6.97	99	805659	35.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	489847	36.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	703536	39.37	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	676476	37.48	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	341299	41.51	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.68	143	371963	43.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	723407	40.98	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.73	131	913007	42.95	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	2077974	41.74	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	2636882	41.77	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	212522	24.88	ng/ul	0.00
57) Fluorene-d10	15.43	176	1732101	40.94	ng/ul	-0.01
62) 4,6-Dinitro-2-methylphenol	15.56	200	115051	16.62	ng/ul	0.00
70) Anthracene-d10	17.29	188	2470803	41.78	ng/ul	0.00
78) Pyrene-d10	19.58	212	2456095	43.83	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.50	264	2632150	42.97	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.90	163	921374	18.484	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061219\
Data File : BM020898.D
Acq On : 12 Jun 2019 11:10
Operator : HP/JU
Sample : K3006-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFHC0

Quant Time: Jun 12 16:18:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jun 09 01:02:58 2019
Response via : Initial Calibration

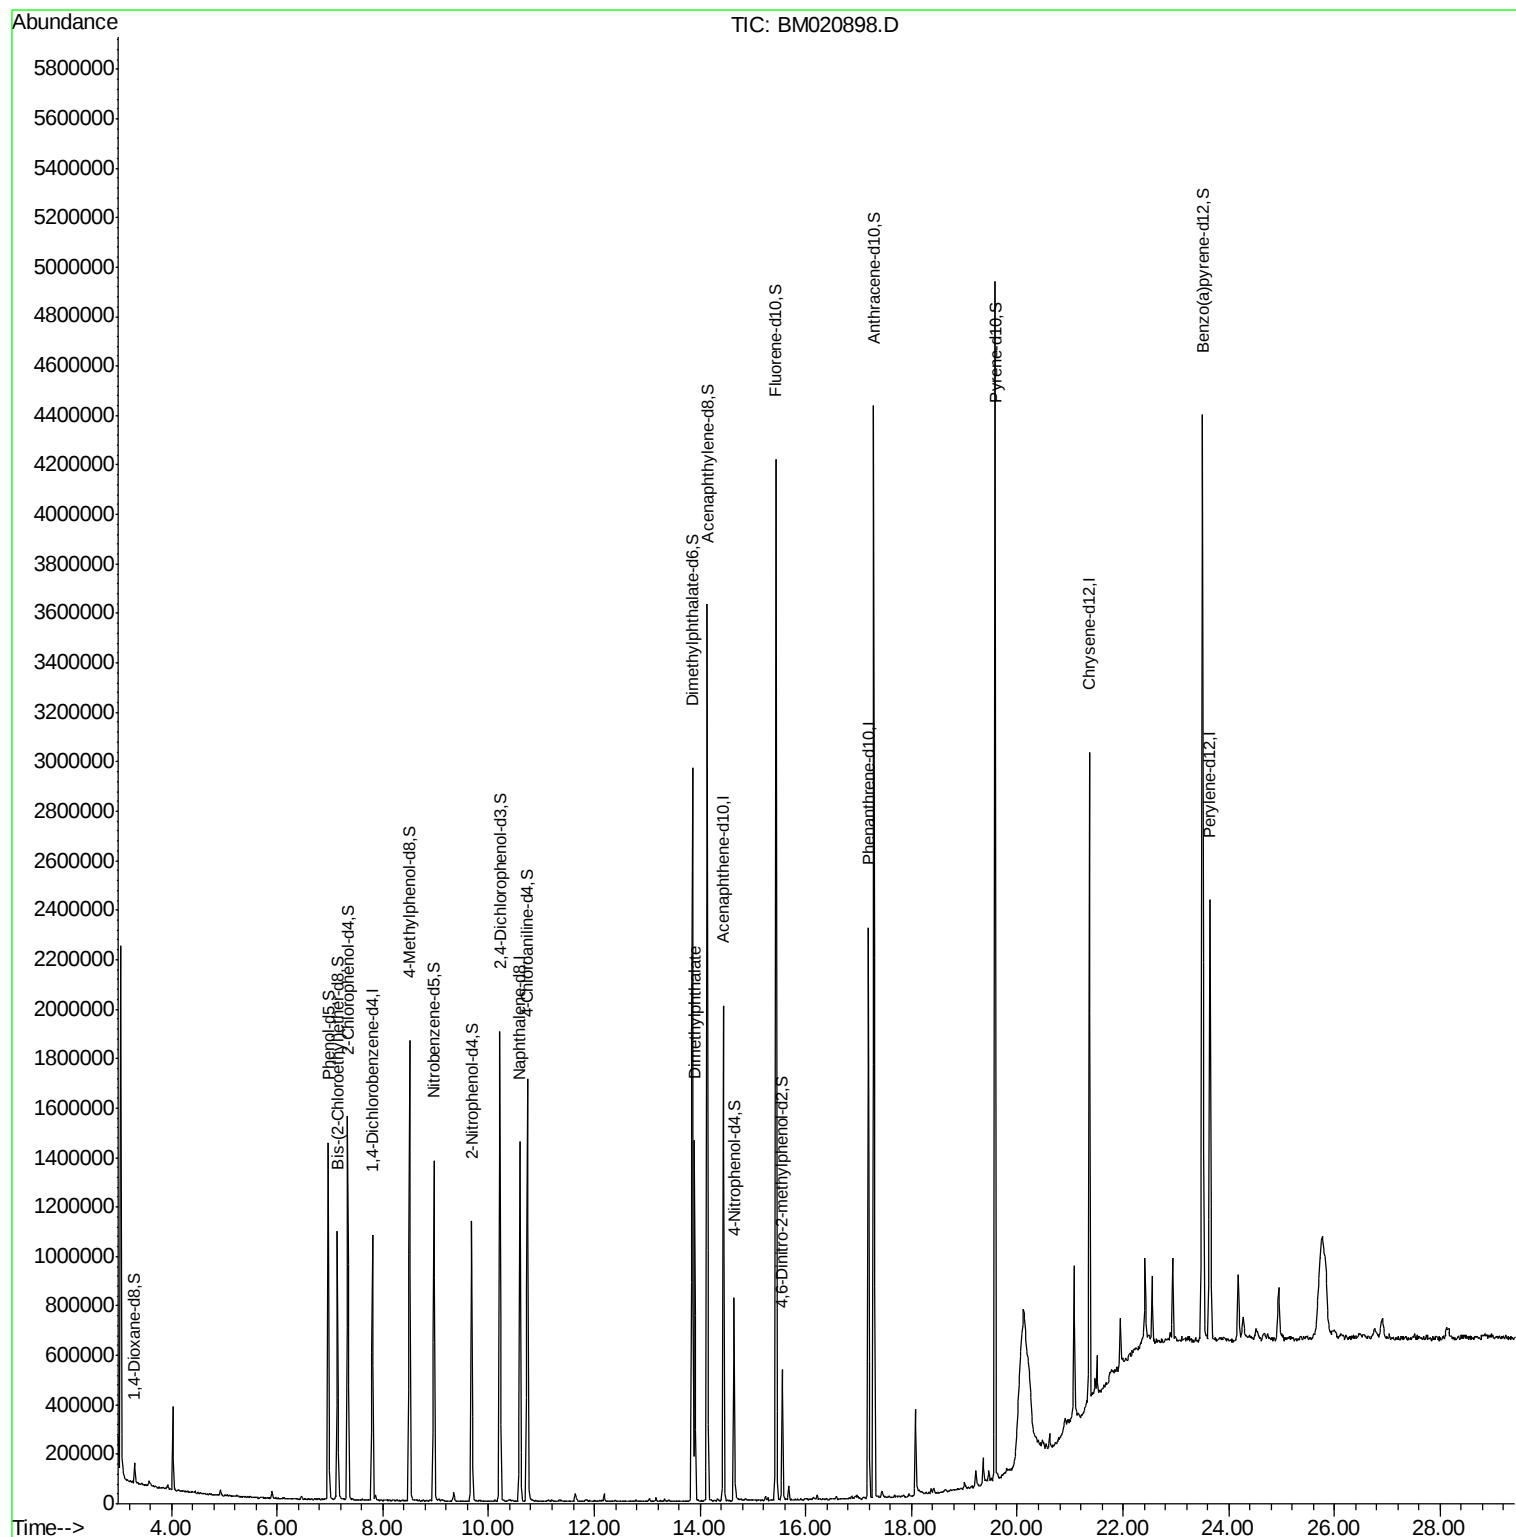

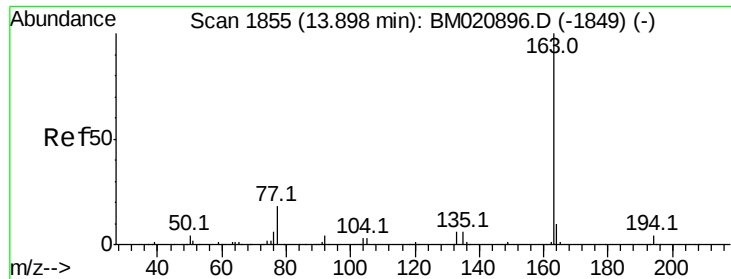

#44

Dimethylphthalate

Concen: 18.484 ng/ul

RT: 13.90 min Scan# 1855

Delta R.T. -0.01 min

Lab File: BM020898.D

Acq: 12 Jun 2019 11:10

Instrument :

BNA_M

ClientSampleId :

BFHC0


Tot Ion:163 Resp: 921374

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 10.2 8.0 12.0

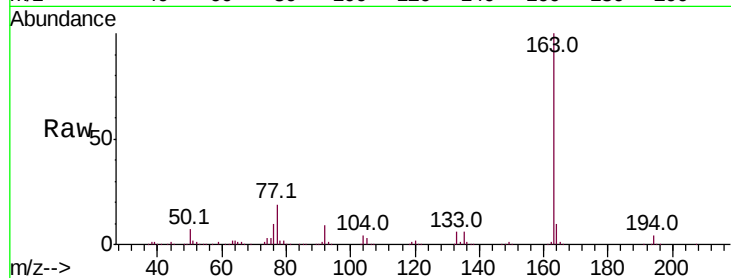

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

