

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061219\
 Data File : BM020917.D
 Acq On : 12 Jun 2019 23:21
 Operator : HP/JU
 Sample : K3215-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DB8J5

Quant Time: Jun 13 04:51:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 13 01:55:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	386731	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	1627460	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.44	164	907620	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	1745784	20.00	ng/ul	0.00
77) Chrysene-d12	21.37	240	1350545	20.00	ng/ul	0.00
85) Perylene-d12	23.65	264	1550852	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	11999	1.48	ng/uL	0.00
5) Phenol-d5	6.97	99	231425	7.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	549790	30.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	662537	28.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	430745	18.09	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	383304	34.51	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.68	143	447497	39.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	803899	33.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	62688	2.18	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	2573462	38.33	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	2984209	35.06	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	72586	6.30	ng/ul	0.00
57) Fluorene-d10	15.44	176	2006133	35.16	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	204762	22.94	ng/ul	0.00
70) Anthracene-d10	17.29	188	2700778	35.42	ng/ul	0.00
78) Pyrene-d10	19.58	212	2624703	40.21	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.50	264	2822556	40.04	ng/ul	0.00

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.90	163	85106	1.266	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061219\
 Data File : BM020917.D
 Acq On : 12 Jun 2019 23:21
 Operator : HP/JU
 Sample : K3215-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DB8J5

Quant Time: Jun 13 04:51:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 13 01:55:55 2019
 Response via : Initial Calibration

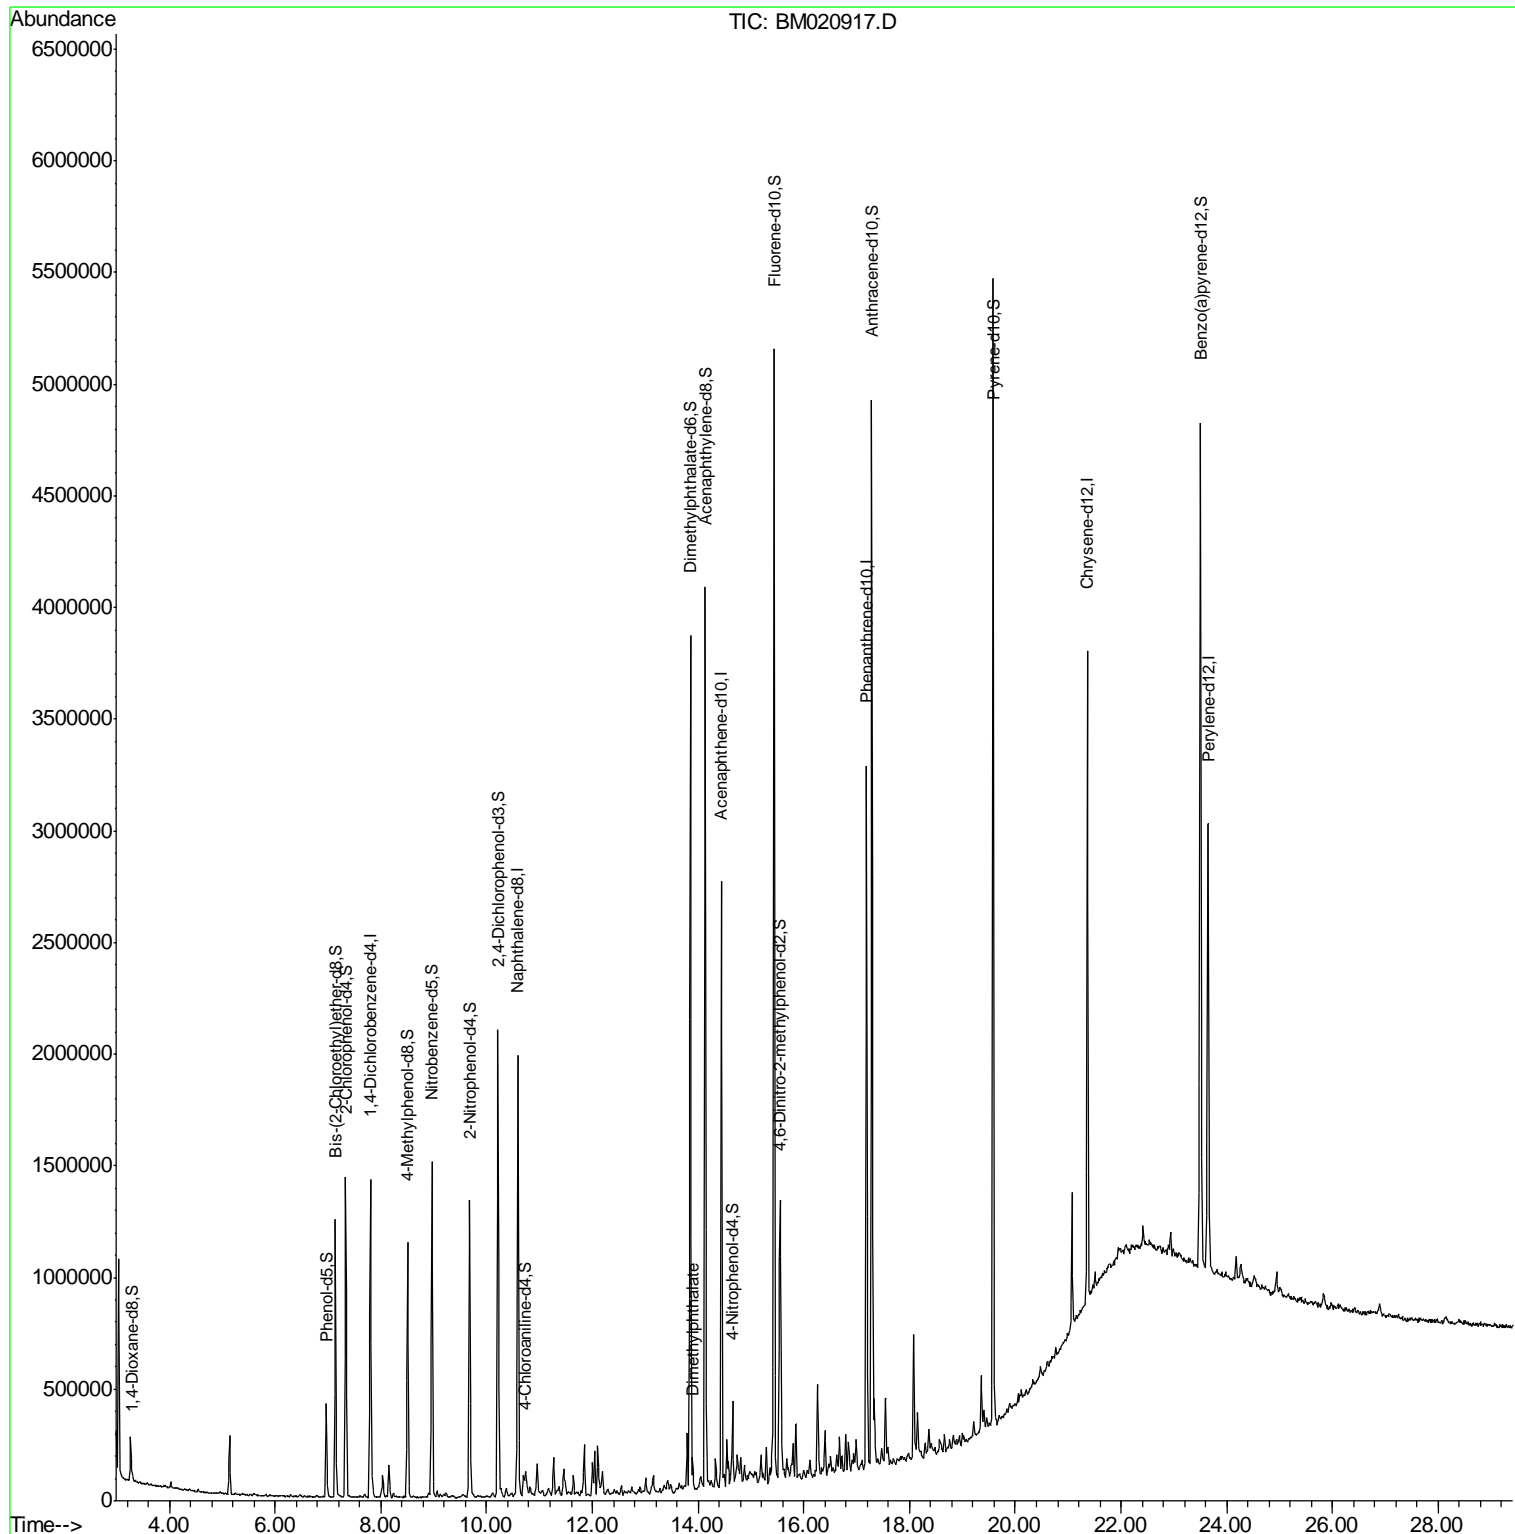

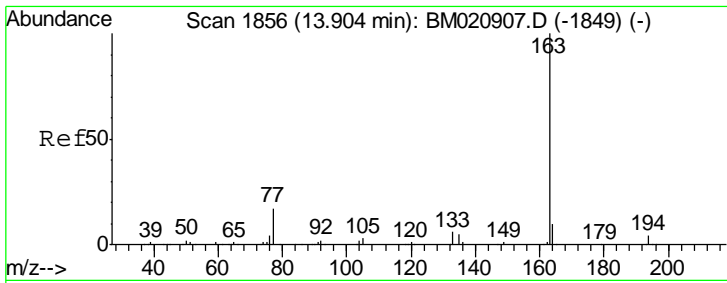

#44
 Dimethylphthalate
 Concen: 1.266 ng/ul
 RT: 13.90 min Scan# 1855
 Delta R.T. -0.01 min
 Lab File: BM020917.D
 Acq: 12 Jun 2019 23:21

Instrument :
 BNA_M
 ClientSampleId :
 DB8J5

Tot Ion:163 Resp: 85106

Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.2	4.8
164	10.0	8.0	12.0

